

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029522.D
 Acq On : 09 Dec 2022 15:34
 Operator : SY/MD
 Sample : N5920-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	216246	214565	15.32%	1.921%
2	1.565	155	163	178	rVB	161215	184288	13.16%	1.650%
3	2.105	320	331	345	rBV	323767	463875	33.12%	4.152%
4	2.404	422	424	427	rBV	203	144	0.01%	0.001%
5	2.558	468	472	479	rBV3	279	356	0.03%	0.003%
6	2.767	529	537	538	rBV2	597	648	0.05%	0.006%
7	2.880	569	572	580	rVB2	291	325	0.02%	0.003%
8	2.918	582	584	587	rBV2	161	102	0.01%	0.001%
9	3.072	628	632	633	rBV2	134	85	0.01%	0.001%
10	3.211	672	675	679	rVB2	350	169	0.01%	0.002%
11	3.278	692	696	701	rBV2	173	181	0.01%	0.002%
12	3.487	759	761	766	rBV	200	173	0.01%	0.002%
13	3.516	766	770	775	rVB2	278	249	0.02%	0.002%
14	3.542	775	778	782	rBV2	241	165	0.01%	0.001%
15	3.590	791	793	797	rBV2	175	120	0.01%	0.001%
16	3.693	821	825	830	rBV2	171	174	0.01%	0.002%
17	3.873	871	881	921	rBV	101189	283243	20.23%	2.535%
18	4.339	1008	1026	1059	rBV	215979	537402	38.37%	4.810%
19	4.603	1106	1108	1112	rBV2	411	216	0.02%	0.002%
20	4.664	1121	1127	1133	rBV3	292	383	0.03%	0.003%
21	4.712	1139	1142	1145	rBV2	201	139	0.01%	0.001%
22	4.741	1150	1151	1152	rVV2	258	68	0.00%	0.001%
23	4.764	1156	1158	1161	rVB2	131	67	0.00%	0.001%
24	4.828	1176	1178	1181	rVB	303	121	0.01%	0.001%
25	4.867	1188	1190	1194	rVB	205	104	0.01%	0.001%
26	4.896	1194	1199	1200	rBV	220	138	0.01%	0.001%
27	4.941	1209	1213	1217	rBV2	197	186	0.01%	0.002%
28	5.040	1226	1244	1283	rBV2	534031	1400407	100.00%	12.536%
29	5.336	1333	1336	1341	rVB2	380	336	0.02%	0.003%
30	5.378	1347	1349	1351	rBV	202	114	0.01%	0.001%
31	5.609	1408	1421	1460	rBV	476105	973377	69.51%	8.713%
32	5.905	1503	1513	1527	rVB7	3901	8350	0.60%	0.075%
33	5.953	1527	1528	1530	rBV	238	71	0.01%	0.001%
34	5.966	1530	1532	1534	rBV2	193	73	0.01%	0.001%
35	6.063	1548	1562	1587	rBV	298090	612736	43.75%	5.485%
36	6.317	1638	1641	1647	rVB3	308	315	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029522.D
 Acq On : 09 Dec 2022 15:34
 Operator : SY/MD
 Sample : N5920-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.384	1659	1662	1665	rBV	245	159	0.01%	0.001%
38	6.426	1673	1675	1679	rVB2	181	83	0.01%	0.001%
39	6.523	1703	1705	1711	rBV2	203	258	0.02%	0.002%
40	6.567	1715	1719	1722	rBV3	254	221	0.02%	0.002%
41	6.622	1727	1736	1739	rBV4	1042	1240	0.09%	0.011%
42	6.735	1768	1771	1772	rBV4	132	73	0.01%	0.001%
43	6.777	1782	1784	1788	rBV2	396	185	0.01%	0.002%
44	6.796	1788	1790	1791	rBV	124	70	0.00%	0.001%
45	6.825	1798	1799	1801	rBV	223	121	0.01%	0.001%
46	6.867	1811	1812	1815	rVB	177	72	0.01%	0.001%
47	6.892	1818	1820	1823	rBV2	360	175	0.01%	0.002%
48	6.934	1828	1833	1835	rBV2	285	226	0.02%	0.002%
49	6.979	1835	1847	1879	rBV	145578	267843	19.13%	2.398%
50	7.307	1936	1949	1987	rBV	656220	1169176	83.49%	10.466%
51	7.612	2034	2044	2063	rBV	101939	181381	12.95%	1.624%
52	7.928	2137	2142	2151	rBV2	2622	4397	0.31%	0.039%
53	8.082	2180	2190	2225	rBV	366885	669888	47.84%	5.996%
54	8.519	2324	2326	2328	rBV2	347	182	0.01%	0.002%
55	8.558	2335	2338	2341	rVB	393	247	0.02%	0.002%
56	8.584	2344	2346	2348	rBV2	371	209	0.01%	0.002%
57	8.657	2365	2369	2371	rBV2	230	162	0.01%	0.001%
58	8.696	2378	2381	2384	rBV3	342	276	0.02%	0.002%
59	8.735	2388	2393	2396	rBV2	414	373	0.03%	0.003%
60	8.764	2399	2402	2403	rBV	364	204	0.01%	0.002%
61	8.844	2414	2427	2462	rBV	684845	1142759	81.60%	10.229%
62	9.137	2514	2518	2527	rVB5	1091	1528	0.11%	0.014%
63	9.172	2527	2529	2533	rBV2	450	341	0.02%	0.003%
64	9.262	2555	2557	2560	rBV2	216	160	0.01%	0.001%
65	9.410	2601	2603	2605	rVB	230	110	0.01%	0.001%
66	9.474	2621	2623	2628	rVB2	334	207	0.01%	0.002%
67	9.542	2638	2644	2650	rBV4	492	693	0.05%	0.006%
68	9.616	2665	2667	2669	rBV2	208	97	0.01%	0.001%
69	9.667	2680	2683	2687	rBV	227	134	0.01%	0.001%
70	9.690	2687	2690	2691	rBV	202	101	0.01%	0.001%
71	9.719	2696	2699	2704	rBV3	318	319	0.02%	0.003%
72	9.770	2711	2715	2718	rBV2	224	180	0.01%	0.002%
73	9.828	2730	2733	2735	rBV2	214	123	0.01%	0.001%
74	9.841	2735	2737	2741	rBV	287	174	0.01%	0.002%
75	9.902	2754	2756	2757	rBV2	281	117	0.01%	0.001%
76	9.956	2771	2773	2775	rBV	228	113	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029522.D
 Acq On : 09 Dec 2022 15:34
 Operator : SY/MD
 Sample : N5920-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.989	2781	2783	2786	rVB2	368	181	0.01%	0.002%
78	10.030	2792	2796	2799	rBV2	338	245	0.02%	0.002%
79	10.162	2827	2837	2841	rBV	22520	32660	2.33%	0.292%
80	10.204	2842	2850	2874	rVB	435755	685449	48.95%	6.136%
81	10.374	2897	2903	2911	rVB3	2716	3980	0.28%	0.036%
82	10.439	2920	2923	2929	rVB3	330	282	0.02%	0.003%
83	10.500	2939	2942	2944	rBV3	235	173	0.01%	0.002%
84	10.529	2945	2951	2953	rBV4	562	573	0.04%	0.005%
85	10.567	2955	2963	2975	rVB2	11272	16976	1.21%	0.152%
86	10.696	3000	3003	3004	rBV2	156	77	0.01%	0.001%
87	10.728	3012	3013	3015	rBV2	181	88	0.01%	0.001%
88	10.902	3062	3067	3076	rBV4	1143	1592	0.11%	0.014%
89	11.021	3102	3104	3110	rVB2	221	126	0.01%	0.001%
90	11.046	3110	3112	3114	rBV	146	78	0.01%	0.001%
91	11.172	3145	3151	3158	rBV5	1198	1496	0.11%	0.013%
92	11.239	3159	3172	3190	rBV	765788	1198367	85.57%	10.727%
93	11.554	3264	3270	3276	rBV4	1674	2359	0.17%	0.021%
94	11.612	3276	3288	3307	rBV	693969	1097353	78.36%	9.823%
95	11.963	3394	3397	3402	rVB3	415	305	0.02%	0.003%
96	12.066	3424	3429	3433	rBV2	439	399	0.03%	0.004%
97	12.210	3472	3474	3475	rBV2	337	141	0.01%	0.001%
98	12.606	3595	3597	3600	rBV	445	305	0.02%	0.003%
99	12.696	3622	3625	3627	rBV2	327	193	0.01%	0.002%
100	13.172	3770	3773	3774	rBV2	474	248	0.02%	0.002%


Sum of corrected areas: 11171488

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029522.D
Acq On : 09 Dec 2022 15:34
Operator : SY/MD
Sample : N5920-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

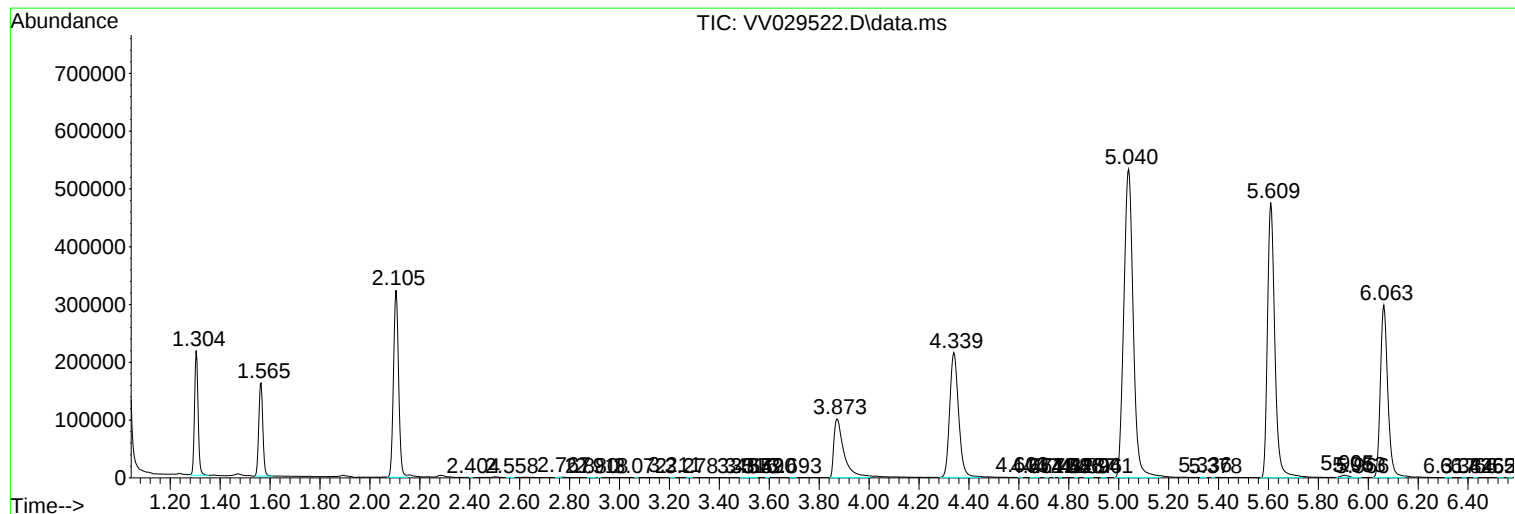

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029522.D
Acq On : 09 Dec 2022 15:34
Operator : SY/MD
Sample : N5920-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029522.D
Acq On : 09 Dec 2022 15:34
Operator : SY/MD
Sample : N5920-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc