

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029523.D
 Acq On : 09 Dec 2022 15:57
 Operator : SY/MD
 Sample : N5920-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	230271	230493	14.67%	1.910%
2	1.564	155	163	177	rVB	187119	208592	13.28%	1.728%
3	2.105	320	331	345	rBV	359507	520592	33.14%	4.314%
4	2.500	450	454	462	rVB5	1319	1848	0.12%	0.015%
5	2.597	482	484	485	rBV5	177	68	0.00%	0.001%
6	2.851	561	563	566	rBV	178	121	0.01%	0.001%
7	2.899	575	578	580	rBV3	212	145	0.01%	0.001%
8	3.011	609	613	615	rBV2	141	107	0.01%	0.001%
9	3.040	620	622	625	rVV2	236	121	0.01%	0.001%
10	3.085	634	636	639	rVB	226	86	0.01%	0.001%
11	3.307	702	705	709	rBV	214	136	0.01%	0.001%
12	3.423	737	741	744	rBV	160	152	0.01%	0.001%
13	3.490	759	762	763	rBV	170	100	0.01%	0.001%
14	3.558	773	783	784	rBV	299	360	0.02%	0.003%
15	3.625	801	804	806	rBV	205	124	0.01%	0.001%
16	3.677	814	820	823	rBV2	247	298	0.02%	0.002%
17	3.719	828	833	836	rBV2	253	169	0.01%	0.001%
18	3.764	843	847	848	rBV2	212	113	0.01%	0.001%
19	3.870	870	880	931	rBV	115131	317935	20.24%	2.634%
20	4.339	1009	1026	1052	rBV	241162	595857	37.93%	4.937%
21	4.593	1103	1105	1108	rBV	260	191	0.01%	0.002%
22	4.635	1115	1118	1120	rBV3	151	107	0.01%	0.001%
23	4.664	1123	1127	1132	rBV3	345	263	0.02%	0.002%
24	4.683	1132	1133	1135	rBV	183	54	0.00%	0.000%
25	4.712	1140	1142	1146	rBV3	254	154	0.01%	0.001%
26	4.757	1151	1156	1158	rBV	198	173	0.01%	0.001%
27	4.831	1177	1179	1183	rVB2	221	116	0.01%	0.001%
28	4.928	1207	1209	1211	rBV	102	50	0.00%	0.000%
29	4.960	1217	1219	1222	rVB	195	64	0.00%	0.001%
30	5.040	1226	1244	1284	rBV2	595964	1570766	100.00%	13.015%
31	5.404	1351	1357	1363	rBV3	494	672	0.04%	0.006%
32	5.471	1373	1378	1381	rBV2	484	481	0.03%	0.004%
33	5.532	1394	1397	1398	rBV2	317	160	0.01%	0.001%
34	5.609	1408	1421	1461	rBV	481308	986369	62.80%	8.173%
35	5.912	1502	1515	1529	rVB9	6095	14060	0.90%	0.116%
36	6.008	1538	1545	1548	rBV3	527	661	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029523.D
 Acq On : 09 Dec 2022 15:57
 Operator : SY/MD
 Sample : N5920-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1548	1562	1590	rBV	335089	690818	43.98%	5.724%
38	6.339	1647	1648	1652	rVB	289	93	0.01%	0.001%
39	6.368	1652	1657	1661	rBV2	274	249	0.02%	0.002%
40	6.384	1661	1662	1664	rBV	207	63	0.00%	0.001%
41	6.420	1669	1673	1674	rBV2	290	192	0.01%	0.002%
42	6.429	1674	1676	1681	rVB2	451	270	0.02%	0.002%
43	6.458	1682	1685	1688	rBV	98	75	0.00%	0.001%
44	6.532	1705	1708	1709	rBV	112	49	0.00%	0.000%
45	6.542	1709	1711	1714	rVB2	242	118	0.01%	0.001%
46	6.561	1714	1717	1721	rBV	165	178	0.01%	0.001%
47	6.625	1729	1737	1744	rBV6	1218	2198	0.14%	0.018%
48	6.709	1761	1763	1765	rBV	293	164	0.01%	0.001%
49	6.776	1782	1784	1786	rBV	192	96	0.01%	0.001%
50	6.793	1787	1789	1793	rBV3	174	112	0.01%	0.001%
51	6.879	1813	1816	1819	rVB	221	88	0.01%	0.001%
52	6.908	1822	1825	1828	rVB2	260	139	0.01%	0.001%
53	6.928	1828	1831	1832	rBV	100	55	0.00%	0.000%
54	6.940	1832	1835	1836	rBV	222	112	0.01%	0.001%
55	6.979	1836	1847	1880	rBV	160412	301096	19.17%	2.495%
56	7.307	1937	1949	1984	rBV	736941	1306840	83.20%	10.828%
57	7.616	2032	2045	2074	rBV	112272	204291	13.01%	1.693%
58	7.799	2101	2102	2112	rBV3	412	397	0.03%	0.003%
59	7.934	2135	2144	2150	rBV4	3162	5714	0.36%	0.047%
60	8.082	2180	2190	2234	rBV	400277	729421	46.44%	6.044%
61	8.648	2364	2366	2368	rBV2	338	192	0.01%	0.002%
62	8.696	2379	2381	2384	rVB	160	96	0.01%	0.001%
63	8.719	2384	2388	2390	rBV2	334	244	0.02%	0.002%
64	8.760	2396	2401	2402	rBV3	257	191	0.01%	0.002%
65	8.844	2415	2427	2456	rBV	704071	1160649	73.89%	9.617%
66	9.191	2533	2535	2537	rVB2	215	83	0.01%	0.001%
67	9.207	2537	2540	2543	rBV	270	169	0.01%	0.001%
68	9.227	2543	2546	2548	rBV2	196	138	0.01%	0.001%
69	9.339	2579	2581	2587	rVB2	352	195	0.01%	0.002%
70	9.368	2587	2590	2594	rBV3	235	186	0.01%	0.002%
71	9.387	2594	2596	2597	rBV	133	74	0.00%	0.001%
72	9.403	2599	2601	2602	rBV2	179	51	0.00%	0.000%
73	9.535	2636	2642	2648	rBV4	713	899	0.06%	0.007%
74	9.564	2648	2651	2652	rBV	211	113	0.01%	0.001%
75	9.670	2682	2684	2686	rBV	206	109	0.01%	0.001%
76	9.706	2692	2695	2696	rBV	173	100	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029523.D
 Acq On : 09 Dec 2022 15:57
 Operator : SY/MD
 Sample : N5920-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.731	2700	2703	2707	rVB2	210	146	0.01%	0.001%
78	9.809	2723	2727	2730	rBV3	274	232	0.01%	0.002%
79	9.825	2730	2732	2735	rVB	423	176	0.01%	0.001%
80	9.844	2735	2738	2740	rBV2	328	219	0.01%	0.002%
81	9.863	2740	2744	2750	rVB2	347	325	0.02%	0.003%
82	9.895	2750	2754	2755	rBV	270	173	0.01%	0.001%
83	9.921	2759	2762	2764	rBV	294	231	0.01%	0.002%
84	10.108	2816	2820	2821	rBV	179	92	0.01%	0.001%
85	10.127	2823	2826	2827	rVV	325	188	0.01%	0.002%
86	10.162	2828	2837	2841	rVV2	26835	38884	2.48%	0.322%
87	10.207	2842	2851	2878	rVB	487722	776248	49.42%	6.432%
88	10.371	2894	2902	2910	rBV5	3464	5843	0.37%	0.048%
89	10.532	2944	2952	2954	rBV4	861	1022	0.07%	0.008%
90	10.567	2955	2963	2974	rVB	13006	20991	1.34%	0.174%
91	10.670	2992	2995	2997	rBV2	184	107	0.01%	0.001%
92	10.728	3009	3013	3014	rBV2	363	224	0.01%	0.002%
93	10.902	3062	3067	3069	rBV4	1207	1052	0.07%	0.009%
94	11.056	3113	3115	3118	rBV	243	185	0.01%	0.002%
95	11.095	3124	3127	3132	rBV3	495	471	0.03%	0.004%
96	11.239	3160	3172	3192	rBV	766775	1198353	76.29%	9.929%
97	11.551	3262	3269	3270	rBV3	1737	1427	0.09%	0.012%
98	11.612	3276	3288	3314	rBV	748499	1163620	74.08%	9.642%
99	11.908	3377	3380	3383	rBV3	216	199	0.01%	0.002%
100	12.194	3468	3469	3473	rVB	362	216	0.01%	0.002%




Sum of corrected areas: 12068699

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029523.D
Acq On : 09 Dec 2022 15:57
Operator : SY/MD
Sample : N5920-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

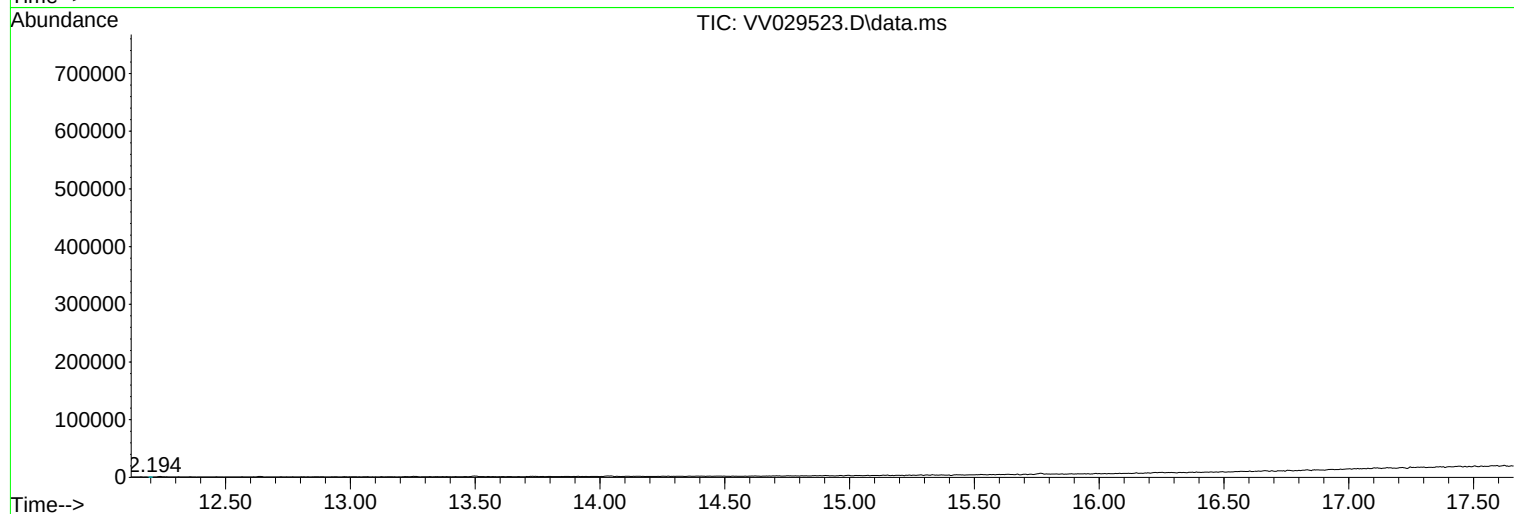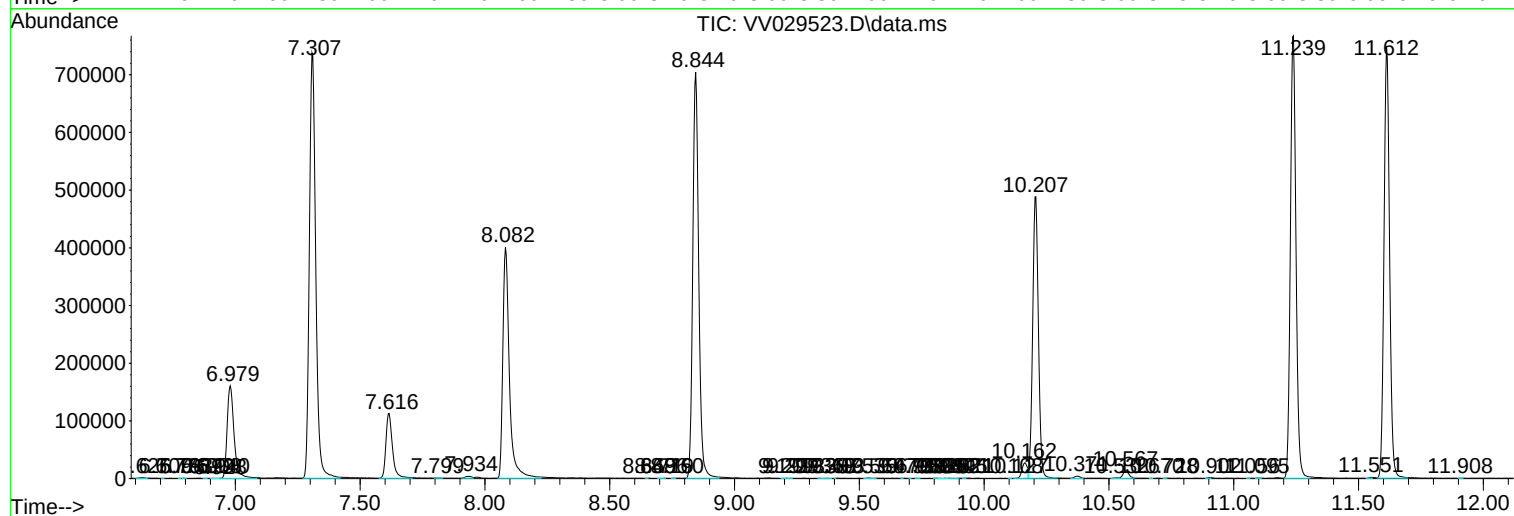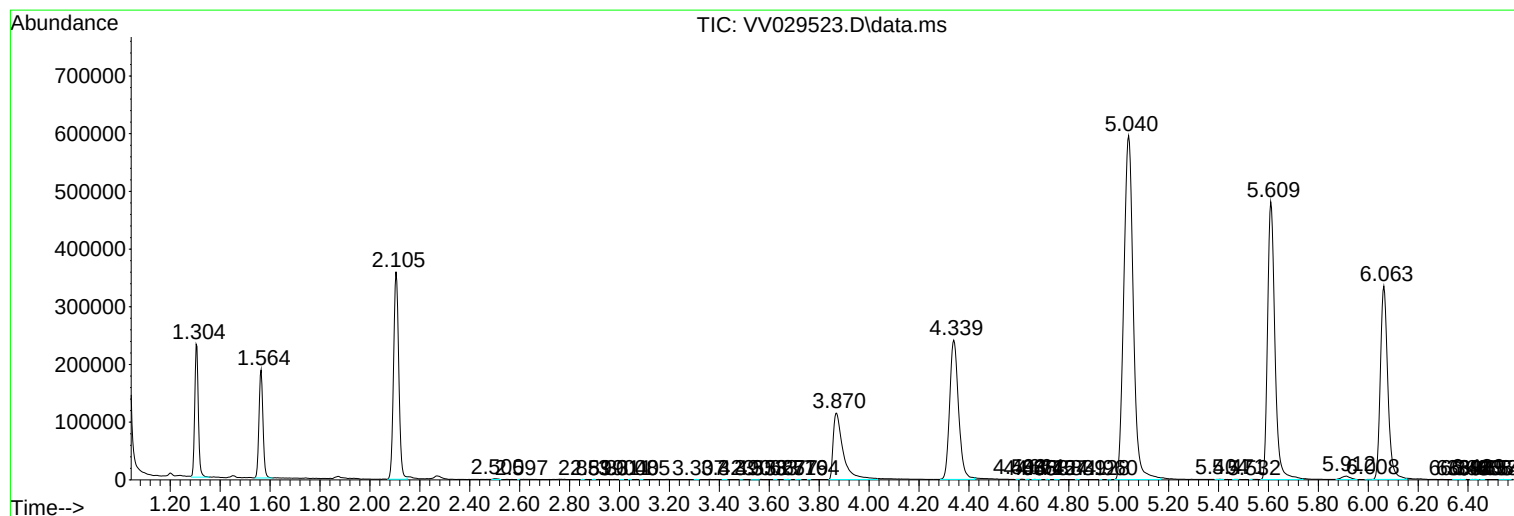

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029523.D
Acq On : 09 Dec 2022 15:57
Operator : SY/MD
Sample : N5920-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029523.D
Acq On : 09 Dec 2022 15:57
Operator : SY/MD
Sample : N5920-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------