

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029525.D
 Acq On : 09 Dec 2022 16:44
 Operator : SY/MD
 Sample : N5959-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	231765	228083	14.63%	1.807%
2	1.564	155	163	180	rVB	188594	209147	13.42%	1.657%
3	2.105	320	331	344	rBV	359333	517526	33.20%	4.101%
4	2.468	441	444	445	rBV	187	114	0.01%	0.001%
5	2.477	445	447	449	rVV	373	216	0.01%	0.002%
6	2.500	449	454	462	rVB3	1557	2331	0.15%	0.018%
7	2.535	462	465	467	rBV3	224	140	0.01%	0.001%
8	2.625	481	493	501	rBV3	2267	4658	0.30%	0.037%
9	2.754	530	533	534	rBV	360	205	0.01%	0.002%
10	2.789	542	544	547	rBV2	301	172	0.01%	0.001%
11	2.812	548	551	554	rVB2	322	223	0.01%	0.002%
12	2.847	558	562	564	rBV	158	122	0.01%	0.001%
13	2.957	593	596	600	rBV2	164	114	0.01%	0.001%
14	2.979	600	603	606	rVB3	285	168	0.01%	0.001%
15	3.339	712	715	719	rVB2	198	126	0.01%	0.001%
16	3.468	752	755	756	rBV	300	139	0.01%	0.001%
17	3.516	767	770	776	rVB2	298	255	0.02%	0.002%
18	3.548	776	780	786	rVB2	197	186	0.01%	0.001%
19	3.661	811	815	817	rBV2	163	126	0.01%	0.001%
20	3.709	826	830	833	rBV2	192	140	0.01%	0.001%
21	3.754	839	844	847	rBV2	159	138	0.01%	0.001%
22	3.870	870	880	920	rBV	113396	313917	20.14%	2.487%
23	4.339	1010	1026	1059	rBV	239662	599883	38.49%	4.753%
24	4.583	1099	1102	1104	rBV3	268	174	0.01%	0.001%
25	4.612	1110	1111	1113	rVB3	340	131	0.01%	0.001%
26	4.661	1123	1126	1128	rBV2	342	223	0.01%	0.002%
27	4.693	1134	1136	1145	rVB3	359	287	0.02%	0.002%
28	4.892	1195	1198	1205	rVB2	342	340	0.02%	0.003%
29	4.937	1205	1212	1216	rBV2	304	321	0.02%	0.003%
30	5.040	1226	1244	1275	rBV2	593607	1558714	100.00%	12.350%
31	5.526	1392	1395	1398	rVB2	251	146	0.01%	0.001%
32	5.609	1407	1421	1455	rBV	529963	1086243	69.69%	8.607%
33	5.908	1502	1514	1541	rBV	71466	152912	9.81%	1.212%
34	6.063	1548	1562	1593	rBV	335151	689634	44.24%	5.464%
35	6.265	1623	1625	1631	rVB4	447	325	0.02%	0.003%
36	6.381	1658	1661	1664	rVV2	218	160	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029525.D
 Acq On : 09 Dec 2022 16:44
 Operator : SY/MD
 Sample : N5959-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.403	1664	1668	1672	rVB	212	113	0.01%	0.001%
38	6.452	1682	1683	1688	rVB	216	153	0.01%	0.001%
39	6.484	1688	1693	1696	rBV	362	348	0.02%	0.003%
40	6.590	1722	1726	1728	rBV2	210	118	0.01%	0.001%
41	6.632	1728	1739	1741	rBV4	1089	1658	0.11%	0.013%
42	6.725	1765	1768	1773	rVB2	361	280	0.02%	0.002%
43	6.754	1773	1777	1780	rBV2	231	149	0.01%	0.001%
44	6.879	1813	1816	1821	rBV2	255	235	0.02%	0.002%
45	6.918	1825	1828	1831	rBV2	213	117	0.01%	0.001%
46	6.979	1836	1847	1880	rBV	163033	303333	19.46%	2.403%
47	7.310	1934	1950	1982	rBV	749164	1309602	84.02%	10.376%
48	7.612	2035	2044	2072	rBV	112583	198675	12.75%	1.574%
49	7.844	2114	2116	2117	rBV	286	125	0.01%	0.001%
50	7.937	2135	2145	2152	rBV3	4089	7540	0.48%	0.060%
51	8.082	2179	2190	2234	rBV	398769	729445	46.80%	5.780%
52	8.564	2336	2340	2342	rBV	253	212	0.01%	0.002%
53	8.709	2383	2385	2388	rBV	236	131	0.01%	0.001%
54	8.844	2415	2427	2456	rBV	772745	1283911	82.37%	10.173%
55	9.095	2503	2505	2509	rVB3	219	132	0.01%	0.001%
56	9.140	2513	2519	2527	rVB5	873	1299	0.08%	0.010%
57	9.207	2537	2540	2542	rVB3	316	163	0.01%	0.001%
58	9.223	2542	2545	2548	rBV3	212	155	0.01%	0.001%
59	9.320	2573	2575	2580	rVB2	249	140	0.01%	0.001%
60	9.349	2581	2584	2587	rVV2	242	206	0.01%	0.002%
61	9.378	2590	2593	2596	rVB	406	246	0.02%	0.002%
62	9.542	2639	2644	2647	rVV3	527	512	0.03%	0.004%
63	9.609	2663	2665	2670	rVB2	238	144	0.01%	0.001%
64	9.635	2670	2673	2677	rBV3	245	220	0.01%	0.002%
65	9.686	2685	2689	2693	rBV2	413	344	0.02%	0.003%
66	9.728	2700	2702	2706	rVB2	295	162	0.01%	0.001%
67	9.754	2706	2710	2714	rBV2	196	157	0.01%	0.001%
68	9.850	2737	2740	2744	rBV	285	227	0.01%	0.002%
69	9.953	2769	2772	2775	rBV2	214	178	0.01%	0.001%
70	10.021	2790	2793	2796	rBV	273	174	0.01%	0.001%
71	10.117	2820	2823	2825	rBV	306	200	0.01%	0.002%
72	10.162	2828	2837	2841	rBV2	24785	36725	2.36%	0.291%
73	10.207	2842	2851	2867	rVB	494124	772642	49.57%	6.122%
74	10.326	2887	2888	2892	rVB2	337	161	0.01%	0.001%
75	10.374	2892	2903	2915	rBV2	4906	8353	0.54%	0.066%
76	10.445	2921	2925	2927	rBV3	227	155	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029525.D
 Acq On : 09 Dec 2022 16:44
 Operator : SY/MD
 Sample : N5959-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.525	2946	2950	2952	rBV3	671	486	0.03%	0.004%
78	10.567	2954	2963	2975	rVB2	12075	19760	1.27%	0.157%
79	10.654	2987	2990	2994	rBV	164	156	0.01%	0.001%
80	10.699	3002	3004	3009	rBV2	378	320	0.02%	0.003%
81	10.722	3009	3011	3015	rBV	198	140	0.01%	0.001%
82	10.840	3045	3048	3051	rBV	380	302	0.02%	0.002%
83	10.863	3053	3055	3057	rVB2	336	153	0.01%	0.001%
84	10.908	3062	3069	3078	rBV4	1025	1638	0.11%	0.013%
85	10.940	3078	3079	3082	rVB2	389	145	0.01%	0.001%
86	10.966	3082	3087	3088	rBV2	263	165	0.01%	0.001%
87	11.066	3115	3118	3121	rBV2	219	162	0.01%	0.001%
88	11.088	3122	3125	3127	rBV2	265	166	0.01%	0.001%
89	11.140	3138	3141	3143	rBV	283	157	0.01%	0.001%
90	11.156	3143	3146	3147	rBV	253	165	0.01%	0.001%
91	11.168	3147	3150	3154	rBV3	885	890	0.06%	0.007%
92	11.236	3159	3171	3197	rBV	843631	1335608	85.69%	10.583%
93	11.558	3265	3271	3276	rBV6	1884	3121	0.20%	0.025%
94	11.612	3277	3288	3317	rVB	777057	1227984	78.78%	9.730%
95	11.815	3348	3351	3358	rBV4	419	477	0.03%	0.004%
96	12.053	3421	3425	3427	rBV2	243	202	0.01%	0.002%
97	12.159	3456	3458	3461	rBV2	276	157	0.01%	0.001%
98	12.638	3602	3607	3608	rBV2	522	464	0.03%	0.004%
99	12.998	3717	3719	3722	rBV3	424	284	0.02%	0.002%
100	13.252	3794	3798	3804	rVB4	1121	1165	0.07%	0.009%




Sum of corrected areas: 12620846

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029525.D
Acq On : 09 Dec 2022 16:44
Operator : SY/MD
Sample : N5959-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

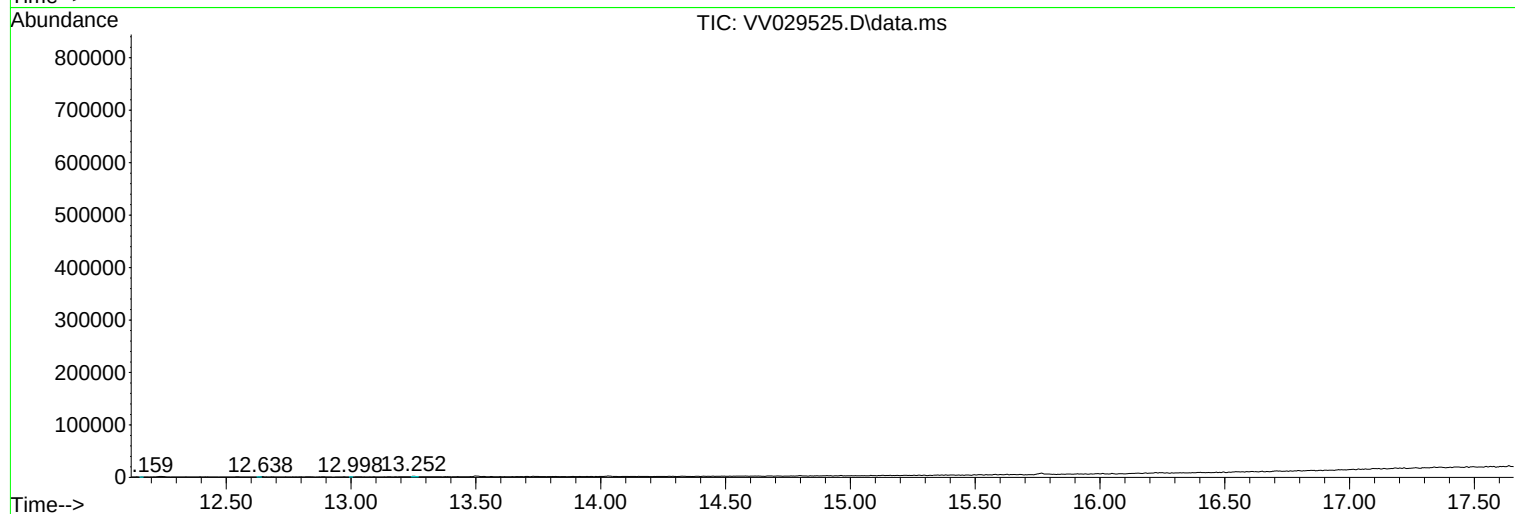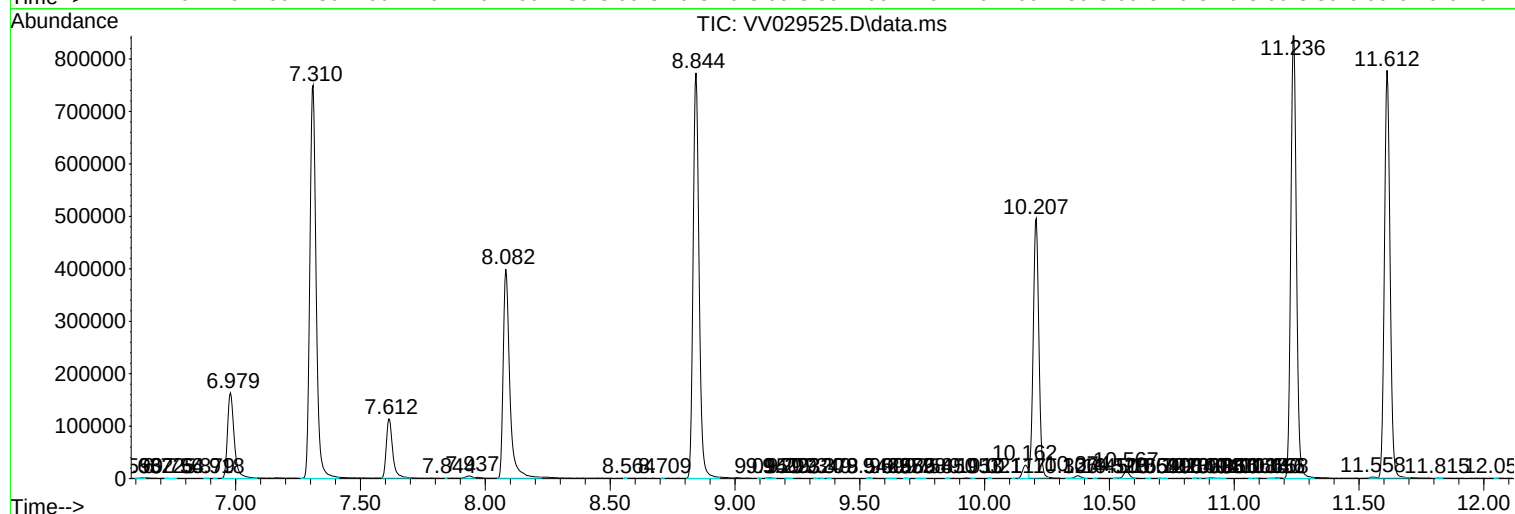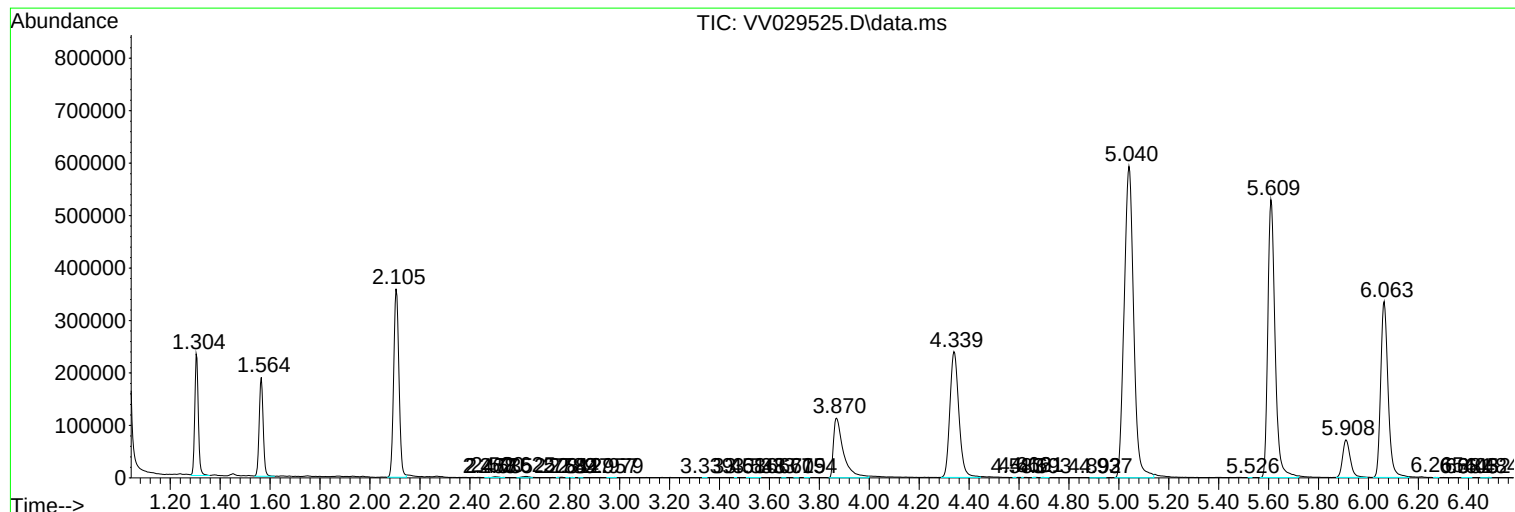

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029525.D
Acq On : 09 Dec 2022 16:44
Operator : SY/MD
Sample : N5959-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029525.D
Acq On : 09 Dec 2022 16:44
Operator : SY/MD
Sample : N5959-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------