

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029526.D
 Acq On : 09 Dec 2022 17:07
 Operator : SY/MD
 Sample : N5959-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	226359	220309	14.23%	1.797%
2	1.564	155	163	176	rVB	180863	199501	12.88%	1.628%
3	2.105	320	331	345	rBV	351275	506341	32.70%	4.131%
4	2.458	436	441	443	rBV2	319	330	0.02%	0.003%
5	2.506	449	456	464	rVB2	1060	1478	0.10%	0.012%
6	2.773	531	539	542	rBV3	441	644	0.04%	0.005%
7	2.825	551	555	557	rBV	173	127	0.01%	0.001%
8	2.838	557	559	561	rVB	218	97	0.01%	0.001%
9	2.931	584	588	590	rBV2	233	163	0.01%	0.001%
10	2.947	591	593	596	rBV2	184	122	0.01%	0.001%
11	3.188	661	668	670	rBV3	325	315	0.02%	0.003%
12	3.320	707	709	713	rBV	256	125	0.01%	0.001%
13	3.535	773	776	779	rBV	196	105	0.01%	0.001%
14	3.580	786	790	794	rBV	378	234	0.02%	0.002%
15	3.677	814	820	825	rBV2	251	282	0.02%	0.002%
16	3.706	827	829	833	rVB2	288	166	0.01%	0.001%
17	3.728	833	836	840	rVB	161	130	0.01%	0.001%
18	3.751	840	843	847	rBV	121	130	0.01%	0.001%
19	3.812	858	862	864	rBV2	178	156	0.01%	0.001%
20	3.870	870	880	924	rBV	114659	318824	20.59%	2.601%
21	4.339	1009	1026	1062	rBV	237542	591251	38.18%	4.824%
22	4.590	1102	1104	1107	rBV2	239	179	0.01%	0.001%
23	4.603	1107	1108	1115	rVB3	370	341	0.02%	0.003%
24	4.677	1129	1131	1134	rBV	236	114	0.01%	0.001%
25	4.715	1139	1143	1146	rBV2	274	225	0.01%	0.002%
26	4.747	1149	1153	1155	rBV	255	197	0.01%	0.002%
27	4.764	1156	1158	1160	rBV2	169	87	0.01%	0.001%
28	4.818	1172	1175	1180	rBV2	235	209	0.01%	0.002%
29	4.860	1184	1188	1190	rBV2	170	125	0.01%	0.001%
30	4.947	1213	1215	1219	rBV2	180	144	0.01%	0.001%
31	4.976	1222	1224	1226	rVB	157	77	0.00%	0.001%
32	5.040	1226	1244	1291	rBV2	588211	1548400	100.00%	12.633%
33	5.609	1408	1421	1452	rBV	524257	1068169	68.99%	8.715%
34	5.989	1538	1539	1542	rBV	191	105	0.01%	0.001%
35	6.063	1548	1562	1596	rBV	330394	680912	43.98%	5.555%
36	6.294	1629	1634	1637	rBV3	415	337	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029526.D
 Acq On : 09 Dec 2022 17:07
 Operator : SY/MD
 Sample : N5959-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.374	1650	1659	1664	rVB3	345	463	0.03%	0.004%
38	6.403	1664	1668	1669	rBV	128	84	0.01%	0.001%
39	6.474	1684	1690	1694	rBV2	208	187	0.01%	0.002%
40	6.516	1700	1703	1704	rBV	156	88	0.01%	0.001%
41	6.542	1707	1711	1715	rVB2	182	151	0.01%	0.001%
42	6.564	1715	1718	1720	rBV	208	101	0.01%	0.001%
43	6.587	1722	1725	1729	rVB2	252	168	0.01%	0.001%
44	6.628	1729	1738	1750	rBV4	1007	2619	0.17%	0.021%
45	6.738	1768	1772	1773	rBV	216	121	0.01%	0.001%
46	6.751	1774	1776	1778	rVV	399	218	0.01%	0.002%
47	6.763	1778	1780	1785	rVV	318	222	0.01%	0.002%
48	6.792	1786	1789	1795	rVB2	194	144	0.01%	0.001%
49	6.821	1796	1798	1801	rBV3	211	159	0.01%	0.001%
50	6.886	1815	1818	1820	rBV2	247	117	0.01%	0.001%
51	6.921	1826	1829	1832	rBV	247	104	0.01%	0.001%
52	6.979	1836	1847	1867	rBV	156568	292282	18.88%	2.385%
53	7.307	1936	1949	1975	rBV	716377	1275177	82.35%	10.404%
54	7.612	2034	2044	2069	rBV	108969	197034	12.73%	1.608%
55	7.808	2102	2105	2108	rBV2	611	505	0.03%	0.004%
56	7.934	2138	2144	2152	rBV2	2729	4457	0.29%	0.036%
57	8.082	2180	2190	2231	rBV	405174	728078	47.02%	5.940%
58	8.561	2334	2339	2341	rBV3	426	442	0.03%	0.004%
59	8.638	2359	2363	2365	rBV2	312	222	0.01%	0.002%
60	8.670	2372	2373	2374	rBV2	303	86	0.01%	0.001%
61	8.779	2405	2407	2410	rVB	346	193	0.01%	0.002%
62	8.844	2412	2427	2463	rBV	783223	1280297	82.69%	10.446%
63	9.082	2499	2501	2502	rBV	264	99	0.01%	0.001%
64	9.140	2512	2519	2525	rVB4	916	1081	0.07%	0.009%
65	9.169	2526	2528	2531	rVB2	385	185	0.01%	0.002%
66	9.259	2553	2556	2561	rBV4	361	249	0.02%	0.002%
67	9.358	2586	2587	2590	rBV	159	70	0.00%	0.001%
68	9.429	2607	2609	2612	rBV2	202	93	0.01%	0.001%
69	9.468	2619	2621	2626	rVB2	224	197	0.01%	0.002%
70	9.542	2640	2644	2645	rBV	389	257	0.02%	0.002%
71	9.599	2657	2662	2663	rBV3	253	178	0.01%	0.001%
72	9.615	2665	2667	2669	rBV2	177	95	0.01%	0.001%
73	9.654	2676	2679	2684	rVB3	282	201	0.01%	0.002%
74	9.776	2713	2717	2719	rBV2	321	232	0.01%	0.002%
75	9.837	2733	2736	2737	rBV	205	133	0.01%	0.001%
76	9.876	2744	2748	2756	rVB3	422	472	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029526.D
 Acq On : 09 Dec 2022 17:07
 Operator : SY/MD
 Sample : N5959-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.918	2757	2761	2764	rBV4	669	559	0.04%	0.005%
78	10.027	2791	2795	2797	rBV3	358	295	0.02%	0.002%
79	10.085	2811	2813	2815	rBV	238	121	0.01%	0.001%
80	10.127	2822	2826	2827	rBV	227	153	0.01%	0.001%
81	10.162	2827	2837	2841	rVV2	26869	37777	2.44%	0.308%
82	10.207	2842	2851	2871	rVB	483713	760273	49.10%	6.203%
83	10.374	2893	2903	2910	rBV3	3205	4656	0.30%	0.038%
84	10.426	2915	2919	2921	rBV2	238	217	0.01%	0.002%
85	10.500	2940	2942	2945	rBV2	324	213	0.01%	0.002%
86	10.567	2956	2963	2977	rVB2	12363	19316	1.25%	0.158%
87	10.693	3000	3002	3004	rBV	226	123	0.01%	0.001%
88	10.805	3034	3037	3038	rBV2	243	140	0.01%	0.001%
89	11.140	3137	3141	3145	rBV3	328	334	0.02%	0.003%
90	11.175	3145	3152	3159	rBV5	968	1453	0.09%	0.012%
91	11.236	3159	3171	3206	rBV	841958	1321841	85.37%	10.785%
92	11.509	3253	3256	3259	rBV2	352	293	0.02%	0.002%
93	11.525	3259	3261	3262	rBV	469	97	0.01%	0.001%
94	11.551	3263	3269	3270	rBV2	2055	1919	0.12%	0.016%
95	11.612	3277	3288	3314	rVB	744140	1177932	76.07%	9.610%
96	11.837	3356	3358	3359	rBV	321	142	0.01%	0.001%
97	11.988	3402	3405	3408	rBV2	380	271	0.02%	0.002%
98	12.461	3548	3552	3553	rBV3	354	258	0.02%	0.002%
99	12.631	3602	3605	3606	rBV2	856	472	0.03%	0.004%
100	12.828	3664	3666	3669	rBV2	340	167	0.01%	0.001%




Sum of corrected areas: 12256734

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029526.D
Acq On : 09 Dec 2022 17:07
Operator : SY/MD
Sample : N5959-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

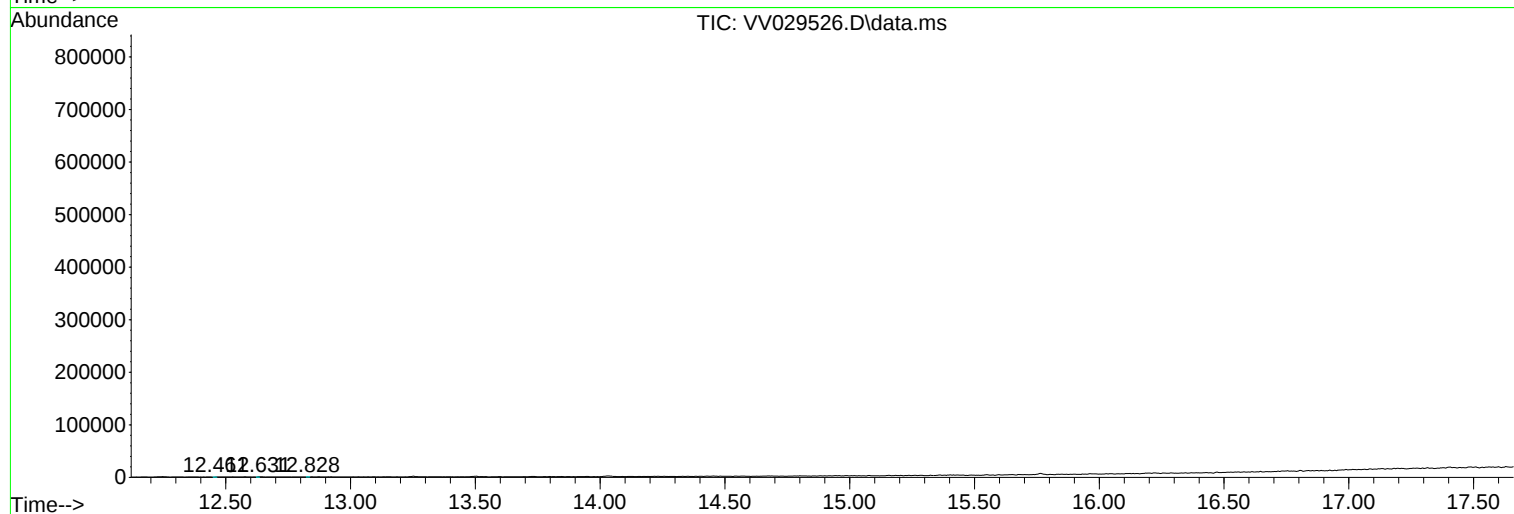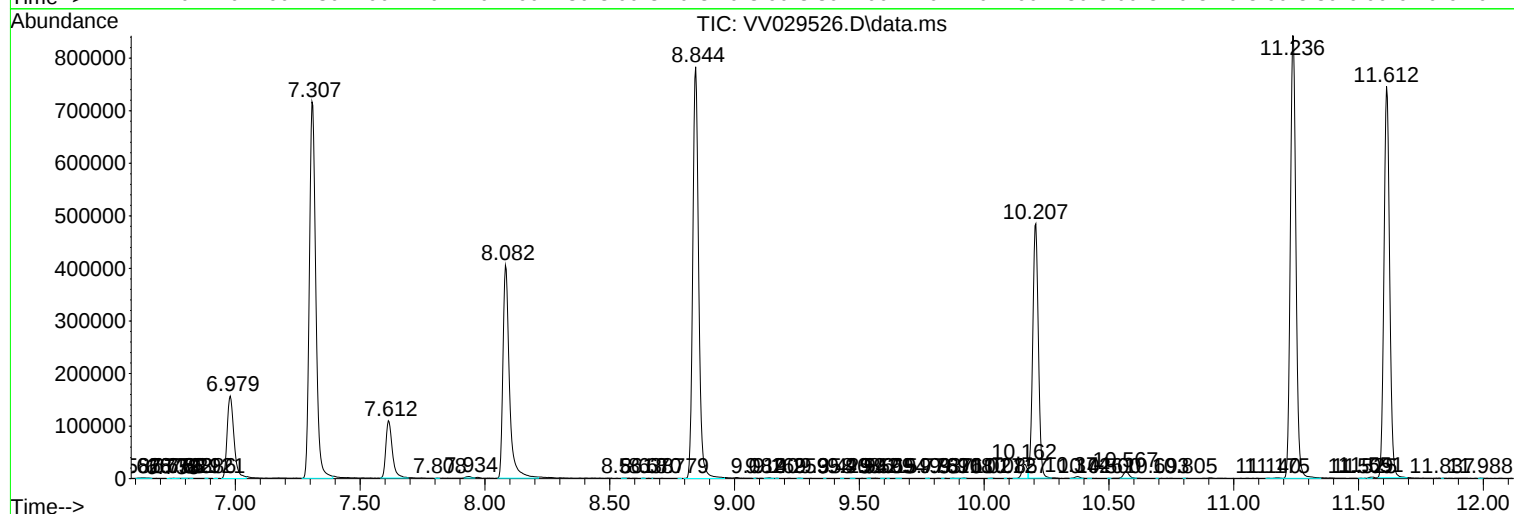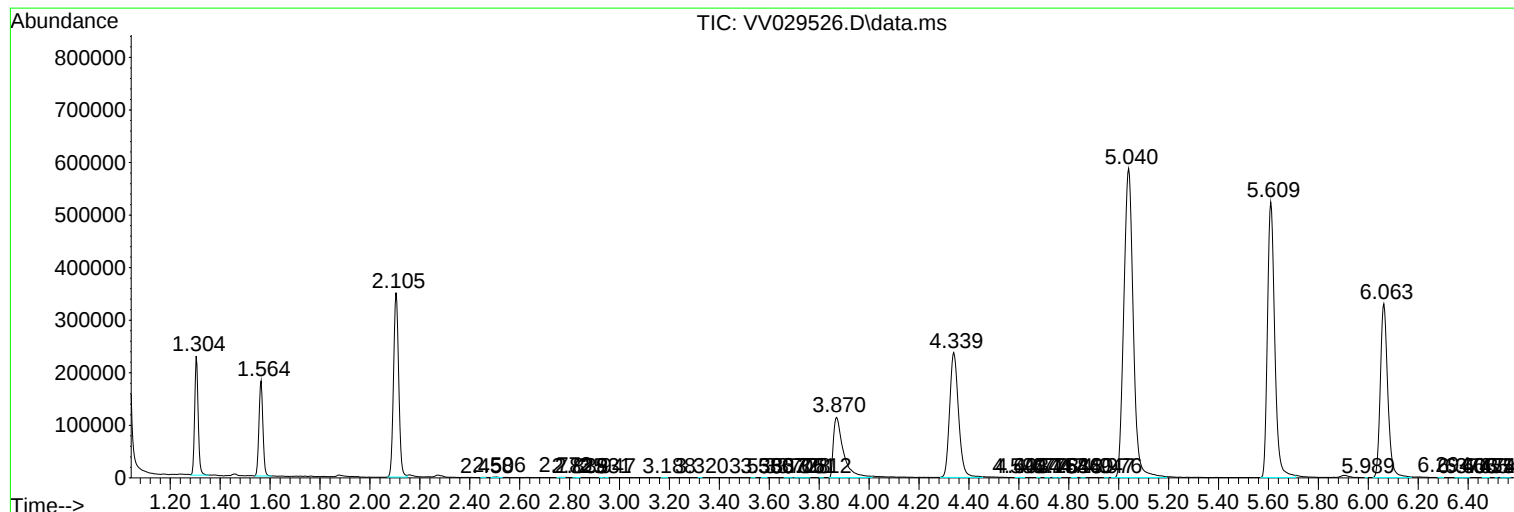

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029526.D
Acq On : 09 Dec 2022 17:07
Operator : SY/MD
Sample : N5959-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029526.D
Acq On : 09 Dec 2022 17:07
Operator : SY/MD
Sample : N5959-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc