

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029527.D
 Acq On : 09 Dec 2022 17:31
 Operator : SY/MD
 Sample : N5959-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	243524	234698	15.20%	1.913%
2	1.565	155	163	177	rVB	179540	203815	13.20%	1.662%
3	2.105	320	331	345	rBV	357564	516892	33.48%	4.214%
4	2.500	448	454	455	rBV2	1085	900	0.06%	0.007%
5	2.587	479	481	483	rBV2	211	114	0.01%	0.001%
6	2.728	522	525	528	rBV2	175	129	0.01%	0.001%
7	2.761	533	535	538	rVB2	333	166	0.01%	0.001%
8	2.934	583	589	592	rBV	387	330	0.02%	0.003%
9	2.954	592	595	599	rBV2	343	256	0.02%	0.002%
10	3.056	625	627	631	rVB2	280	152	0.01%	0.001%
11	3.159	655	659	661	rBV2	156	110	0.01%	0.001%
12	3.185	664	667	670	rVB2	264	184	0.01%	0.002%
13	3.243	682	685	688	rBV	234	146	0.01%	0.001%
14	3.365	718	723	727	rBV2	113	145	0.01%	0.001%
15	3.423	738	741	745	rBV2	217	179	0.01%	0.001%
16	3.529	771	774	780	rBV2	188	141	0.01%	0.001%
17	3.587	788	792	799	rVB	254	307	0.02%	0.003%
18	3.700	822	827	829	rBV	242	127	0.01%	0.001%
19	3.799	854	858	860	rBV	240	137	0.01%	0.001%
20	3.867	869	879	917	rBV	115439	311104	20.15%	2.536%
21	4.339	1009	1026	1054	rBV	236024	594946	38.53%	4.850%
22	4.590	1102	1104	1106	rBV	445	296	0.02%	0.002%
23	4.661	1123	1126	1129	rVV2	406	285	0.02%	0.002%
24	4.751	1149	1154	1157	rBV2	216	224	0.01%	0.002%
25	4.799	1167	1169	1172	rVB2	269	125	0.01%	0.001%
26	4.815	1172	1174	1180	rBV3	283	220	0.01%	0.002%
27	4.892	1192	1198	1202	rBV2	96	124	0.01%	0.001%
28	4.918	1202	1206	1210	rVB2	184	140	0.01%	0.001%
29	5.040	1225	1244	1272	rBV2	590415	1544072	100.00%	12.588%
30	5.481	1376	1381	1386	rBV3	450	606	0.04%	0.005%
31	5.609	1408	1421	1456	rBV	503600	1025244	66.40%	8.358%
32	5.912	1501	1515	1531	rBV5	32432	68503	4.44%	0.558%
33	6.063	1543	1562	1598	rBV	333080	687172	44.50%	5.602%
34	6.294	1631	1634	1638	rVB2	376	275	0.02%	0.002%
35	6.388	1658	1663	1666	rBV3	228	179	0.01%	0.001%
36	6.439	1674	1679	1682	rBV2	241	226	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029527.D
 Acq On : 09 Dec 2022 17:31
 Operator : SY/MD
 Sample : N5959-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.458	1683	1685	1690	rVV2	223	144	0.01%	0.001%
38	6.481	1690	1692	1698	rVB3	294	261	0.02%	0.002%
39	6.539	1706	1710	1712	rBV	159	129	0.01%	0.001%
40	6.619	1727	1735	1737	rBV4	916	898	0.06%	0.007%
41	6.744	1772	1774	1777	rBV	251	199	0.01%	0.002%
42	6.799	1784	1791	1792	rBV2	306	233	0.02%	0.002%
43	6.818	1792	1797	1799	rVV2	386	386	0.02%	0.003%
44	6.847	1802	1806	1809	rBV2	276	191	0.01%	0.002%
45	6.892	1817	1820	1822	rBV	248	159	0.01%	0.001%
46	6.979	1835	1847	1870	rBV	159461	293761	19.03%	2.395%
47	7.307	1937	1949	1986	rBV	733834	1303198	84.40%	10.624%
48	7.577	2030	2033	2034	rBV	553	333	0.02%	0.003%
49	7.613	2034	2044	2074	rVV	113351	198352	12.85%	1.617%
50	7.757	2086	2089	2091	rBV3	524	312	0.02%	0.003%
51	8.082	2180	2190	2225	rBV	404332	732920	47.47%	5.975%
52	8.481	2309	2314	2317	rBV3	382	441	0.03%	0.004%
53	8.577	2339	2344	2350	rVB4	397	450	0.03%	0.004%
54	8.703	2381	2383	2387	rBV3	185	116	0.01%	0.001%
55	8.731	2389	2392	2396	rBV4	282	277	0.02%	0.002%
56	8.754	2396	2399	2404	rBV4	326	301	0.02%	0.002%
57	8.780	2404	2407	2413	rBV2	329	326	0.02%	0.003%
58	8.844	2414	2427	2454	rBV	740888	1212735	78.54%	9.887%
59	9.063	2492	2495	2497	rBV3	464	240	0.02%	0.002%
60	9.133	2513	2517	2518	rBV3	412	325	0.02%	0.003%
61	9.172	2527	2529	2532	rVB	281	113	0.01%	0.001%
62	9.191	2532	2535	2537	rBV2	197	142	0.01%	0.001%
63	9.281	2561	2563	2568	rBV2	301	210	0.01%	0.002%
64	9.330	2575	2578	2583	rVB4	339	319	0.02%	0.003%
65	9.391	2594	2597	2599	rBV2	178	132	0.01%	0.001%
66	9.445	2611	2614	2618	rVB2	216	176	0.01%	0.001%
67	9.567	2650	2652	2655	rVB2	318	120	0.01%	0.001%
68	9.648	2669	2677	2683	rBV4	351	532	0.03%	0.004%
69	9.911	2756	2759	2765	rBV4	359	408	0.03%	0.003%
70	9.960	2771	2774	2777	rBV2	183	133	0.01%	0.001%
71	10.037	2795	2798	2804	rBV2	286	236	0.02%	0.002%
72	10.101	2815	2818	2823	rBV3	163	135	0.01%	0.001%
73	10.162	2826	2837	2841	rBV	26548	39178	2.54%	0.319%
74	10.204	2842	2850	2877	rVB	482339	771356	49.96%	6.288%
75	10.329	2887	2889	2893	rBV2	258	119	0.01%	0.001%
76	10.374	2893	2903	2912	rBV4	2988	5112	0.33%	0.042%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029527.D
 Acq On : 09 Dec 2022 17:31
 Operator : SY/MD
 Sample : N5959-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.429	2918	2920	2923	rVB2	274	155	0.01%	0.001%
78	10.448	2923	2926	2931	rBV3	379	319	0.02%	0.003%
79	10.529	2946	2951	2952	rBV2	667	585	0.04%	0.005%
80	10.567	2955	2963	2974	rVB	13202	20336	1.32%	0.166%
81	10.645	2984	2987	2990	rBV2	228	199	0.01%	0.002%
82	10.709	3004	3007	3010	rBV	180	119	0.01%	0.001%
83	10.731	3010	3014	3018	rVB3	311	300	0.02%	0.002%
84	10.834	3043	3046	3047	rBV2	200	116	0.01%	0.001%
85	10.860	3051	3054	3055	rBV	223	107	0.01%	0.001%
86	10.911	3063	3070	3071	rBV2	765	751	0.05%	0.006%
87	10.998	3094	3097	3103	rVB3	292	274	0.02%	0.002%
88	11.034	3105	3108	3110	rBV	243	137	0.01%	0.001%
89	11.046	3110	3112	3117	rVB2	310	243	0.02%	0.002%
90	11.075	3117	3121	3123	rBV	355	271	0.02%	0.002%
91	11.117	3129	3134	3143	rBV4	348	616	0.04%	0.005%
92	11.172	3147	3151	3157	rVB5	712	783	0.05%	0.006%
93	11.239	3159	3172	3198	rBV	814454	1269529	82.22%	10.350%
94	11.612	3276	3288	3312	rBV	771339	1212353	78.52%	9.883%
95	11.889	3372	3374	3377	rBV2	363	249	0.02%	0.002%
96	11.944	3388	3391	3392	rBV	283	171	0.01%	0.001%
97	12.069	3427	3430	3436	rBV3	336	387	0.03%	0.003%
98	12.165	3456	3460	3462	rBV2	400	378	0.02%	0.003%
99	12.564	3581	3584	3586	rBV2	291	187	0.01%	0.002%
100	12.628	3602	3604	3605	rBV	415	138	0.01%	0.001%




Sum of corrected areas: 12266480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029527.D
Acq On : 09 Dec 2022 17:31
Operator : SY/MD
Sample : N5959-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

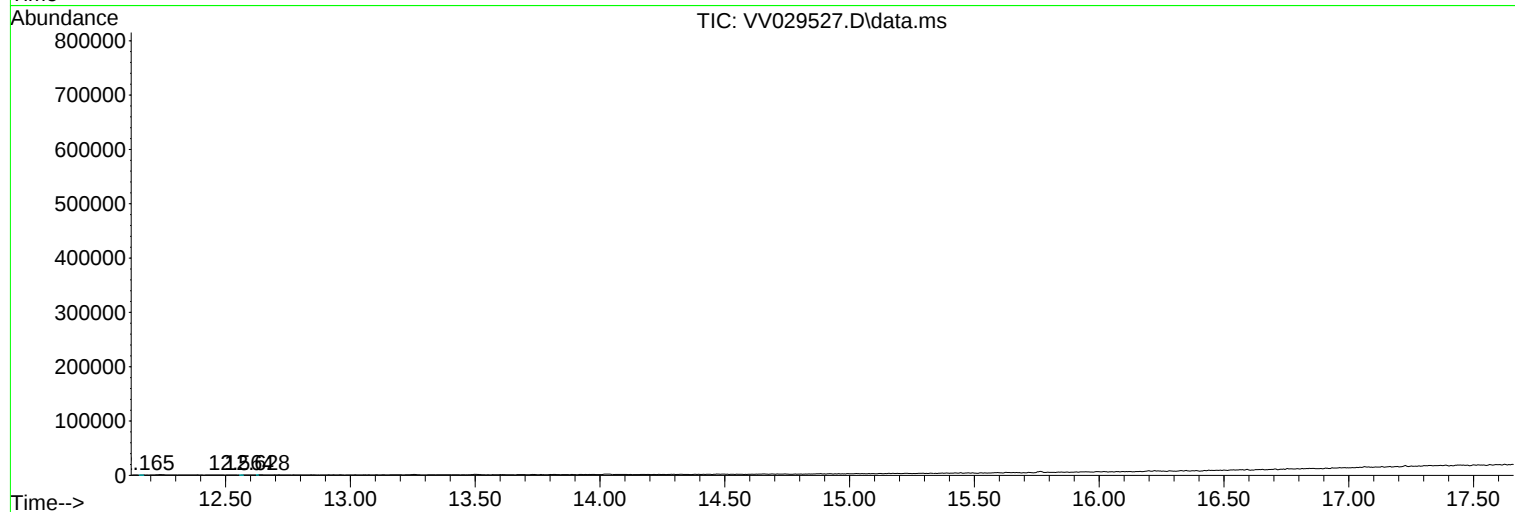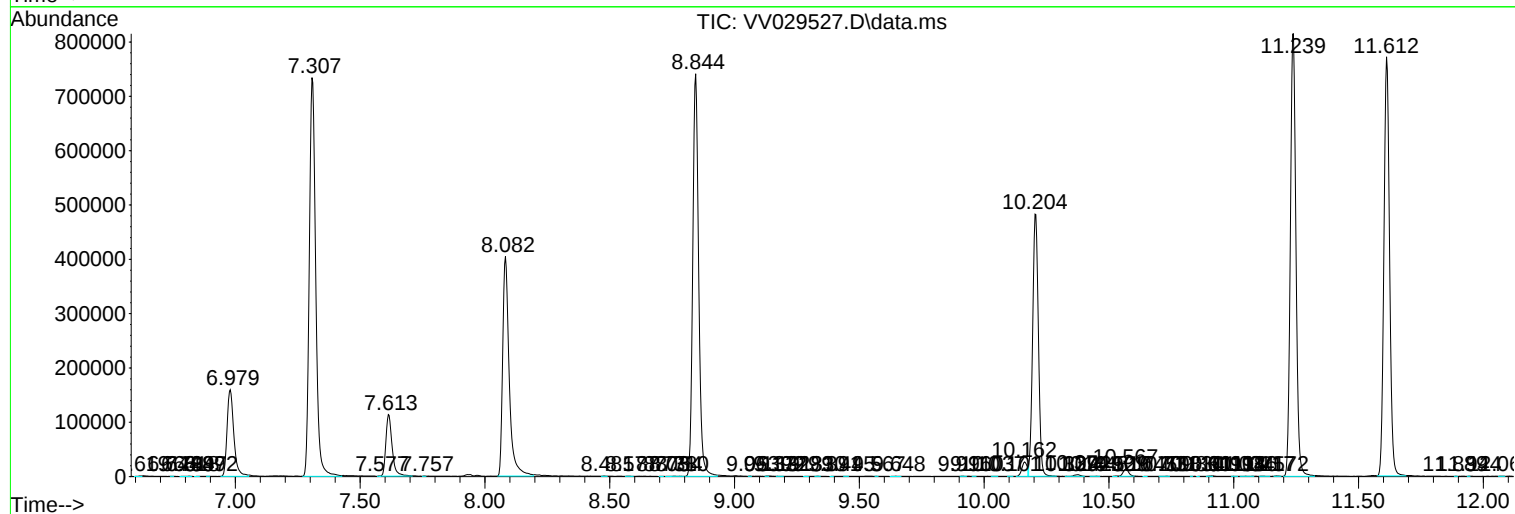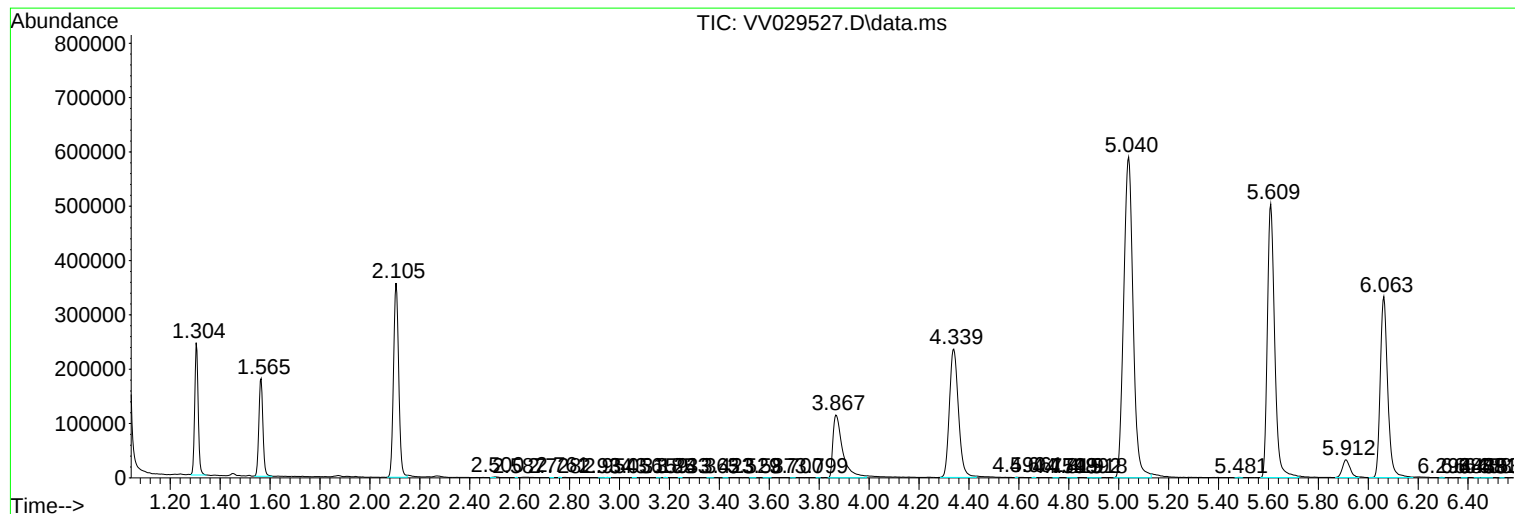

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029527.D
Acq On : 09 Dec 2022 17:31
Operator : SY/MD
Sample : N5959-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029527.D
Acq On : 09 Dec 2022 17:31
Operator : SY/MD
Sample : N5959-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------