

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029528.D
 Acq On : 09 Dec 2022 17:54
 Operator : SY/MD
 Sample : N5959-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	224393	225144	14.79%	1.823%
2	1.564	155	163	177	rVB	177477	200083	13.14%	1.620%
3	2.105	321	331	345	rBV2	368037	558069	36.66%	4.520%
4	2.372	411	414	415	rBV	327	143	0.01%	0.001%
5	2.651	498	501	503	rVB	262	100	0.01%	0.001%
6	2.748	526	531	533	rBV3	361	312	0.02%	0.003%
7	2.831	554	557	561	rVB2	264	183	0.01%	0.001%
8	2.973	599	601	608	rVB	337	193	0.01%	0.002%
9	3.005	608	611	615	rVB	379	184	0.01%	0.001%
10	3.027	615	618	621	rBV2	262	207	0.01%	0.002%
11	3.162	656	660	661	rBV2	332	186	0.01%	0.002%
12	3.185	661	667	680	rVB4	1073	2016	0.13%	0.016%
13	3.478	753	758	765	rBV2	295	366	0.02%	0.003%
14	3.510	765	768	769	rBV	147	66	0.00%	0.001%
15	3.545	777	779	783	rBV	149	92	0.01%	0.001%
16	3.571	783	787	790	rVB2	284	193	0.01%	0.002%
17	3.638	800	808	812	rBV2	227	294	0.02%	0.002%
18	3.661	812	815	817	rBV2	124	72	0.00%	0.001%
19	3.706	825	829	834	rVB2	298	288	0.02%	0.002%
20	3.744	837	841	843	rVB	186	97	0.01%	0.001%
21	3.761	843	846	848	rBV	136	106	0.01%	0.001%
22	3.870	870	880	916	rBV	114824	363042	23.85%	2.940%
23	4.339	1009	1026	1057	rBV	236473	590148	38.77%	4.780%
24	4.606	1093	1109	1122	rBV4	9432	24244	1.59%	0.196%
25	4.706	1137	1140	1148	rVB3	284	281	0.02%	0.002%
26	4.744	1149	1152	1159	rVB2	175	193	0.01%	0.002%
27	4.812	1159	1173	1174	rBV4	542	774	0.05%	0.006%
28	4.886	1193	1196	1200	rVV2	342	225	0.01%	0.002%
29	4.918	1202	1206	1208	rVV	148	97	0.01%	0.001%
30	4.947	1213	1215	1219	rBV2	182	112	0.01%	0.001%
31	4.973	1219	1223	1226	rVB2	398	273	0.02%	0.002%
32	5.040	1226	1244	1273	rBV2	580569	1522143	100.00%	12.328%
33	5.394	1351	1354	1358	rBV3	325	283	0.02%	0.002%
34	5.465	1372	1376	1378	rBV2	471	361	0.02%	0.003%
35	5.503	1386	1388	1392	rVB2	285	168	0.01%	0.001%
36	5.609	1406	1421	1460	rBV	536042	1094590	71.91%	8.865%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029528.D
 Acq On : 09 Dec 2022 17:54
 Operator : SY/MD
 Sample : N5959-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.902	1502	1512	1529	rVB8	4363	9244	0.61%	0.075%
38	6.063	1547	1562	1598	rBV	330495	680366	44.70%	5.510%
39	6.301	1634	1636	1638	rBV2	108	69	0.00%	0.001%
40	6.326	1641	1644	1646	rVV2	182	144	0.01%	0.001%
41	6.339	1646	1648	1651	rVB	284	103	0.01%	0.001%
42	6.381	1659	1661	1664	rBV	200	92	0.01%	0.001%
43	6.436	1673	1678	1680	rBV2	238	182	0.01%	0.001%
44	6.484	1690	1693	1695	rBV	272	211	0.01%	0.002%
45	6.596	1724	1728	1730	rBV2	278	228	0.01%	0.002%
46	6.703	1756	1761	1762	rBV	210	163	0.01%	0.001%
47	6.799	1788	1791	1793	rBV2	326	185	0.01%	0.001%
48	6.815	1794	1796	1800	rBV2	193	146	0.01%	0.001%
49	6.854	1806	1808	1809	rBV2	124	71	0.00%	0.001%
50	6.876	1812	1815	1817	rBV	168	146	0.01%	0.001%
51	6.899	1818	1822	1824	rVB2	260	193	0.01%	0.002%
52	6.912	1824	1826	1829	rBV	160	119	0.01%	0.001%
53	6.979	1834	1847	1875	rBV	154328	289942	19.05%	2.348%
54	7.172	1904	1907	1911	rBV3	491	430	0.03%	0.003%
55	7.307	1937	1949	1983	rBV	718877	1275171	83.77%	10.327%
56	7.612	2034	2044	2062	rBV	110039	194150	12.76%	1.572%
57	7.838	2107	2114	2124	rBV8	1808	2823	0.19%	0.023%
58	7.937	2135	2145	2151	rBV4	3371	6055	0.40%	0.049%
59	8.037	2169	2176	2180	rBV4	435	644	0.04%	0.005%
60	8.082	2180	2190	2224	rBV	397774	722759	47.48%	5.854%
61	8.574	2341	2343	2347	rBV4	361	220	0.01%	0.002%
62	8.664	2367	2371	2375	rBV3	364	456	0.03%	0.004%
63	8.696	2378	2381	2383	rBV3	349	236	0.02%	0.002%
64	8.738	2391	2394	2396	rBV	309	160	0.01%	0.001%
65	8.751	2396	2398	2402	rVB3	371	193	0.01%	0.002%
66	8.844	2414	2427	2450	rBV	779290	1292411	84.91%	10.467%
67	9.053	2489	2492	2493	rBV	297	140	0.01%	0.001%
68	9.127	2510	2515	2517	rBV3	882	619	0.04%	0.005%
69	9.185	2531	2533	2539	rVB2	605	483	0.03%	0.004%
70	9.233	2546	2548	2553	rBV3	217	222	0.01%	0.002%
71	9.265	2556	2558	2561	rVB2	420	193	0.01%	0.002%
72	9.320	2573	2575	2577	rVB	313	127	0.01%	0.001%
73	9.333	2577	2579	2581	rBV	184	105	0.01%	0.001%
74	9.371	2588	2591	2594	rBV	158	102	0.01%	0.001%
75	9.542	2638	2644	2649	rBV2	496	750	0.05%	0.006%
76	9.648	2673	2677	2680	rBV2	225	166	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029528.D
 Acq On : 09 Dec 2022 17:54
 Operator : SY/MD
 Sample : N5959-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.670	2680	2684	2686	rBV2	190	147	0.01%	0.001%
78	9.722	2697	2700	2702	rVB	248	132	0.01%	0.001%
79	9.735	2702	2704	2706	rBV2	217	104	0.01%	0.001%
80	9.780	2717	2718	2720	rBV2	215	74	0.00%	0.001%
81	9.985	2780	2782	2784	rBV	136	78	0.01%	0.001%
82	10.124	2822	2825	2827	rBV	248	114	0.01%	0.001%
83	10.162	2827	2837	2841	rBV2	25574	38470	2.53%	0.312%
84	10.207	2842	2851	2873	rVB	482042	760683	49.97%	6.161%
85	10.374	2896	2903	2915	rVB3	2750	4499	0.30%	0.036%
86	10.484	2934	2937	2939	rBV	263	225	0.01%	0.002%
87	10.567	2955	2963	2975	rVB2	12026	18389	1.21%	0.149%
88	10.866	3054	3056	3058	rBV2	162	92	0.01%	0.001%
89	10.898	3063	3066	3067	rBV	703	370	0.02%	0.003%
90	11.159	3145	3147	3148	rBV	359	163	0.01%	0.001%
91	11.236	3159	3171	3201	rBV	840923	1309604	86.04%	10.606%
92	11.500	3250	3253	3257	rBV2	235	249	0.02%	0.002%
93	11.522	3257	3260	3261	rVV2	309	172	0.01%	0.001%
94	11.558	3264	3271	3276	rVV7	1928	2975	0.20%	0.024%
95	11.612	3276	3288	3321	rVB	725238	1144313	75.18%	9.268%
96	11.754	3331	3332	3334	rBV	426	114	0.01%	0.001%
97	11.831	3354	3356	3360	rBV2	396	217	0.01%	0.002%
98	11.898	3374	3377	3379	rBV2	212	107	0.01%	0.001%
99	11.985	3400	3404	3408	rBV	451	411	0.03%	0.003%
100	12.313	3503	3506	3509	rBV2	328	185	0.01%	0.001%




Sum of corrected areas: 12347434

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029528.D
Acq On : 09 Dec 2022 17:54
Operator : SY/MD
Sample : N5959-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

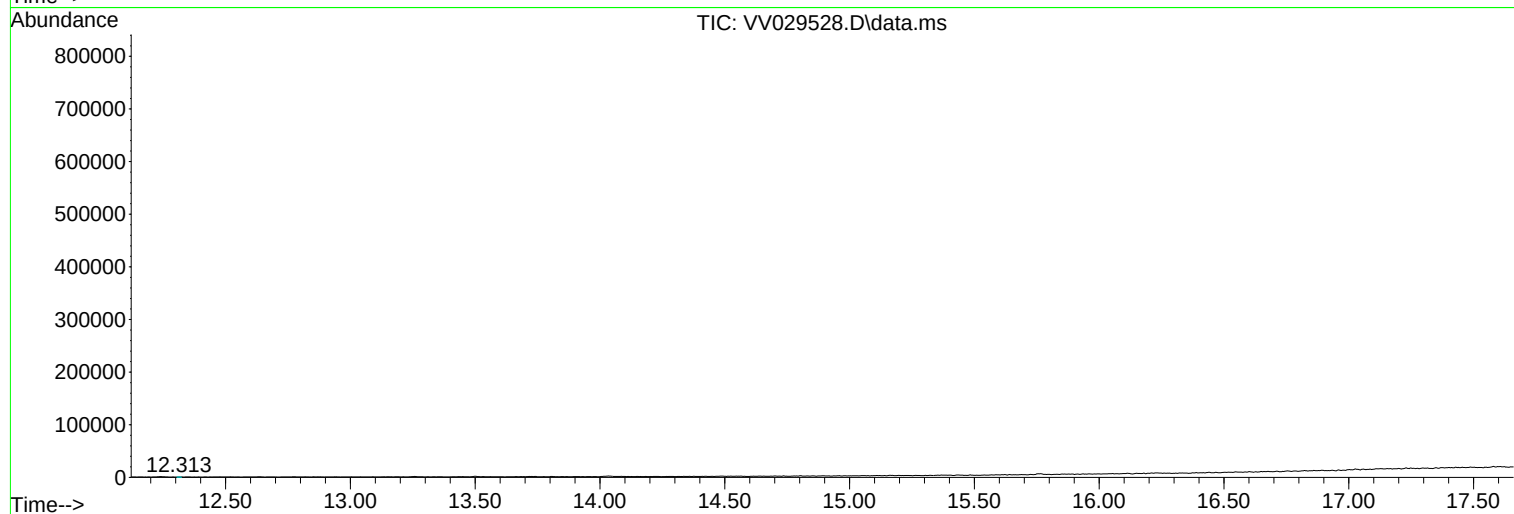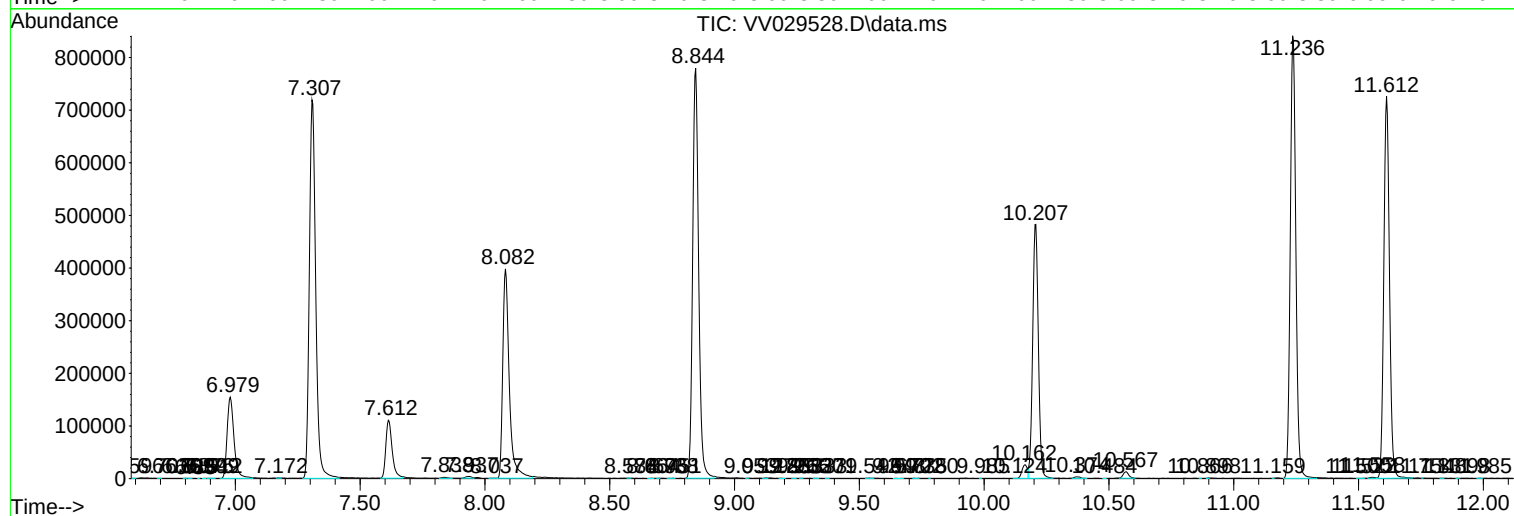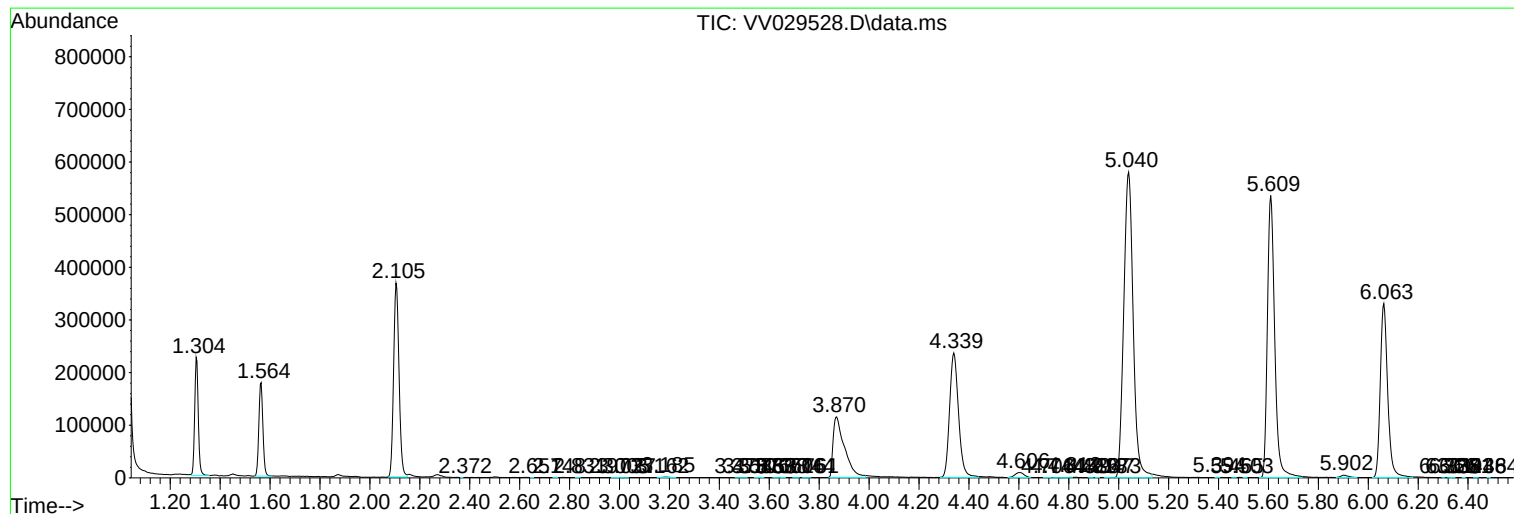

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029528.D
Acq On : 09 Dec 2022 17:54
Operator : SY/MD
Sample : N5959-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029528.D
Acq On : 09 Dec 2022 17:54
Operator : SY/MD
Sample : N5959-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc