

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029529.D
 Acq On : 09 Dec 2022 18:18
 Operator : SY/MD
 Sample : N5959-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	224192	221416	15.05%	1.703%
2	1.449	124	127	133	rVB4	3585	3460	0.24%	0.027%
3	1.564	155	163	177	rVB	176316	197682	13.44%	1.521%
4	1.873	252	259	270	rVB	5238	8504	0.58%	0.065%
5	2.056	314	316	319	rBV2	524	315	0.02%	0.002%
6	2.105	320	331	360	rVV2	357546	541264	36.80%	4.164%
7	2.269	375	382	400	rVB	8417	15935	1.08%	0.123%
8	2.400	421	423	427	rVB	358	199	0.01%	0.002%
9	2.503	449	455	466	rVB6	1117	1697	0.12%	0.013%
10	2.622	489	492	497	rVB2	262	216	0.01%	0.002%
11	2.770	532	538	545	rBV4	593	690	0.05%	0.005%
12	2.953	592	595	604	rVB2	250	323	0.02%	0.002%
13	3.130	645	650	653	rBV3	258	256	0.02%	0.002%
14	3.191	658	669	680	rVB4	1034	2551	0.17%	0.020%
15	3.870	870	880	931	rBV	108102	358551	24.38%	2.759%
16	4.339	1008	1026	1055	rBV	224810	565258	38.43%	4.349%
17	4.600	1093	1107	1126	rVB3	9805	24844	1.69%	0.191%
18	4.703	1136	1139	1142	rBV2	346	219	0.01%	0.002%
19	5.040	1225	1244	1279	rBV2	550784	1470908	100.00%	11.317%
20	5.281	1315	1319	1322	rVV2	416	335	0.02%	0.003%
21	5.339	1334	1337	1345	rVB3	393	375	0.03%	0.003%
22	5.468	1374	1377	1380	rBV3	434	390	0.03%	0.003%
23	5.545	1398	1401	1405	rVB3	273	225	0.02%	0.002%
24	5.609	1405	1421	1467	rBV	515903	1057491	71.89%	8.136%
25	5.821	1485	1487	1491	rBV	298	234	0.02%	0.002%
26	5.905	1499	1513	1548	rBV	477973	956661	65.04%	7.360%
27	6.063	1548	1562	1596	rVB	312070	645423	43.88%	4.966%
28	6.281	1627	1630	1634	rVB3	274	210	0.01%	0.002%
29	6.330	1642	1645	1650	rVB3	293	240	0.02%	0.002%
30	6.403	1663	1668	1672	rVB2	250	250	0.02%	0.002%
31	6.622	1728	1736	1740	rBV4	1122	1404	0.10%	0.011%
32	6.722	1761	1767	1772	rBV4	447	505	0.03%	0.004%
33	6.812	1791	1795	1800	rBV3	338	304	0.02%	0.002%
34	6.895	1814	1821	1826	rBV4	358	385	0.03%	0.003%
35	6.979	1836	1847	1876	rBV	150237	275637	18.74%	2.121%
36	7.120	1888	1891	1895	rVB3	292	246	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029529.D
 Acq On : 09 Dec 2022 18:18
 Operator : SY/MD
 Sample : N5959-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.172	1900	1907	1911	rBV5	811	1049	0.07%	0.008%
38	7.191	1911	1913	1923	rVB5	564	659	0.04%	0.005%
39	7.307	1937	1949	1979	rBV	696128	1229252	83.57%	9.457%
40	7.612	2034	2044	2072	rBV	106611	188259	12.80%	1.448%
41	7.844	2109	2116	2121	rVB4	779	1023	0.07%	0.008%
42	7.873	2121	2125	2128	rVB3	406	288	0.02%	0.002%
43	7.931	2133	2143	2152	rBV2	4592	8935	0.61%	0.069%
44	8.018	2166	2170	2172	rBV2	393	283	0.02%	0.002%
45	8.082	2180	2190	2222	rBV	377808	681723	46.35%	5.245%
46	8.455	2303	2306	2310	rBV	266	208	0.01%	0.002%
47	8.484	2313	2315	2321	rVB3	411	347	0.02%	0.003%
48	8.516	2321	2325	2329	rBV4	346	301	0.02%	0.002%
49	8.574	2338	2343	2345	rBV3	295	213	0.01%	0.002%
50	8.645	2362	2365	2369	rBV2	318	234	0.02%	0.002%
51	8.786	2401	2409	2412	rBV3	363	360	0.02%	0.003%
52	8.844	2414	2427	2459	rBV	756988	1247564	84.82%	9.598%
53	8.995	2470	2474	2476	rBV2	383	322	0.02%	0.002%
54	9.140	2510	2519	2524	rVV4	944	1317	0.09%	0.010%
55	9.178	2527	2531	2534	rBV2	356	311	0.02%	0.002%
56	9.194	2534	2536	2540	rVB2	412	241	0.02%	0.002%
57	9.217	2540	2543	2546	rBV	330	224	0.02%	0.002%
58	9.345	2580	2583	2588	rBV3	349	256	0.02%	0.002%
59	9.374	2588	2592	2597	rVB3	220	222	0.02%	0.002%
60	9.481	2620	2625	2630	rBV2	396	433	0.03%	0.003%
61	9.542	2637	2644	2649	rBV4	734	1039	0.07%	0.008%
62	9.571	2649	2653	2658	rVV2	505	401	0.03%	0.003%
63	9.898	2749	2755	2758	rBV3	244	221	0.02%	0.002%
64	9.927	2758	2764	2765	rBV	476	377	0.03%	0.003%
65	10.027	2791	2795	2802	rBV2	295	411	0.03%	0.003%
66	10.075	2805	2810	2815	rVB3	305	353	0.02%	0.003%
67	10.162	2826	2837	2841	rBV3	25282	36825	2.50%	0.283%
68	10.204	2841	2850	2870	rVB	460895	730285	49.65%	5.619%
69	10.374	2892	2903	2912	rBV3	4599	7087	0.48%	0.055%
70	10.445	2921	2925	2927	rBV2	447	272	0.02%	0.002%
71	10.522	2946	2949	2950	rVV2	467	279	0.02%	0.002%
72	10.532	2950	2952	2954	rVV2	736	408	0.03%	0.003%
73	10.567	2954	2963	2976	rVV2	11967	19612	1.33%	0.151%
74	10.683	2997	2999	3005	rVB3	342	215	0.01%	0.002%
75	10.844	3045	3049	3052	rBV2	386	309	0.02%	0.002%
76	10.905	3063	3068	3076	rVV5	1066	1614	0.11%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029529.D
 Acq On : 09 Dec 2022 18:18
 Operator : SY/MD
 Sample : N5959-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.169	3147	3150	3151	rBV	467	262	0.02%	0.002%
78	11.239	3159	3172	3201	rBV	828337	1297286	88.20%	9.981%
79	11.506	3252	3255	3257	rBV2	374	247	0.02%	0.002%
80	11.551	3262	3269	3275	rBV5	1528	2502	0.17%	0.019%
81	11.612	3275	3288	3326	rVB	739184	1169884	79.53%	9.001%
82	11.892	3372	3375	3378	rVB	321	206	0.01%	0.002%
83	11.976	3399	3401	3407	rBV2	242	242	0.02%	0.002%
84	12.242	3477	3484	3491	rVB3	789	1197	0.08%	0.009%
85	12.464	3550	3553	3556	rBV2	283	212	0.01%	0.002%
86	12.689	3620	3623	3626	rBV3	317	256	0.02%	0.002%
87	12.844	3669	3671	3675	rBV2	355	261	0.02%	0.002%
88	12.908	3688	3691	3695	rBV	392	271	0.02%	0.002%
89	13.046	3731	3734	3736	rVB3	411	203	0.01%	0.002%
90	13.123	3754	3758	3760	rBV3	354	254	0.02%	0.002%
91	13.175	3771	3774	3779	rVB3	617	375	0.03%	0.003%
92	13.252	3795	3798	3806	rVB6	832	925	0.06%	0.007%
93	13.320	3817	3819	3824	rVB3	567	338	0.02%	0.003%
94	13.493	3867	3873	3876	rBV4	1505	1749	0.12%	0.013%
95	13.731	3943	3947	3954	rBV4	791	1202	0.08%	0.009%
96	13.821	3973	3975	3976	rBV	456	221	0.02%	0.002%
97	13.860	3984	3987	3988	rBV3	470	249	0.02%	0.002%
98	13.905	3996	4001	4002	rBV2	451	388	0.03%	0.003%
99	14.821	4284	4286	4289	rBV3	742	419	0.03%	0.003%
100	15.133	4381	4383	4385	rBV3	872	356	0.02%	0.003%


Sum of corrected areas: 12997840

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029529.D
Acq On : 09 Dec 2022 18:18
Operator : SY/MD
Sample : N5959-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

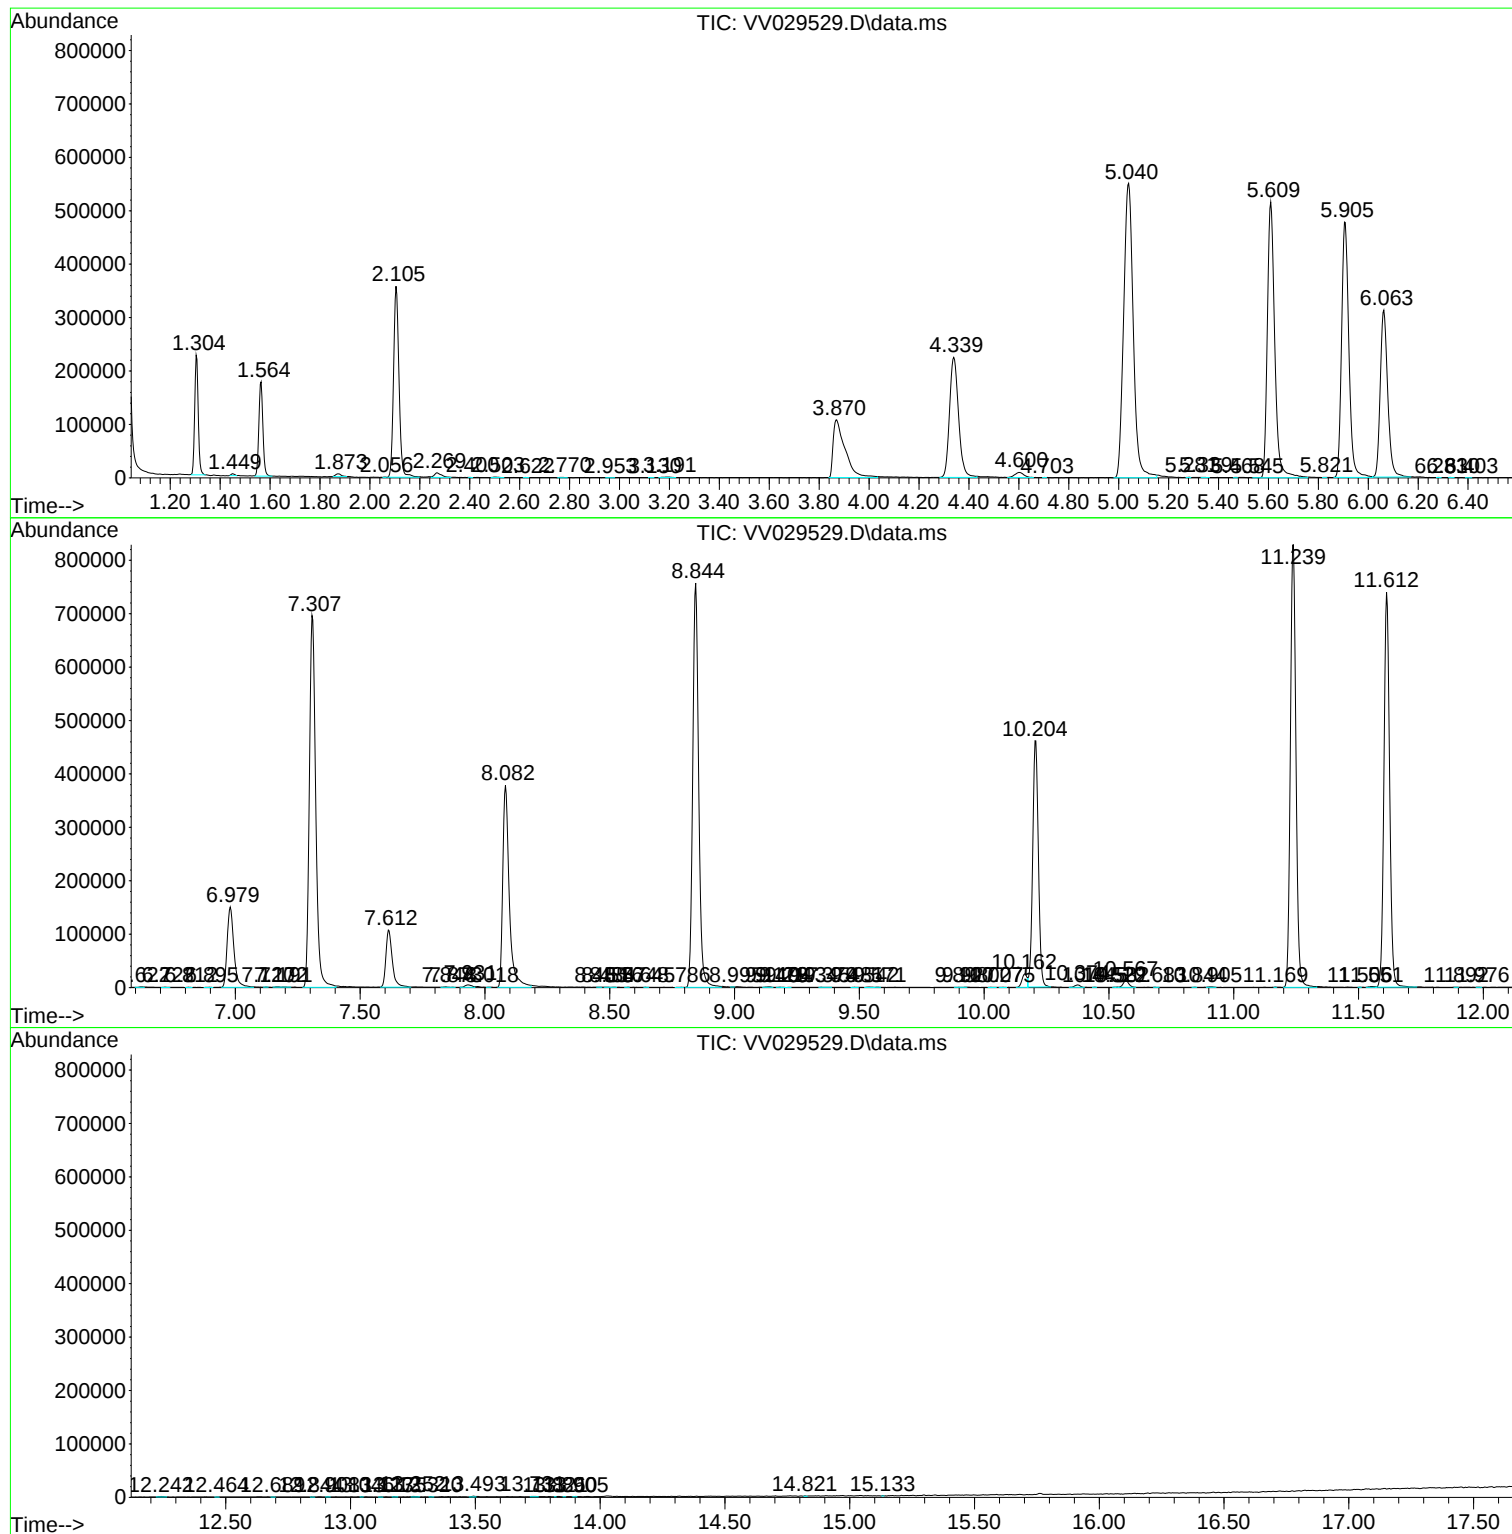

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029529.D
Acq On : 09 Dec 2022 18:18
Operator : SY/MD
Sample : N5959-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029529.D
Acq On : 09 Dec 2022 18:18
Operator : SY/MD
Sample : N5959-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------