

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029530.D
 Acq On : 09 Dec 2022 18:42
 Operator : SY/MD
 Sample : N5959-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	225046	225597	14.36%	1.818%
2	1.564	155	163	180	rVB	181458	207677	13.22%	1.674%
3	2.104	319	331	344	rBV	362208	517789	32.97%	4.173%
4	2.413	423	427	430	rBV2	288	278	0.02%	0.002%
5	2.558	467	472	477	rBV2	258	309	0.02%	0.002%
6	2.860	563	566	569	rBV2	207	136	0.01%	0.001%
7	3.368	722	724	727	rVB2	188	89	0.01%	0.001%
8	3.767	846	848	850	rVB	157	48	0.00%	0.000%
9	3.821	863	865	868	rBV	93	69	0.00%	0.001%
10	3.870	870	880	911	rBV	115841	308212	19.63%	2.484%
11	4.339	1009	1026	1060	rBV	244927	611764	38.95%	4.930%
12	4.535	1085	1087	1094	rVB3	604	428	0.03%	0.003%
13	4.628	1113	1116	1123	rVB3	172	159	0.01%	0.001%
14	4.657	1123	1125	1127	rBV2	279	181	0.01%	0.001%
15	4.725	1144	1146	1147	rBV2	119	49	0.00%	0.000%
16	4.744	1147	1152	1159	rVV4	283	383	0.02%	0.003%
17	4.773	1159	1161	1162	rBV	327	91	0.01%	0.001%
18	4.796	1167	1168	1171	rVB	131	37	0.00%	0.000%
19	4.870	1188	1191	1194	rVB	310	166	0.01%	0.001%
20	4.889	1194	1197	1201	rVB2	184	152	0.01%	0.001%
21	4.911	1201	1204	1206	rBV	236	146	0.01%	0.001%
22	5.040	1222	1244	1279	rBV2	600683	1570495	100.00%	12.656%
23	5.445	1367	1370	1371	rBV	224	131	0.01%	0.001%
24	5.519	1391	1393	1394	rBV	172	70	0.00%	0.001%
25	5.564	1406	1407	1408	rBV	171	48	0.00%	0.000%
26	5.609	1408	1421	1444	rBV	522717	1063722	67.73%	8.572%
27	5.905	1503	1513	1532	rVB8	4630	11446	0.73%	0.092%
28	5.976	1533	1535	1539	rBV2	251	140	0.01%	0.001%
29	6.063	1547	1562	1590	rBV	336908	694319	44.21%	5.595%
30	6.423	1671	1674	1676	rBV2	174	134	0.01%	0.001%
31	6.464	1681	1687	1694	rVV4	311	456	0.03%	0.004%
32	6.513	1700	1702	1703	rBV	214	92	0.01%	0.001%
33	6.596	1723	1728	1730	rBV	204	155	0.01%	0.001%
34	6.776	1779	1784	1787	rBV3	293	294	0.02%	0.002%
35	6.841	1803	1804	1808	rBV	127	45	0.00%	0.000%
36	6.979	1835	1847	1876	rBV	158359	297187	18.92%	2.395%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029530.D
 Acq On : 09 Dec 2022 18:42
 Operator : SY/MD
 Sample : N5959-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.310	1937	1950	1982	rBV	734814	1312496	83.57%	10.577%
38	7.612	2035	2044	2069	rBV	112995	198633	12.65%	1.601%
39	8.082	2179	2190	2227	rBV	409244	743594	47.35%	5.992%
40	8.574	2341	2343	2345	rBV2	289	167	0.01%	0.001%
41	8.709	2383	2385	2389	rBV	337	227	0.01%	0.002%
42	8.754	2395	2399	2403	rBV2	375	353	0.02%	0.003%
43	8.844	2415	2427	2465	rBV	772151	1276946	81.31%	10.291%
44	9.127	2512	2515	2516	rBV	597	356	0.02%	0.003%
45	9.181	2529	2532	2534	rBV3	175	106	0.01%	0.001%
46	9.275	2559	2561	2563	rVB2	173	49	0.00%	0.000%
47	9.300	2567	2569	2571	rVB	181	76	0.00%	0.001%
48	9.506	2631	2633	2635	rBV	146	86	0.01%	0.001%
49	9.535	2639	2642	2645	rBV2	597	490	0.03%	0.004%
50	9.593	2658	2660	2662	rBV3	395	196	0.01%	0.002%
51	9.664	2680	2682	2684	rVB	252	88	0.01%	0.001%
52	9.680	2685	2687	2689	rVB2	189	82	0.01%	0.001%
53	9.699	2691	2693	2696	rVV2	171	83	0.01%	0.001%
54	9.744	2705	2707	2710	rBB2	212	111	0.01%	0.001%
55	9.763	2711	2713	2718	rVB2	272	160	0.01%	0.001%
56	9.863	2742	2744	2747	rBV2	134	63	0.00%	0.001%
57	9.918	2759	2761	2762	rBV	472	175	0.01%	0.001%
58	10.066	2806	2807	2810	rBV	241	93	0.01%	0.001%
59	10.095	2814	2816	2820	rBV2	321	222	0.01%	0.002%
60	10.117	2820	2823	2827	rBV3	369	374	0.02%	0.003%
61	10.162	2827	2837	2841	rBV	27798	39632	2.52%	0.319%
62	10.207	2842	2851	2878	rVB	497502	782358	49.82%	6.305%
63	10.371	2894	2902	2913	rVB4	3965	6114	0.39%	0.049%
64	10.484	2935	2937	2938	rBV	237	78	0.00%	0.001%
65	10.532	2947	2952	2954	rBV2	714	767	0.05%	0.006%
66	10.567	2955	2963	2976	rVB	12687	21049	1.34%	0.170%
67	10.750	3017	3020	3024	rBV2	254	138	0.01%	0.001%
68	10.824	3040	3043	3046	rBV2	367	281	0.02%	0.002%
69	10.844	3047	3049	3051	rBV2	481	236	0.02%	0.002%
70	10.889	3061	3063	3064	rBV	275	89	0.01%	0.001%
71	10.998	3095	3097	3099	rBV	290	187	0.01%	0.002%
72	11.053	3111	3114	3116	rBV2	183	130	0.01%	0.001%
73	11.123	3133	3136	3141	rBV3	589	491	0.03%	0.004%
74	11.175	3145	3152	3156	rBV2	718	885	0.06%	0.007%
75	11.239	3160	3172	3198	rBV	834855	1305762	83.14%	10.523%
76	11.529	3259	3262	3264	rBV	384	293	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029530.D
Acq On : 09 Dec 2022 18:42
Operator : SY/MD
Sample : N5959-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

77	11.612	3277	3288	3311	rBV	758866	1199630	76.39%	9.667%
78	11.988	3401	3405	3412	rBV	337	334	0.02%	0.003%
79	12.017	3412	3414	3417	rBV	339	201	0.01%	0.002%
80	12.239	3475	3483	3491	rBV3	833	1492	0.10%	0.012%
81	12.532	3571	3574	3577	rBV2	311	175	0.01%	0.001%
82	12.638	3603	3607	3612	rVB3	905	873	0.06%	0.007%




Sum of corrected areas: 12408915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029530.D
Acq On : 09 Dec 2022 18:42
Operator : SY/MD
Sample : N5959-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

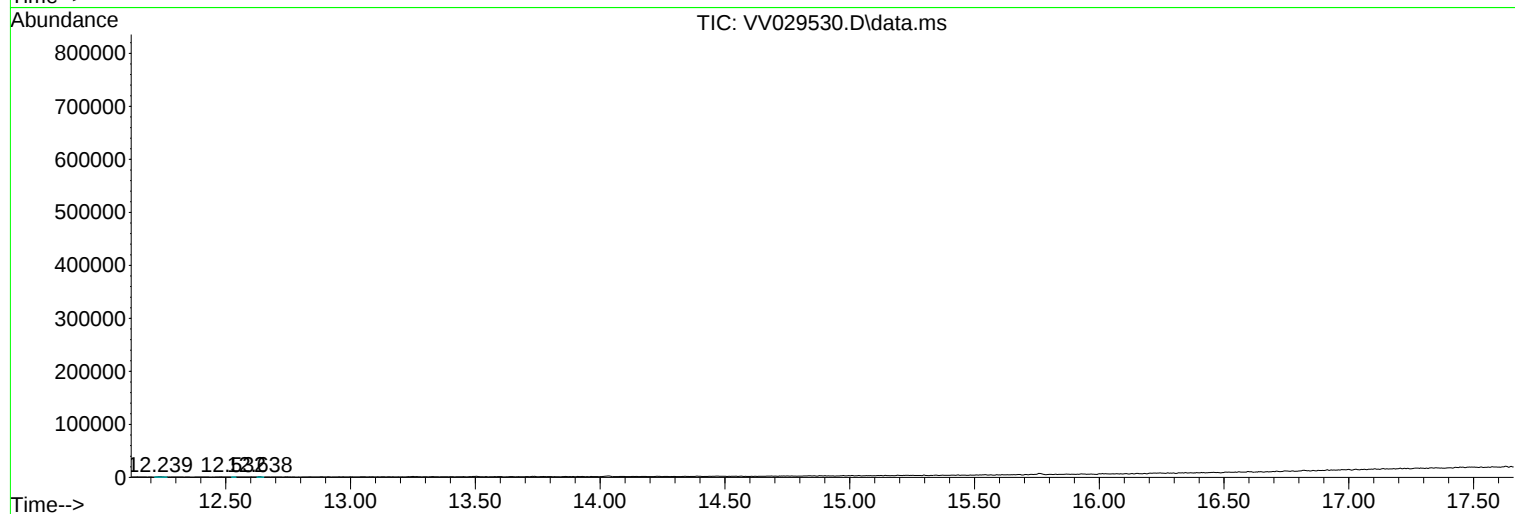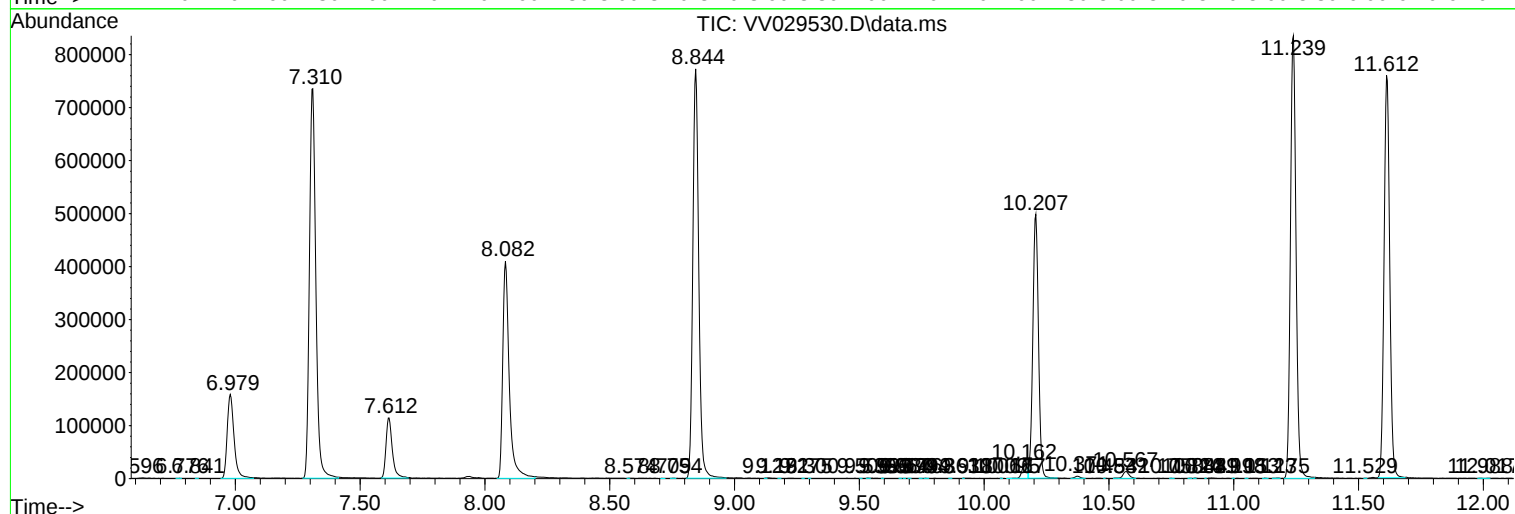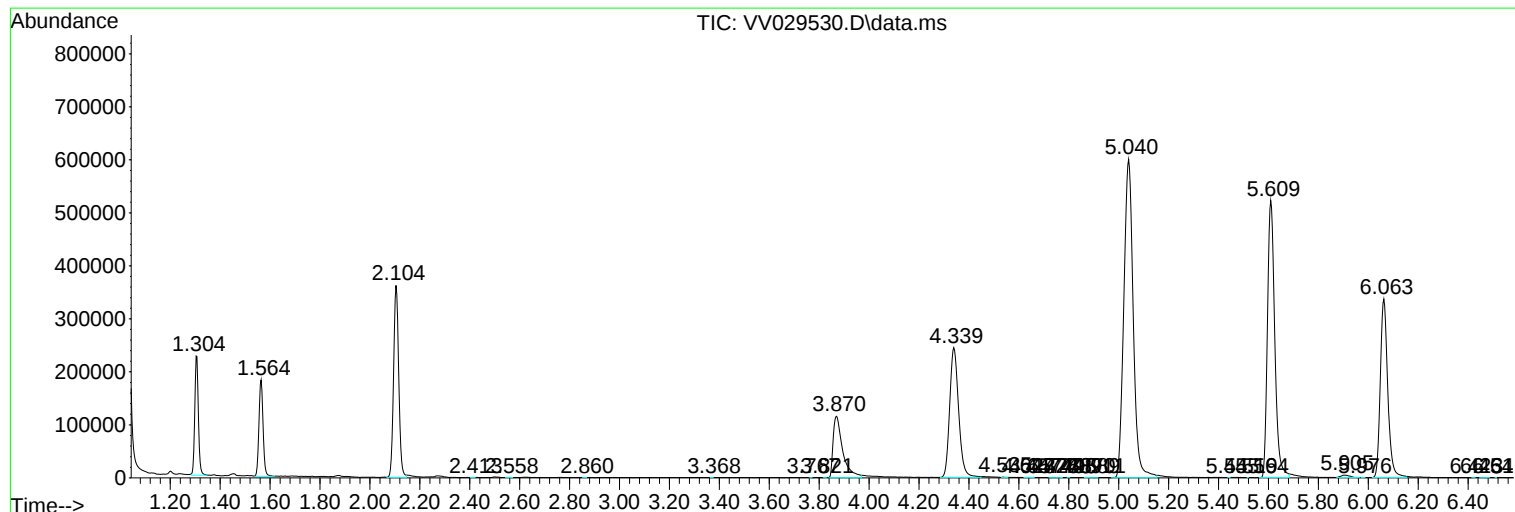

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029530.D
Acq On : 09 Dec 2022 18:42
Operator : SY/MD
Sample : N5959-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029530.D
Acq On : 09 Dec 2022 18:42
Operator : SY/MD
Sample : N5959-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------