

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029531.D
 Acq On : 09 Dec 2022 19:05
 Operator : SY/MD
 Sample : N5959-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	220850	214532	8.55%	1.491%
2	1.564	155	163	181	rVB	166776	192446	7.67%	1.338%
3	1.883	255	262	274	rBV4	2842	5463	0.22%	0.038%
4	2.050	312	314	320	rBV4	359	452	0.02%	0.003%
5	2.105	320	331	347	rBV3	373969	596957	23.80%	4.149%
6	2.278	377	385	404	rVB3	3957	8244	0.33%	0.057%
7	2.420	424	429	430	rBV2	308	260	0.01%	0.002%
8	2.503	446	455	462	rVB4	1284	2028	0.08%	0.014%
9	2.632	484	495	504	rBV5	1615	3265	0.13%	0.023%
10	2.706	511	518	520	rBV2	302	256	0.01%	0.002%
11	2.764	532	536	540	rBV4	455	469	0.02%	0.003%
12	2.806	544	549	552	rBV2	263	267	0.01%	0.002%
13	2.973	597	601	606	rBV	205	197	0.01%	0.001%
14	2.998	606	609	617	rVB2	279	326	0.01%	0.002%
15	3.185	657	667	680	rVB3	1480	3013	0.12%	0.021%
16	3.343	710	716	720	rBV2	200	192	0.01%	0.001%
17	3.873	870	881	924	rBV2	105629	373657	14.90%	2.597%
18	4.339	1009	1026	1050	rBV	221800	547844	21.84%	3.808%
19	4.600	1091	1107	1129	rVV3	31110	78897	3.15%	0.548%
20	4.687	1132	1134	1139	rVB5	320	220	0.01%	0.002%
21	4.844	1179	1183	1187	rVB2	276	193	0.01%	0.001%
22	5.040	1226	1244	1295	rBV2	544438	1440709	57.44%	10.014%
23	5.400	1354	1356	1362	rVB2	330	333	0.01%	0.002%
24	5.439	1362	1368	1372	rVB2	375	402	0.02%	0.003%
25	5.474	1375	1379	1384	rBV4	610	541	0.02%	0.004%
26	5.609	1408	1421	1476	rVV	500798	1024774	40.86%	7.123%
27	5.905	1498	1513	1549	rBV	1276762	2508300	100.00%	17.435%
28	6.063	1549	1562	1589	rVB	302274	624397	24.89%	4.340%
29	6.185	1598	1600	1603	rBV3	622	358	0.01%	0.002%
30	6.272	1626	1627	1633	rVB2	482	289	0.01%	0.002%
31	6.307	1633	1638	1640	rBV	308	219	0.01%	0.002%
32	6.625	1732	1737	1738	rBV2	818	569	0.02%	0.004%
33	6.751	1772	1776	1779	rBV2	364	236	0.01%	0.002%
34	6.912	1820	1826	1828	rBV3	266	263	0.01%	0.002%
35	6.979	1836	1847	1872	rBV	150762	275893	11.00%	1.918%
36	7.146	1896	1899	1902	rBV2	408	324	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029531.D
 Acq On : 09 Dec 2022 19:05
 Operator : SY/MD
 Sample : N5959-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.307	1935	1949	1986	rBV	675952	1197349	47.74%	8.323%
38	7.558	2023	2027	2028	rBV3	294	228	0.01%	0.002%
39	7.616	2034	2045	2075	rVB	102881	184759	7.37%	1.284%
40	7.796	2098	2101	2106	rVB3	403	368	0.01%	0.003%
41	7.838	2106	2114	2115	rBV4	1358	1495	0.06%	0.010%
42	7.934	2135	2144	2150	rBV2	4592	7336	0.29%	0.051%
43	8.027	2167	2173	2175	rBV2	221	230	0.01%	0.002%
44	8.082	2180	2190	2228	rBV	375265	675646	26.94%	4.696%
45	8.291	2252	2255	2258	rBV4	454	323	0.01%	0.002%
46	8.358	2273	2276	2278	rBV2	352	239	0.01%	0.002%
47	8.574	2336	2343	2346	rBV2	565	592	0.02%	0.004%
48	8.590	2346	2348	2352	rVV2	338	242	0.01%	0.002%
49	8.609	2352	2354	2357	rVV3	302	210	0.01%	0.001%
50	8.657	2362	2369	2373	rBV3	522	629	0.03%	0.004%
51	8.680	2373	2376	2380	rVB2	508	376	0.01%	0.003%
52	8.725	2384	2390	2392	rBV3	350	332	0.01%	0.002%
53	8.776	2401	2406	2408	rBV3	326	329	0.01%	0.002%
54	8.844	2414	2427	2451	rBV	742821	1211574	48.30%	8.422%
55	9.056	2490	2493	2498	rBV4	324	330	0.01%	0.002%
56	9.140	2516	2519	2524	rVV2	556	436	0.02%	0.003%
57	9.191	2529	2535	2536	rBV2	332	248	0.01%	0.002%
58	9.310	2567	2572	2578	rBV2	290	353	0.01%	0.002%
59	9.358	2585	2587	2590	rVB	377	222	0.01%	0.002%
60	9.378	2590	2593	2598	rBV2	202	191	0.01%	0.001%
61	9.403	2598	2601	2605	rVB2	392	249	0.01%	0.002%
62	9.535	2637	2642	2644	rBV2	500	365	0.01%	0.003%
63	9.548	2644	2646	2649	rVB3	482	265	0.01%	0.002%
64	9.982	2777	2781	2784	rBV2	267	187	0.01%	0.001%
65	10.063	2803	2806	2812	rBV3	291	301	0.01%	0.002%
66	10.162	2826	2837	2841	rBV2	24101	35276	1.41%	0.245%
67	10.207	2841	2851	2872	rVB	450829	716236	28.55%	4.979%
68	10.378	2894	2904	2916	rVB2	4858	7942	0.32%	0.055%
69	10.464	2926	2931	2935	rBV3	379	396	0.02%	0.003%
70	10.532	2944	2952	2955	rBV3	718	739	0.03%	0.005%
71	10.567	2955	2963	2977	rVB	11618	17937	0.72%	0.125%
72	10.747	3017	3019	3023	rVV	281	208	0.01%	0.001%
73	10.911	3063	3070	3074	rVB3	908	1066	0.04%	0.007%
74	11.178	3150	3153	3159	rVB3	747	738	0.03%	0.005%
75	11.236	3159	3171	3191	rBV	820365	1270839	50.67%	8.834%
76	11.407	3222	3224	3232	rVB4	475	488	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029531.D
 Acq On : 09 Dec 2022 19:05
 Operator : SY/MD
 Sample : N5959-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.487	3243	3249	3253	rBV3	396	463	0.02%	0.003%
78	11.506	3253	3255	3259	rVB3	266	190	0.01%	0.001%
79	11.554	3262	3270	3275	rBV3	2409	3714	0.15%	0.026%
80	11.612	3276	3288	3307	rVV	711568	1130114	45.05%	7.855%
81	11.966	3396	3398	3406	rVB2	318	290	0.01%	0.002%
82	12.072	3427	3431	3436	rBV2	383	386	0.02%	0.003%
83	12.114	3441	3444	3448	rBV2	257	216	0.01%	0.002%
84	12.236	3478	3482	3483	rBV	791	593	0.02%	0.004%
85	12.297	3498	3501	3505	rBV3	296	221	0.01%	0.002%
86	12.439	3540	3545	3546	rBV2	332	244	0.01%	0.002%
87	12.455	3547	3550	3556	rVV4	524	535	0.02%	0.004%
88	12.635	3603	3606	3612	rVB4	563	539	0.02%	0.004%
89	12.693	3621	3624	3628	rBV3	453	334	0.01%	0.002%
90	12.796	3654	3656	3660	rBV2	418	277	0.01%	0.002%
91	13.255	3795	3799	3803	rVB3	559	487	0.02%	0.003%
92	13.361	3829	3832	3835	rBV3	454	367	0.01%	0.003%
93	13.500	3871	3875	3879	rVB3	761	713	0.03%	0.005%
94	13.538	3885	3887	3890	rBV3	329	195	0.01%	0.001%
95	13.615	3907	3911	3917	rBV3	357	409	0.02%	0.003%
96	13.728	3944	3946	3949	rBV4	451	311	0.01%	0.002%
97	13.818	3969	3974	3977	rBV3	524	596	0.02%	0.004%
98	13.979	4020	4024	4027	rBV4	597	563	0.02%	0.004%
99	14.088	4056	4058	4061	rBV3	560	395	0.02%	0.003%
100	14.275	4113	4116	4118	rVB3	610	310	0.01%	0.002%




Sum of corrected areas: 14386516

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029531.D
Acq On : 09 Dec 2022 19:05
Operator : SY/MD
Sample : N5959-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

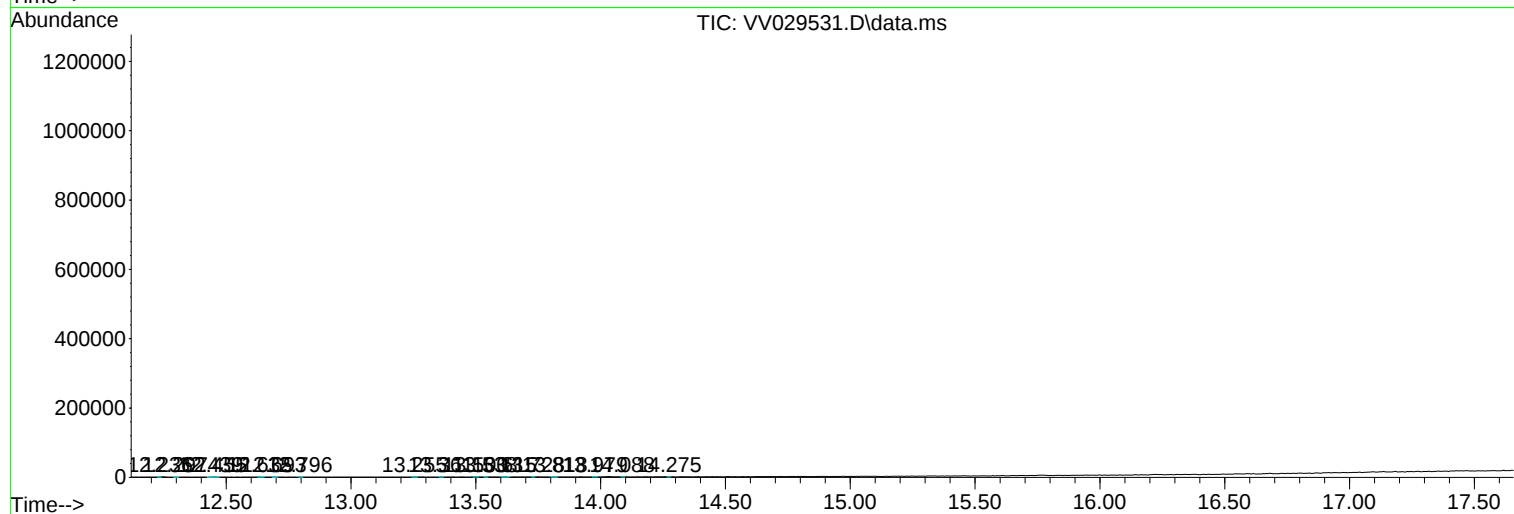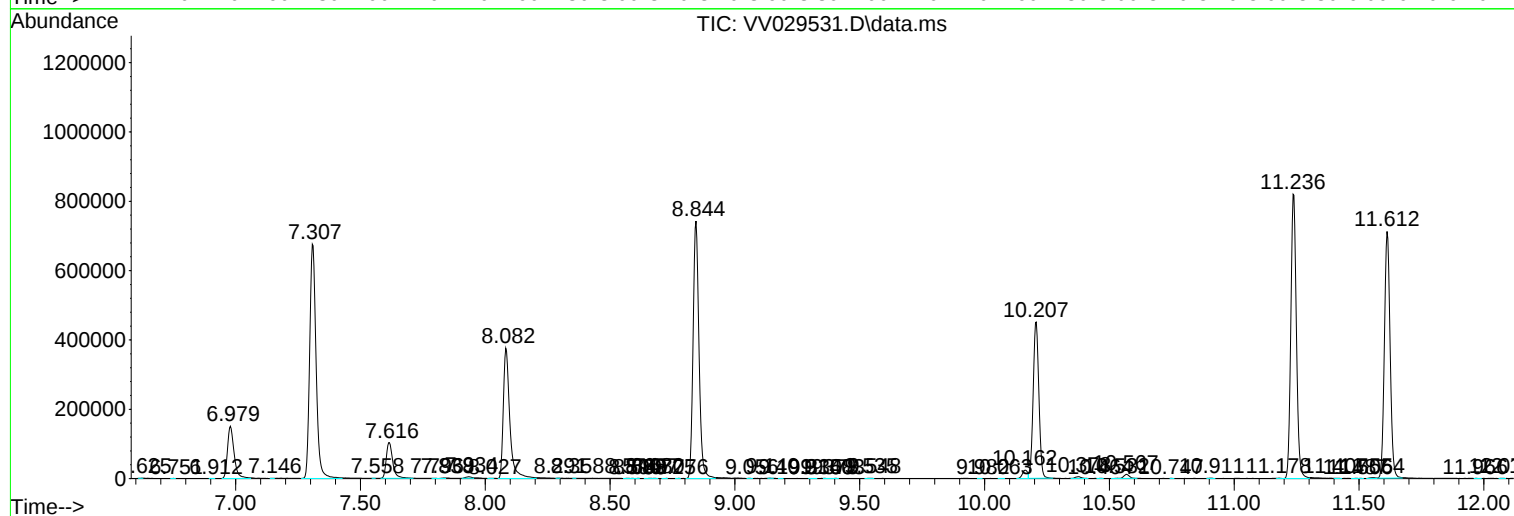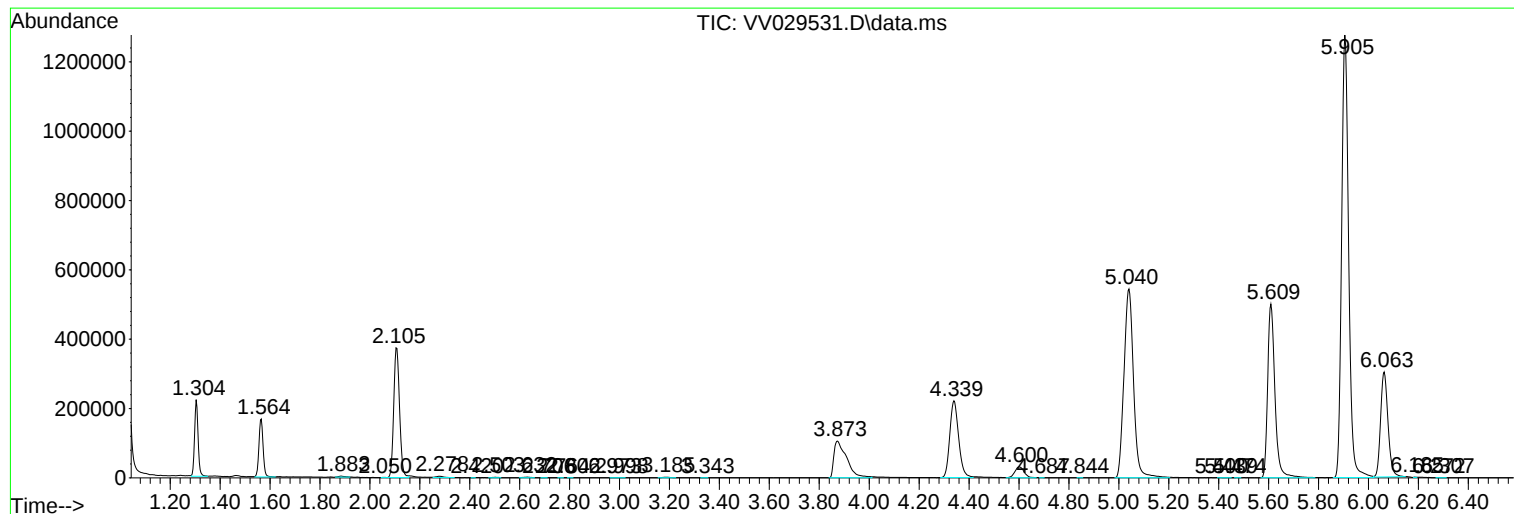

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029531.D
Acq On : 09 Dec 2022 19:05
Operator : SY/MD
Sample : N5959-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029531.D
Acq On : 09 Dec 2022 19:05
Operator : SY/MD
Sample : N5959-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc