

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029532.D
 Acq On : 09 Dec 2022 19:27
 Operator : SY/MD
 Sample : N5959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	217403	217100	14.49%	1.796%
2	1.564	155	163	177	rBV	176057	195548	13.06%	1.618%
3	1.995	295	297	300	rBV3	407	283	0.02%	0.002%
4	2.104	320	331	344	rBV	338560	493955	32.98%	4.087%
5	2.278	378	385	396	rVB4	4390	7992	0.53%	0.066%
6	2.368	411	413	419	rVB2	387	251	0.02%	0.002%
7	2.429	431	432	436	rVB2	379	208	0.01%	0.002%
8	2.506	450	456	465	rVB4	1395	2124	0.14%	0.018%
9	2.632	486	495	496	rBV3	508	564	0.04%	0.005%
10	2.757	530	534	535	rVV2	465	278	0.02%	0.002%
11	2.793	543	545	549	rVB2	440	251	0.02%	0.002%
12	2.937	587	590	593	rVB3	351	220	0.01%	0.002%
13	3.185	662	667	669	rBV	482	375	0.03%	0.003%
14	3.265	685	692	697	rVB2	291	331	0.02%	0.003%
15	3.294	697	701	704	rBV	236	219	0.01%	0.002%
16	3.699	823	827	834	rBV2	178	261	0.02%	0.002%
17	3.873	872	881	911	rBV	107638	295558	19.73%	2.446%
18	4.342	1009	1027	1058	rBV	230512	570865	38.11%	4.724%
19	4.612	1108	1111	1114	rVB2	344	284	0.02%	0.002%
20	4.645	1114	1121	1122	rBV2	340	313	0.02%	0.003%
21	4.937	1207	1212	1217	rBV2	292	262	0.02%	0.002%
22	5.043	1227	1245	1298	rBV2	567889	1497877	100.00%	12.394%
23	5.288	1318	1321	1326	rVB2	638	474	0.03%	0.004%
24	5.397	1353	1355	1359	rBV2	356	232	0.02%	0.002%
25	5.474	1374	1379	1386	rBV4	411	553	0.04%	0.005%
26	5.612	1408	1422	1463	rBV	517386	1069884	71.43%	8.853%
27	5.911	1502	1515	1527	rBV	6639	15545	1.04%	0.129%
28	6.066	1549	1563	1600	rBV	317174	655719	43.78%	5.426%
29	6.628	1730	1738	1740	rBV3	1026	1186	0.08%	0.010%
30	6.699	1758	1760	1764	rVB3	495	302	0.02%	0.002%
31	6.728	1764	1769	1771	rBV	330	312	0.02%	0.003%
32	6.812	1790	1795	1797	rBV3	261	228	0.02%	0.002%
33	6.876	1811	1815	1821	rBV2	218	202	0.01%	0.002%
34	6.982	1836	1848	1870	rBV	151245	278930	18.62%	2.308%
35	7.152	1896	1901	1902	rBV3	492	398	0.03%	0.003%
36	7.233	1923	1926	1929	rVB3	313	234	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029532.D
 Acq On : 09 Dec 2022 19:27
 Operator : SY/MD
 Sample : N5959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.255	1929	1933	1936	rVB3	428	407	0.03%	0.003%
38	7.310	1936	1950	1992	rBV	710725	1244360	83.07%	10.296%
39	7.615	2035	2045	2074	rBV	107771	188134	12.56%	1.557%
40	7.850	2115	2118	2123	rVB2	343	283	0.02%	0.002%
41	7.889	2126	2130	2133	rBV2	408	474	0.03%	0.004%
42	7.937	2135	2145	2152	rBV4	4019	7233	0.48%	0.060%
43	8.085	2177	2191	2238	rBV	393726	720502	48.10%	5.962%
44	8.262	2243	2246	2252	rVB4	1220	1154	0.08%	0.010%
45	8.355	2273	2275	2279	rVB2	350	220	0.01%	0.002%
46	8.461	2306	2308	2310	rBV3	447	259	0.02%	0.002%
47	8.474	2310	2312	2313	rVV2	561	291	0.02%	0.002%
48	8.496	2317	2319	2325	rVV3	348	320	0.02%	0.003%
49	8.535	2327	2331	2334	rVV2	294	264	0.02%	0.002%
50	8.554	2335	2337	2340	rVB2	544	236	0.02%	0.002%
51	8.683	2375	2377	2380	rVB2	404	228	0.02%	0.002%
52	8.722	2387	2389	2393	rVB3	489	270	0.02%	0.002%
53	8.844	2415	2427	2463	rBV	760368	1273500	85.02%	10.537%
54	9.056	2490	2493	2495	rBV3	633	328	0.02%	0.003%
55	9.210	2537	2541	2545	rBV3	359	286	0.02%	0.002%
56	9.291	2561	2566	2568	rBV2	271	221	0.01%	0.002%
57	9.329	2574	2578	2582	rBV2	283	289	0.02%	0.002%
58	9.390	2592	2597	2600	rBV2	256	246	0.02%	0.002%
59	9.577	2651	2655	2658	rVB2	481	360	0.02%	0.003%
60	9.879	2742	2749	2755	rVB3	373	515	0.03%	0.004%
61	9.918	2756	2761	2764	rBV3	671	576	0.04%	0.005%
62	9.956	2768	2773	2777	rBV2	231	200	0.01%	0.002%
63	9.975	2777	2779	2782	rBV	267	201	0.01%	0.002%
64	10.017	2788	2792	2796	rBV2	272	219	0.01%	0.002%
65	10.069	2804	2808	2810	rBV3	347	245	0.02%	0.002%
66	10.165	2827	2838	2841	rBV2	24279	34785	2.32%	0.288%
67	10.207	2842	2851	2876	rVB	478902	746942	49.87%	6.180%
68	10.374	2888	2903	2913	rVB3	5045	8620	0.58%	0.071%
69	10.490	2934	2939	2942	rBV3	368	368	0.02%	0.003%
70	10.570	2955	2964	2978	rVB	11975	19362	1.29%	0.160%
71	10.683	2992	2999	3001	rBV3	318	328	0.02%	0.003%
72	10.911	3063	3070	3075	rVB4	858	1054	0.07%	0.009%
73	11.033	3105	3108	3112	rVB2	394	274	0.02%	0.002%
74	11.136	3136	3140	3143	rBV3	233	247	0.02%	0.002%
75	11.184	3153	3155	3159	rBV	371	289	0.02%	0.002%
76	11.239	3159	3172	3200	rBV	874649	1330142	88.80%	11.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029532.D
 Acq On : 09 Dec 2022 19:27
 Operator : SY/MD
 Sample : N5959-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.442	3232	3235	3239	rVB	344	256	0.02%	0.002%
78	11.467	3239	3243	3251	rBV3	385	379	0.03%	0.003%
79	11.512	3253	3257	3262	rBV2	356	399	0.03%	0.003%
80	11.554	3263	3270	3276	rVV6	2592	3868	0.26%	0.032%
81	11.612	3277	3288	3322	rVB	737153	1176993	78.58%	9.739%
82	11.831	3353	3356	3358	rBV	380	253	0.02%	0.002%
83	11.873	3366	3369	3372	rBV3	307	228	0.02%	0.002%
84	11.975	3396	3401	3402	rBV3	280	213	0.01%	0.002%
85	12.239	3477	3483	3492	rVB3	1455	2200	0.15%	0.018%
86	12.339	3511	3514	3518	rVB3	297	228	0.02%	0.002%
87	12.419	3537	3539	3544	rVV2	309	306	0.02%	0.003%
88	12.538	3573	3576	3580	rBV3	431	334	0.02%	0.003%
89	12.638	3600	3607	3611	rBV6	624	869	0.06%	0.007%
90	12.676	3617	3619	3628	rVB3	255	276	0.02%	0.002%
91	12.911	3688	3692	3694	rBV3	304	261	0.02%	0.002%
92	13.030	3726	3729	3736	rBV4	553	481	0.03%	0.004%
93	13.107	3749	3753	3755	rVB3	461	284	0.02%	0.002%
94	13.188	3776	3778	3783	rVB3	394	361	0.02%	0.003%
95	13.258	3792	3800	3803	rBV3	888	1208	0.08%	0.010%
96	13.319	3817	3819	3823	rBV4	498	360	0.02%	0.003%
97	13.493	3869	3873	3875	rBV3	543	424	0.03%	0.004%
98	13.731	3944	3947	3952	rVB5	904	852	0.06%	0.007%
99	13.798	3966	3968	3971	rBV	460	300	0.02%	0.002%
100	13.824	3971	3976	3980	rVB4	644	704	0.05%	0.006%


Sum of corrected areas: 12085587

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029532.D
Acq On : 09 Dec 2022 19:27
Operator : SY/MD
Sample : N5959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

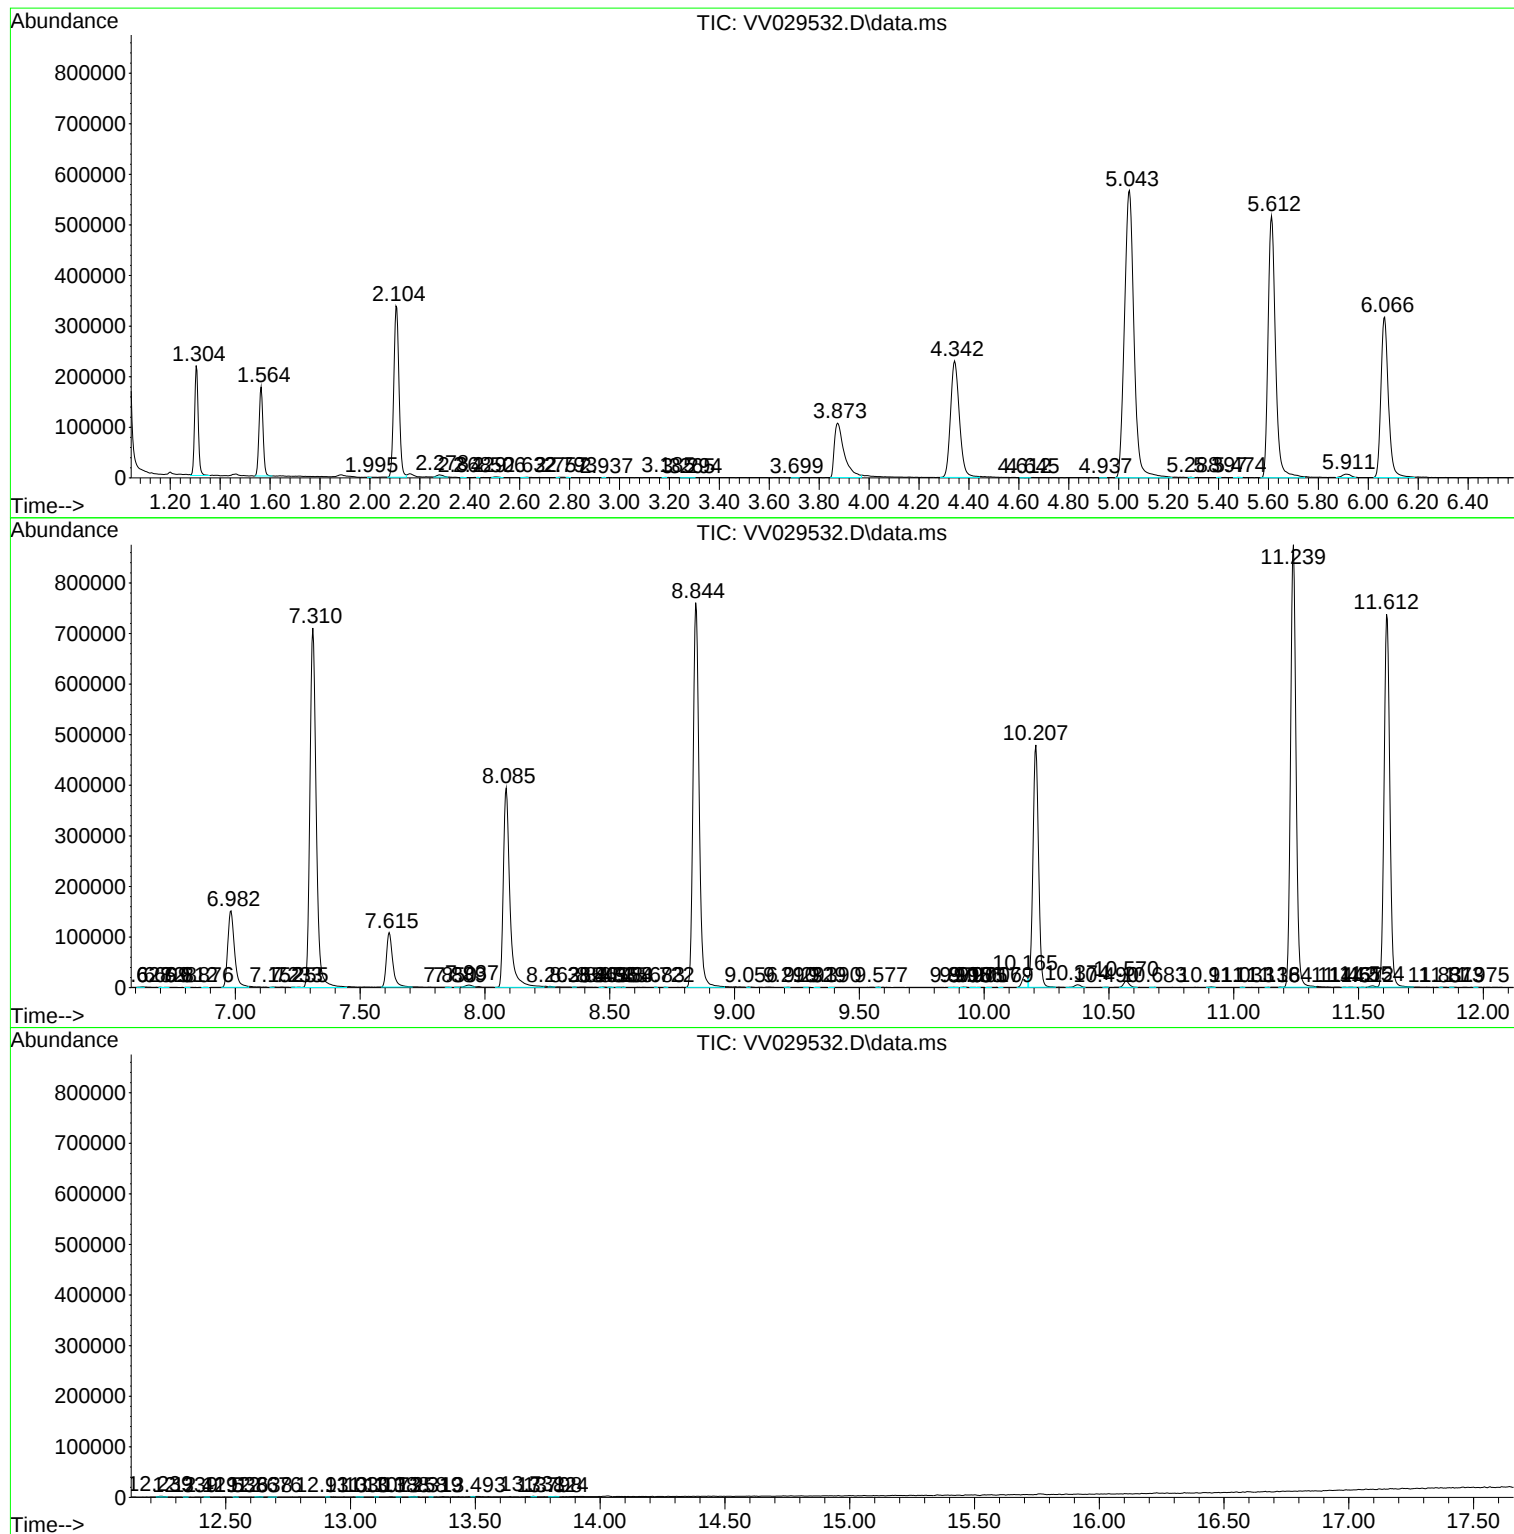

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029532.D
Acq On : 09 Dec 2022 19:27
Operator : SY/MD
Sample : N5959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029532.D
Acq On : 09 Dec 2022 19:27
Operator : SY/MD
Sample : N5959-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------