

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029533.D
 Acq On : 09 Dec 2022 19:50
 Operator : SY/MD
 Sample : N5959-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	219874	218080	14.19%	1.782%
2	1.564	155	163	179	rVB	182398	203138	13.22%	1.660%
3	1.982	290	293	296	rBV2	634	424	0.03%	0.003%
4	2.105	320	331	347	rBV	350519	505466	32.90%	4.130%
5	2.275	379	384	397	rVB4	2975	4798	0.31%	0.039%
6	2.397	418	422	424	rBV3	291	241	0.02%	0.002%
7	2.506	447	456	462	rVV3	1233	1687	0.11%	0.014%
8	2.616	484	490	491	rBV3	862	650	0.04%	0.005%
9	2.751	530	532	533	rBV	393	203	0.01%	0.002%
10	3.034	615	620	625	rBV2	232	280	0.02%	0.002%
11	3.185	659	667	673	rVV3	419	607	0.04%	0.005%
12	3.249	685	687	692	rVB3	287	241	0.02%	0.002%
13	3.362	719	722	730	rVB2	222	233	0.02%	0.002%
14	3.410	730	737	741	rBV3	353	374	0.02%	0.003%
15	3.551	775	781	786	rBV2	266	319	0.02%	0.003%
16	3.870	869	880	921	rBV	109632	304978	19.85%	2.492%
17	4.339	1008	1026	1058	rBV	237357	585049	38.08%	4.780%
18	4.635	1115	1118	1121	rVB2	495	281	0.02%	0.002%
19	4.667	1125	1128	1129	rBV2	434	203	0.01%	0.002%
20	4.677	1129	1131	1136	rVB2	462	287	0.02%	0.002%
21	4.770	1153	1160	1162	rBV	213	213	0.01%	0.002%
22	5.040	1226	1244	1293	rBV2	579160	1536497	100.00%	12.555%
23	5.403	1355	1357	1361	rVB3	347	230	0.01%	0.002%
24	5.609	1407	1421	1463	rBV	510435	1047181	68.15%	8.557%
25	5.911	1502	1515	1533	rBV2	48257	101146	6.58%	0.826%
26	6.063	1546	1562	1595	rBV	327044	674506	43.90%	5.511%
27	6.567	1715	1719	1722	rVB2	319	227	0.01%	0.002%
28	6.625	1731	1737	1739	rBV3	1040	1026	0.07%	0.008%
29	6.747	1771	1775	1778	rVV3	370	383	0.02%	0.003%
30	6.767	1778	1781	1784	rVV2	291	207	0.01%	0.002%
31	6.792	1787	1789	1792	rVV	324	213	0.01%	0.002%
32	6.812	1792	1795	1799	rVB3	290	225	0.01%	0.002%
33	6.837	1799	1803	1808	rBV3	286	209	0.01%	0.002%
34	6.979	1834	1847	1875	rBV	155589	288453	18.77%	2.357%
35	7.108	1885	1887	1890	rVB3	394	216	0.01%	0.002%
36	7.162	1899	1904	1906	rBV3	465	399	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029533.D
 Acq On : 09 Dec 2022 19:50
 Operator : SY/MD
 Sample : N5959-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.175	1906	1908	1910	rBV2	449	263	0.02%	0.002%
38	7.233	1924	1926	1932	rVB2	700	585	0.04%	0.005%
39	7.259	1932	1934	1937	rBV2	358	203	0.01%	0.002%
40	7.307	1937	1949	1982	rBV	718256	1267890	82.52%	10.360%
41	7.612	2034	2044	2066	rBV	109188	194802	12.68%	1.592%
42	7.770	2089	2093	2095	rBV2	254	205	0.01%	0.002%
43	7.808	2103	2105	2108	rBV2	386	237	0.02%	0.002%
44	7.850	2115	2118	2121	rBV4	371	272	0.02%	0.002%
45	7.873	2121	2125	2128	rBV2	276	270	0.02%	0.002%
46	7.934	2136	2144	2151	rBV3	3220	5327	0.35%	0.044%
47	7.966	2151	2154	2160	rVB4	1234	1245	0.08%	0.010%
48	8.082	2180	2190	2233	rVV	401636	731224	47.59%	5.975%
49	8.371	2278	2280	2283	rVB	402	244	0.02%	0.002%
50	8.426	2294	2297	2300	rVB4	403	249	0.02%	0.002%
51	8.452	2302	2305	2310	rBV3	544	582	0.04%	0.005%
52	8.516	2322	2325	2329	rVB3	291	215	0.01%	0.002%
53	8.570	2339	2342	2347	rVB3	480	409	0.03%	0.003%
54	8.641	2360	2364	2366	rVV2	274	215	0.01%	0.002%
55	8.757	2397	2400	2405	rVB2	379	330	0.02%	0.003%
56	8.844	2415	2427	2461	rBV	755591	1241305	80.79%	10.143%
57	9.008	2475	2478	2483	rVV3	660	541	0.04%	0.004%
58	9.133	2512	2517	2519	rBV3	447	423	0.03%	0.003%
59	9.165	2525	2527	2531	rVB	467	223	0.01%	0.002%
60	9.197	2532	2537	2540	rBV3	298	285	0.02%	0.002%
61	9.812	2726	2728	2732	rBV2	419	236	0.02%	0.002%
62	9.860	2738	2743	2749	rVB3	353	445	0.03%	0.004%
63	9.889	2749	2752	2755	rBV	429	237	0.02%	0.002%
64	9.918	2755	2761	2763	rBV3	549	528	0.03%	0.004%
65	10.162	2826	2837	2841	rBV2	25459	36504	2.38%	0.298%
66	10.207	2841	2851	2872	rVB	477006	756981	49.27%	6.185%
67	10.307	2879	2882	2887	rBV4	349	279	0.02%	0.002%
68	10.374	2894	2903	2913	rBV4	3631	5709	0.37%	0.047%
69	10.435	2920	2922	2927	rVV3	466	337	0.02%	0.003%
70	10.529	2946	2951	2952	rBV4	531	465	0.03%	0.004%
71	10.567	2954	2963	2976	rVB2	11613	19327	1.26%	0.158%
72	10.783	3027	3030	3034	rBV2	341	238	0.02%	0.002%
73	10.844	3045	3049	3052	rBV	374	244	0.02%	0.002%
74	10.914	3063	3071	3080	rVB2	751	1383	0.09%	0.011%
75	11.168	3141	3150	3153	rBV4	727	774	0.05%	0.006%
76	11.239	3159	3172	3196	rBV	825923	1279617	83.28%	10.456%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029533.D
 Acq On : 09 Dec 2022 19:50
 Operator : SY/MD
 Sample : N5959-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.381	3215	3216	3219	rVB2	508	208	0.01%	0.002%
78	11.500	3247	3253	3254	rBV3	373	366	0.02%	0.003%
79	11.551	3261	3269	3276	rBV4	2391	4229	0.28%	0.035%
80	11.612	3276	3288	3320	rVV	750729	1193305	77.66%	9.751%
81	11.776	3337	3339	3345	rVB3	522	399	0.03%	0.003%
82	11.953	3390	3394	3398	rVB3	381	300	0.02%	0.002%
83	11.988	3404	3405	3409	rVB	487	230	0.01%	0.002%
84	12.011	3409	3412	3415	rBV2	341	302	0.02%	0.002%
85	12.091	3434	3437	3442	rBV3	263	207	0.01%	0.002%
86	12.239	3476	3483	3491	rBV4	714	1169	0.08%	0.010%
87	12.519	3562	3570	3573	rBV3	374	487	0.03%	0.004%
88	12.619	3598	3601	3602	rBV3	368	204	0.01%	0.002%
89	12.792	3651	3655	3663	rBV4	758	946	0.06%	0.008%
90	12.824	3663	3665	3669	rVV2	295	219	0.01%	0.002%
91	12.902	3686	3689	3691	rVB	364	205	0.01%	0.002%
92	13.088	3744	3747	3751	rBV3	473	329	0.02%	0.003%
93	13.120	3754	3757	3760	rBV2	382	232	0.02%	0.002%
94	13.246	3794	3796	3799	rBV2	627	484	0.03%	0.004%
95	13.297	3807	3812	3815	rBV2	487	498	0.03%	0.004%
96	13.387	3833	3840	3846	rBV6	540	907	0.06%	0.007%
97	13.503	3866	3876	3880	rBV5	1200	2222	0.14%	0.018%
98	13.773	3957	3960	3961	rBV2	432	247	0.02%	0.002%
99	14.220	4096	4099	4101	rBV3	495	311	0.02%	0.003%
100	14.429	4160	4164	4166	rBV2	633	627	0.04%	0.005%




Sum of corrected areas: 12238351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029533.D
Acq On : 09 Dec 2022 19:50
Operator : SY/MD
Sample : N5959-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

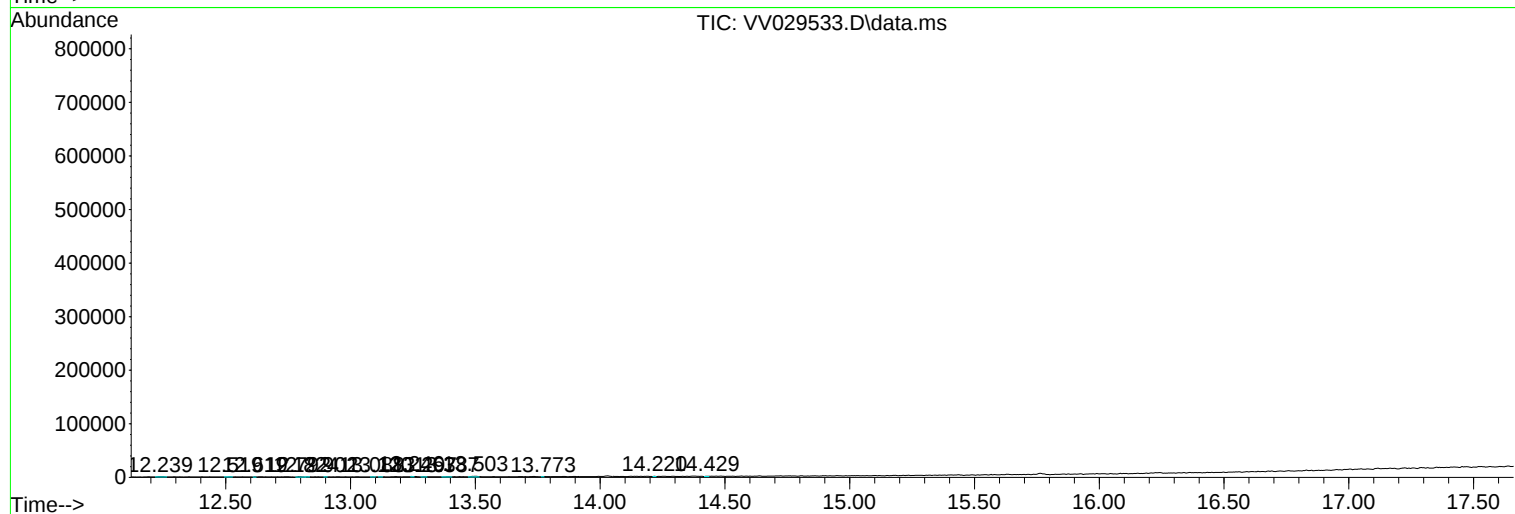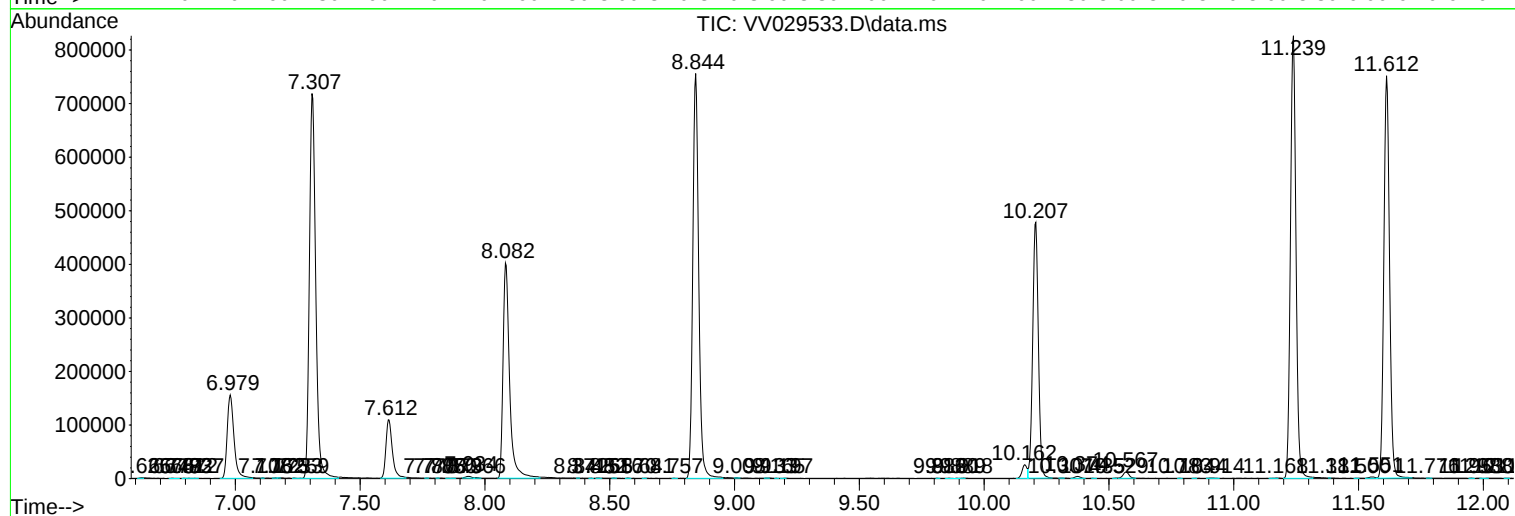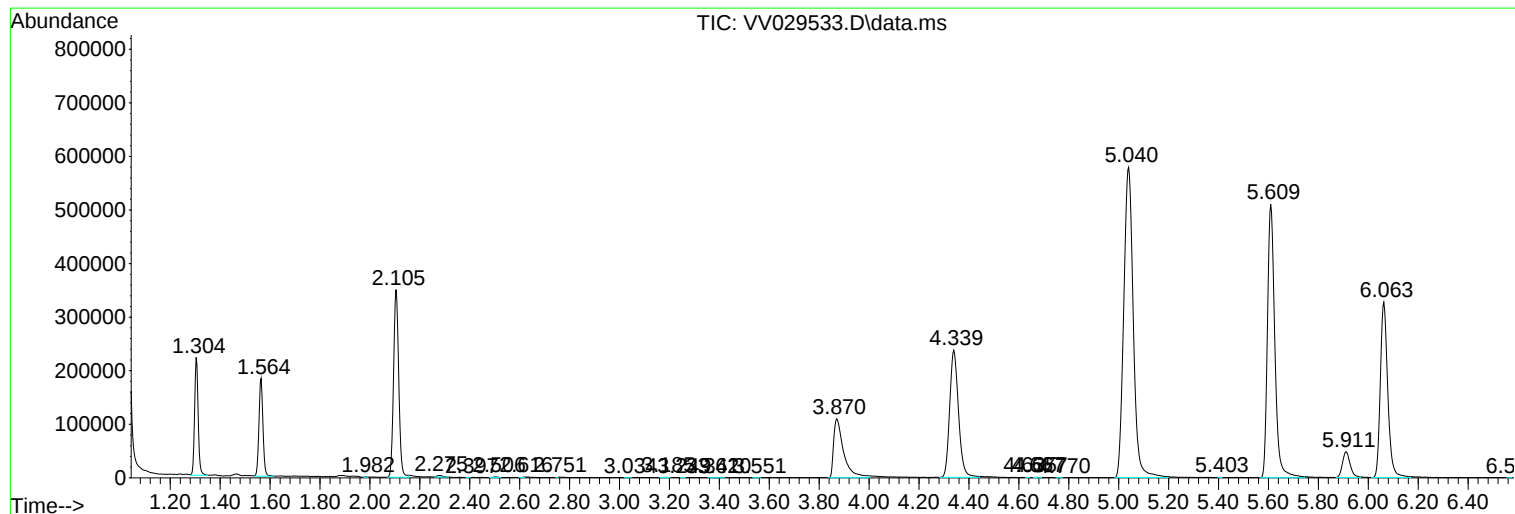

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029533.D
Acq On : 09 Dec 2022 19:50
Operator : SY/MD
Sample : N5959-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029533.D
Acq On : 09 Dec 2022 19:50
Operator : SY/MD
Sample : N5959-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------