

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029536.D
 Acq On : 09 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5959-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	220232	220551	14.37%	1.820%
2	1.565	155	163	177	rVB	174258	199926	13.03%	1.650%
3	2.105	321	331	345	rBV	349247	503520	32.81%	4.154%
4	2.507	449	456	462	rBV2	1131	1444	0.09%	0.012%
5	2.542	466	467	471	rVB3	277	153	0.01%	0.001%
6	2.571	474	476	481	rVB	243	147	0.01%	0.001%
7	2.632	488	495	497	rBV	962	1167	0.08%	0.010%
8	2.716	517	521	526	rBV2	334	289	0.02%	0.002%
9	2.870	566	569	576	rVB3	324	350	0.02%	0.003%
10	2.928	585	587	590	rBV	186	113	0.01%	0.001%
11	2.944	590	592	595	rVB2	268	137	0.01%	0.001%
12	2.973	598	601	602	rBV2	153	100	0.01%	0.001%
13	3.002	607	610	615	rVB2	217	170	0.01%	0.001%
14	3.101	638	641	645	rBB2	201	148	0.01%	0.001%
15	3.124	645	648	652	rBV2	241	197	0.01%	0.002%
16	3.188	660	668	679	rVB	1200	2170	0.14%	0.018%
17	3.253	684	688	691	rBV	261	195	0.01%	0.002%
18	3.330	704	712	715	rBV2	298	349	0.02%	0.003%
19	3.449	746	749	751	rBV	150	97	0.01%	0.001%
20	3.664	812	816	817	rBV	208	107	0.01%	0.001%
21	3.722	831	834	837	rVB	179	106	0.01%	0.001%
22	3.745	837	841	846	rVB2	204	173	0.01%	0.001%
23	3.777	846	851	854	rBV2	133	126	0.01%	0.001%
24	3.796	854	857	862	rVB2	143	132	0.01%	0.001%
25	3.873	871	881	919	rBV	109756	319788	20.84%	2.639%
26	4.339	1010	1026	1059	rBV	235393	587416	38.28%	4.847%
27	4.831	1174	1179	1182	rVB4	409	281	0.02%	0.002%
28	4.963	1215	1220	1222	rBV	169	145	0.01%	0.001%
29	5.040	1226	1244	1290	rBV2	583224	1534566	100.00%	12.662%
30	5.281	1316	1319	1323	rBV3	391	332	0.02%	0.003%
31	5.465	1374	1376	1377	rBV	301	122	0.01%	0.001%
32	5.609	1408	1421	1458	rVV	518461	1058803	69.00%	8.736%
33	5.915	1502	1516	1531	rVB8	7139	17711	1.15%	0.146%
34	5.979	1531	1536	1540	rBV2	380	324	0.02%	0.003%
35	6.063	1548	1562	1600	rBV	322243	672272	43.81%	5.547%
36	6.426	1672	1675	1679	rBV2	195	147	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029536.D
 Acq On : 09 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5959-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.523	1701	1705	1708	rBV2	220	163	0.01%	0.001%
38	6.555	1713	1715	1718	rVB3	189	126	0.01%	0.001%
39	6.622	1730	1736	1737	rBV2	900	819	0.05%	0.007%
40	6.687	1755	1756	1759	rBV2	219	132	0.01%	0.001%
41	6.751	1772	1776	1779	rVB2	211	152	0.01%	0.001%
42	6.773	1779	1783	1784	rBV2	200	136	0.01%	0.001%
43	6.870	1810	1813	1815	rBV	268	202	0.01%	0.002%
44	6.921	1825	1829	1831	rBV2	324	249	0.02%	0.002%
45	6.979	1835	1847	1876	rBV	155465	289321	18.85%	2.387%
46	7.127	1889	1893	1895	rBV2	428	303	0.02%	0.003%
47	7.233	1924	1926	1929	rVB2	532	319	0.02%	0.003%
48	7.249	1929	1931	1934	rVB	286	107	0.01%	0.001%
49	7.310	1936	1950	1990	rBV	724105	1280457	83.44%	10.565%
50	7.616	2035	2045	2075	rBV	110091	195024	12.71%	1.609%
51	7.931	2135	2143	2144	rBV4	4375	4117	0.27%	0.034%
52	8.082	2180	2190	2230	rBV	397039	720869	46.98%	5.948%
53	8.513	2322	2324	2325	rBV	358	183	0.01%	0.002%
54	8.555	2334	2337	2339	rBV2	398	221	0.01%	0.002%
55	8.622	2354	2358	2362	rBV2	399	379	0.02%	0.003%
56	8.703	2379	2383	2387	rVB3	421	382	0.02%	0.003%
57	8.728	2387	2391	2392	rBV	312	179	0.01%	0.001%
58	8.770	2402	2404	2408	rVB2	179	102	0.01%	0.001%
59	8.844	2415	2427	2453	rBV	765831	1249985	81.46%	10.313%
60	9.092	2502	2504	2507	rVB	299	144	0.01%	0.001%
61	9.233	2544	2548	2552	rBV3	290	227	0.01%	0.002%
62	9.330	2573	2578	2579	rBV2	184	159	0.01%	0.001%
63	9.458	2614	2618	2622	rBV	285	240	0.02%	0.002%
64	9.596	2658	2661	2663	rBV2	245	182	0.01%	0.002%
65	9.641	2671	2675	2676	rBV	192	104	0.01%	0.001%
66	9.683	2686	2688	2691	rVB2	239	153	0.01%	0.001%
67	9.786	2716	2720	2723	rBV	222	162	0.01%	0.001%
68	9.850	2737	2740	2742	rBV2	285	154	0.01%	0.001%
69	9.908	2754	2758	2759	rBV2	313	212	0.01%	0.002%
70	9.924	2759	2763	2765	rVV2	538	425	0.03%	0.004%
71	9.976	2777	2779	2784	rVB3	385	246	0.02%	0.002%
72	10.005	2786	2788	2791	rVV	163	105	0.01%	0.001%
73	10.030	2791	2796	2801	rVB2	241	312	0.02%	0.003%
74	10.162	2826	2837	2841	rBV	25033	36032	2.35%	0.297%
75	10.207	2842	2851	2868	rVB	479635	753924	49.13%	6.221%
76	10.339	2890	2892	2895	rBV3	230	102	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029536.D
 Acq On : 09 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5959-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.375	2895	2903	2911	rBV2	4278	6898	0.45%	0.057%
78	10.445	2921	2925	2927	rBV2	332	238	0.02%	0.002%
79	10.474	2930	2934	2937	rBV2	322	278	0.02%	0.002%
80	10.567	2956	2963	2979	rVB	12521	19529	1.27%	0.161%
81	10.651	2986	2989	2992	rBV	364	175	0.01%	0.001%
82	10.770	3023	3026	3032	rBV3	317	306	0.02%	0.003%
83	10.879	3057	3060	3062	rBV2	147	108	0.01%	0.001%
84	10.911	3064	3070	3076	rVV5	1035	1466	0.10%	0.012%
85	11.037	3105	3109	3112	rBV2	208	181	0.01%	0.001%
86	11.059	3113	3116	3119	rVB2	233	142	0.01%	0.001%
87	11.082	3120	3123	3126	rBV	167	120	0.01%	0.001%
88	11.133	3137	3139	3144	rVB3	368	284	0.02%	0.002%
89	11.175	3144	3152	3160	rBV4	1573	2424	0.16%	0.020%
90	11.236	3160	3171	3201	rBV	806359	1258806	82.03%	10.386%
91	11.612	3276	3288	3315	rBV	740164	1145867	74.67%	9.454%
92	11.812	3348	3350	3356	rBV5	398	336	0.02%	0.003%
93	12.091	3434	3437	3441	rBV	464	320	0.02%	0.003%
94	12.243	3476	3484	3489	rBV5	1172	1880	0.12%	0.016%
95	12.394	3529	3531	3537	rVB3	348	245	0.02%	0.002%
96	12.509	3562	3567	3572	rBV3	311	384	0.03%	0.003%
97	12.635	3601	3606	3613	rVB5	1739	2156	0.14%	0.018%
98	12.667	3614	3616	3621	rBV4	499	422	0.03%	0.003%
99	13.252	3791	3798	3807	rVB7	2530	3814	0.25%	0.031%
100	13.497	3864	3874	3884	rBV2	7593	12947	0.84%	0.107%




Sum of corrected areas: 12119910

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029536.D
Acq On : 09 Dec 2022 21:19
Operator : SY/MD
Sample : N5959-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

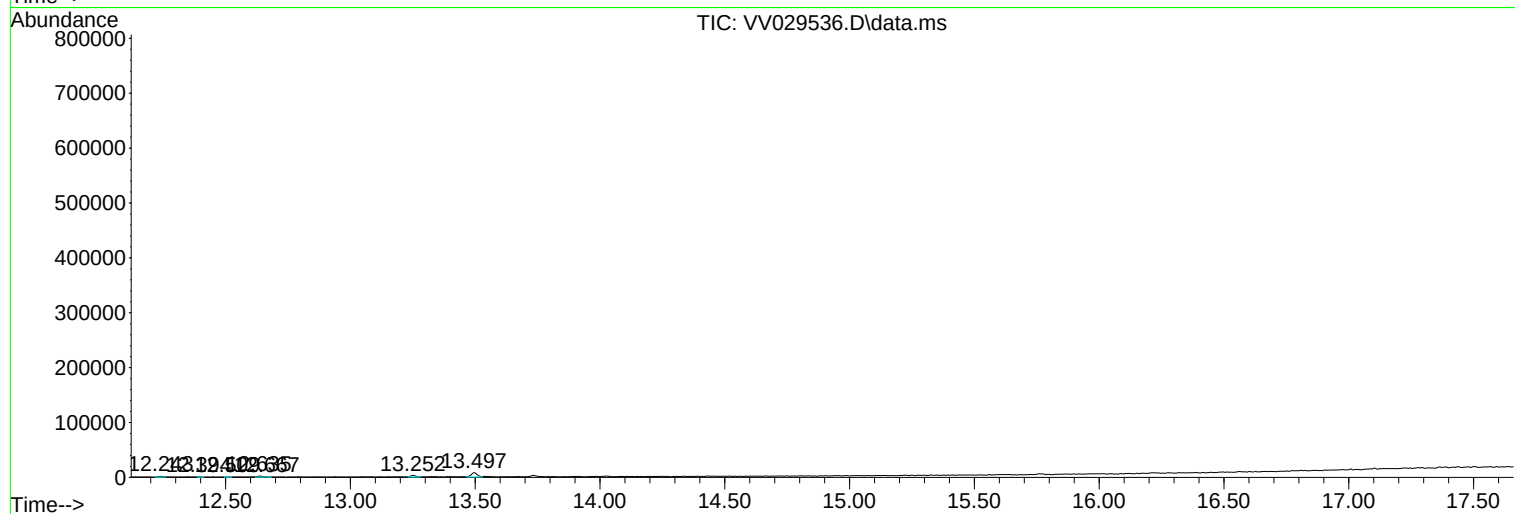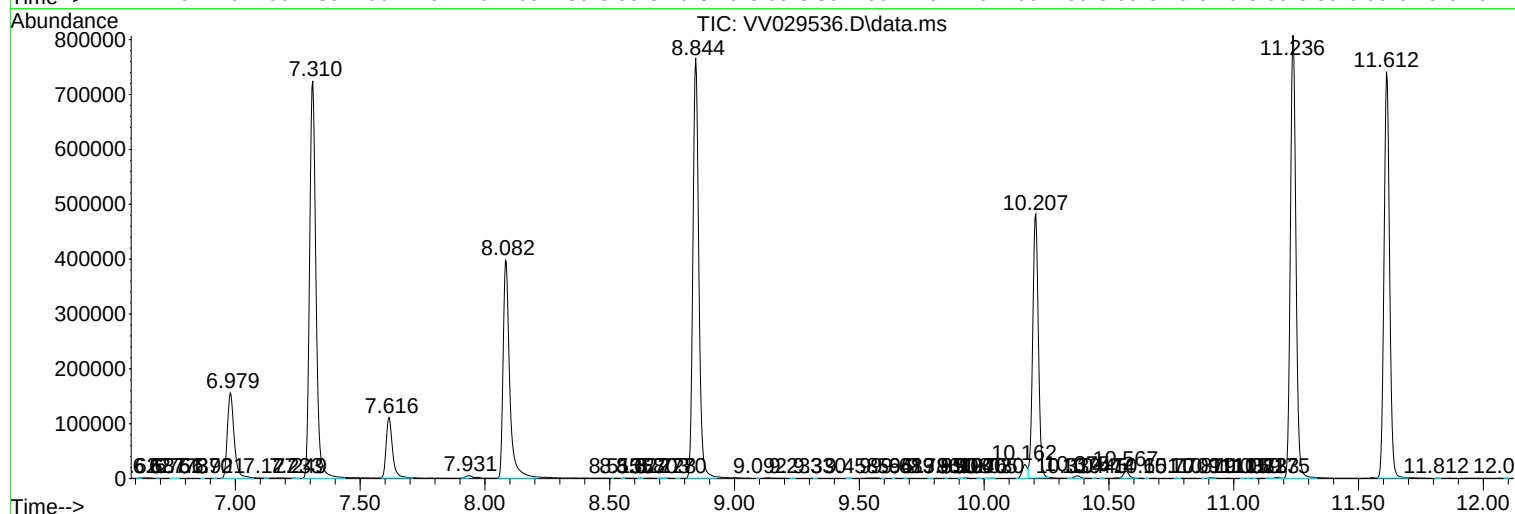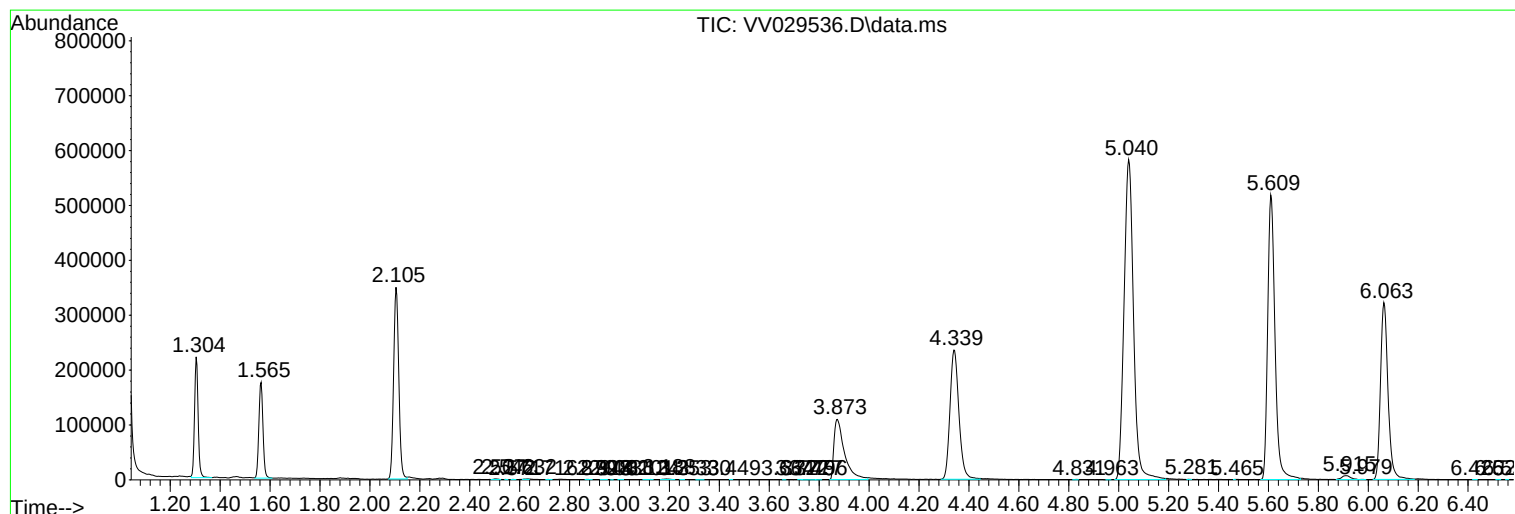

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029536.D
Acq On : 09 Dec 2022 21:19
Operator : SY/MD
Sample : N5959-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029536.D
Acq On : 09 Dec 2022 21:19
Operator : SY/MD
Sample : N5959-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc