

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029537.D
 Acq On : 09 Dec 2022 21:43
 Operator : SY/MD
 Sample : N5959-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	222894	219173	14.78%	1.738%
2	1.565	155	163	175	rVB	175672	198130	13.36%	1.571%
3	2.105	320	331	346	rBV2	350890	524638	35.39%	4.161%
4	2.452	437	439	440	rBV	337	73	0.00%	0.001%
5	2.500	449	454	462	rVB4	1104	1566	0.11%	0.012%
6	2.719	516	522	524	rBV2	219	230	0.02%	0.002%
7	2.860	564	566	568	rBV2	195	102	0.01%	0.001%
8	2.989	604	606	611	rBV	150	159	0.01%	0.001%
9	3.230	677	681	683	rBV2	188	163	0.01%	0.001%
10	3.410	731	737	739	rBV2	184	187	0.01%	0.001%
11	3.478	755	758	759	rBV	141	79	0.01%	0.001%
12	3.642	804	809	811	rBV	114	88	0.01%	0.001%
13	3.671	816	818	824	rVB3	218	146	0.01%	0.001%
14	3.719	831	833	836	rBV	224	120	0.01%	0.001%
15	3.873	871	881	934	rBV2	108048	346494	23.37%	2.748%
16	4.339	1010	1026	1050	rBV	227769	561039	37.84%	4.450%
17	4.725	1144	1146	1150	rBV	168	116	0.01%	0.001%
18	4.838	1179	1181	1182	rBV	168	70	0.00%	0.001%
19	4.902	1197	1201	1204	rBV3	241	219	0.01%	0.002%
20	4.934	1208	1211	1213	rBV	213	102	0.01%	0.001%
21	4.963	1217	1220	1224	rBV2	111	77	0.01%	0.001%
22	5.040	1226	1244	1294	rBV2	563176	1482548	100.00%	11.758%
23	5.462	1372	1375	1377	rBV2	255	187	0.01%	0.001%
24	5.507	1388	1389	1392	rVB	253	76	0.01%	0.001%
25	5.526	1393	1395	1397	rBV	166	78	0.01%	0.001%
26	5.609	1408	1421	1447	rBV	513754	1044421	70.45%	8.283%
27	5.908	1500	1514	1549	rBV	342492	694799	46.87%	5.510%
28	6.063	1549	1562	1597	rVB	315155	651165	43.92%	5.164%
29	6.294	1631	1634	1636	rVB2	258	132	0.01%	0.001%
30	6.355	1650	1653	1655	rBV3	195	108	0.01%	0.001%
31	6.555	1711	1715	1717	rBV2	189	125	0.01%	0.001%
32	6.571	1717	1720	1724	rBV	265	145	0.01%	0.001%
33	6.622	1730	1736	1739	rBV4	1076	1222	0.08%	0.010%
34	6.732	1768	1770	1772	rVB4	371	159	0.01%	0.001%
35	6.793	1787	1789	1793	rBV	288	229	0.02%	0.002%
36	6.841	1801	1804	1807	rVB	163	86	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029537.D
 Acq On : 09 Dec 2022 21:43
 Operator : SY/MD
 Sample : N5959-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COEL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.863	1807	1811	1813	rBV2	139	109	0.01%	0.001%
38	6.879	1814	1816	1820	rVV2	196	96	0.01%	0.001%
39	6.918	1826	1828	1831	rVB	257	86	0.01%	0.001%
40	6.979	1835	1847	1872	rBV	150807	279483	18.85%	2.217%
41	7.153	1899	1901	1902	rBV	412	163	0.01%	0.001%
42	7.230	1923	1925	1928	rBV3	366	264	0.02%	0.002%
43	7.307	1936	1949	1982	rBV	700551	1229922	82.96%	9.755%
44	7.613	2034	2044	2077	rBV	107609	191755	12.93%	1.521%
45	7.931	2136	2143	2150	rBV4	3573	5926	0.40%	0.047%
46	8.085	2180	2191	2232	rBV	386974	714553	48.20%	5.667%
47	8.429	2295	2298	2301	rBV2	464	318	0.02%	0.003%
48	8.661	2367	2370	2371	rBV	242	168	0.01%	0.001%
49	8.693	2378	2380	2383	rBV	248	142	0.01%	0.001%
50	8.725	2387	2390	2391	rBV2	171	100	0.01%	0.001%
51	8.748	2394	2397	2400	rVB	248	179	0.01%	0.001%
52	8.767	2400	2403	2404	rBV	423	217	0.01%	0.002%
53	8.844	2415	2427	2454	rBV	770159	1236499	83.40%	9.807%
54	9.050	2488	2491	2493	rBV2	448	327	0.02%	0.003%
55	9.140	2511	2519	2522	rBV4	854	994	0.07%	0.008%
56	9.188	2531	2534	2535	rBV	191	111	0.01%	0.001%
57	9.220	2542	2544	2547	rVB	278	136	0.01%	0.001%
58	9.233	2547	2548	2552	rVB2	184	102	0.01%	0.001%
59	9.252	2552	2554	2557	rBV	249	183	0.01%	0.001%
60	9.317	2570	2574	2575	rBV2	137	124	0.01%	0.001%
61	9.349	2580	2584	2586	rBV	216	186	0.01%	0.001%
62	9.420	2603	2606	2607	rBV2	199	106	0.01%	0.001%
63	9.432	2607	2610	2613	rVV2	183	101	0.01%	0.001%
64	9.474	2619	2623	2626	rBV2	209	147	0.01%	0.001%
65	9.513	2629	2635	2638	rBV2	323	327	0.02%	0.003%
66	9.539	2641	2643	2648	rVB3	457	319	0.02%	0.003%
67	9.606	2661	2664	2666	rBV	185	92	0.01%	0.001%
68	9.641	2670	2675	2683	rVB3	296	420	0.03%	0.003%
69	9.728	2700	2702	2705	rBV2	138	71	0.00%	0.001%
70	9.850	2738	2740	2742	rVB	210	89	0.01%	0.001%
71	9.870	2742	2746	2748	rBV2	206	134	0.01%	0.001%
72	9.924	2757	2763	2770	rBV2	787	957	0.06%	0.008%
73	10.008	2787	2789	2792	rBV2	219	122	0.01%	0.001%
74	10.162	2826	2837	2841	rBV2	22771	33718	2.27%	0.267%
75	10.204	2842	2850	2874	rVB	462407	729591	49.21%	5.786%
76	10.378	2896	2904	2913	rVB4	4256	6486	0.44%	0.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029537.D
 Acq On : 09 Dec 2022 21:43
 Operator : SY/MD
 Sample : N5959-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.461	2928	2930	2933	rVB	185	83	0.01%	0.001%
78	10.487	2933	2938	2941	rBV2	478	318	0.02%	0.003%
79	10.506	2942	2944	2946	rVV	166	91	0.01%	0.001%
80	10.529	2946	2951	2952	rVV2	804	660	0.04%	0.005%
81	10.571	2956	2964	2980	rVV2	10916	18515	1.25%	0.147%
82	10.632	2981	2983	2992	rVB2	263	345	0.02%	0.003%
83	10.670	2992	2995	3001	rVB2	369	307	0.02%	0.002%
84	10.905	3060	3068	3076	rBV5	1242	1822	0.12%	0.014%
85	11.069	3115	3119	3120	rBV	207	157	0.01%	0.001%
86	11.149	3142	3144	3147	rVB	495	288	0.02%	0.002%
87	11.172	3147	3151	3153	rBV2	1034	857	0.06%	0.007%
88	11.236	3160	3171	3197	rBV	822324	1280188	86.35%	10.153%
89	11.439	3232	3234	3238	rVB2	352	238	0.02%	0.002%
90	11.458	3238	3240	3242	rBV2	251	137	0.01%	0.001%
91	11.519	3257	3259	3262	rBV	269	145	0.01%	0.001%
92	11.558	3264	3271	3276	rVV5	1788	2561	0.17%	0.020%
93	11.612	3276	3288	3309	rVV	709365	1137389	76.72%	9.021%
94	11.844	3357	3360	3362	rBV2	215	136	0.01%	0.001%
95	11.866	3363	3367	3370	rVV2	359	285	0.02%	0.002%
96	11.915	3379	3382	3383	rBV2	381	163	0.01%	0.001%
97	12.082	3431	3434	3436	rBV2	312	210	0.01%	0.002%
98	12.136	3448	3451	3453	rBV	292	220	0.01%	0.002%
99	12.452	3547	3549	3551	rBV3	391	160	0.01%	0.001%
100	12.622	3600	3602	3603	rBV3	493	202	0.01%	0.002%

Sum of corrected areas: 12608751




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029537.D
Acq On : 09 Dec 2022 21:43
Operator : SY/MD
Sample : N5959-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

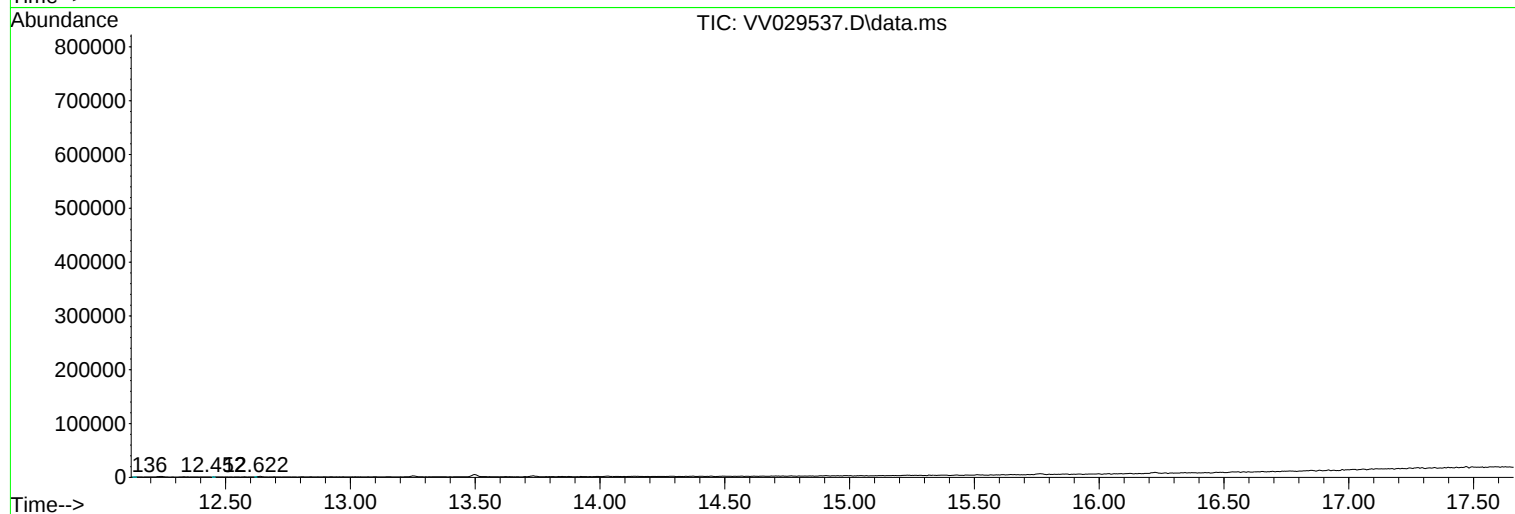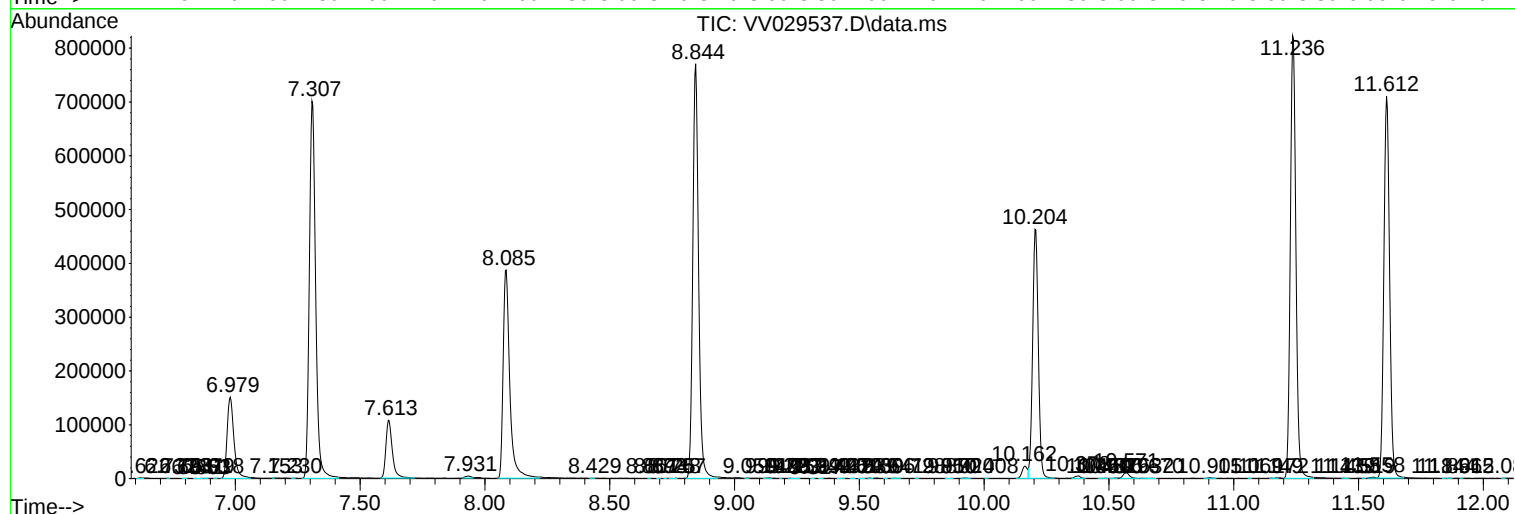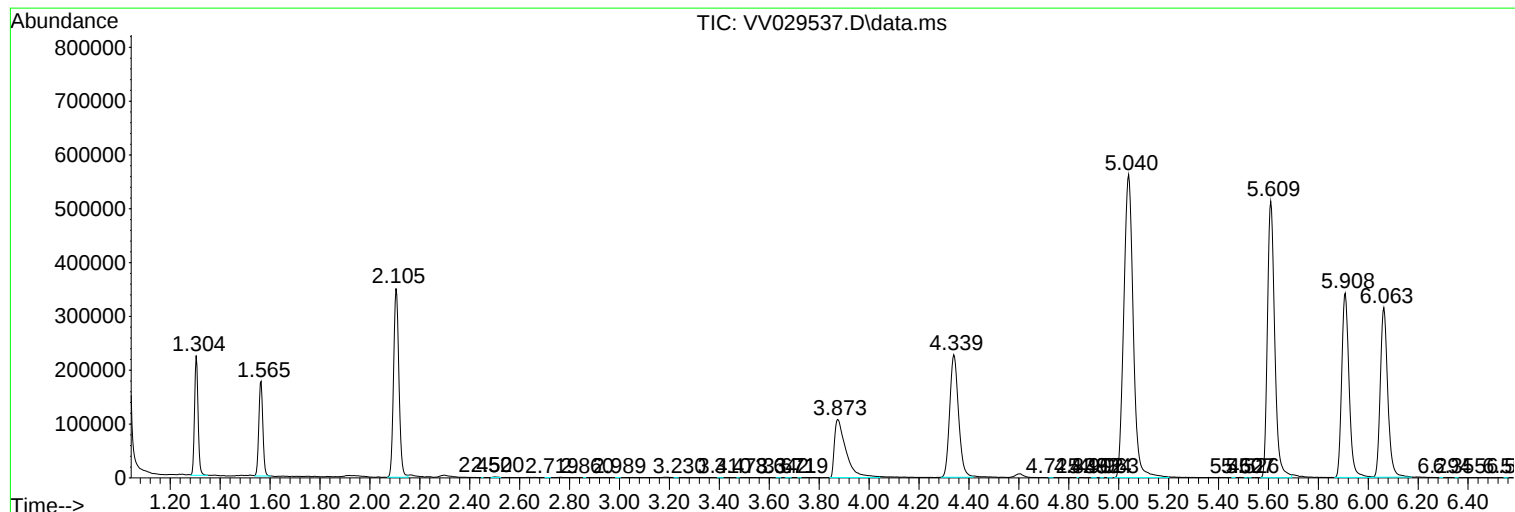

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029537.D
Acq On : 09 Dec 2022 21:43
Operator : SY/MD
Sample : N5959-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029537.D
Acq On : 09 Dec 2022 21:43
Operator : SY/MD
Sample : N5959-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc