

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029538.D
 Acq On : 09 Dec 2022 22:05
 Operator : SY/MD
 Sample : N5959-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rVB	215088	209562	13.99%	1.755%
2	1.565	155	163	182	rVB	175898	199212	13.29%	1.668%
3	2.105	320	331	362	rBV	343089	494584	33.01%	4.142%
4	2.507	449	456	464	rBV3	1276	1965	0.13%	0.016%
5	2.626	487	493	496	rBV4	1171	1504	0.10%	0.013%
6	2.738	525	528	530	rBV	340	225	0.02%	0.002%
7	2.761	533	535	537	rBV2	310	158	0.01%	0.001%
8	2.773	537	539	540	rBV2	243	90	0.01%	0.001%
9	2.854	559	564	565	rBV2	224	163	0.01%	0.001%
10	2.995	605	608	613	rBV	228	173	0.01%	0.001%
11	3.040	620	622	626	rBV	225	162	0.01%	0.001%
12	3.092	635	638	640	rBV	220	121	0.01%	0.001%
13	3.339	710	715	718	rBV2	143	141	0.01%	0.001%
14	3.362	718	722	728	rVV2	195	217	0.01%	0.002%
15	3.429	740	743	746	rBV2	111	91	0.01%	0.001%
16	3.577	786	789	796	rVB2	280	296	0.02%	0.002%
17	3.693	819	825	830	rBV2	247	324	0.02%	0.003%
18	3.773	847	850	854	rVB	144	113	0.01%	0.001%
19	3.796	854	857	858	rBV	238	110	0.01%	0.001%
20	3.809	858	861	869	rVB2	149	173	0.01%	0.001%
21	3.870	871	880	911	rBV	107405	289265	19.30%	2.422%
22	4.339	1010	1026	1060	rBV	232268	573772	38.29%	4.805%
23	4.619	1110	1113	1115	rBV3	263	227	0.02%	0.002%
24	4.761	1152	1157	1160	rBV2	154	129	0.01%	0.001%
25	4.796	1165	1168	1171	rBV2	190	148	0.01%	0.001%
26	4.828	1177	1178	1183	rVB	328	160	0.01%	0.001%
27	4.966	1219	1221	1224	rBV2	261	104	0.01%	0.001%
28	5.040	1226	1244	1296	rBV2	566428	1498414	100.00%	12.548%
29	5.471	1375	1378	1380	rBV2	391	270	0.02%	0.002%
30	5.564	1404	1407	1409	rBV2	200	146	0.01%	0.001%
31	5.609	1409	1421	1458	rBV	523030	1065776	71.13%	8.925%
32	5.908	1503	1514	1528	rVB10	4491	9909	0.66%	0.083%
33	6.063	1548	1562	1599	rBV	316893	660998	44.11%	5.535%
34	6.314	1638	1640	1643	rVB	352	147	0.01%	0.001%
35	6.349	1647	1651	1653	rVB2	287	180	0.01%	0.002%
36	6.397	1664	1666	1669	rBV2	198	89	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029538.D
 Acq On : 09 Dec 2022 22:05
 Operator : SY/MD
 Sample : N5959-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.526	1703	1706	1713	rVB3	351	317	0.02%	0.003%
38	6.568	1717	1719	1722	rBV	241	158	0.01%	0.001%
39	6.587	1722	1725	1728	rBV2	298	202	0.01%	0.002%
40	6.629	1731	1738	1743	rBV2	1122	1689	0.11%	0.014%
41	6.690	1755	1757	1762	rVB3	294	193	0.01%	0.002%
42	6.719	1762	1766	1770	rBV3	293	265	0.02%	0.002%
43	6.741	1770	1773	1776	rVB2	240	156	0.01%	0.001%
44	6.770	1780	1782	1787	rVB3	199	152	0.01%	0.001%
45	6.799	1787	1791	1792	rBV3	176	90	0.01%	0.001%
46	6.838	1801	1803	1807	rBV2	183	110	0.01%	0.001%
47	6.979	1836	1847	1878	rBV	153687	282972	18.88%	2.370%
48	7.162	1900	1904	1906	rBV2	994	669	0.04%	0.006%
49	7.230	1923	1925	1927	rBV	256	102	0.01%	0.001%
50	7.310	1936	1950	1983	rBV	704098	1240733	82.80%	10.390%
51	7.616	2034	2045	2070	rBV	107124	191027	12.75%	1.600%
52	7.937	2135	2145	2152	rBV3	4727	8049	0.54%	0.067%
53	8.082	2180	2190	2231	rBV	393774	714152	47.66%	5.981%
54	8.535	2329	2331	2333	rBV2	274	130	0.01%	0.001%
55	8.616	2352	2356	2361	rVB3	360	296	0.02%	0.002%
56	8.696	2379	2381	2384	rBV	277	203	0.01%	0.002%
57	8.715	2385	2387	2392	rVB4	367	256	0.02%	0.002%
58	8.776	2401	2406	2408	rBV2	230	224	0.01%	0.002%
59	8.844	2414	2427	2459	rBV	780598	1269911	84.75%	10.635%
60	9.085	2500	2502	2504	rBV	265	131	0.01%	0.001%
61	9.207	2537	2540	2545	rVB2	334	298	0.02%	0.002%
62	9.288	2563	2565	2568	rBV2	192	127	0.01%	0.001%
63	9.323	2573	2576	2577	rBV	176	99	0.01%	0.001%
64	9.410	2601	2603	2605	rBV	191	102	0.01%	0.001%
65	9.448	2611	2615	2617	rBV2	154	116	0.01%	0.001%
66	9.468	2617	2621	2623	rVB3	457	354	0.02%	0.003%
67	9.487	2623	2627	2628	rBV	242	161	0.01%	0.001%
68	9.538	2638	2643	2647	rBV3	769	795	0.05%	0.007%
69	9.596	2659	2661	2664	rBV2	217	109	0.01%	0.001%
70	9.657	2677	2680	2682	rBV2	200	148	0.01%	0.001%
71	9.731	2701	2703	2704	rBV2	223	103	0.01%	0.001%
72	9.931	2763	2765	2768	rVB2	462	180	0.01%	0.002%
73	10.098	2815	2817	2819	rBV2	255	182	0.01%	0.002%
74	10.162	2825	2837	2841	rBV2	24601	35106	2.34%	0.294%
75	10.207	2842	2851	2872	rVB	471082	744272	49.67%	6.233%
76	10.378	2896	2904	2913	rVB3	5184	8678	0.58%	0.073%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029538.D
 Acq On : 09 Dec 2022 22:05
 Operator : SY/MD
 Sample : N5959-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.458	2927	2929	2931	rBV	350	179	0.01%	0.001%
78	10.490	2935	2939	2945	rBV2	449	567	0.04%	0.005%
79	10.522	2945	2949	2950	rBV2	523	392	0.03%	0.003%
80	10.567	2955	2963	2978	rVB	12148	19428	1.30%	0.163%
81	10.657	2988	2991	2995	rBV2	273	219	0.01%	0.002%
82	10.818	3038	3041	3043	rBV	230	169	0.01%	0.001%
83	10.841	3046	3048	3052	rVV	392	273	0.02%	0.002%
84	10.908	3063	3069	3073	rBV4	1119	1225	0.08%	0.010%
85	10.985	3090	3093	3094	rBV	301	158	0.01%	0.001%
86	11.046	3107	3112	3115	rVB3	321	311	0.02%	0.003%
87	11.079	3118	3122	3125	rBV3	239	191	0.01%	0.002%
88	11.143	3139	3142	3145	rVB	266	205	0.01%	0.002%
89	11.172	3145	3151	3160	rBV6	891	1393	0.09%	0.012%
90	11.239	3160	3172	3196	rBV	824699	1279113	85.36%	10.712%
91	11.503	3251	3254	3258	rBV	396	272	0.02%	0.002%
92	11.561	3264	3272	3276	rBV4	1895	3047	0.20%	0.026%
93	11.612	3277	3288	3311	rVV	703049	1119082	74.68%	9.372%
94	11.857	3361	3364	3368	rBV2	466	407	0.03%	0.003%
95	12.040	3418	3421	3422	rBV2	256	100	0.01%	0.001%
96	12.140	3449	3452	3455	rBV2	286	210	0.01%	0.002%
97	12.709	3627	3629	3631	rBV	320	154	0.01%	0.001%
98	13.185	3775	3777	3780	rBV2	317	121	0.01%	0.001%
99	13.252	3791	3798	3804	rVB8	1090	1621	0.11%	0.014%
100	13.410	3843	3847	3848	rBV2	470	352	0.02%	0.003%




Sum of corrected areas: 11941324

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029538.D
Acq On : 09 Dec 2022 22:05
Operator : SY/MD
Sample : N5959-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

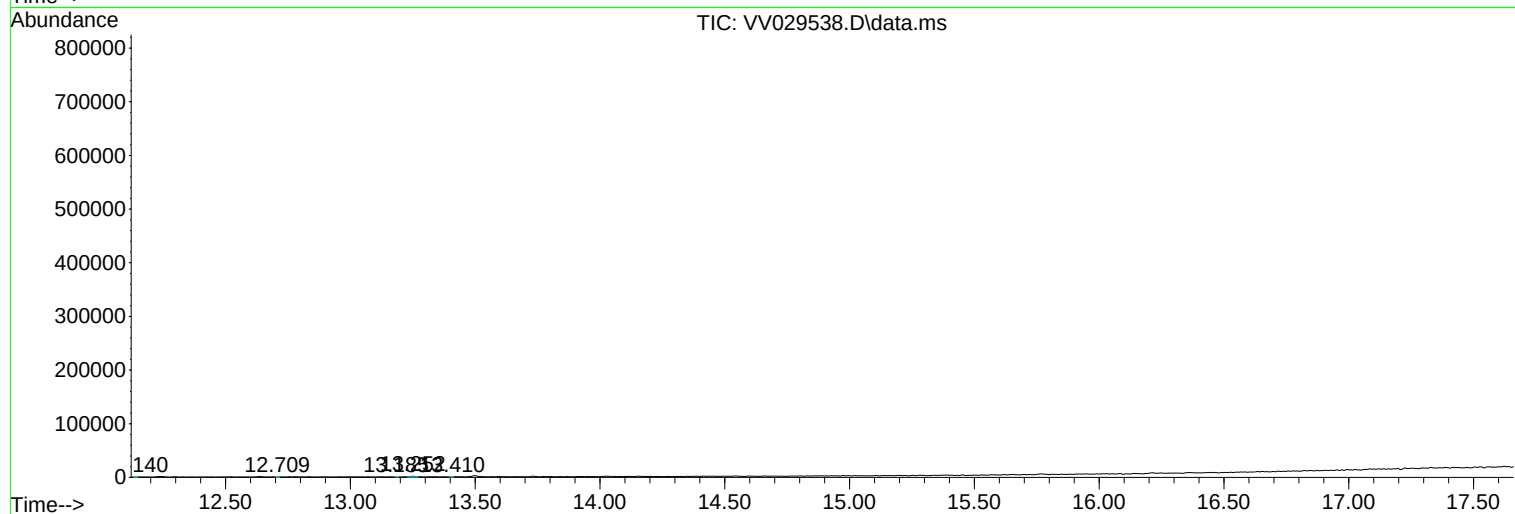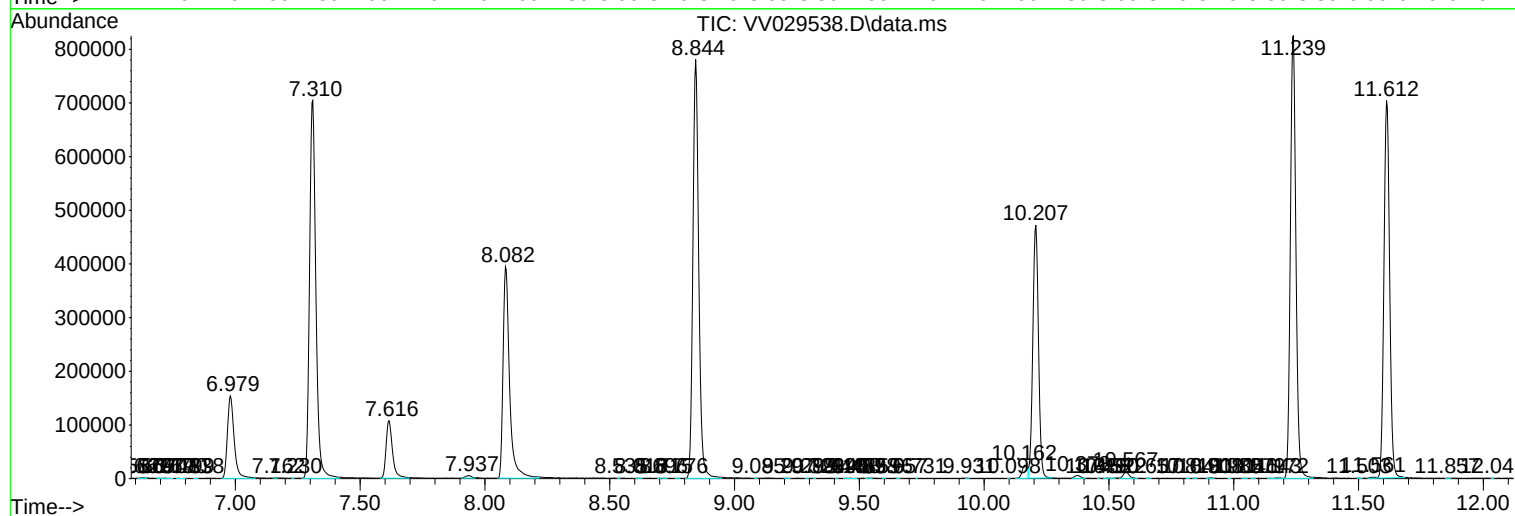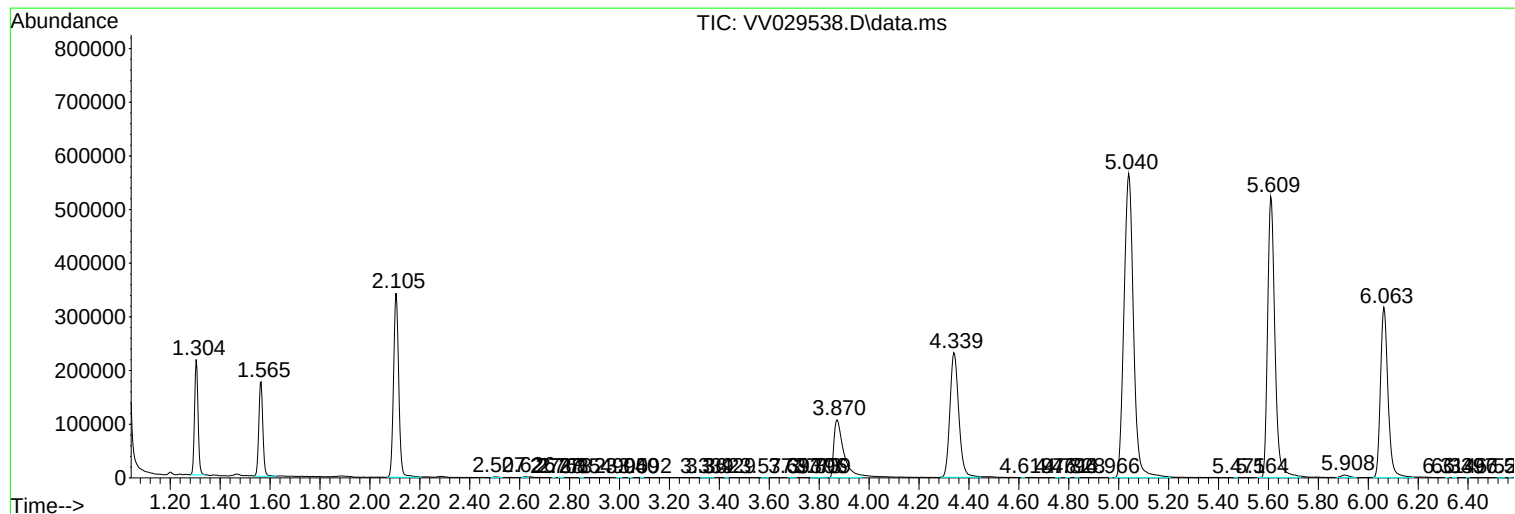

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029538.D
Acq On : 09 Dec 2022 22:05
Operator : SY/MD
Sample : N5959-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029538.D
Acq On : 09 Dec 2022 22:05
Operator : SY/MD
Sample : N5959-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc