

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029539.D
 Acq On : 09 Dec 2022 22:28
 Operator : SY/MD
 Sample : N5959-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	212117	212679	14.57%	1.806%
2	1.564	155	163	180	rVB	174940	193002	13.23%	1.639%
3	2.105	320	331	345	rBV	333611	487978	33.44%	4.145%
4	2.500	448	454	462	rVB5	1320	1817	0.12%	0.015%
5	2.809	546	550	552	rBV	236	163	0.01%	0.001%
6	2.886	571	574	577	rBV2	217	168	0.01%	0.001%
7	3.072	629	632	634	rBV	186	113	0.01%	0.001%
8	3.172	659	663	667	rBV	211	185	0.01%	0.002%
9	3.191	667	669	672	rVV2	202	117	0.01%	0.001%
10	3.397	729	733	735	rBV2	142	96	0.01%	0.001%
11	3.548	776	780	783	rBV2	147	134	0.01%	0.001%
12	3.590	789	793	795	rBV2	123	88	0.01%	0.001%
13	3.629	802	805	808	rBV2	150	105	0.01%	0.001%
14	3.686	816	823	828	rBV2	207	286	0.02%	0.002%
15	3.751	840	843	845	rBV2	208	97	0.01%	0.001%
16	3.799	855	858	861	rVB	142	79	0.01%	0.001%
17	3.815	861	863	865	rBV	132	78	0.01%	0.001%
18	3.873	871	881	925	rBV2	105799	293153	20.09%	2.490%
19	4.342	1011	1027	1053	rBV	221388	554553	38.00%	4.710%
20	4.657	1122	1125	1129	rBV2	302	162	0.01%	0.001%
21	4.744	1149	1152	1155	rVV2	166	109	0.01%	0.001%
22	4.780	1158	1163	1166	rBV2	205	205	0.01%	0.002%
23	4.818	1171	1175	1178	rVB3	159	136	0.01%	0.001%
24	4.924	1205	1208	1213	rBV2	200	182	0.01%	0.002%
25	5.043	1226	1245	1291	rBV2	553701	1459249	100.00%	12.394%
26	5.310	1325	1328	1330	rBV2	225	137	0.01%	0.001%
27	5.612	1408	1422	1463	rBV	494965	1025578	70.28%	8.711%
28	5.911	1503	1515	1543	rBV2	74682	156537	10.73%	1.330%
29	6.063	1549	1562	1598	rBV	309486	635991	43.58%	5.402%
30	6.400	1663	1667	1669	rBV2	197	149	0.01%	0.001%
31	6.452	1681	1683	1685	rVB	205	87	0.01%	0.001%
32	6.481	1690	1692	1696	rVB2	223	115	0.01%	0.001%
33	6.529	1703	1707	1710	rBV2	206	127	0.01%	0.001%
34	6.735	1768	1771	1774	rBV	305	169	0.01%	0.001%
35	6.757	1774	1778	1781	rVV2	468	313	0.02%	0.003%
36	6.770	1781	1782	1784	rVV	208	92	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029539.D
 Acq On : 09 Dec 2022 22:28
 Operator : SY/MD
 Sample : N5959-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.796	1788	1790	1794	rBV2	213	129	0.01%	0.001%
38	6.834	1798	1802	1804	rBV	234	150	0.01%	0.001%
39	6.866	1810	1812	1815	rVB3	313	165	0.01%	0.001%
40	6.905	1819	1824	1827	rBV2	248	207	0.01%	0.002%
41	6.979	1836	1847	1874	rBV	147854	273829	18.77%	2.326%
42	7.310	1937	1950	1971	rBV	684663	1204904	82.57%	10.234%
43	7.616	2035	2045	2071	rBV	103777	183477	12.57%	1.558%
44	7.873	2122	2125	2127	rBV	388	331	0.02%	0.003%
45	8.085	2180	2191	2223	rBV	374864	682131	46.75%	5.794%
46	8.397	2286	2288	2295	rBV3	479	339	0.02%	0.003%
47	8.564	2335	2340	2342	rBV2	360	320	0.02%	0.003%
48	8.670	2368	2373	2376	rBV3	296	287	0.02%	0.002%
49	8.686	2376	2378	2381	rVB	440	224	0.02%	0.002%
50	8.702	2381	2383	2385	rBV2	292	186	0.01%	0.002%
51	8.734	2392	2393	2396	rBV	252	127	0.01%	0.001%
52	8.754	2396	2399	2403	rBV2	490	375	0.03%	0.003%
53	8.844	2415	2427	2458	rBV	738857	1214580	83.23%	10.316%
54	9.001	2473	2476	2477	rBV2	697	408	0.03%	0.003%
55	9.104	2507	2508	2510	rBV	215	109	0.01%	0.001%
56	9.130	2513	2516	2517	rBV2	445	228	0.02%	0.002%
57	9.169	2526	2528	2534	rBV2	182	182	0.01%	0.002%
58	9.226	2543	2546	2549	rBV	323	170	0.01%	0.001%
59	9.316	2572	2574	2575	rBV	198	87	0.01%	0.001%
60	9.378	2589	2593	2596	rBV2	365	318	0.02%	0.003%
61	9.419	2604	2606	2608	rBV2	202	95	0.01%	0.001%
62	9.461	2617	2619	2625	rVB2	279	227	0.02%	0.002%
63	9.538	2639	2643	2647	rBV3	731	765	0.05%	0.006%
64	9.567	2650	2652	2656	rVB3	516	314	0.02%	0.003%
65	9.670	2680	2684	2686	rBV2	245	132	0.01%	0.001%
66	9.705	2692	2695	2696	rBV	181	121	0.01%	0.001%
67	9.715	2696	2698	2702	rVV2	298	239	0.02%	0.002%
68	9.734	2702	2704	2707	rVV2	159	100	0.01%	0.001%
69	9.770	2712	2715	2718	rBV	286	187	0.01%	0.002%
70	9.799	2721	2724	2726	rBV2	355	233	0.02%	0.002%
71	9.879	2745	2749	2752	rVB3	288	200	0.01%	0.002%
72	9.902	2754	2756	2758	rVB2	206	92	0.01%	0.001%
73	9.924	2758	2763	2767	rBV3	533	502	0.03%	0.004%
74	9.979	2777	2780	2782	rBV	213	129	0.01%	0.001%
75	10.085	2811	2813	2815	rBV	171	80	0.01%	0.001%
76	10.162	2828	2837	2841	rBV	23491	33627	2.30%	0.286%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029539.D
 Acq On : 09 Dec 2022 22:28
 Operator : SY/MD
 Sample : N5959-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.207	2842	2851	2877	rVB	456238	722194	49.49%	6.134%
78	10.419	2914	2917	2919	rBV2	259	178	0.01%	0.002%
79	10.532	2944	2952	2956	rBV5	666	1071	0.07%	0.009%
80	10.567	2956	2963	2977	rVB	12245	18795	1.29%	0.160%
81	10.648	2985	2988	2993	rVB2	293	260	0.02%	0.002%
82	10.677	2995	2997	3001	rVB	273	151	0.01%	0.001%
83	10.699	3001	3004	3006	rVB	301	185	0.01%	0.002%
84	10.715	3006	3009	3015	rBV4	249	313	0.02%	0.003%
85	10.776	3025	3028	3029	rBV	119	87	0.01%	0.001%
86	10.828	3041	3044	3046	rBV2	234	131	0.01%	0.001%
87	10.844	3046	3049	3052	rBV3	478	343	0.02%	0.003%
88	10.956	3081	3084	3086	rBV	172	111	0.01%	0.001%
89	11.014	3098	3102	3106	rBV2	229	216	0.01%	0.002%
90	11.101	3126	3129	3132	rBV2	232	229	0.02%	0.002%
91	11.140	3138	3141	3144	rBV3	511	376	0.03%	0.003%
92	11.239	3159	3172	3198	rBV	807474	1262767	86.54%	10.725%
93	11.500	3248	3253	3255	rBV2	354	314	0.02%	0.003%
94	11.561	3263	3272	3276	rBV5	1866	3101	0.21%	0.026%
95	11.612	3276	3288	3311	rVV	715946	1135537	77.82%	9.645%
96	11.840	3354	3359	3361	rBV3	418	332	0.02%	0.003%
97	12.143	3449	3453	3456	rBV3	453	398	0.03%	0.003%
98	12.467	3551	3554	3556	rBV2	235	181	0.01%	0.002%
99	12.628	3601	3604	3605	rBV2	579	351	0.02%	0.003%
100	13.252	3793	3798	3804	rBV6	1050	1374	0.09%	0.012%




Sum of corrected areas: 11773530

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029539.D
Acq On : 09 Dec 2022 22:28
Operator : SY/MD
Sample : N5959-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

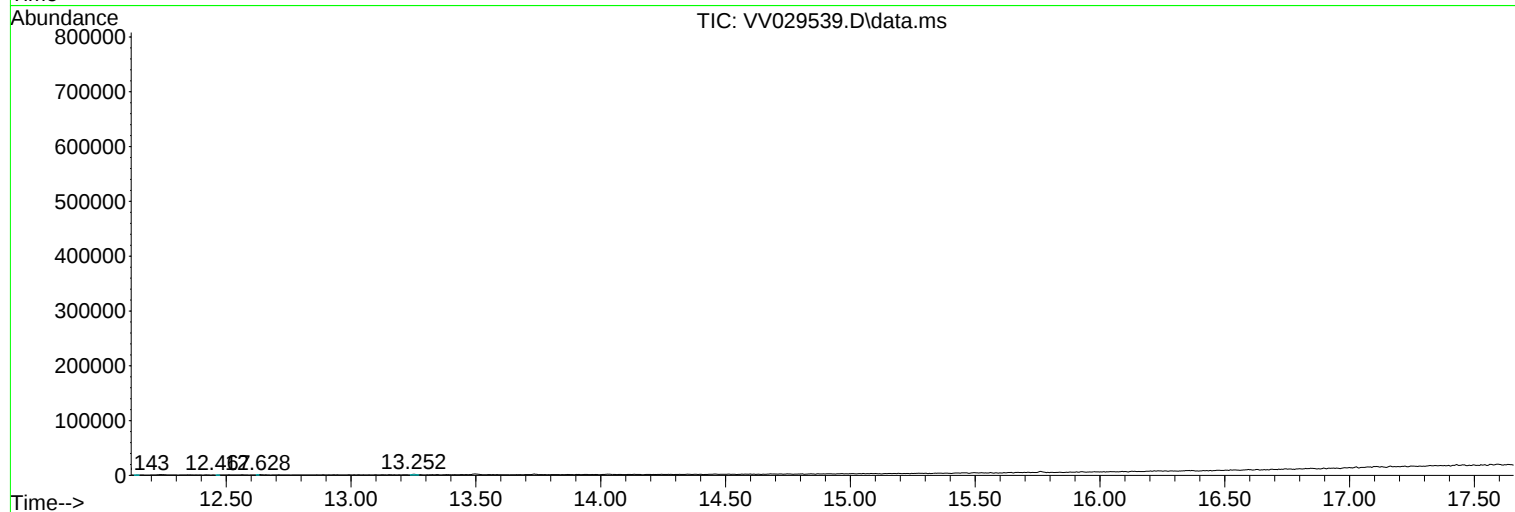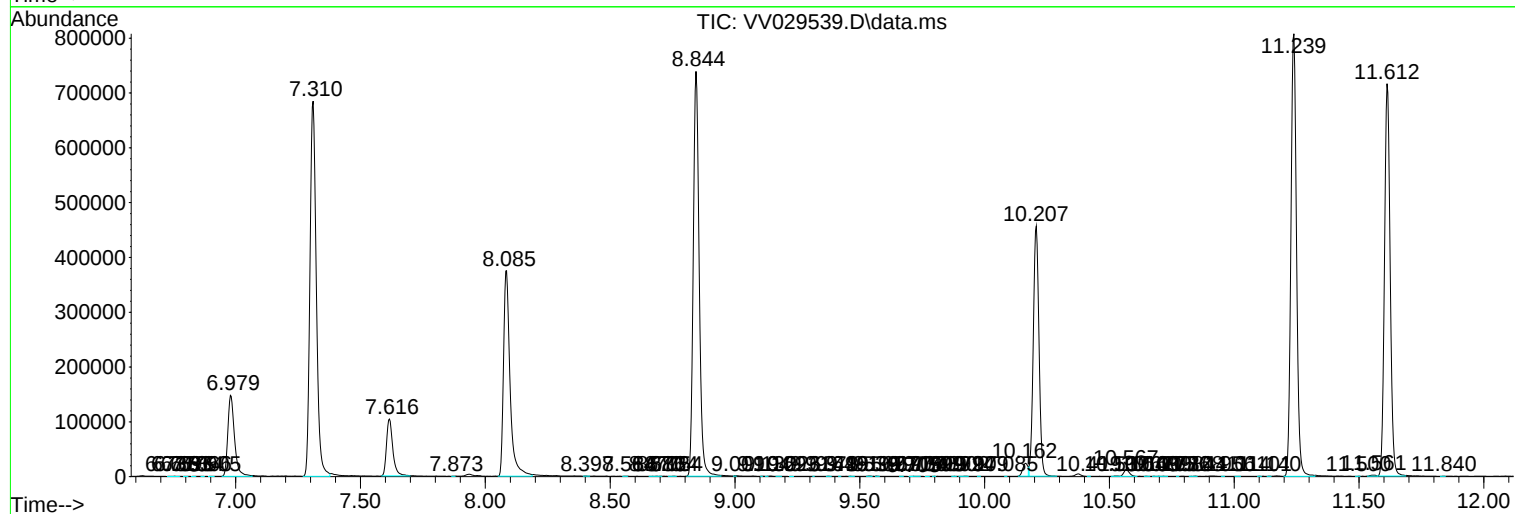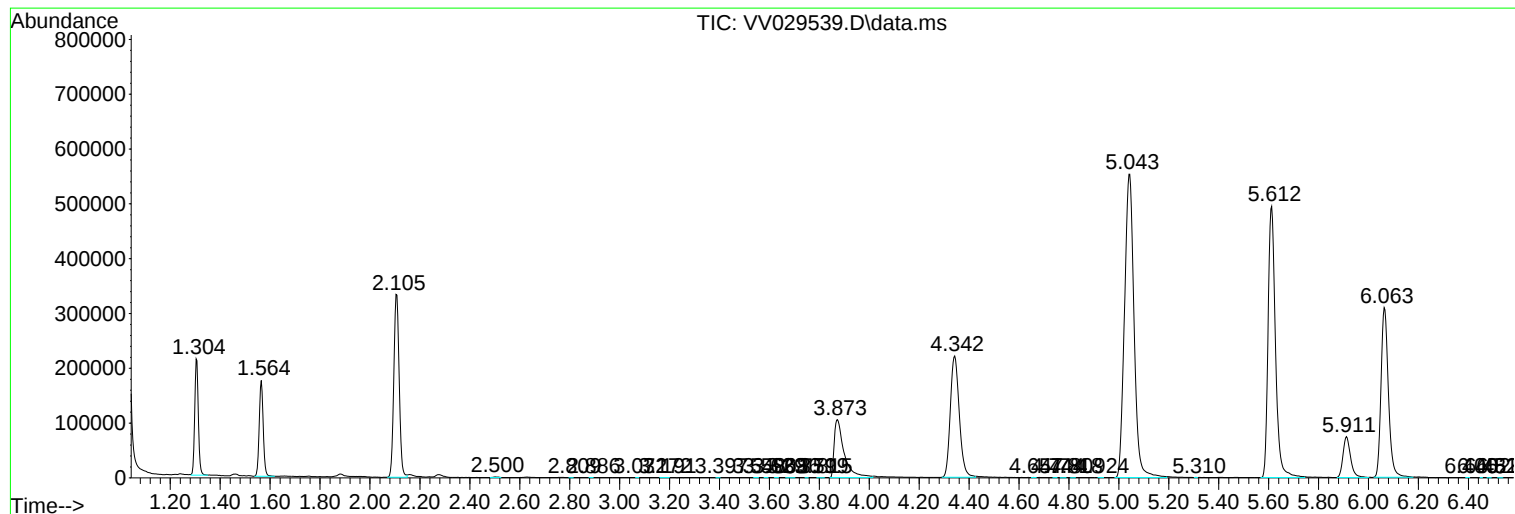

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029539.D
Acq On : 09 Dec 2022 22:28
Operator : SY/MD
Sample : N5959-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029539.D
Acq On : 09 Dec 2022 22:28
Operator : SY/MD
Sample : N5959-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------