

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029540.D
 Acq On : 09 Dec 2022 22:49
 Operator : SY/MD
 Sample : N5959-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	216966	215739	14.15%	1.794%
2	1.564	156	163	178	rVB	182477	202019	13.25%	1.680%
3	2.108	320	332	346	rBV	340712	495881	32.53%	4.123%
4	2.413	424	427	432	rBV3	418	388	0.03%	0.003%
5	2.452	437	439	443	rBV	309	180	0.01%	0.001%
6	2.471	443	445	448	rBV	227	123	0.01%	0.001%
7	2.503	449	455	462	rVB6	1166	1878	0.12%	0.016%
8	2.542	462	467	472	rBV2	442	301	0.02%	0.003%
9	2.571	472	476	478	rBV	177	154	0.01%	0.001%
10	2.584	478	480	482	rBV	234	119	0.01%	0.001%
11	2.651	498	501	504	rVB3	440	303	0.02%	0.003%
12	2.696	512	515	516	rBV	262	155	0.01%	0.001%
13	2.773	536	539	543	rVB2	523	323	0.02%	0.003%
14	2.834	555	558	561	rVV2	325	227	0.01%	0.002%
15	2.921	582	585	590	rBV2	167	153	0.01%	0.001%
16	2.969	598	600	603	rBV2	336	179	0.01%	0.001%
17	3.175	661	664	669	rVV2	157	152	0.01%	0.001%
18	3.272	689	694	696	rBV	167	141	0.01%	0.001%
19	3.635	803	807	810	rBV	171	159	0.01%	0.001%
20	3.686	820	823	826	rBV2	300	138	0.01%	0.001%
21	3.732	832	837	841	rBV2	107	132	0.01%	0.001%
22	3.802	856	859	866	rBV2	213	257	0.02%	0.002%
23	3.876	872	882	921	rBV	103375	294073	19.29%	2.445%
24	4.342	1011	1027	1062	rBV	233701	580772	38.10%	4.829%
25	4.632	1114	1117	1120	rBV3	231	166	0.01%	0.001%
26	4.696	1134	1137	1140	rBV	294	187	0.01%	0.002%
27	5.043	1226	1245	1289	rBV2	578460	1524403	100.00%	12.676%
28	5.522	1392	1394	1403	rVB2	295	349	0.02%	0.003%
29	5.561	1403	1406	1408	rBV3	226	152	0.01%	0.001%
30	5.612	1409	1422	1458	rBV	509795	1036465	67.99%	8.618%
31	5.911	1504	1515	1528	rBV9	4154	9451	0.62%	0.079%
32	6.066	1545	1563	1598	rBV	325931	675766	44.33%	5.619%
33	6.252	1618	1621	1623	rBV3	257	161	0.01%	0.001%
34	6.272	1623	1627	1631	rVV3	340	327	0.02%	0.003%
35	6.291	1631	1633	1636	rVB	289	151	0.01%	0.001%
36	6.304	1636	1637	1640	rVB	289	133	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029540.D
 Acq On : 09 Dec 2022 22:49
 Operator : SY/MD
 Sample : N5959-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.323	1640	1643	1645	rBV2	233	153	0.01%	0.001%
38	6.378	1657	1660	1665	rBV2	155	189	0.01%	0.002%
39	6.413	1669	1671	1674	rVB2	378	138	0.01%	0.001%
40	6.432	1674	1677	1680	rBV3	251	184	0.01%	0.002%
41	6.493	1693	1696	1697	rBV2	241	125	0.01%	0.001%
42	6.506	1697	1700	1703	rVB3	168	116	0.01%	0.001%
43	6.535	1707	1709	1711	rBV2	232	128	0.01%	0.001%
44	6.632	1731	1739	1742	rBV3	1056	1756	0.12%	0.015%
45	6.693	1756	1758	1762	rVB3	263	117	0.01%	0.001%
46	6.792	1785	1789	1792	rBV2	173	153	0.01%	0.001%
47	6.825	1794	1799	1802	rVB3	466	258	0.02%	0.002%
48	6.857	1802	1809	1813	rBV2	235	372	0.02%	0.003%
49	6.982	1836	1848	1877	rBV	155746	285313	18.72%	2.372%
50	7.310	1938	1950	1976	rBV	719908	1265971	83.05%	10.527%
51	7.616	2035	2045	2078	rBV	110041	196420	12.89%	1.633%
52	7.821	2107	2109	2114	rVB2	529	479	0.03%	0.004%
53	7.847	2114	2117	2118	rBV2	418	229	0.02%	0.002%
54	8.085	2181	2191	2228	rBV	391623	712814	46.76%	5.927%
55	8.548	2332	2335	2337	rBV	366	214	0.01%	0.002%
56	8.583	2342	2346	2348	rBV2	458	339	0.02%	0.003%
57	8.644	2361	2365	2370	rVB4	409	366	0.02%	0.003%
58	8.673	2370	2374	2376	rBV2	620	441	0.03%	0.004%
59	8.706	2381	2384	2387	rVV2	410	264	0.02%	0.002%
60	8.799	2409	2413	2415	rBV	276	196	0.01%	0.002%
61	8.844	2415	2427	2456	rBV	741402	1226596	80.46%	10.199%
62	9.127	2513	2515	2517	rBV2	431	304	0.02%	0.003%
63	9.201	2535	2538	2541	rVB2	302	227	0.01%	0.002%
64	9.278	2559	2562	2564	rVB	232	124	0.01%	0.001%
65	9.291	2564	2566	2569	rBV	268	147	0.01%	0.001%
66	9.313	2572	2573	2577	rVV	203	111	0.01%	0.001%
67	9.368	2588	2590	2592	rBV	288	148	0.01%	0.001%
68	9.509	2628	2634	2638	rVB2	308	285	0.02%	0.002%
69	9.542	2638	2644	2647	rBV3	525	642	0.04%	0.005%
70	9.616	2661	2667	2670	rBV2	295	289	0.02%	0.002%
71	9.673	2683	2685	2690	rVB	345	195	0.01%	0.002%
72	9.808	2722	2727	2729	rBV3	275	227	0.01%	0.002%
73	9.850	2737	2740	2741	rBV	194	138	0.01%	0.001%
74	9.924	2758	2763	2772	rVB3	663	782	0.05%	0.007%
75	9.960	2772	2774	2777	rBV	263	139	0.01%	0.001%
76	9.982	2777	2781	2783	rBV	301	244	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029540.D
 Acq On : 09 Dec 2022 22:49
 Operator : SY/MD
 Sample : N5959-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.043	2796	2800	2804	rBV2	356	350	0.02%	0.003%
78	10.165	2828	2838	2841	rBV	23381	32471	2.13%	0.270%
79	10.207	2842	2851	2871	rVB	481179	751831	49.32%	6.252%
80	10.374	2893	2903	2916	rBV4	4567	8038	0.53%	0.067%
81	10.468	2928	2932	2934	rBV	400	312	0.02%	0.003%
82	10.516	2940	2947	2948	rBV	379	332	0.02%	0.003%
83	10.567	2956	2963	2979	rVB2	11350	17992	1.18%	0.150%
84	10.699	3001	3004	3007	rBV3	234	151	0.01%	0.001%
85	10.767	3021	3025	3027	rBV2	317	244	0.02%	0.002%
86	10.844	3047	3049	3054	rBV2	290	189	0.01%	0.002%
87	10.908	3064	3069	3073	rBV3	880	855	0.06%	0.007%
88	10.966	3085	3087	3088	rBV3	307	119	0.01%	0.001%
89	11.123	3133	3136	3140	rBV	283	221	0.01%	0.002%
90	11.181	3147	3154	3159	rBV4	679	987	0.06%	0.008%
91	11.239	3159	3172	3195	rBV	826345	1282583	84.14%	10.665%
92	11.500	3251	3253	3256	rVB3	372	174	0.01%	0.001%
93	11.516	3256	3258	3260	rBV	322	125	0.01%	0.001%
94	11.551	3264	3269	3276	rBV7	1580	2300	0.15%	0.019%
95	11.612	3277	3288	3309	rBV	752334	1183567	77.64%	9.841%
96	12.403	3532	3534	3535	rBV	332	136	0.01%	0.001%
97	13.130	3758	3760	3762	rBV	507	281	0.02%	0.002%
98	13.246	3793	3796	3801	rBV4	1137	1113	0.07%	0.009%
99	13.500	3867	3875	3883	rBV3	1257	2354	0.15%	0.020%
100	13.728	3943	3946	3947	rBV2	1009	588	0.04%	0.005%




Sum of corrected areas: 12026303

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029540.D
Acq On : 09 Dec 2022 22:49
Operator : SY/MD
Sample : N5959-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

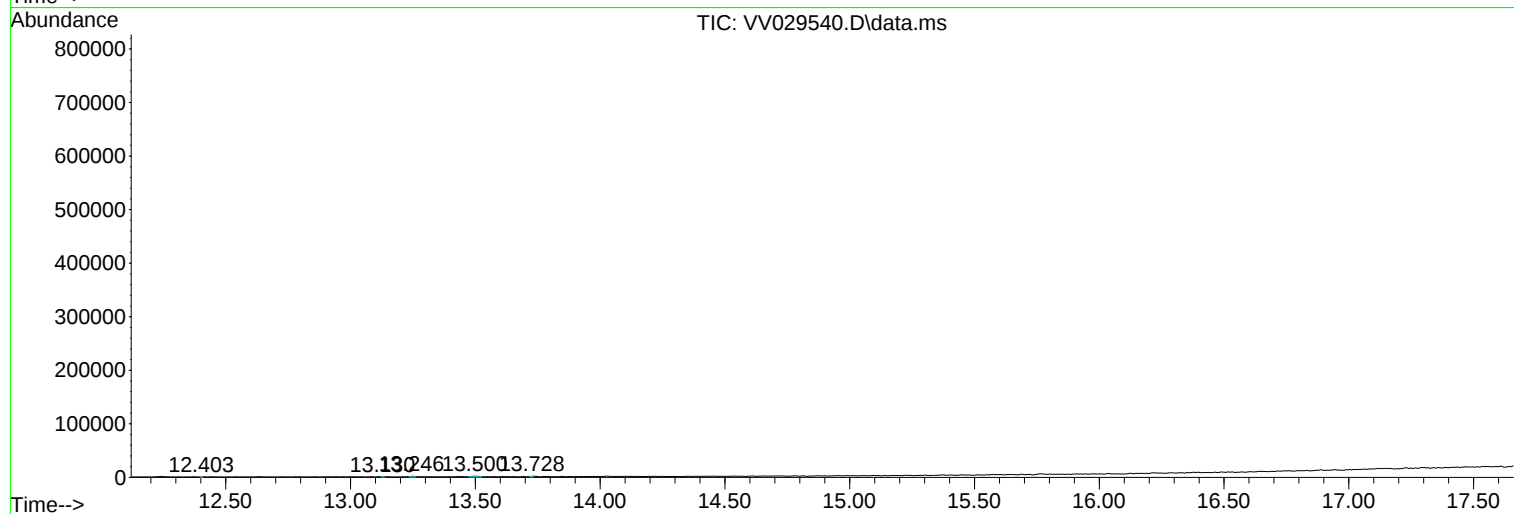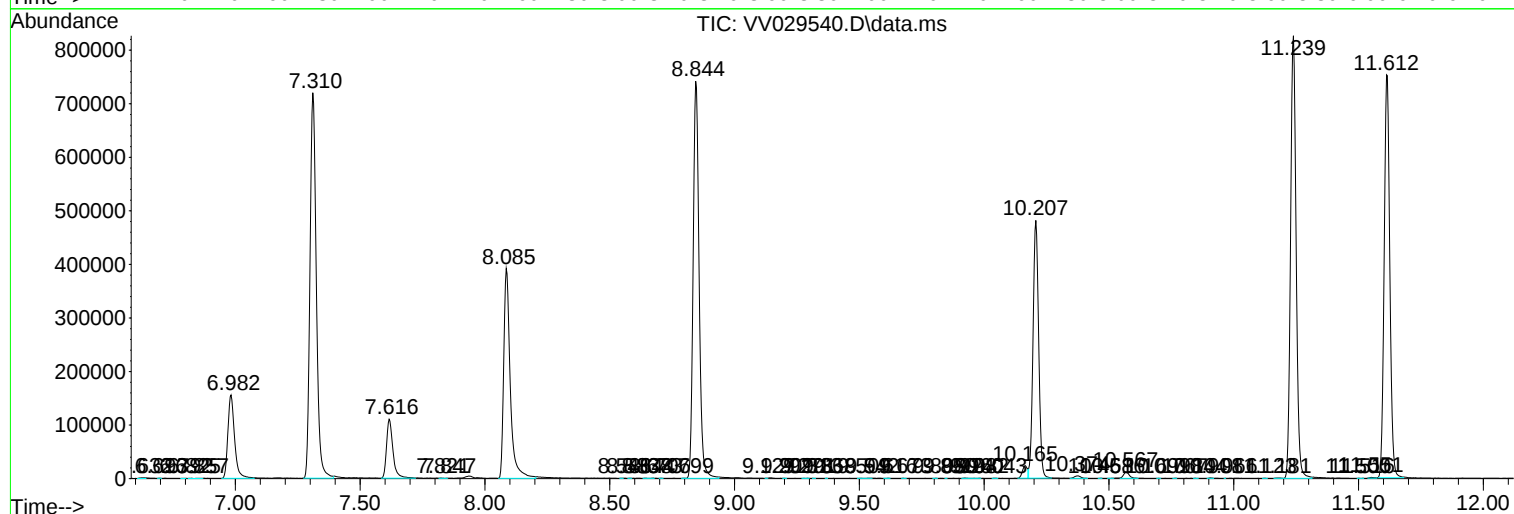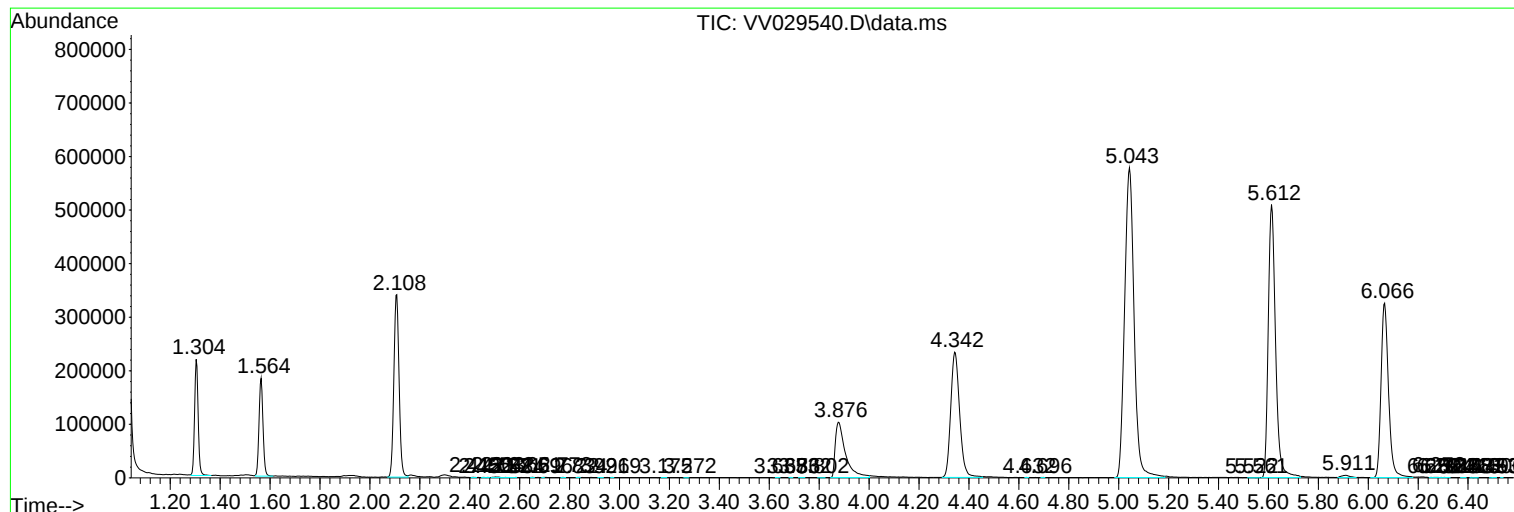

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029540.D
Acq On : 09 Dec 2022 22:49
Operator : SY/MD
Sample : N5959-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029540.D
Acq On : 09 Dec 2022 22:49
Operator : SY/MD
Sample : N5959-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------