

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029542.D
 Acq On : 09 Dec 2022 23:35
 Operator : SY/MD
 Sample : N5959-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	222555	218307	14.98%	1.870%
2	1.565	155	163	178	rVB	178854	199169	13.67%	1.706%
3	2.105	320	331	345	rBV	336749	483773	33.20%	4.143%
4	2.439	428	435	440	rBV3	657	837	0.06%	0.007%
5	2.503	449	455	461	rBV2	1023	1242	0.09%	0.011%
6	2.565	472	474	475	rBV	245	106	0.01%	0.001%
7	2.645	488	499	501	rBV5	1532	2133	0.15%	0.018%
8	2.754	531	533	538	rBV3	440	325	0.02%	0.003%
9	2.825	553	555	557	rBV	185	90	0.01%	0.001%
10	2.954	591	595	600	rVB2	429	427	0.03%	0.004%
11	3.227	677	680	683	rBV	253	165	0.01%	0.001%
12	3.420	737	740	742	rBV	203	120	0.01%	0.001%
13	3.487	759	761	766	rVB	170	136	0.01%	0.001%
14	3.532	772	775	779	rBV2	139	133	0.01%	0.001%
15	3.764	845	847	849	rBV	261	128	0.01%	0.001%
16	3.873	868	881	923	rBV	102611	297696	20.43%	2.549%
17	4.339	1009	1026	1064	rBV	222727	564902	38.77%	4.838%
18	4.600	1103	1107	1108	rBV	311	226	0.02%	0.002%
19	4.638	1115	1119	1122	rVB3	406	320	0.02%	0.003%
20	4.658	1122	1125	1128	rBV	352	190	0.01%	0.002%
21	4.680	1128	1132	1134	rBV2	240	214	0.01%	0.002%
22	4.799	1165	1169	1172	rBV2	271	254	0.02%	0.002%
23	5.040	1226	1244	1280	rBV2	554234	1456966	100.00%	12.477%
24	5.391	1350	1353	1355	rBV3	219	134	0.01%	0.001%
25	5.439	1365	1368	1373	rBV2	235	200	0.01%	0.002%
26	5.471	1373	1378	1385	rBV2	477	615	0.04%	0.005%
27	5.523	1390	1394	1398	rBV3	227	188	0.01%	0.002%
28	5.542	1398	1400	1401	rBV3	281	115	0.01%	0.001%
29	5.561	1404	1406	1408	rBV	180	103	0.01%	0.001%
30	5.609	1408	1421	1468	rBV	491568	1007038	69.12%	8.624%
31	5.905	1503	1513	1526	rVB7	4389	9902	0.68%	0.085%
32	5.973	1529	1534	1536	rBV2	334	242	0.02%	0.002%
33	6.063	1546	1562	1597	rBV	312382	649358	44.57%	5.561%
34	6.256	1620	1622	1623	rBV	280	119	0.01%	0.001%
35	6.297	1627	1635	1655	rBV6	5327	14104	0.97%	0.121%
36	6.455	1680	1684	1689	rBV	398	262	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029542.D
 Acq On : 09 Dec 2022 23:35
 Operator : SY/MD
 Sample : N5959-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.510	1697	1701	1702	rBV2	404	219	0.02%	0.002%
38	6.532	1703	1708	1718	rVB4	1158	1987	0.14%	0.017%
39	6.622	1733	1736	1742	rVV4	899	1033	0.07%	0.009%
40	6.806	1787	1793	1796	rBV3	414	339	0.02%	0.003%
41	6.841	1797	1804	1805	rBV	167	157	0.01%	0.001%
42	6.867	1809	1812	1815	rVB2	226	122	0.01%	0.001%
43	6.883	1815	1817	1818	rBV2	246	101	0.01%	0.001%
44	6.924	1826	1830	1835	rVB3	259	236	0.02%	0.002%
45	6.979	1835	1847	1873	rBV	148796	276712	18.99%	2.370%
46	7.307	1937	1949	1970	rBV	680288	1210928	83.11%	10.370%
47	7.616	2034	2045	2071	rBV	103136	186189	12.78%	1.595%
48	7.860	2119	2121	2124	rVB	433	170	0.01%	0.001%
49	7.873	2124	2125	2126	rBV	251	95	0.01%	0.001%
50	8.085	2180	2191	2226	rBV	391169	709791	48.72%	6.079%
51	8.545	2330	2334	2337	rBV2	337	248	0.02%	0.002%
52	8.593	2346	2349	2354	rVB2	428	305	0.02%	0.003%
53	8.619	2354	2357	2359	rVB	269	113	0.01%	0.001%
54	8.635	2359	2362	2365	rBV2	341	213	0.01%	0.002%
55	8.651	2365	2367	2369	rBV2	125	93	0.01%	0.001%
56	8.715	2384	2387	2389	rBV3	214	159	0.01%	0.001%
57	8.751	2395	2398	2400	rVB2	297	158	0.01%	0.001%
58	8.844	2415	2427	2451	rBV	717788	1186744	81.45%	10.163%
59	9.101	2502	2507	2509	rBV2	392	340	0.02%	0.003%
60	9.133	2509	2517	2527	rVB5	1921	3405	0.23%	0.029%
61	9.185	2531	2533	2537	rBV2	381	247	0.02%	0.002%
62	9.207	2537	2540	2546	rVB2	281	261	0.02%	0.002%
63	9.243	2546	2551	2553	rBV	403	268	0.02%	0.002%
64	9.339	2577	2581	2584	rBV3	222	200	0.01%	0.002%
65	9.468	2616	2621	2624	rVV2	294	283	0.02%	0.002%
66	9.561	2641	2650	2661	rVB4	6680	11117	0.76%	0.095%
67	9.632	2669	2672	2674	rBV	255	172	0.01%	0.001%
68	9.657	2678	2680	2683	rBV	155	110	0.01%	0.001%
69	9.690	2688	2690	2692	rBV	192	103	0.01%	0.001%
70	9.722	2698	2700	2706	rVB3	201	166	0.01%	0.001%
71	9.805	2720	2726	2735	rBV5	2008	2774	0.19%	0.024%
72	9.908	2755	2758	2760	rBV2	366	254	0.02%	0.002%
73	9.995	2779	2785	2787	rBV2	310	268	0.02%	0.002%
74	10.021	2789	2793	2797	rVV2	304	265	0.02%	0.002%
75	10.069	2804	2808	2812	rBV2	250	192	0.01%	0.002%
76	10.162	2825	2837	2841	rBV	22983	33408	2.29%	0.286%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029542.D
 Acq On : 09 Dec 2022 23:35
 Operator : SY/MD
 Sample : N5959-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.204	2842	2850	2868	rVB	456944	720061	49.42%	6.167%
78	10.374	2895	2903	2915	rVB2	3610	5620	0.39%	0.048%
79	10.452	2925	2927	2929	rBV	274	161	0.01%	0.001%
80	10.522	2946	2949	2951	rBV	469	341	0.02%	0.003%
81	10.567	2955	2963	2974	rVV	9980	16186	1.11%	0.139%
82	10.702	3001	3005	3008	rBV3	243	200	0.01%	0.002%
83	10.767	3022	3025	3030	rVB	243	151	0.01%	0.001%
84	10.792	3030	3033	3034	rBV2	228	109	0.01%	0.001%
85	10.802	3034	3036	3037	rBV2	419	175	0.01%	0.001%
86	10.854	3050	3052	3056	rBV2	192	102	0.01%	0.001%
87	10.918	3061	3072	3080	rBV5	1244	3230	0.22%	0.028%
88	10.992	3092	3095	3102	rBV3	244	312	0.02%	0.003%
89	11.146	3139	3143	3147	rVB3	591	437	0.03%	0.004%
90	11.169	3147	3150	3152	rBV2	795	580	0.04%	0.005%
91	11.239	3160	3172	3196	rBV	807746	1245399	85.48%	10.666%
92	11.551	3260	3269	3275	rBV6	4618	7408	0.51%	0.063%
93	11.612	3277	3288	3315	rVB	717694	1132882	77.76%	9.702%
94	11.847	3359	3361	3365	rBV3	292	260	0.02%	0.002%
95	11.940	3388	3390	3391	rBV	243	101	0.01%	0.001%
96	12.227	3475	3479	3480	rBV3	724	544	0.04%	0.005%
97	12.339	3510	3514	3524	rVB5	1237	1075	0.07%	0.009%
98	12.442	3540	3546	3547	rBV2	307	300	0.02%	0.003%
99	12.632	3602	3605	3610	rBB2	460	449	0.03%	0.004%
100	13.394	3837	3842	3845	rBV4	520	547	0.04%	0.005%




Sum of corrected areas: 11676814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029542.D
Acq On : 09 Dec 2022 23:35
Operator : SY/MD
Sample : N5959-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

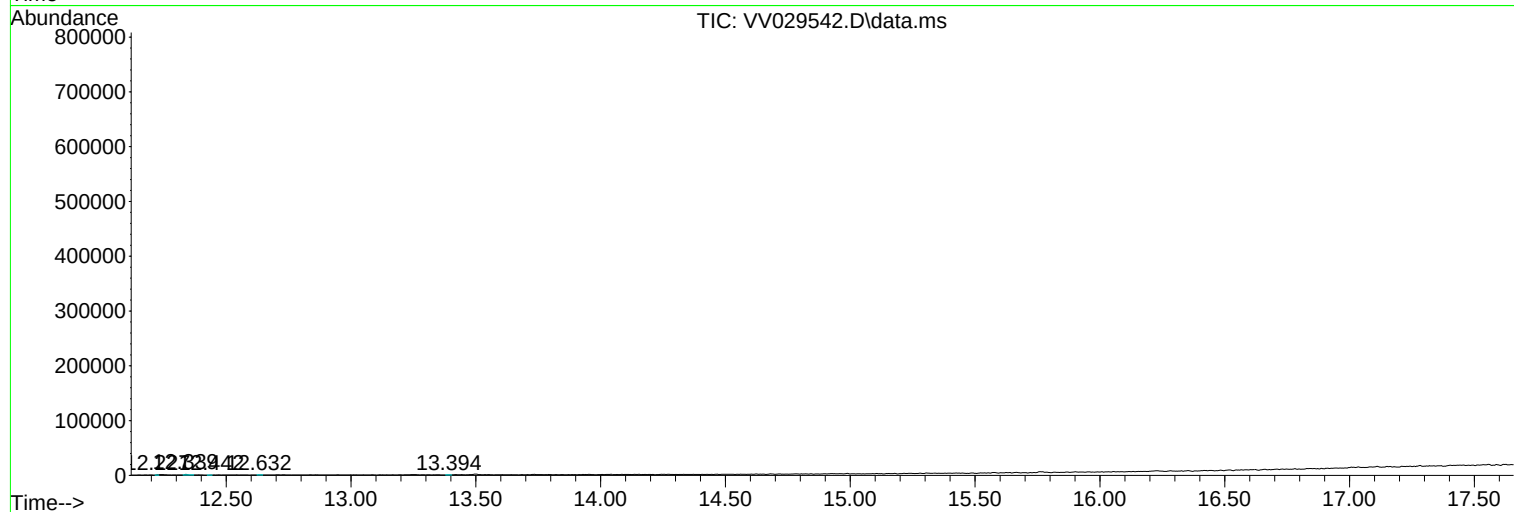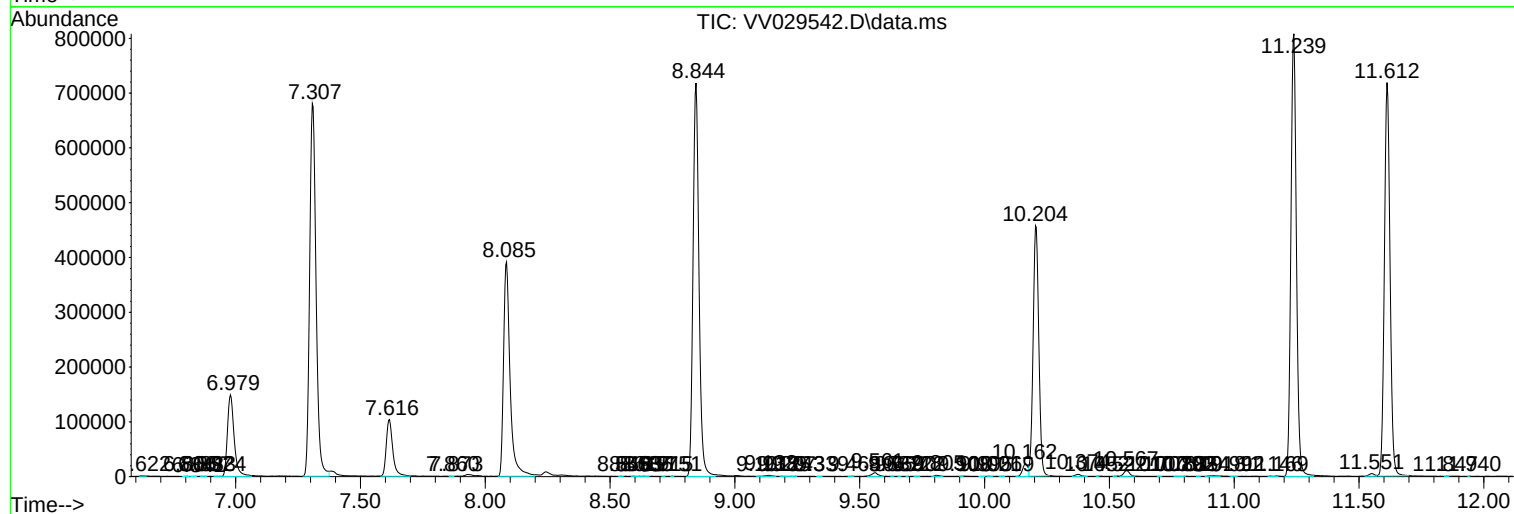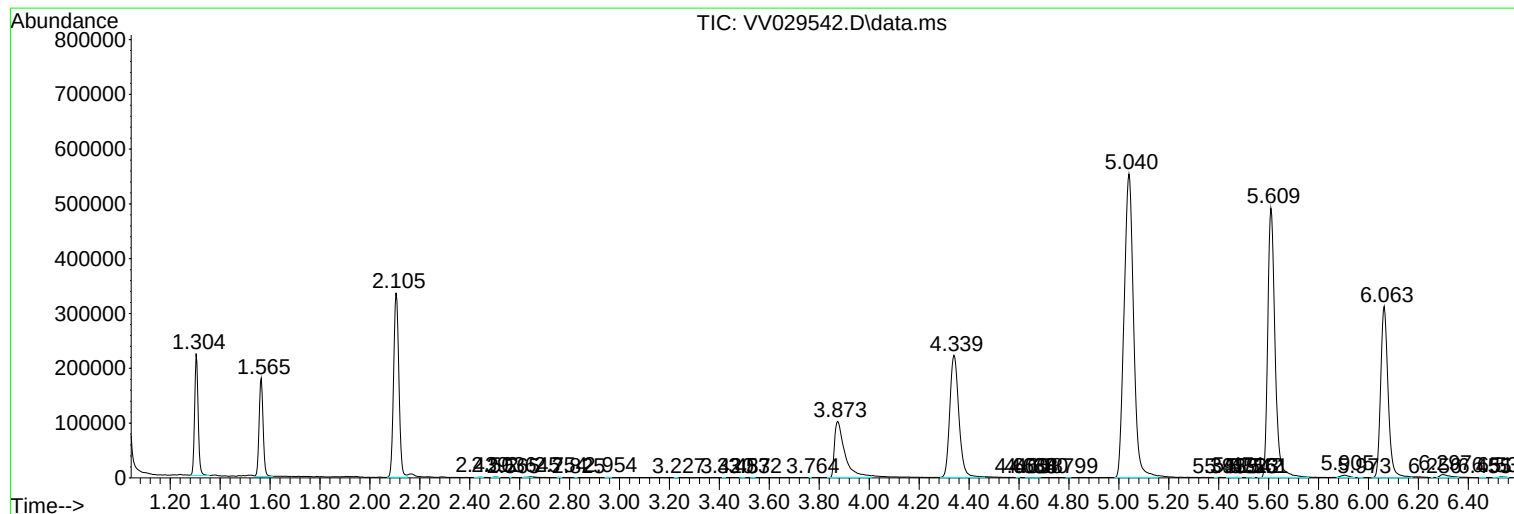

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029542.D
Acq On : 09 Dec 2022 23:35
Operator : SY/MD
Sample : N5959-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029542.D
Acq On : 09 Dec 2022 23:35
Operator : SY/MD
Sample : N5959-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc