

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029543.D
 Acq On : 09 Dec 2022 23:58
 Operator : SY/MD
 Sample : N5959-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	221601	218574	14.25%	1.812%
2	1.564	155	163	178	rVB	182297	205886	13.43%	1.706%
3	2.105	320	331	346	rBV	347704	502026	32.74%	4.161%
4	2.281	382	386	387	rBV2	965	711	0.05%	0.006%
5	2.442	432	436	443	rVB3	321	401	0.03%	0.003%
6	2.503	449	455	465	rVB4	1233	2057	0.13%	0.017%
7	2.651	489	501	507	rBV4	1417	3164	0.21%	0.026%
8	2.754	530	533	538	rVB3	291	305	0.02%	0.003%
9	2.857	563	565	567	rVB2	450	214	0.01%	0.002%
10	2.957	593	596	602	rVB4	334	371	0.02%	0.003%
11	2.989	602	606	610	rBV	339	293	0.02%	0.002%
12	3.371	718	725	726	rBV	302	259	0.02%	0.002%
13	3.439	741	746	752	rVB2	217	263	0.02%	0.002%
14	3.542	776	778	783	rVB	332	197	0.01%	0.002%
15	3.706	825	829	833	rVV2	374	267	0.02%	0.002%
16	3.876	872	882	919	rBV	108530	312564	20.38%	2.591%
17	4.224	987	990	994	rVB2	396	301	0.02%	0.002%
18	4.339	1008	1026	1057	rBV	234676	592744	38.65%	4.913%
19	4.584	1098	1102	1103	rBV2	525	382	0.02%	0.003%
20	4.674	1126	1130	1134	rVB2	262	268	0.02%	0.002%
21	4.728	1142	1147	1150	rBV2	228	201	0.01%	0.002%
22	4.789	1162	1166	1168	rBV2	235	200	0.01%	0.002%
23	4.828	1174	1178	1181	rBV2	341	288	0.02%	0.002%
24	5.040	1226	1244	1284	rBV2	583223	1533528	100.00%	12.710%
25	5.246	1306	1308	1313	rVB3	421	321	0.02%	0.003%
26	5.281	1316	1319	1323	rBV4	468	388	0.03%	0.003%
27	5.416	1360	1361	1366	rVB2	353	195	0.01%	0.002%
28	5.609	1408	1421	1457	rBV	509567	1052782	68.65%	8.726%
29	5.905	1502	1513	1527	rVB8	3772	8376	0.55%	0.069%
30	5.989	1537	1539	1545	rVB	302	243	0.02%	0.002%
31	6.063	1546	1562	1595	rBV	326278	680319	44.36%	5.639%
32	6.281	1627	1630	1633	rBV2	370	274	0.02%	0.002%
33	6.371	1654	1658	1662	rVB2	353	195	0.01%	0.002%
34	6.629	1729	1738	1739	rBV2	1068	1273	0.08%	0.011%
35	6.770	1777	1782	1785	rVB2	301	212	0.01%	0.002%
36	6.854	1803	1808	1811	rBV2	421	287	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029543.D
 Acq On : 09 Dec 2022 23:58
 Operator : SY/MD
 Sample : N5959-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COENO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.979	1834	1847	1876	rBV	154989	289763	18.90%	2.402%
38	7.239	1925	1928	1932	rBV3	348	296	0.02%	0.002%
39	7.307	1937	1949	1982	rBV	712787	1265083	82.49%	10.486%
40	7.612	2033	2044	2071	rBV	110060	195472	12.75%	1.620%
41	7.825	2106	2110	2112	rBV3	295	283	0.02%	0.002%
42	7.857	2118	2120	2125	rVB4	606	373	0.02%	0.003%
43	7.889	2125	2130	2136	rBV3	473	588	0.04%	0.005%
44	7.931	2136	2143	2152	rBV4	3322	5962	0.39%	0.049%
45	7.995	2160	2163	2166	rVB3	320	203	0.01%	0.002%
46	8.085	2180	2191	2227	rBV	407073	745635	48.62%	6.180%
47	8.349	2271	2273	2277	rBV3	546	329	0.02%	0.003%
48	8.384	2280	2284	2288	rVB3	306	268	0.02%	0.002%
49	8.429	2294	2298	2300	rBV2	402	299	0.02%	0.002%
50	8.500	2315	2320	2323	rBV2	391	437	0.03%	0.004%
51	8.699	2380	2382	2387	rBV3	332	249	0.02%	0.002%
52	8.776	2401	2406	2412	rBV2	296	286	0.02%	0.002%
53	8.844	2414	2427	2452	rBV	748792	1238865	80.79%	10.268%
54	9.127	2511	2515	2517	rVV2	412	304	0.02%	0.003%
55	9.140	2517	2519	2522	rVB2	583	259	0.02%	0.002%
56	9.233	2546	2548	2553	rVB2	329	231	0.02%	0.002%
57	9.426	2605	2608	2615	rBV2	297	287	0.02%	0.002%
58	9.538	2638	2643	2644	rBV2	455	384	0.03%	0.003%
59	9.548	2644	2646	2648	rVV	466	205	0.01%	0.002%
60	9.590	2655	2659	2662	rVV3	297	337	0.02%	0.003%
61	9.625	2665	2670	2672	rVV	263	218	0.01%	0.002%
62	9.651	2676	2678	2684	rVB2	313	223	0.01%	0.002%
63	9.686	2684	2689	2691	rBV	354	234	0.02%	0.002%
64	9.918	2756	2761	2763	rBV2	387	439	0.03%	0.004%
65	9.982	2775	2781	2785	rBV3	434	508	0.03%	0.004%
66	10.037	2795	2798	2806	rVB2	404	452	0.03%	0.004%
67	10.079	2807	2811	2816	rVB2	416	390	0.03%	0.003%
68	10.162	2827	2837	2841	rBV2	22576	32712	2.13%	0.271%
69	10.207	2841	2851	2868	rVB	480986	757775	49.41%	6.281%
70	10.297	2876	2879	2882	rVB	396	275	0.02%	0.002%
71	10.374	2896	2903	2914	rVB3	2872	4343	0.28%	0.036%
72	10.535	2943	2953	2955	rBV3	982	1389	0.09%	0.012%
73	10.567	2955	2963	2975	rVB2	10832	17244	1.12%	0.143%
74	10.657	2985	2991	2993	rBV2	445	361	0.02%	0.003%
75	10.776	3022	3028	3033	rBV2	314	339	0.02%	0.003%
76	10.828	3041	3044	3046	rVV2	275	220	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029543.D
 Acq On : 09 Dec 2022 23:58
 Operator : SY/MD
 Sample : N5959-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.841	3046	3048	3052	rVV3	553	340	0.02%	0.003%
78	10.905	3064	3068	3071	rBV4	776	747	0.05%	0.006%
79	11.050	3107	3113	3118	rBV3	389	454	0.03%	0.004%
80	11.175	3147	3152	3158	rBV6	1028	1235	0.08%	0.010%
81	11.239	3158	3172	3205	rBV	790668	1237689	80.71%	10.258%
82	11.480	3242	3247	3250	rBV2	405	333	0.02%	0.003%
83	11.551	3259	3269	3277	rBV5	3309	6241	0.41%	0.052%
84	11.612	3277	3288	3308	rVV	721798	1128679	73.60%	9.355%
85	11.860	3359	3365	3367	rBV3	379	337	0.02%	0.003%
86	12.040	3416	3421	3423	rBV2	251	230	0.01%	0.002%
87	12.172	3460	3462	3468	rVB2	438	353	0.02%	0.003%
88	12.201	3468	3471	3474	rBV2	479	413	0.03%	0.003%
89	12.361	3518	3521	3525	rVB2	496	381	0.02%	0.003%
90	12.384	3525	3528	3531	rBV2	512	382	0.02%	0.003%
91	12.487	3557	3560	3563	rVB4	428	271	0.02%	0.002%
92	12.564	3580	3584	3587	rVB2	377	215	0.01%	0.002%
93	12.625	3602	3603	3607	rBV	288	238	0.02%	0.002%
94	12.853	3672	3674	3681	rBV3	361	298	0.02%	0.002%
95	12.924	3693	3696	3699	rBV2	411	289	0.02%	0.002%
96	13.104	3747	3752	3754	rBV2	486	438	0.03%	0.004%
97	13.201	3780	3782	3787	rVB4	417	222	0.01%	0.002%
98	13.246	3794	3796	3797	rBV	411	220	0.01%	0.002%
99	14.458	4171	4173	4175	rBV3	692	440	0.03%	0.004%
100	14.609	4218	4220	4226	rBV4	737	769	0.05%	0.006%




Sum of corrected areas: 12065063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029543.D
Acq On : 09 Dec 2022 23:58
Operator : SY/MD
Sample : N5959-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COEN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

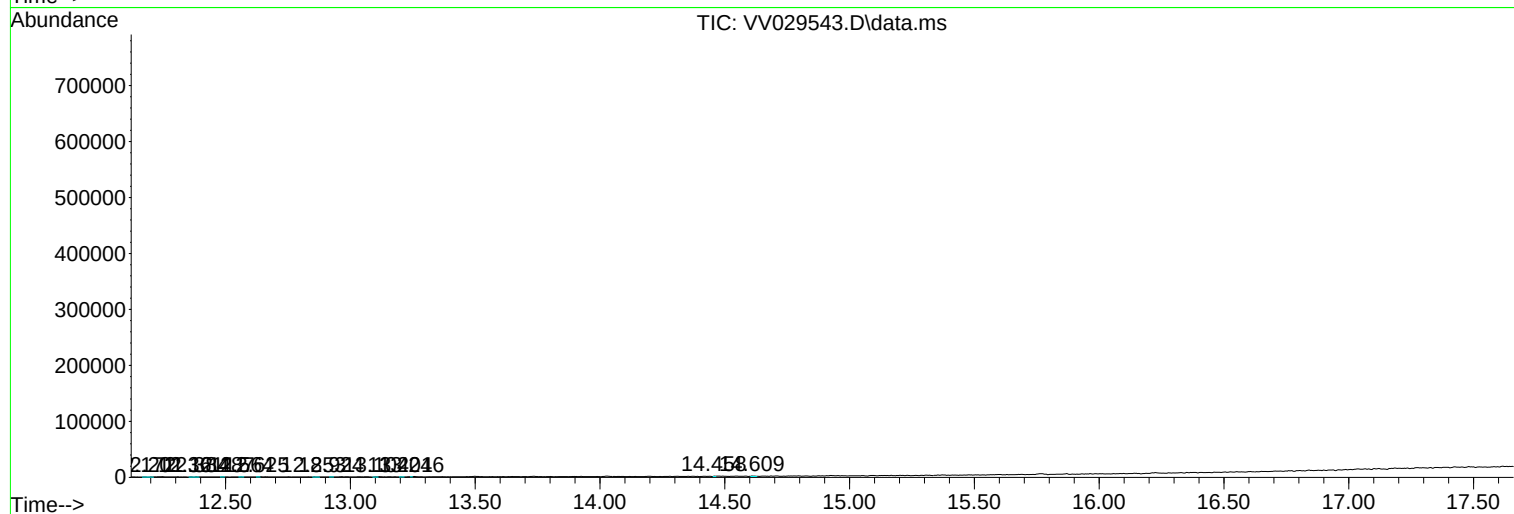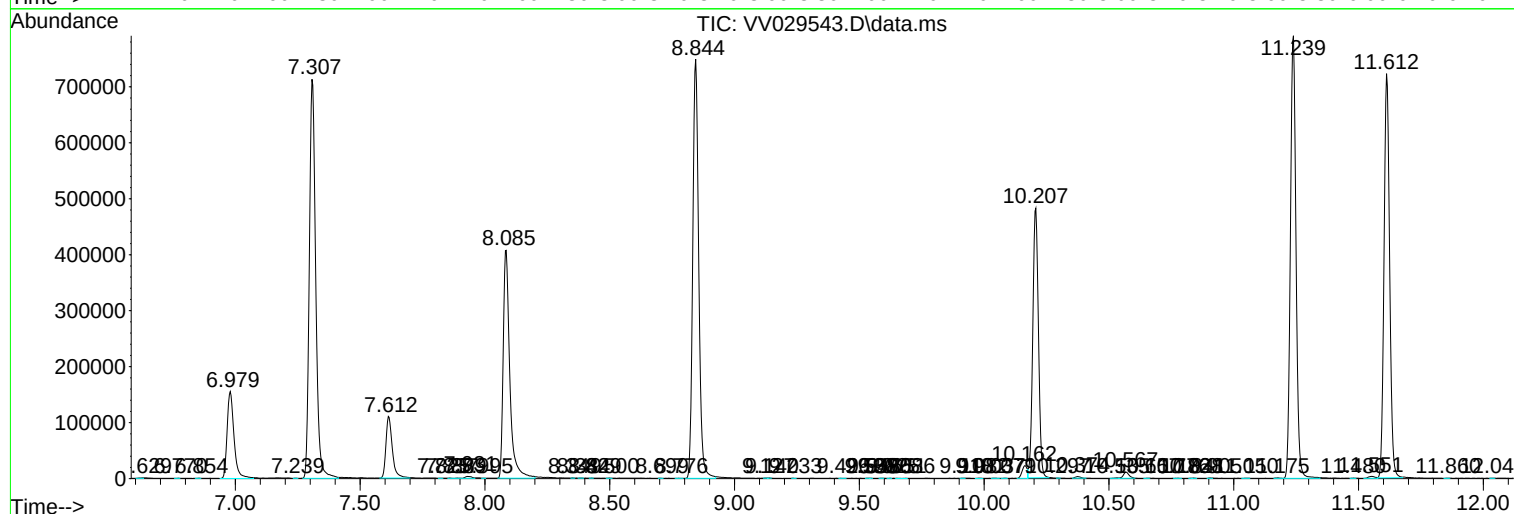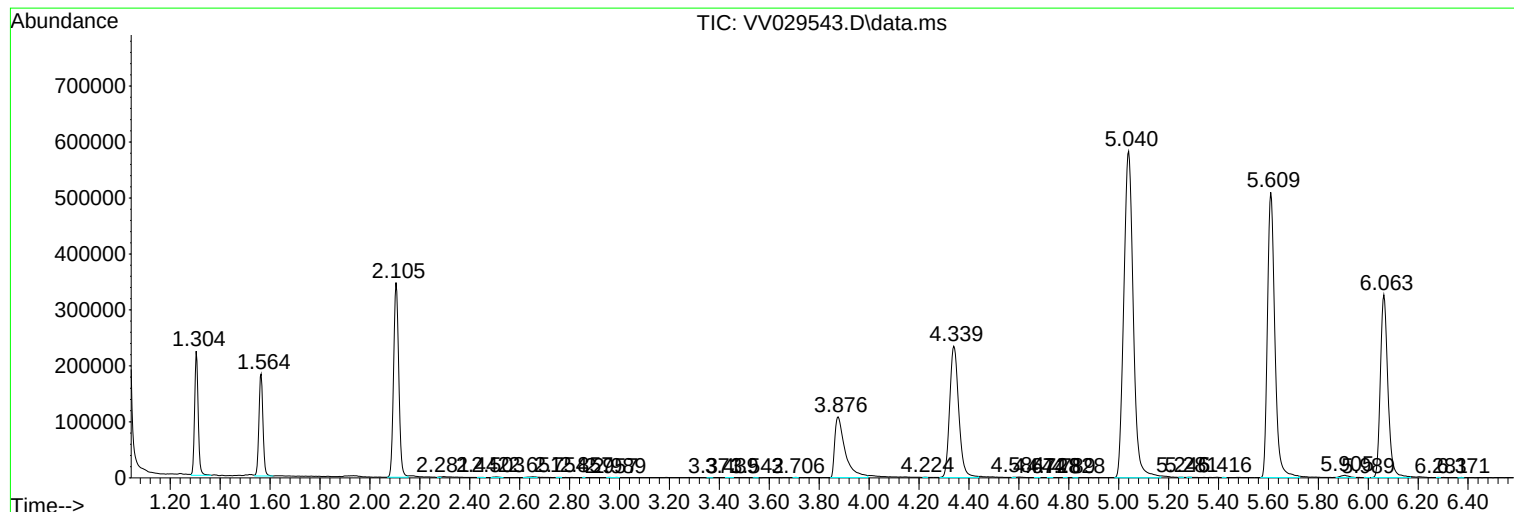

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029543.D
Acq On : 09 Dec 2022 23:58
Operator : SY/MD
Sample : N5959-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029543.D
Acq On : 09 Dec 2022 23:58
Operator : SY/MD
Sample : N5959-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------