

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029545.D
 Acq On : 10 Dec 2022 00:45
 Operator : SY/MD
 Sample : N5915-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	217260	215031	14.09%	1.712%
2	1.565	155	163	175	rVB	180900	200953	13.17%	1.600%
3	2.105	320	331	345	rBV	346672	498497	32.67%	3.968%
4	2.372	411	414	419	rBV2	331	307	0.02%	0.002%
5	2.468	442	444	447	rBV2	281	129	0.01%	0.001%
6	2.500	451	454	462	rVB4	1219	1621	0.11%	0.013%
7	2.838	557	559	561	rBV	189	84	0.01%	0.001%
8	2.902	577	579	582	rBV2	122	71	0.00%	0.001%
9	2.957	588	596	598	rBV4	551	641	0.04%	0.005%
10	3.175	653	664	675	rBV4	3791	7982	0.52%	0.064%
11	3.217	675	677	678	rVB4	286	92	0.01%	0.001%
12	3.236	680	683	685	rBV2	324	150	0.01%	0.001%
13	3.384	726	729	730	rBV	164	71	0.00%	0.001%
14	3.413	735	738	743	rBV	118	135	0.01%	0.001%
15	3.574	786	788	791	rVB	230	91	0.01%	0.001%
16	3.690	820	824	827	rBV	331	226	0.01%	0.002%
17	3.741	837	840	843	rVB2	177	94	0.01%	0.001%
18	3.828	862	867	871	rVB2	222	217	0.01%	0.002%
19	3.870	871	880	911	rBV	125208	342874	22.47%	2.729%
20	4.339	1009	1026	1055	rBV	236493	588245	38.55%	4.682%
21	4.667	1126	1128	1131	rBV2	288	135	0.01%	0.001%
22	4.741	1146	1151	1154	rBV3	252	254	0.02%	0.002%
23	4.831	1177	1179	1183	rVB	254	124	0.01%	0.001%
24	4.867	1188	1190	1192	rBV	179	75	0.00%	0.001%
25	4.896	1192	1199	1204	rBV3	360	500	0.03%	0.004%
26	4.976	1220	1224	1226	rBV	191	179	0.01%	0.001%
27	5.040	1226	1244	1271	rBV2	585387	1526000	100.00%	12.147%
28	5.355	1340	1342	1344	rBV2	263	128	0.01%	0.001%
29	5.420	1358	1362	1367	rBV2	254	260	0.02%	0.002%
30	5.523	1390	1394	1402	rBV	380	527	0.03%	0.004%
31	5.609	1407	1421	1453	rBV	544919	1101881	72.21%	8.771%
32	5.905	1503	1513	1527	rVB8	4893	10688	0.70%	0.085%
33	6.008	1542	1545	1546	rBV2	309	189	0.01%	0.002%
34	6.063	1548	1562	1597	rVV	328231	677854	44.42%	5.396%
35	6.275	1626	1628	1630	rBV	212	91	0.01%	0.001%
36	6.310	1636	1639	1641	rBV	149	103	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029545.D
 Acq On : 10 Dec 2022 00:45
 Operator : SY/MD
 Sample : N5915-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.323	1641	1643	1646	rVB2	191	72	0.00%	0.001%
38	6.481	1690	1692	1695	rVB3	256	156	0.01%	0.001%
39	6.513	1695	1702	1704	rBV2	365	362	0.02%	0.003%
40	6.625	1731	1737	1752	rVB8	1026	2316	0.15%	0.018%
41	6.680	1752	1754	1757	rBV2	476	220	0.01%	0.002%
42	6.699	1758	1760	1762	rBV2	267	126	0.01%	0.001%
43	6.738	1770	1772	1774	rBV2	305	181	0.01%	0.001%
44	6.777	1782	1784	1788	rVB2	222	111	0.01%	0.001%
45	6.799	1788	1791	1796	rBV2	427	322	0.02%	0.003%
46	6.854	1805	1808	1811	rBV	159	85	0.01%	0.001%
47	6.870	1811	1813	1814	rVV	212	97	0.01%	0.001%
48	6.892	1817	1820	1825	rVB3	224	173	0.01%	0.001%
49	6.918	1825	1828	1829	rBV3	207	93	0.01%	0.001%
50	6.979	1835	1847	1873	rBV	155226	286736	18.79%	2.282%
51	7.307	1936	1949	1988	rBV	720039	1278412	83.78%	10.176%
52	7.613	2034	2044	2070	rBV	111906	195687	12.82%	1.558%
53	7.931	2137	2143	2152	rBV4	3058	4896	0.32%	0.039%
54	8.082	2180	2190	2229	rBV	489180	873669	57.25%	6.954%
55	8.625	2356	2359	2365	rVB3	358	353	0.02%	0.003%
56	8.683	2375	2377	2380	rBV2	297	119	0.01%	0.001%
57	8.757	2395	2400	2401	rBV	330	211	0.01%	0.002%
58	8.844	2415	2427	2456	rBV	787743	1298002	85.06%	10.332%
59	9.108	2507	2509	2512	rBV	341	192	0.01%	0.002%
60	9.130	2514	2516	2518	rBV2	559	310	0.02%	0.002%
61	9.188	2531	2534	2536	rVV2	349	239	0.02%	0.002%
62	9.217	2540	2543	2547	rVV3	448	351	0.02%	0.003%
63	9.246	2550	2552	2555	rVB	238	97	0.01%	0.001%
64	9.268	2555	2559	2562	rBV2	364	271	0.02%	0.002%
65	9.284	2562	2564	2567	rBV	199	103	0.01%	0.001%
66	9.301	2567	2569	2572	rVB3	275	163	0.01%	0.001%
67	9.317	2572	2574	2575	rBV3	199	87	0.01%	0.001%
68	9.371	2589	2591	2593	rBV2	244	103	0.01%	0.001%
69	9.458	2614	2618	2619	rBV2	300	192	0.01%	0.002%
70	9.503	2627	2632	2637	rBV2	267	269	0.02%	0.002%
71	9.535	2637	2642	2646	rBV5	744	727	0.05%	0.006%
72	9.632	2669	2672	2674	rBV	229	170	0.01%	0.001%
73	9.664	2679	2682	2687	rBV2	265	235	0.02%	0.002%
74	9.690	2687	2690	2692	rBV2	193	95	0.01%	0.001%
75	9.760	2710	2712	2716	rBV	205	93	0.01%	0.001%
76	9.786	2718	2720	2724	rVB2	337	152	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029545.D
 Acq On : 10 Dec 2022 00:45
 Operator : SY/MD
 Sample : N5915-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.921	2756	2762	2766	rBV3	690	737	0.05%	0.006%
78	10.040	2796	2799	2800	rBV	236	137	0.01%	0.001%
79	10.079	2809	2811	2814	rBV2	161	96	0.01%	0.001%
80	10.162	2824	2837	2841	rBV	23937	35102	2.30%	0.279%
81	10.204	2842	2850	2874	rVB	498949	793878	52.02%	6.319%
82	10.374	2895	2903	2912	rBV2	3816	5955	0.39%	0.047%
83	10.468	2927	2932	2933	rBV2	168	149	0.01%	0.001%
84	10.526	2948	2950	2951	rBV2	353	152	0.01%	0.001%
85	10.567	2955	2963	2986	rVB3	11384	19265	1.26%	0.153%
86	10.686	2998	3000	3002	rBV3	214	110	0.01%	0.001%
87	10.908	3064	3069	3074	rBV3	900	1035	0.07%	0.008%
88	11.024	3103	3105	3107	rVB	178	73	0.00%	0.001%
89	11.043	3108	3111	3112	rBV	187	94	0.01%	0.001%
90	11.239	3160	3172	3208	rBV	881517	1366158	89.53%	10.875%
91	11.493	3249	3251	3255	rBV	319	215	0.01%	0.002%
92	11.516	3255	3258	3262	rBV4	401	311	0.02%	0.002%
93	11.551	3262	3269	3276	rBV5	2516	4212	0.28%	0.034%
94	11.612	3277	3288	3314	rVB	771325	1211254	79.37%	9.642%
95	11.841	3357	3359	3361	rVB	266	114	0.01%	0.001%
96	12.027	3415	3417	3419	rBV	179	77	0.01%	0.001%
97	12.127	3444	3448	3453	rBV4	548	556	0.04%	0.004%
98	12.387	3527	3529	3530	rBV4	288	130	0.01%	0.001%
99	12.423	3537	3540	3543	rBV3	242	116	0.01%	0.001%
100	12.873	3679	3680	3682	rBV2	312	143	0.01%	0.001%




Sum of corrected areas: 12562816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029545.D
Acq On : 10 Dec 2022 00:45
Operator : SY/MD
Sample : N5915-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

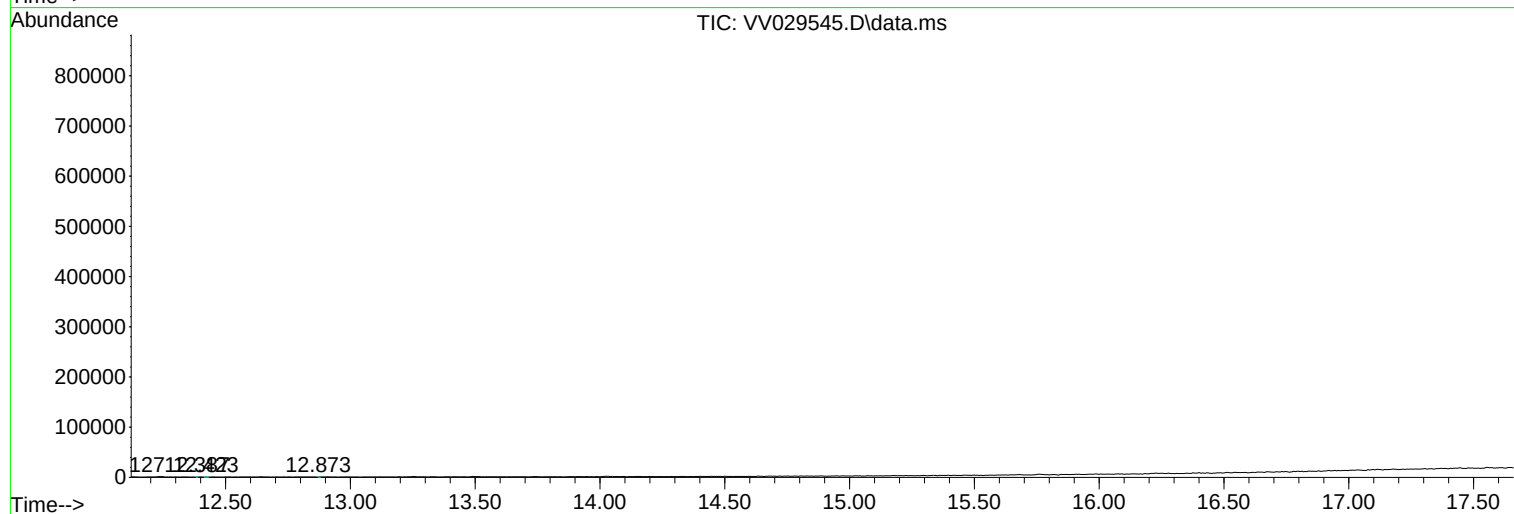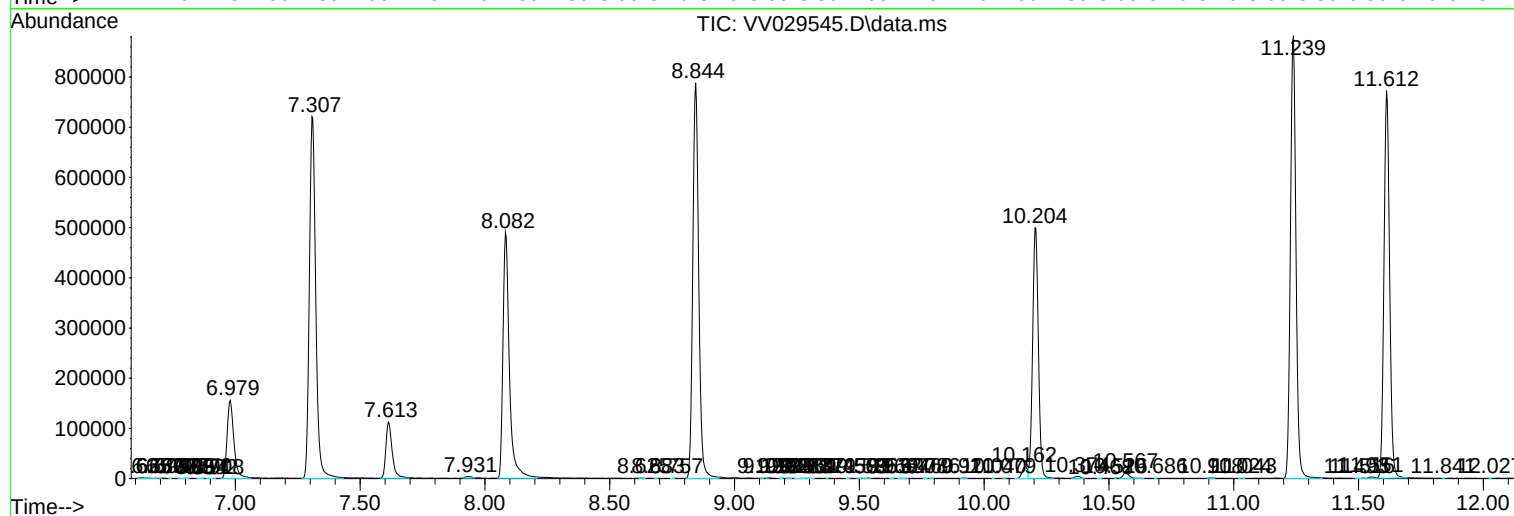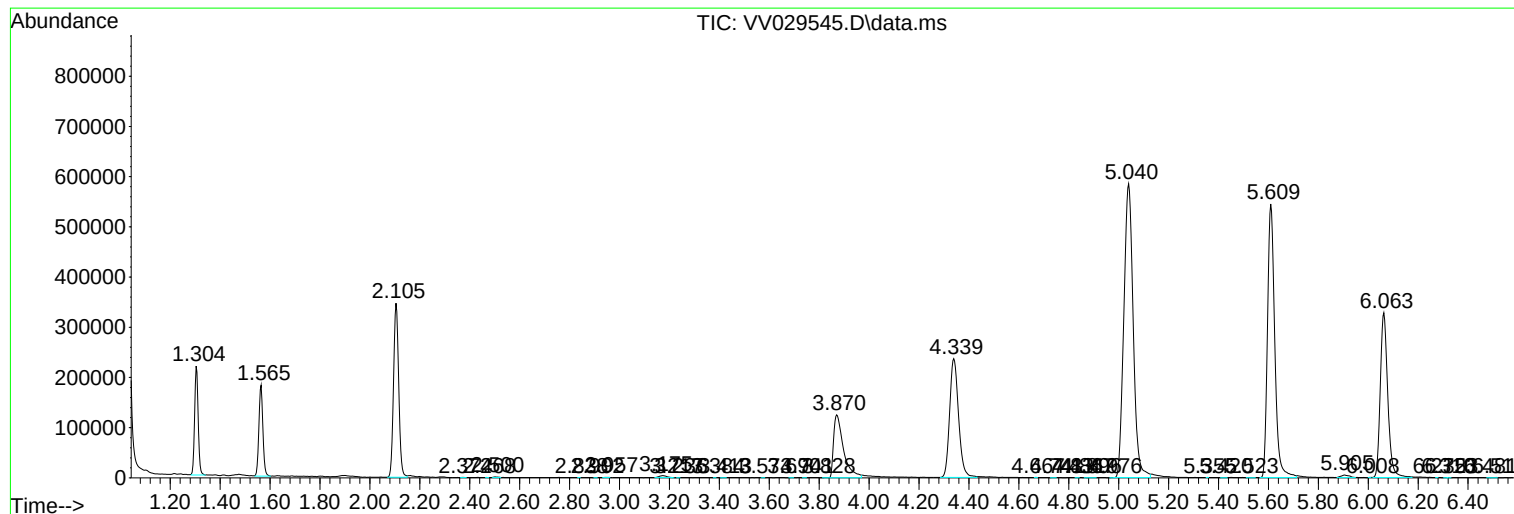

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029545.D
Acq On : 10 Dec 2022 00:45
Operator : SY/MD
Sample : N5915-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029545.D
Acq On : 10 Dec 2022 00:45
Operator : SY/MD
Sample : N5915-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc