

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029546.D
 Acq On : 10 Dec 2022 01:09
 Operator : SY/MD
 Sample : N5915-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	216943	216050	14.61%	1.823%
2	1.564	155	163	176	rVB	171053	194314	13.14%	1.639%
3	2.105	320	331	345	rBV	336030	482705	32.65%	4.073%
4	2.506	450	456	464	rVB5	1654	2471	0.17%	0.021%
5	2.545	464	468	470	rBV	208	134	0.01%	0.001%
6	2.722	521	523	526	rBV2	175	95	0.01%	0.001%
7	2.921	582	585	587	rBV2	183	125	0.01%	0.001%
8	2.950	593	594	599	rBV2	157	89	0.01%	0.001%
9	3.034	616	620	625	rBV2	239	224	0.02%	0.002%
10	3.095	637	639	640	rBV2	126	59	0.00%	0.000%
11	3.330	709	712	716	rVB	180	125	0.01%	0.001%
12	3.391	729	731	734	rBV2	151	80	0.01%	0.001%
13	3.423	737	741	745	rBV2	197	146	0.01%	0.001%
14	3.449	745	749	752	rBV2	209	148	0.01%	0.001%
15	3.545	776	779	782	rBV	197	122	0.01%	0.001%
16	3.664	813	816	820	rBV	108	71	0.00%	0.001%
17	3.873	871	881	913	rBV	105388	295701	20.00%	2.495%
18	4.339	1009	1026	1056	rBV	232815	578365	39.12%	4.880%
19	4.667	1126	1128	1130	rBV	210	100	0.01%	0.001%
20	4.706	1137	1140	1142	rBV2	159	96	0.01%	0.001%
21	4.738	1147	1150	1153	rBV2	205	161	0.01%	0.001%
22	4.809	1169	1172	1174	rBV	146	81	0.01%	0.001%
23	4.822	1174	1176	1184	rVB	238	216	0.01%	0.002%
24	4.860	1186	1188	1190	rVB2	195	61	0.00%	0.001%
25	4.899	1199	1200	1203	rVB	333	105	0.01%	0.001%
26	4.921	1203	1207	1210	rBV	171	166	0.01%	0.001%
27	4.937	1210	1212	1214	rVB	143	43	0.00%	0.000%
28	4.960	1217	1219	1221	rBV	172	92	0.01%	0.001%
29	5.040	1226	1244	1285	rBV2	565140	1478464	100.00%	12.474%
30	5.461	1373	1375	1377	rBV2	290	146	0.01%	0.001%
31	5.609	1407	1421	1462	rBV	524632	1062113	71.84%	8.961%
32	5.902	1502	1512	1527	rVB9	4967	11356	0.77%	0.096%
33	6.063	1548	1562	1599	rBV	317915	657999	44.51%	5.552%
34	6.284	1630	1631	1634	rBV2	220	106	0.01%	0.001%
35	6.304	1635	1637	1639	rVB2	258	85	0.01%	0.001%
36	6.320	1639	1642	1644	rBV	177	91	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029546.D
 Acq On : 10 Dec 2022 01:09
 Operator : SY/MD
 Sample : N5915-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.461	1683	1686	1690	rBV2	339	215	0.01%	0.002%
38	6.500	1696	1698	1700	rVB	132	54	0.00%	0.000%
39	6.516	1700	1703	1704	rBV	179	91	0.01%	0.001%
40	6.542	1708	1711	1713	rBV2	148	98	0.01%	0.001%
41	6.564	1716	1718	1722	rVB2	225	132	0.01%	0.001%
42	6.616	1728	1734	1735	rBV	783	546	0.04%	0.005%
43	6.780	1783	1785	1787	rVB	166	72	0.00%	0.001%
44	6.812	1787	1795	1800	rBV3	254	298	0.02%	0.003%
45	6.863	1810	1811	1812	rBV3	111	42	0.00%	0.000%
46	6.979	1835	1847	1879	rBV	150741	281777	19.06%	2.377%
47	7.117	1887	1890	1896	rBV4	469	369	0.02%	0.003%
48	7.307	1937	1949	1975	rBV	694888	1222645	82.70%	10.315%
49	7.612	2033	2044	2072	rBV	104453	188538	12.75%	1.591%
50	8.001	2162	2165	2167	rBV2	334	252	0.02%	0.002%
51	8.082	2180	2190	2228	rBV	388477	712673	48.20%	6.013%
52	8.571	2341	2342	2343	rBV	242	77	0.01%	0.001%
53	8.596	2347	2350	2353	rVV3	478	359	0.02%	0.003%
54	8.622	2355	2358	2365	rVB3	257	264	0.02%	0.002%
55	8.648	2365	2366	2368	rVB	230	58	0.00%	0.000%
56	8.673	2371	2374	2375	rBV	394	185	0.01%	0.002%
57	8.844	2414	2427	2449	rBV	752380	1249811	84.53%	10.545%
58	9.130	2512	2516	2517	rBV	387	300	0.02%	0.003%
59	9.169	2527	2528	2532	rVB2	468	213	0.01%	0.002%
60	9.249	2550	2553	2556	rBV2	228	167	0.01%	0.001%
61	9.310	2567	2572	2577	rBV2	227	280	0.02%	0.002%
62	9.336	2577	2580	2583	rVV2	256	125	0.01%	0.001%
63	9.400	2598	2600	2603	rBV2	189	116	0.01%	0.001%
64	9.445	2613	2614	2616	rVB	228	47	0.00%	0.000%
65	9.497	2628	2630	2633	rBV	263	137	0.01%	0.001%
66	9.603	2657	2663	2667	rBV4	567	656	0.04%	0.006%
67	9.760	2710	2712	2715	rBV2	261	145	0.01%	0.001%
68	9.828	2729	2733	2736	rBV2	192	170	0.01%	0.001%
69	9.873	2745	2747	2750	rVB2	306	144	0.01%	0.001%
70	10.040	2797	2799	2806	rVB	251	173	0.01%	0.001%
71	10.101	2814	2818	2821	rVB2	465	343	0.02%	0.003%
72	10.162	2827	2837	2841	rBV	22812	32197	2.18%	0.272%
73	10.207	2842	2851	2872	rVB	469753	731782	49.50%	6.174%
74	10.326	2885	2888	2890	rBV3	325	218	0.01%	0.002%
75	10.419	2913	2917	2920	rBV2	314	289	0.02%	0.002%
76	10.525	2947	2950	2953	rBV3	519	431	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029546.D
 Acq On : 10 Dec 2022 01:09
 Operator : SY/MD
 Sample : N5915-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.567	2955	2963	2976	rVB2	10330	16509	1.12%	0.139%
78	10.661	2991	2992	2995	rBV	132	74	0.01%	0.001%
79	10.696	3001	3003	3006	rVB2	213	124	0.01%	0.001%
80	10.722	3006	3011	3014	rBV3	317	338	0.02%	0.003%
81	10.770	3024	3026	3029	rVB	176	89	0.01%	0.001%
82	10.834	3042	3046	3049	rBV3	286	206	0.01%	0.002%
83	10.850	3049	3051	3052	rVV3	190	50	0.00%	0.000%
84	10.892	3062	3064	3065	rBV2	330	125	0.01%	0.001%
85	10.972	3086	3089	3094	rVB3	224	207	0.01%	0.002%
86	11.017	3100	3103	3107	rVB	262	187	0.01%	0.002%
87	11.037	3107	3109	3110	rBV	167	69	0.00%	0.001%
88	11.101	3126	3129	3132	rBV	287	256	0.02%	0.002%
89	11.172	3147	3151	3160	rVB6	873	1042	0.07%	0.009%
90	11.239	3160	3172	3190	rBV	825398	1275597	86.28%	10.762%
91	11.551	3260	3269	3276	rBV4	5906	10138	0.69%	0.086%
92	11.612	3277	3288	3312	rVB	712659	1137920	76.97%	9.601%
93	12.030	3416	3418	3419	rBV	269	112	0.01%	0.001%
94	12.043	3420	3422	3427	rVB2	214	159	0.01%	0.001%
95	13.291	3807	3810	3812	rBV2	484	371	0.03%	0.003%




Sum of corrected areas: 11852567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029546.D
Acq On : 10 Dec 2022 01:09
Operator : SY/MD
Sample : N5915-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

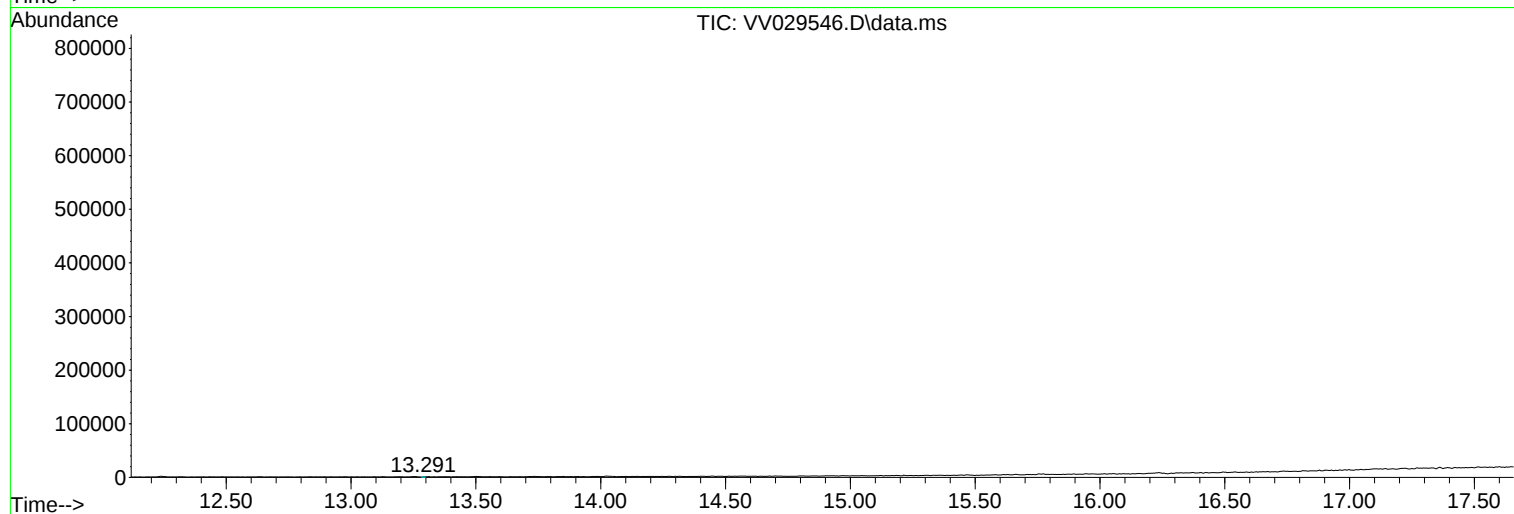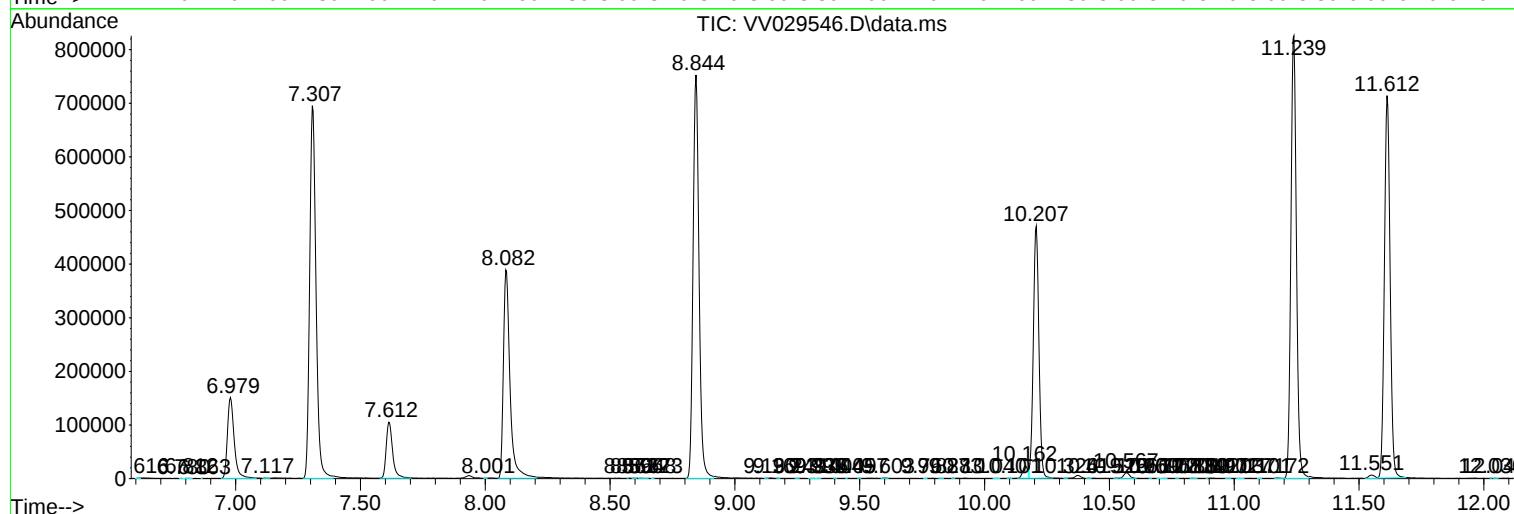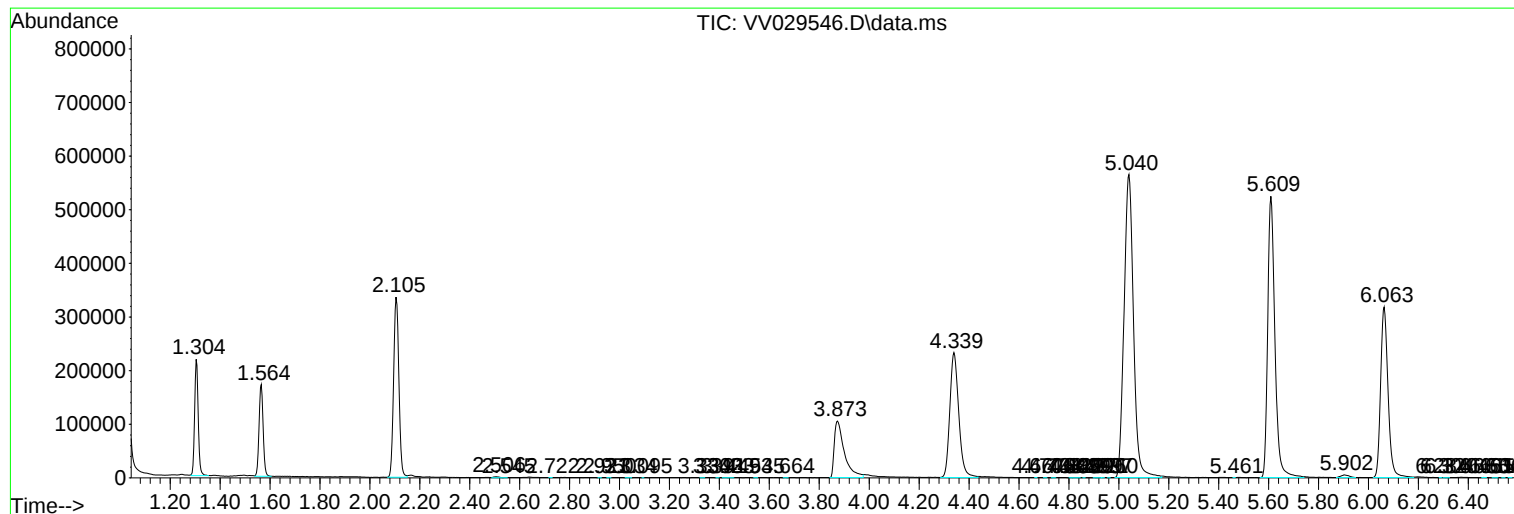

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029546.D
Acq On : 10 Dec 2022 01:09
Operator : SY/MD
Sample : N5915-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029546.D
Acq On : 10 Dec 2022 01:09
Operator : SY/MD
Sample : N5915-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------