

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029547.D
 Acq On : 10 Dec 2022 01:32
 Operator : SY/MD
 Sample : N5915-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	221983	221405	13.94%	1.739%
2	1.564	155	163	177	rVB	188993	209480	13.19%	1.645%
3	2.105	320	331	345	rBV	351806	505904	31.85%	3.973%
4	2.497	448	453	464	rVB5	1124	1998	0.13%	0.016%
5	2.542	464	467	473	rVB2	293	339	0.02%	0.003%
6	2.574	473	477	482	rBV2	161	171	0.01%	0.001%
7	2.850	561	563	567	rBV	325	171	0.01%	0.001%
8	2.928	584	587	589	rBV2	174	93	0.01%	0.001%
9	2.944	589	592	596	rBV2	267	167	0.01%	0.001%
10	2.960	596	597	603	rVB	190	138	0.01%	0.001%
11	3.040	618	622	625	rVB2	244	181	0.01%	0.001%
12	3.159	655	659	662	rBV	302	213	0.01%	0.002%
13	3.336	710	714	717	rBV2	198	195	0.01%	0.002%
14	3.413	734	738	739	rBV2	183	129	0.01%	0.001%
15	3.510	765	768	774	rBV2	271	219	0.01%	0.002%
16	3.539	774	777	781	rBV	264	205	0.01%	0.002%
17	3.577	786	789	791	rBV	166	118	0.01%	0.001%
18	3.622	801	803	807	rVB2	283	167	0.01%	0.001%
19	3.648	807	811	814	rBV2	133	122	0.01%	0.001%
20	3.831	865	868	871	rBV2	162	97	0.01%	0.001%
21	3.873	871	881	919	rBV	113285	322886	20.32%	2.536%
22	4.339	1010	1026	1053	rBV	247178	617217	38.85%	4.847%
23	4.577	1097	1100	1104	rBV3	432	306	0.02%	0.002%
24	4.664	1122	1127	1128	rBV2	350	250	0.02%	0.002%
25	4.699	1135	1138	1139	rBV	177	97	0.01%	0.001%
26	4.744	1147	1152	1157	rBV2	197	212	0.01%	0.002%
27	4.783	1162	1164	1169	rVV	129	75	0.00%	0.001%
28	4.873	1189	1192	1196	rBV2	124	132	0.01%	0.001%
29	4.928	1204	1209	1212	rBV2	180	157	0.01%	0.001%
30	4.944	1212	1214	1217	rVB3	159	91	0.01%	0.001%
31	4.960	1217	1219	1221	rBV	194	86	0.01%	0.001%
32	4.969	1221	1222	1225	rBV	140	77	0.00%	0.001%
33	5.040	1225	1244	1291	rBV2	595660	1588635	100.00%	12.476%
34	5.609	1407	1421	1461	rBV	554974	1131790	71.24%	8.888%
35	5.905	1502	1513	1523	rBV7	4759	10503	0.66%	0.082%
36	6.063	1548	1562	1596	rBV	343800	703144	44.26%	5.522%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029547.D
 Acq On : 10 Dec 2022 01:32
 Operator : SY/MD
 Sample : N5915-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.355	1651	1653	1655	rBV	177	75	0.00%	0.001%
38	6.394	1663	1665	1666	rBV	265	84	0.01%	0.001%
39	6.445	1679	1681	1683	rBV2	132	71	0.00%	0.001%
40	6.474	1687	1690	1692	rBV2	253	115	0.01%	0.001%
41	6.535	1707	1709	1712	rVB3	230	131	0.01%	0.001%
42	6.571	1716	1720	1724	rVB3	477	338	0.02%	0.003%
43	6.593	1724	1727	1728	rBV	183	81	0.01%	0.001%
44	6.632	1728	1739	1745	rBV3	1227	2247	0.14%	0.018%
45	6.809	1791	1794	1796	rVB2	287	155	0.01%	0.001%
46	6.821	1796	1798	1801	rBV2	364	301	0.02%	0.002%
47	6.882	1812	1817	1819	rBV	193	122	0.01%	0.001%
48	6.979	1834	1847	1873	rBV	160998	299616	18.86%	2.353%
49	7.227	1922	1924	1927	rBV3	439	290	0.02%	0.002%
50	7.307	1936	1949	1969	rBV	731679	1305330	82.17%	10.251%
51	7.616	2034	2045	2071	rBV	111922	202373	12.74%	1.589%
52	7.899	2130	2133	2136	rBV2	474	498	0.03%	0.004%
53	7.937	2136	2145	2152	rVV3	4227	7575	0.48%	0.059%
54	8.085	2181	2191	2228	rBV	431001	778138	48.98%	6.111%
55	8.561	2334	2339	2342	rBV3	490	420	0.03%	0.003%
56	8.580	2342	2345	2346	rBV	299	153	0.01%	0.001%
57	8.661	2367	2370	2373	rBV3	209	117	0.01%	0.001%
58	8.722	2386	2389	2391	rBV	296	157	0.01%	0.001%
59	8.754	2396	2399	2401	rBV	193	91	0.01%	0.001%
60	8.844	2414	2427	2449	rBV	823478	1331708	83.83%	10.458%
61	9.104	2505	2508	2509	rBV2	404	218	0.01%	0.002%
62	9.136	2510	2518	2530	rVB3	3130	4973	0.31%	0.039%
63	9.214	2540	2542	2545	rVB	197	77	0.00%	0.001%
64	9.233	2545	2548	2550	rBV	163	111	0.01%	0.001%
65	9.249	2550	2553	2556	rVB	367	167	0.01%	0.001%
66	9.271	2556	2560	2562	rBV2	385	331	0.02%	0.003%
67	9.310	2569	2572	2576	rBV	322	192	0.01%	0.002%
68	9.439	2609	2612	2616	rVB2	303	204	0.01%	0.002%
69	9.480	2623	2625	2633	rVB2	298	265	0.02%	0.002%
70	9.513	2633	2635	2636	rBV	155	81	0.01%	0.001%
71	9.545	2636	2645	2653	rBV6	1471	2934	0.18%	0.023%
72	9.648	2673	2677	2683	rBV2	121	128	0.01%	0.001%
73	9.673	2683	2685	2687	rBV	232	130	0.01%	0.001%
74	9.799	2722	2724	2726	rBV	163	82	0.01%	0.001%
75	9.921	2758	2762	2763	rBV2	620	481	0.03%	0.004%
76	9.985	2780	2782	2784	rBV	232	131	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029547.D
 Acq On : 10 Dec 2022 01:32
 Operator : SY/MD
 Sample : N5915-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.998	2784	2786	2788	rVV3	165	79	0.00%	0.001%
78	10.062	2804	2806	2808	rBV	234	137	0.01%	0.001%
79	10.165	2826	2838	2841	rBV2	24344	35907	2.26%	0.282%
80	10.207	2842	2851	2873	rVB	500427	786704	49.52%	6.178%
81	10.342	2888	2893	2894	rBV2	385	273	0.02%	0.002%
82	10.374	2896	2903	2913	rVB3	5710	9115	0.57%	0.072%
83	10.416	2913	2916	2918	rBV2	154	93	0.01%	0.001%
84	10.468	2930	2932	2936	rVB2	298	185	0.01%	0.001%
85	10.567	2956	2963	2975	rVB2	11728	17981	1.13%	0.141%
86	10.680	2993	2998	3003	rVB3	267	296	0.02%	0.002%
87	10.702	3003	3005	3006	rBV3	288	107	0.01%	0.001%
88	10.734	3010	3015	3018	rBV3	318	315	0.02%	0.002%
89	10.847	3048	3050	3054	rBV2	405	262	0.02%	0.002%
90	10.908	3062	3069	3074	rBV2	1636	2342	0.15%	0.018%
91	10.988	3091	3094	3095	rBV	189	99	0.01%	0.001%
92	11.056	3112	3115	3116	rBV	238	146	0.01%	0.001%
93	11.085	3122	3124	3126	rBV	183	96	0.01%	0.001%
94	11.136	3137	3140	3142	rBV2	284	203	0.01%	0.002%
95	11.239	3160	3172	3196	rBV	883490	1382730	87.04%	10.859%
96	11.445	3233	3236	3239	rBV2	418	301	0.02%	0.002%
97	11.551	3263	3269	3276	rBV6	2544	4308	0.27%	0.034%
98	11.612	3276	3288	3308	rBV	782473	1233722	77.66%	9.689%
99	11.847	3359	3361	3362	rBV	183	77	0.00%	0.001%
100	12.860	3675	3676	3681	rVB3	507	297	0.02%	0.002%




Sum of corrected areas: 12733636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029547.D
Acq On : 10 Dec 2022 01:32
Operator : SY/MD
Sample : N5915-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

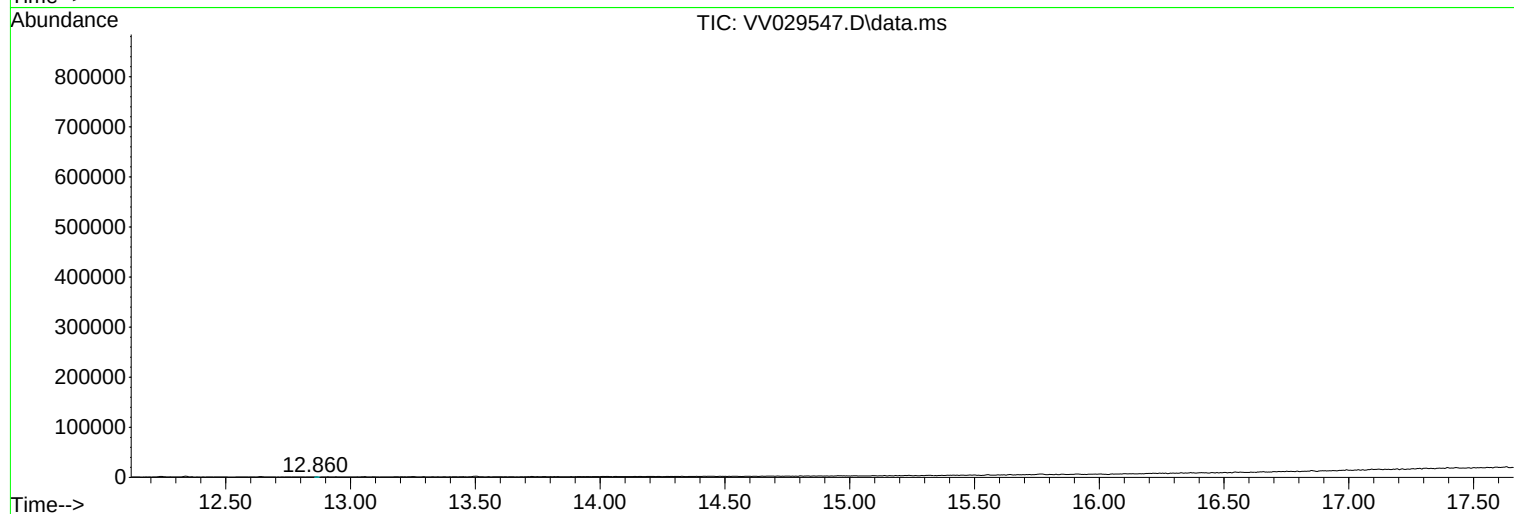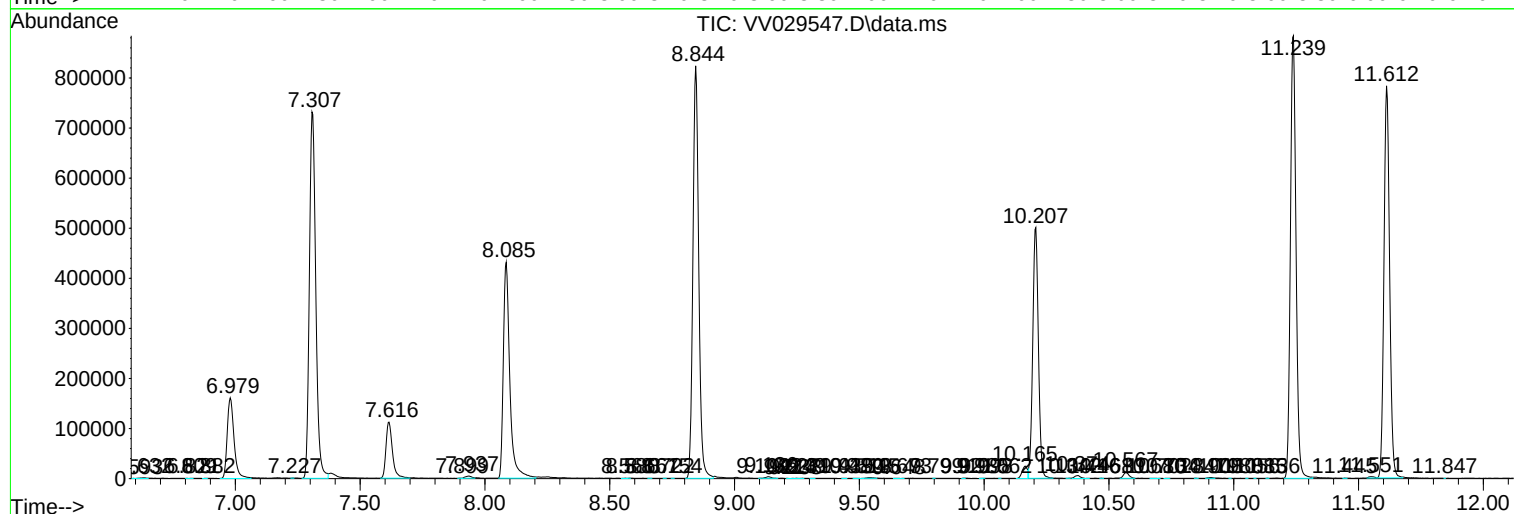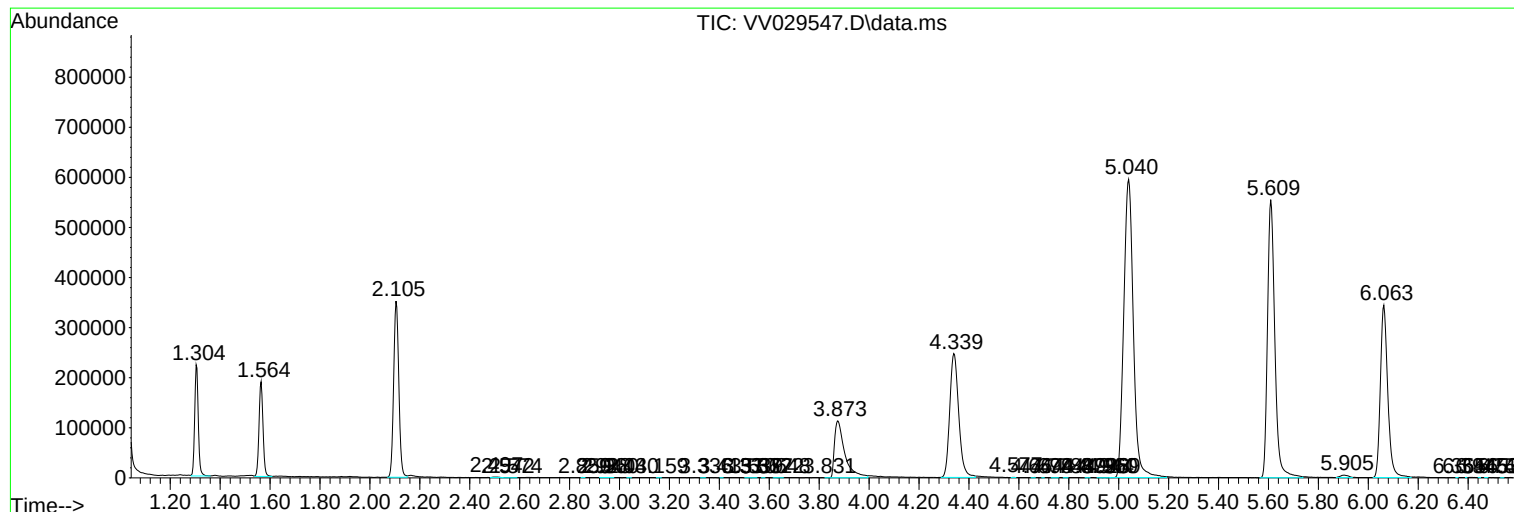

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029547.D
Acq On : 10 Dec 2022 01:32
Operator : SY/MD
Sample : N5915-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029547.D
Acq On : 10 Dec 2022 01:32
Operator : SY/MD
Sample : N5915-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc