

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029548.D
 Acq On : 10 Dec 2022 01:56
 Operator : SY/MD
 Sample : N5915-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	214823	211646	13.72%	1.695%
2	1.564	155	163	173	rVB	180693	200966	13.02%	1.610%
3	2.105	320	331	345	rBV	345372	497921	32.27%	3.989%
4	2.339	402	404	407	rBV2	347	170	0.01%	0.001%
5	2.481	445	448	449	rBV	165	74	0.00%	0.001%
6	2.503	449	455	464	rVV4	1208	1795	0.12%	0.014%
7	2.629	491	494	496	rBV	381	224	0.01%	0.002%
8	2.677	506	509	510	rBV	224	141	0.01%	0.001%
9	2.741	528	529	531	rBV2	139	40	0.00%	0.000%
10	2.764	533	536	542	rBV2	321	333	0.02%	0.003%
11	2.995	606	608	610	rBV2	207	95	0.01%	0.001%
12	3.159	656	659	662	rBV2	328	166	0.01%	0.001%
13	3.195	667	670	672	rBV2	216	113	0.01%	0.001%
14	3.249	686	687	688	rVB	229	44	0.00%	0.000%
15	3.262	689	691	693	rVV	163	73	0.00%	0.001%
16	3.294	697	701	703	rBV2	275	174	0.01%	0.001%
17	3.568	784	786	788	rBV	175	72	0.00%	0.001%
18	3.674	817	819	821	rBV	156	59	0.00%	0.000%
19	3.703	825	828	829	rBV	152	70	0.00%	0.001%
20	3.831	865	868	872	rBV	164	140	0.01%	0.001%
21	3.873	872	881	916	rBV	110526	313480	20.32%	2.511%
22	4.339	1009	1026	1062	rBV	240108	606298	39.29%	4.857%
23	4.603	1105	1108	1114	rVB3	427	329	0.02%	0.003%
24	4.687	1132	1134	1137	rVB2	192	112	0.01%	0.001%
25	4.706	1138	1140	1142	rBV	191	73	0.00%	0.001%
26	4.751	1152	1154	1156	rBV	161	81	0.01%	0.001%
27	4.802	1164	1170	1173	rBV2	260	270	0.02%	0.002%
28	4.822	1173	1176	1177	rBV	208	88	0.01%	0.001%
29	4.876	1190	1193	1195	rBV	244	129	0.01%	0.001%
30	4.908	1200	1203	1204	rBV	157	79	0.01%	0.001%
31	5.040	1226	1244	1299	rBV2	585899	1543090	100.00%	12.361%
32	5.413	1358	1360	1364	rBV2	247	148	0.01%	0.001%
33	5.471	1374	1378	1379	rBV	430	304	0.02%	0.002%
34	5.513	1389	1391	1395	rVB2	173	93	0.01%	0.001%
35	5.532	1395	1397	1398	rBV2	140	74	0.00%	0.001%
36	5.609	1408	1421	1459	rBV	554584	1134929	73.55%	9.091%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029548.D
 Acq On : 10 Dec 2022 01:56
 Operator : SY/MD
 Sample : N5915-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.905	1502	1513	1526	rVV9	4912	10418	0.68%	0.083%
38	5.953	1526	1528	1530	rVB	229	69	0.00%	0.001%
39	5.995	1539	1541	1542	rBV2	256	105	0.01%	0.001%
40	6.063	1548	1562	1599	rBV	327463	682578	44.23%	5.468%
41	6.330	1644	1645	1647	rVB	143	31	0.00%	0.000%
42	6.484	1691	1693	1695	rVB2	202	83	0.01%	0.001%
43	6.526	1702	1706	1710	rBV3	423	353	0.02%	0.003%
44	6.574	1717	1721	1724	rBV3	219	166	0.01%	0.001%
45	6.619	1730	1735	1736	rBV3	847	719	0.05%	0.006%
46	6.677	1750	1753	1759	rVB4	493	292	0.02%	0.002%
47	6.728	1766	1769	1775	rVB2	264	214	0.01%	0.002%
48	6.751	1775	1776	1778	rBV	283	107	0.01%	0.001%
49	6.764	1778	1780	1782	rBV	241	83	0.01%	0.001%
50	6.805	1790	1793	1795	rBV	162	125	0.01%	0.001%
51	6.979	1834	1847	1869	rBV	155957	288358	18.69%	2.310%
52	7.137	1893	1896	1898	rBV2	600	375	0.02%	0.003%
53	7.307	1936	1949	1969	rBV	715889	1263646	81.89%	10.122%
54	7.612	2034	2044	2064	rBV	109488	194301	12.59%	1.556%
55	7.796	2099	2101	2102	rBV	319	157	0.01%	0.001%
56	8.085	2180	2191	2228	rBV	413112	760338	49.27%	6.091%
57	8.374	2278	2281	2283	rBV3	629	397	0.03%	0.003%
58	8.558	2336	2338	2341	rBV	199	113	0.01%	0.001%
59	8.654	2365	2368	2371	rVB2	258	145	0.01%	0.001%
60	8.680	2371	2376	2377	rBV3	409	283	0.02%	0.002%
61	8.709	2382	2385	2387	rBV	349	249	0.02%	0.002%
62	8.735	2391	2393	2396	rVB2	288	159	0.01%	0.001%
63	8.783	2405	2408	2414	rBV2	331	257	0.02%	0.002%
64	8.844	2414	2427	2457	rBV	809900	1341786	86.95%	10.748%
65	9.136	2510	2518	2526	rBV3	2678	4101	0.27%	0.033%
66	9.194	2531	2536	2537	rBV2	237	180	0.01%	0.001%
67	9.358	2582	2587	2590	rVB3	303	286	0.02%	0.002%
68	9.407	2601	2602	2605	rBV2	187	77	0.00%	0.001%
69	9.442	2610	2613	2616	rBV2	192	99	0.01%	0.001%
70	9.468	2617	2621	2624	rBV3	285	187	0.01%	0.001%
71	9.538	2636	2643	2646	rBV5	1449	1801	0.12%	0.014%
72	9.600	2659	2662	2663	rBV5	259	106	0.01%	0.001%
73	9.664	2679	2682	2684	rBV3	196	103	0.01%	0.001%
74	9.677	2684	2686	2688	rVB	256	117	0.01%	0.001%
75	9.693	2688	2691	2693	rVB2	135	76	0.00%	0.001%
76	9.718	2693	2699	2702	rBV3	532	717	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029548.D
 Acq On : 10 Dec 2022 01:56
 Operator : SY/MD
 Sample : N5915-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.847	2737	2739	2740	rBV	148	71	0.00%	0.001%
78	9.886	2750	2751	2754	rBV	150	59	0.00%	0.000%
79	9.960	2771	2774	2778	rVB	253	191	0.01%	0.002%
80	9.985	2778	2782	2786	rBV3	304	273	0.02%	0.002%
81	10.024	2789	2794	2795	rBV	381	327	0.02%	0.003%
82	10.162	2826	2837	2841	rBV	22917	34496	2.24%	0.276%
83	10.207	2842	2851	2866	rVB	485670	758048	49.13%	6.072%
84	10.371	2896	2902	2915	rVB2	4831	8009	0.52%	0.064%
85	10.439	2917	2923	2926	rBV3	466	574	0.04%	0.005%
86	10.526	2947	2950	2952	rBV	520	394	0.03%	0.003%
87	10.567	2955	2963	2977	rVB	11272	18887	1.22%	0.151%
88	10.728	3010	3013	3018	rBV3	431	359	0.02%	0.003%
89	10.763	3021	3024	3030	rBV2	329	385	0.02%	0.003%
90	11.040	3108	3110	3112	rBV2	199	99	0.01%	0.001%
91	11.169	3147	3150	3159	rVB4	1021	1094	0.07%	0.009%
92	11.236	3159	3171	3204	rBV	896733	1401437	90.82%	11.226%
93	11.516	3254	3258	3260	rBV2	568	452	0.03%	0.004%
94	11.551	3262	3269	3276	rVV6	3385	5835	0.38%	0.047%
95	11.612	3276	3288	3307	rVV	769373	1181071	76.54%	9.461%
96	12.001	3406	3409	3413	rBV2	356	410	0.03%	0.003%
97	12.339	3506	3514	3520	rBV5	2128	2753	0.18%	0.022%
98	12.789	3650	3654	3656	rBV	474	365	0.02%	0.003%
99	13.484	3867	3870	3872	rBV3	790	602	0.04%	0.005%




Sum of corrected areas: 12483841

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029548.D
Acq On : 10 Dec 2022 01:56
Operator : SY/MD
Sample : N5915-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

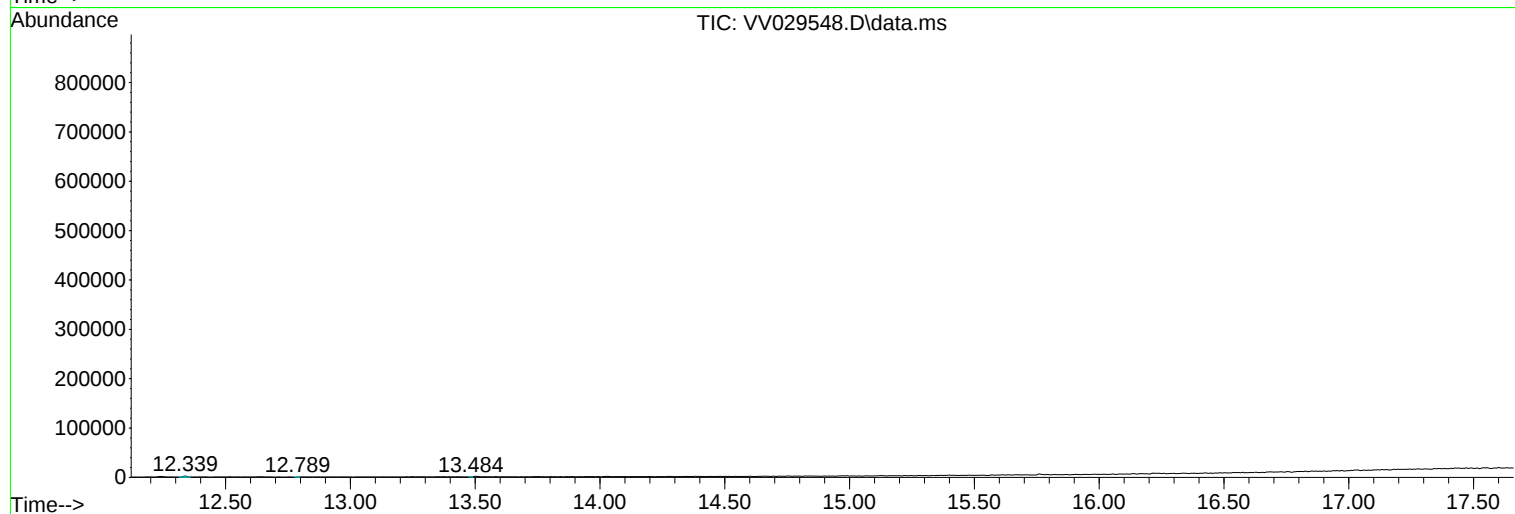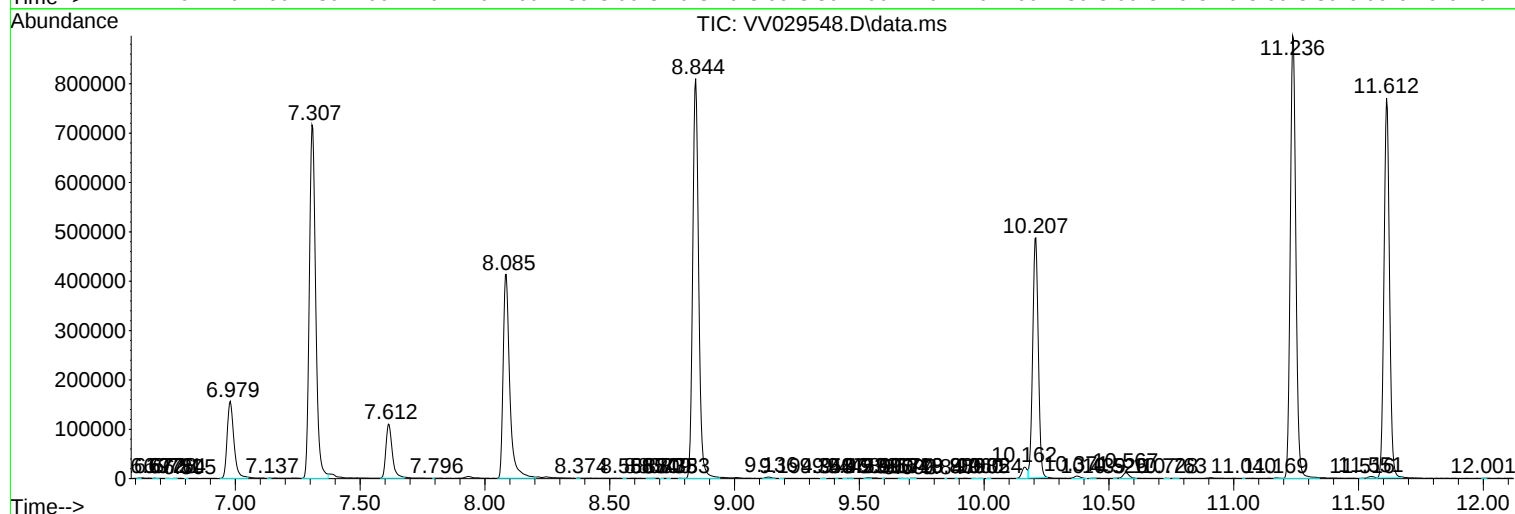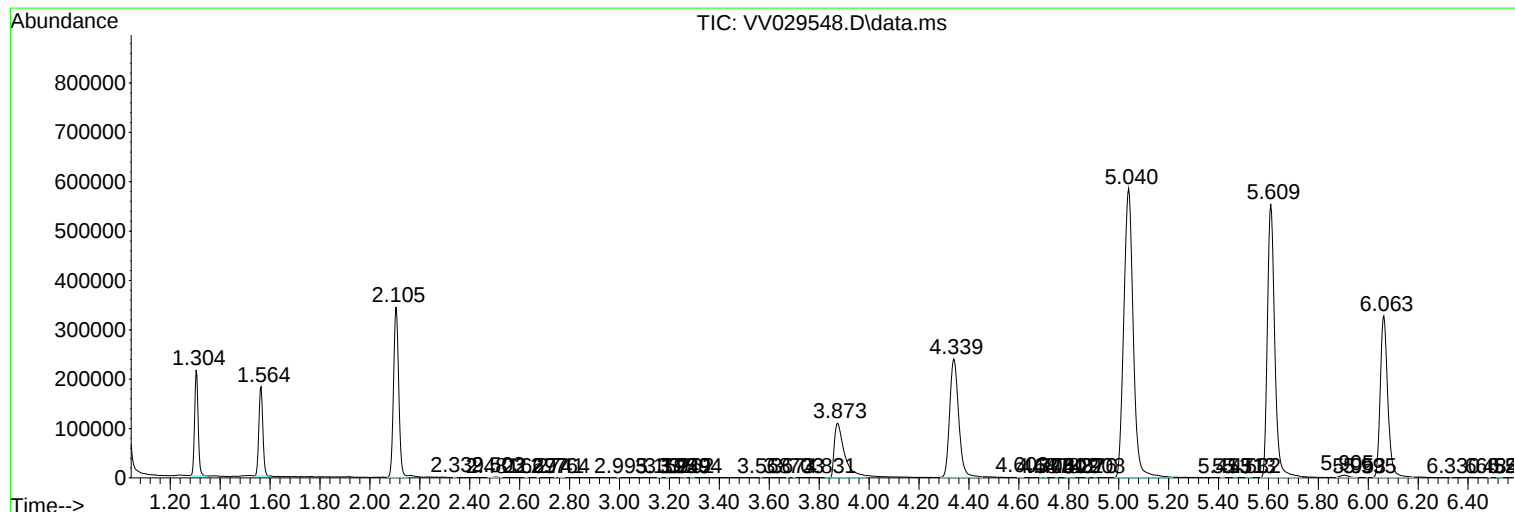

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029548.D
Acq On : 10 Dec 2022 01:56
Operator : SY/MD
Sample : N5915-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029548.D
Acq On : 10 Dec 2022 01:56
Operator : SY/MD
Sample : N5915-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc