

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029549.D
 Acq On : 10 Dec 2022 02:19
 Operator : SY/MD
 Sample : N5915-02DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	213183	216421	15.13%	1.740%
2	1.561	155	162	177	rVB	173791	193632	13.54%	1.557%
3	2.111	320	333	361	rBV3	659674	1121922	78.46%	9.022%
4	2.359	408	410	414	rBV2	301	249	0.02%	0.002%
5	2.503	446	455	465	rBV	4458	7056	0.49%	0.057%
6	2.825	548	555	558	rBV2	303	341	0.02%	0.003%
7	2.880	570	572	574	rVB	189	79	0.01%	0.001%
8	3.018	612	615	617	rBV	305	156	0.01%	0.001%
9	3.056	624	627	631	rBV2	154	127	0.01%	0.001%
10	3.076	631	633	636	rVB	259	97	0.01%	0.001%
11	3.095	636	639	641	rBV2	153	94	0.01%	0.001%
12	3.105	641	642	643	rVB	180	35	0.00%	0.000%
13	3.140	650	653	655	rBV2	214	125	0.01%	0.001%
14	3.188	661	668	679	rVB2	1311	2630	0.18%	0.021%
15	3.288	696	699	702	rBV	115	74	0.01%	0.001%
16	3.330	708	712	713	rBV	270	143	0.01%	0.001%
17	3.368	722	724	729	rVB2	283	165	0.01%	0.001%
18	3.548	775	780	782	rBV	256	216	0.02%	0.002%
19	3.642	806	809	815	rVB	353	252	0.02%	0.002%
20	3.722	831	834	836	rBV	144	96	0.01%	0.001%
21	3.793	852	856	859	rBV	136	129	0.01%	0.001%
22	3.873	869	881	920	rBV2	111662	342310	23.94%	2.753%
23	4.339	1010	1026	1051	rBV	219103	548358	38.35%	4.410%
24	4.642	1117	1120	1122	rBV2	287	146	0.01%	0.001%
25	4.715	1140	1143	1145	rBV2	153	99	0.01%	0.001%
26	4.770	1157	1160	1165	rVB2	279	219	0.02%	0.002%
27	4.796	1166	1168	1171	rVB	141	81	0.01%	0.001%
28	4.815	1171	1174	1176	rBV2	110	74	0.01%	0.001%
29	4.863	1184	1189	1193	rBV	182	181	0.01%	0.001%
30	4.905	1200	1202	1206	rVB	150	102	0.01%	0.001%
31	4.931	1206	1210	1211	rBV	230	125	0.01%	0.001%
32	4.970	1220	1222	1223	rBV	149	55	0.00%	0.000%
33	5.040	1226	1244	1276	rBV2	542331	1430005	100.00%	11.499%
34	5.304	1323	1326	1329	rBV3	281	211	0.01%	0.002%
35	5.465	1374	1376	1378	rBV	307	186	0.01%	0.001%
36	5.539	1397	1399	1402	rBV2	256	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029549.D
 Acq On : 10 Dec 2022 02:19
 Operator : SY/MD
 Sample : N5915-02DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1404	1421	1465	rBV	521532	1078242	75.40%	8.670%
38	5.902	1503	1512	1528	rVB8	4673	10423	0.73%	0.084%
39	5.963	1528	1531	1533	rBV2	199	144	0.01%	0.001%
40	6.063	1548	1562	1599	rBV	305146	633705	44.31%	5.096%
41	6.310	1638	1639	1640	rBV	98	30	0.00%	0.000%
42	6.342	1646	1649	1651	rBV2	154	107	0.01%	0.001%
43	6.413	1666	1671	1676	rBV2	216	221	0.02%	0.002%
44	6.458	1681	1685	1688	rBV2	171	152	0.01%	0.001%
45	6.529	1705	1707	1709	rBV	165	78	0.01%	0.001%
46	6.590	1722	1726	1730	rBV2	212	212	0.01%	0.002%
47	6.625	1731	1737	1742	rBV4	716	1004	0.07%	0.008%
48	6.722	1765	1767	1770	rVB	143	62	0.00%	0.000%
49	6.793	1787	1789	1793	rVB2	208	122	0.01%	0.001%
50	6.815	1794	1796	1800	rVB3	198	129	0.01%	0.001%
51	6.838	1800	1803	1805	rVB	255	145	0.01%	0.001%
52	6.870	1805	1813	1815	rBV3	275	314	0.02%	0.003%
53	6.924	1828	1830	1832	rBV2	177	80	0.01%	0.001%
54	6.979	1835	1847	1872	rBV	146603	270276	18.90%	2.173%
55	7.307	1936	1949	1982	rBV	672711	1192442	83.39%	9.589%
56	7.612	2034	2044	2071	rBV	101747	182423	12.76%	1.467%
57	7.841	2111	2115	2117	rBV2	327	235	0.02%	0.002%
58	8.082	2180	2190	2222	rBV	383177	695794	48.66%	5.595%
59	8.436	2297	2300	2303	rBV2	352	259	0.02%	0.002%
60	8.580	2342	2345	2348	rBV2	377	213	0.01%	0.002%
61	8.677	2373	2375	2377	rBV2	208	137	0.01%	0.001%
62	8.776	2403	2406	2409	rBV2	269	162	0.01%	0.001%
63	8.844	2415	2427	2453	rBV	777347	1270809	88.87%	10.219%
64	9.130	2513	2516	2517	rBV2	499	286	0.02%	0.002%
65	9.188	2531	2534	2539	rBV3	383	380	0.03%	0.003%
66	9.233	2546	2548	2550	rBV	180	113	0.01%	0.001%
67	9.294	2561	2567	2572	rBV3	307	376	0.03%	0.003%
68	9.323	2573	2576	2579	rVV3	225	156	0.01%	0.001%
69	9.342	2579	2582	2584	rVB2	299	158	0.01%	0.001%
70	9.381	2591	2594	2598	rBV2	165	152	0.01%	0.001%
71	9.400	2598	2600	2602	rVV	180	96	0.01%	0.001%
72	9.484	2623	2626	2628	rBV	158	83	0.01%	0.001%
73	9.500	2628	2631	2634	rVB2	255	128	0.01%	0.001%
74	9.522	2635	2638	2639	rBV	255	133	0.01%	0.001%
75	9.571	2651	2653	2656	rBV2	146	72	0.01%	0.001%
76	9.612	2665	2666	2668	rVB	128	26	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029549.D
 Acq On : 10 Dec 2022 02:19
 Operator : SY/MD
 Sample : N5915-02DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.635	2671	2673	2676	rVV	174	99	0.01%	0.001%
78	9.680	2684	2687	2689	rBV2	171	92	0.01%	0.001%
79	9.735	2699	2704	2706	rBV2	426	298	0.02%	0.002%
80	9.831	2731	2734	2737	rBV	282	208	0.01%	0.002%
81	9.854	2740	2741	2744	rVB	298	127	0.01%	0.001%
82	9.873	2745	2747	2749	rBV2	166	75	0.01%	0.001%
83	10.040	2796	2799	2803	rVB2	352	215	0.02%	0.002%
84	10.162	2826	2837	2841	rBV	22377	33240	2.32%	0.267%
85	10.204	2842	2850	2869	rVB	457213	718952	50.28%	5.781%
86	10.371	2899	2902	2907	rVB3	955	888	0.06%	0.007%
87	10.452	2925	2927	2930	rBV	219	153	0.01%	0.001%
88	10.516	2944	2947	2948	rBV	279	150	0.01%	0.001%
89	10.567	2955	2963	2975	rVB3	10598	17324	1.21%	0.139%
90	10.635	2982	2984	2985	rBV	176	72	0.01%	0.001%
91	10.718	3003	3010	3012	rBV3	293	338	0.02%	0.003%
92	10.751	3018	3020	3021	rBV	142	54	0.00%	0.000%
93	10.847	3048	3050	3053	rVB2	417	144	0.01%	0.001%
94	11.069	3115	3119	3121	rBV2	297	265	0.02%	0.002%
95	11.117	3131	3134	3136	rBV2	219	166	0.01%	0.001%
96	11.156	3141	3146	3147	rBV	438	307	0.02%	0.002%
97	11.236	3159	3171	3210	rBV	859163	1337391	93.52%	10.754%
98	11.612	3275	3288	3310	rBV	710110	1118491	78.22%	8.994%
99	13.448	3857	3859	3863	rBV3	559	364	0.03%	0.003%




Sum of corrected areas: 12435803

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029549.D
Acq On : 10 Dec 2022 02:19
Operator : SY/MD
Sample : N5915-02DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

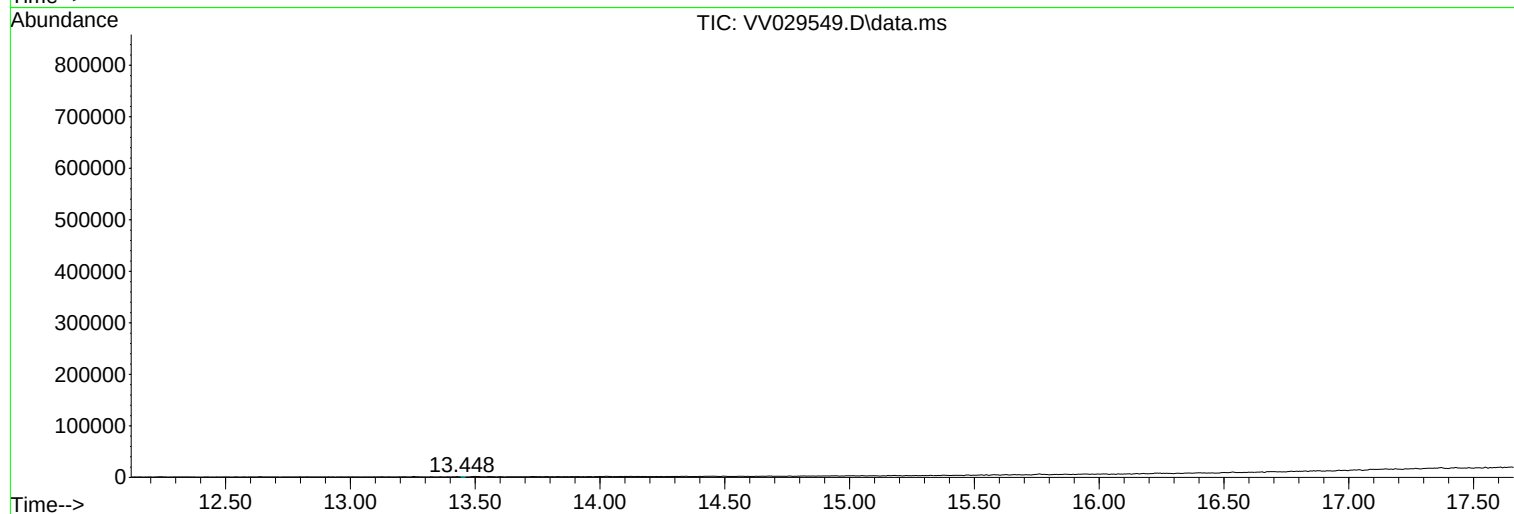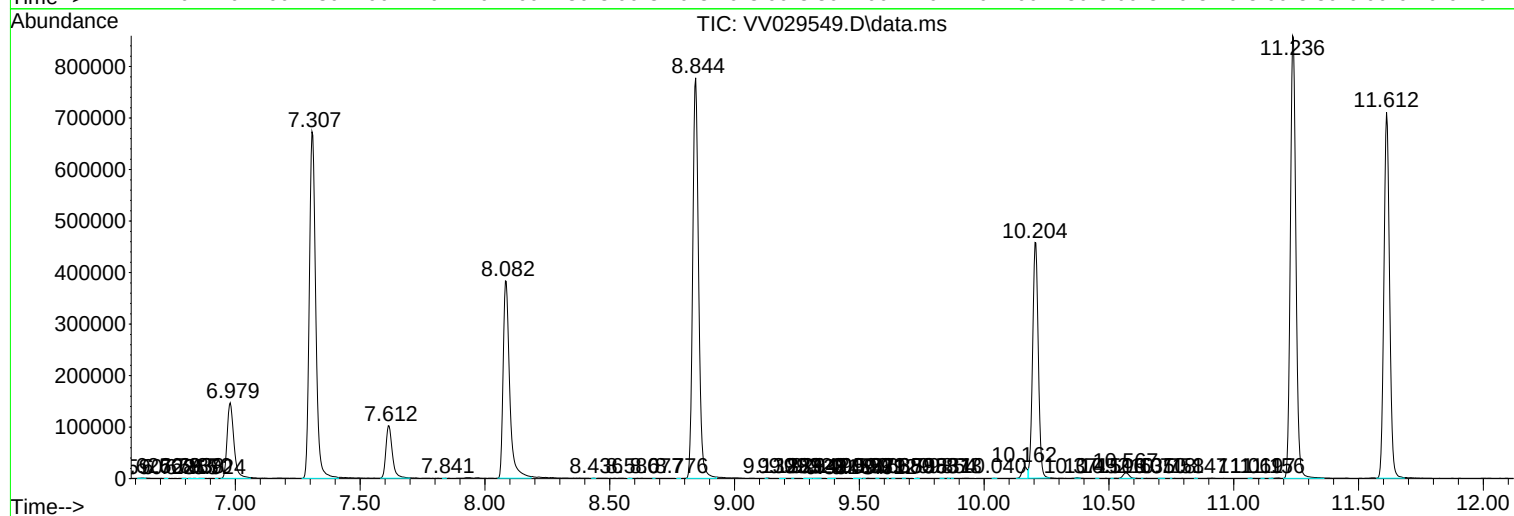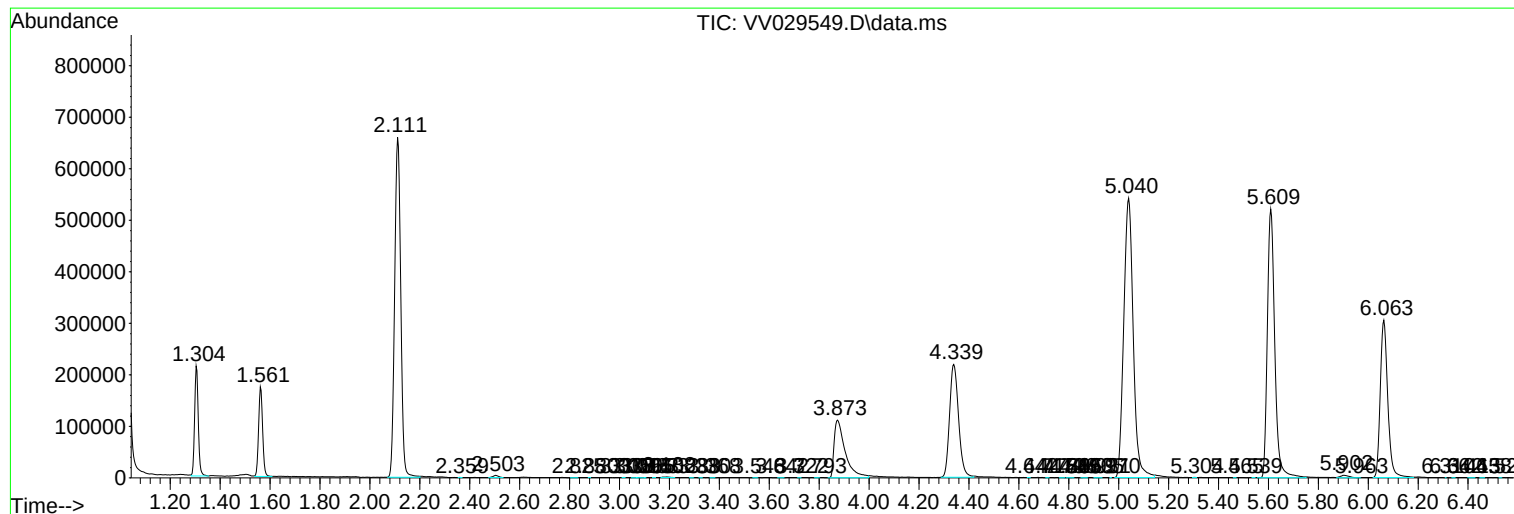

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029549.D
Acq On : 10 Dec 2022 02:19
Operator : SY/MD
Sample : N5915-02DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029549.D
Acq On : 10 Dec 2022 02:19
Operator : SY/MD
Sample : N5915-02DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------