

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029550.D
 Acq On : 10 Dec 2022 02:43
 Operator : SY/MD
 Sample : N5915-10DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N09DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	211006	211927	10.40%	1.563%
2	1.564	156	163	178	rVB	178431	197609	9.70%	1.458%
3	2.105	321	331	350	rBV	337192	488915	24.00%	3.606%
4	2.407	422	425	428	rBV2	319	205	0.01%	0.002%
5	2.452	436	439	442	rBV2	394	267	0.01%	0.002%
6	2.503	447	455	466	rVV3	3368	5232	0.26%	0.039%
7	2.760	529	535	541	rVB4	755	1104	0.05%	0.008%
8	2.960	594	597	603	rBV2	254	161	0.01%	0.001%
9	3.082	632	635	637	rBV	143	99	0.00%	0.001%
10	3.400	732	734	737	rBV	191	128	0.01%	0.001%
11	3.561	781	784	788	rBV	91	96	0.00%	0.001%
12	3.831	865	868	869	rBV	227	123	0.01%	0.001%
13	3.873	871	881	918	rBV2	120128	367898	18.06%	2.714%
14	4.339	1009	1026	1059	rBV	233041	579867	28.47%	4.277%
15	4.564	1093	1096	1098	rBV2	279	211	0.01%	0.002%
16	4.612	1108	1111	1114	rBV3	411	268	0.01%	0.002%
17	4.658	1123	1125	1127	rBV	184	64	0.00%	0.000%
18	4.709	1139	1141	1143	rBV	105	67	0.00%	0.000%
19	4.725	1143	1146	1152	rVV2	293	236	0.01%	0.002%
20	4.751	1152	1154	1156	rVB	160	66	0.00%	0.000%
21	4.793	1164	1167	1172	rVB2	265	215	0.01%	0.002%
22	4.847	1182	1184	1187	rBV	174	76	0.00%	0.001%
23	4.863	1187	1189	1191	rVB	232	74	0.00%	0.001%
24	4.892	1195	1198	1202	rVB2	210	115	0.01%	0.001%
25	4.953	1214	1217	1221	rBV	196	148	0.01%	0.001%
26	5.040	1226	1244	1299	rBV2	571422	1518474	74.54%	11.201%
27	5.355	1340	1342	1345	rBV2	196	123	0.01%	0.001%
28	5.471	1374	1378	1383	rVB3	427	410	0.02%	0.003%
29	5.539	1397	1399	1401	rBV	129	64	0.00%	0.000%
30	5.551	1402	1403	1404	rBV	139	44	0.00%	0.000%
31	5.609	1408	1421	1464	rBV	543790	1112693	54.62%	8.208%
32	5.902	1503	1512	1526	rVB7	4617	9646	0.47%	0.071%
33	6.063	1548	1562	1598	rBV	324200	669613	32.87%	4.939%
34	6.291	1632	1633	1634	rVB	160	31	0.00%	0.000%
35	6.374	1657	1659	1663	rBV	318	198	0.01%	0.001%
36	6.420	1671	1673	1674	rBV	199	74	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029550.D
 Acq On : 10 Dec 2022 02:43
 Operator : SY/MD
 Sample : N5915-10DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N09DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.452	1681	1683	1686	rVB2	174	69	0.00%	0.001%
38	6.516	1700	1703	1705	rBV	197	133	0.01%	0.001%
39	6.555	1711	1715	1716	rBV2	143	73	0.00%	0.001%
40	6.580	1721	1723	1725	rBV	210	87	0.00%	0.001%
41	6.741	1772	1773	1776	rVB	151	49	0.00%	0.000%
42	6.760	1777	1779	1780	rBV2	261	89	0.00%	0.001%
43	6.799	1789	1791	1793	rBV	234	122	0.01%	0.001%
44	6.883	1813	1817	1818	rBV	178	93	0.00%	0.001%
45	6.905	1822	1824	1828	rBV2	185	151	0.01%	0.001%
46	6.928	1828	1831	1832	rBV	177	83	0.00%	0.001%
47	6.979	1836	1847	1877	rVV	151184	279525	13.72%	2.062%
48	7.149	1897	1900	1902	rBV3	552	368	0.02%	0.003%
49	7.307	1937	1949	1978	rBV	701519	1244193	61.08%	9.178%
50	7.612	2034	2044	2071	rBV	108794	191465	9.40%	1.412%
51	7.966	2152	2154	2157	rBV4	757	489	0.02%	0.004%
52	8.085	2180	2191	2229	rBV	408074	750976	36.87%	5.539%
53	8.699	2381	2382	2386	rVB2	318	176	0.01%	0.001%
54	8.844	2414	2427	2430	rBV	860962	1219137	59.85%	8.993%
55	9.265	2555	2558	2562	rBV2	369	283	0.01%	0.002%
56	9.416	2603	2605	2609	rBV2	396	235	0.01%	0.002%
57	9.439	2609	2612	2613	rVV	183	75	0.00%	0.001%
58	9.452	2614	2616	2618	rBV	187	85	0.00%	0.001%
59	9.603	2661	2663	2665	rBV	231	95	0.00%	0.001%
60	9.751	2706	2709	2710	rBV	197	110	0.01%	0.001%
61	9.837	2735	2736	2739	rBV2	260	113	0.01%	0.001%
62	9.992	2778	2784	2787	rBV2	458	510	0.03%	0.004%
63	10.040	2796	2799	2803	rBV3	313	284	0.01%	0.002%
64	10.162	2827	2837	2841	rBV	21731	31091	1.53%	0.229%
65	10.207	2842	2851	2869	rVB	477006	749517	36.79%	5.529%
66	10.345	2892	2894	2900	rBV2	677	643	0.03%	0.005%
67	10.413	2912	2915	2917	rBV	214	165	0.01%	0.001%
68	10.461	2928	2930	2932	rBV2	144	80	0.00%	0.001%
69	10.567	2954	2963	2973	rVB2	9783	15784	0.77%	0.116%
70	10.654	2988	2990	2992	rBV2	162	57	0.00%	0.000%
71	10.683	2995	2999	3002	rBV2	328	279	0.01%	0.002%
72	10.789	3029	3032	3035	rBV2	301	192	0.01%	0.001%
73	10.847	3048	3050	3053	rBV	425	232	0.01%	0.002%
74	11.037	3107	3109	3110	rBV	379	139	0.01%	0.001%
75	11.082	3120	3123	3127	rVB2	443	417	0.02%	0.003%
76	11.140	3138	3141	3142	rBV2	256	128	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029550.D
 Acq On : 10 Dec 2022 02:43
 Operator : SY/MD
 Sample : N5915-10DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N09DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

77	11.172	3142	3151	3160	rBV3	14116	21082	1.03%	0.156%
78	11.239	3160	3172	3197	rBV2	921976	1833781	90.02%	13.527%
79	11.516	3252	3258	3268	rVB4	3791	5663	0.28%	0.042%
80	11.615	3276	3289	3323	rBV2	873959	2037083	100.00%	15.026%
81	11.815	3348	3351	3356	rBV	447	456	0.02%	0.003%
82	12.008	3404	3411	3418	rBV4	1793	2688	0.13%	0.020%
83	12.136	3449	3451	3458	rVB3	256	182	0.01%	0.001%
84	12.400	3528	3533	3541	rBV3	1154	1644	0.08%	0.012%




Sum of corrected areas: 13556912

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029550.D
Acq On : 10 Dec 2022 02:43
Operator : SY/MD
Sample : N5915-10DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N09DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

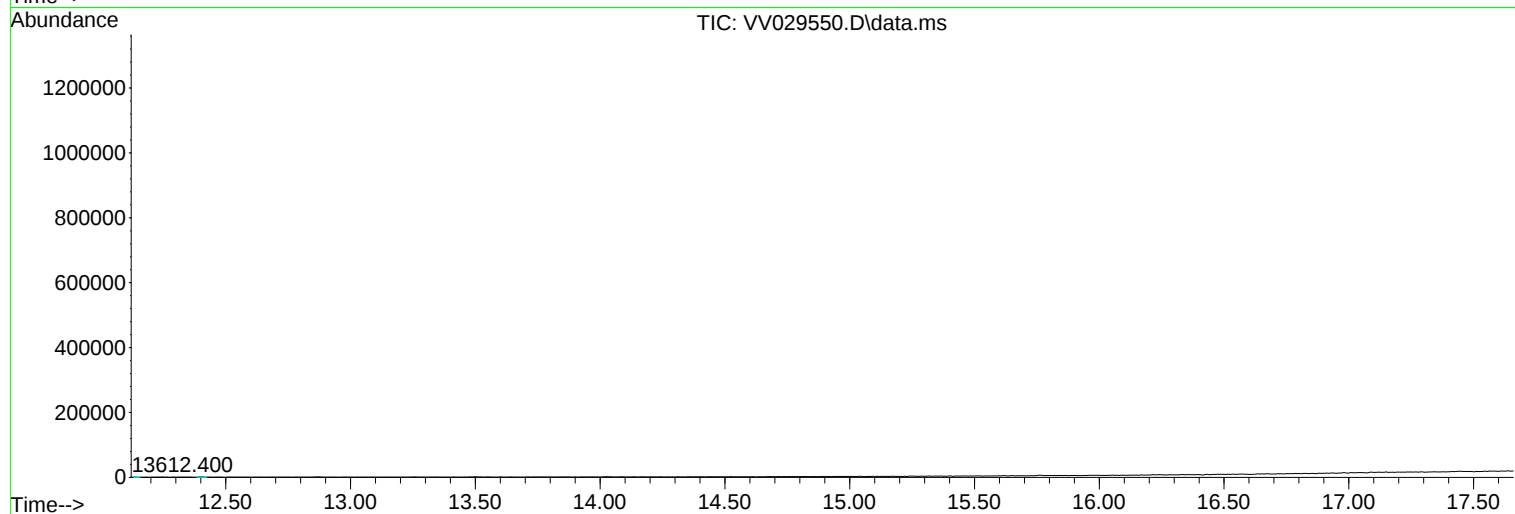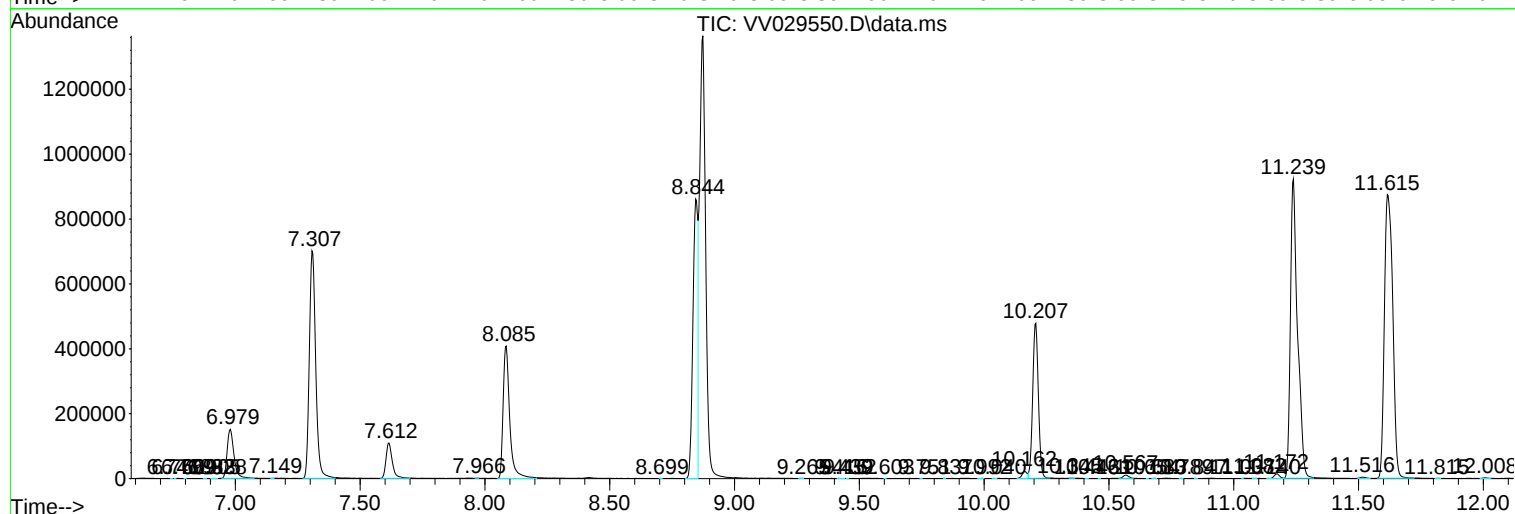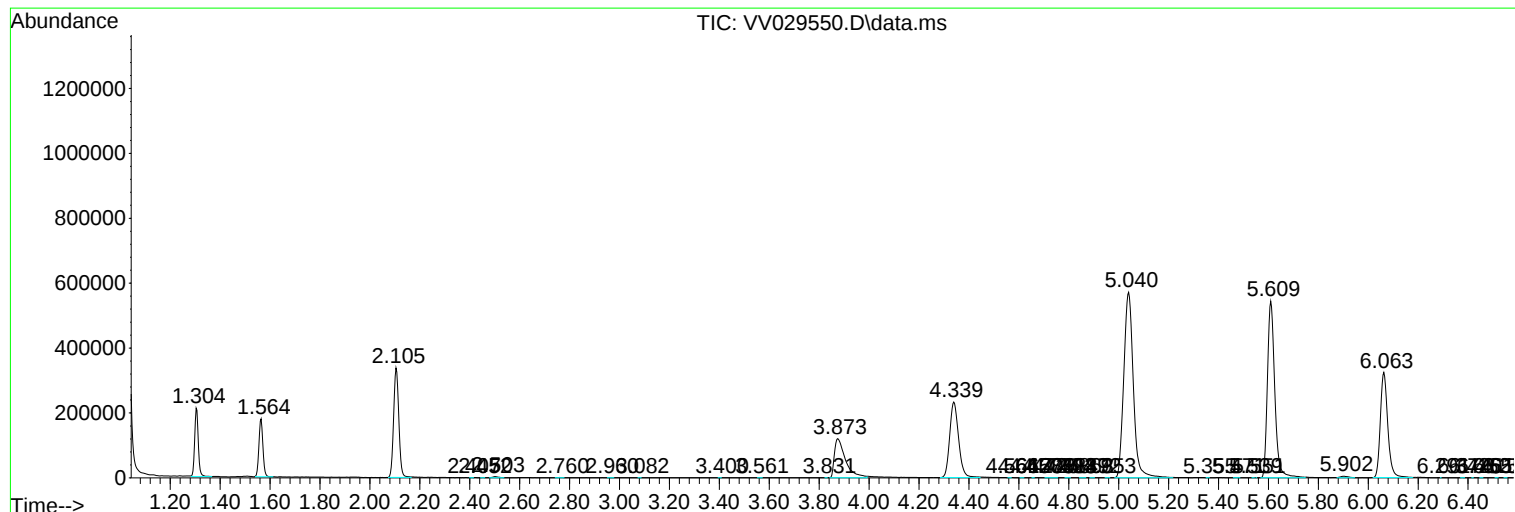

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029550.D
Acq On : 10 Dec 2022 02:43
Operator : SY/MD
Sample : N5915-10DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N09DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029550.D
Acq On : 10 Dec 2022 02:43
Operator : SY/MD
Sample : N5915-10DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N09DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc