

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029551.D
 Acq On : 10 Dec 2022 03:06
 Operator : SY/MD
 Sample : N5915-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	211427	212957	6.44%	1.469%
2	1.564	155	163	175	rVB	177267	194382	5.87%	1.341%
3	2.114	320	334	369	rBV2	2141561	3309082	100.00%	22.828%
4	2.506	447	456	465	rVV3	4093	6296	0.19%	0.043%
5	2.613	484	489	493	rBV2	537	679	0.02%	0.005%
6	2.706	513	518	522	rBV3	281	250	0.01%	0.002%
7	2.757	529	534	537	rBV2	382	277	0.01%	0.002%
8	3.185	658	667	677	rBV3	1727	3229	0.10%	0.022%
9	3.262	689	691	696	rVB2	287	205	0.01%	0.001%
10	3.294	697	701	707	rBV2	312	430	0.01%	0.003%
11	3.725	829	835	839	rBV2	160	201	0.01%	0.001%
12	3.876	869	882	928	rBV2	114685	363366	10.98%	2.507%
13	4.246	995	997	1003	rVB4	383	376	0.01%	0.003%
14	4.339	1008	1026	1060	rBV	225286	559259	16.90%	3.858%
15	4.677	1128	1131	1135	rBV2	605	608	0.02%	0.004%
16	4.725	1144	1146	1151	rVB2	337	293	0.01%	0.002%
17	4.770	1157	1160	1167	rVB	353	281	0.01%	0.002%
18	4.812	1167	1173	1175	rBV	394	301	0.01%	0.002%
19	4.879	1185	1194	1197	rBV2	143	202	0.01%	0.001%
20	5.040	1226	1244	1292	rBV2	550996	1452356	43.89%	10.019%
21	5.477	1375	1380	1382	rBV2	259	234	0.01%	0.002%
22	5.564	1403	1407	1408	rBV2	314	185	0.01%	0.001%
23	5.609	1408	1421	1452	rBV	504411	1014909	30.67%	7.001%
24	5.844	1492	1494	1498	rVB2	335	185	0.01%	0.001%
25	5.908	1503	1514	1528	rVB9	6095	13276	0.40%	0.092%
26	6.063	1548	1562	1595	rBV	307146	635446	19.20%	4.384%
27	6.619	1729	1735	1736	rBV2	730	457	0.01%	0.003%
28	6.828	1796	1800	1806	rVB3	453	410	0.01%	0.003%
29	6.979	1836	1847	1878	rBV	145343	269616	8.15%	1.860%
30	7.130	1890	1894	1898	rBV3	289	338	0.01%	0.002%
31	7.162	1898	1904	1906	rBV4	581	530	0.02%	0.004%
32	7.307	1936	1949	1982	rBV	666435	1180979	35.69%	8.147%
33	7.551	2023	2025	2030	rBV3	338	259	0.01%	0.002%
34	7.616	2033	2045	2067	rBV	102610	182256	5.51%	1.257%
35	7.802	2101	2103	2109	rBV3	317	349	0.01%	0.002%
36	7.841	2113	2115	2118	rVV3	308	190	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029551.D
 Acq On : 10 Dec 2022 03:06
 Operator : SY/MD
 Sample : N5915-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.857	2118	2120	2123	rVV3	289	199	0.01%	0.001%
38	7.931	2137	2143	2149	rBV2	611	983	0.03%	0.007%
39	7.972	2149	2156	2167	rVB5	2166	3557	0.11%	0.025%
40	8.021	2167	2171	2172	rBV3	272	198	0.01%	0.001%
41	8.085	2178	2191	2227	rBV	391453	710661	21.48%	4.903%
42	8.416	2286	2294	2307	rVB3	2425	4368	0.13%	0.030%
43	8.519	2323	2326	2329	rBV3	380	222	0.01%	0.002%
44	8.538	2329	2332	2336	rVB2	260	195	0.01%	0.001%
45	8.567	2338	2341	2343	rBV3	282	207	0.01%	0.001%
46	8.599	2349	2351	2357	rVB4	435	329	0.01%	0.002%
47	8.641	2359	2364	2366	rBV2	373	313	0.01%	0.002%
48	8.706	2380	2384	2390	rVB4	376	358	0.01%	0.002%
49	8.844	2414	2427	2458	rBV	739616	1215216	36.72%	8.383%
50	9.066	2493	2496	2501	rBV2	542	387	0.01%	0.003%
51	9.091	2501	2504	2506	rBV2	260	187	0.01%	0.001%
52	9.130	2511	2516	2522	rVB5	360	408	0.01%	0.003%
53	9.323	2572	2576	2580	rVV2	210	234	0.01%	0.002%
54	9.371	2589	2591	2597	rVB4	443	432	0.01%	0.003%
55	9.480	2623	2625	2631	rVB2	195	194	0.01%	0.001%
56	9.535	2638	2642	2644	rBV	380	246	0.01%	0.002%
57	9.667	2675	2683	2685	rBV	195	217	0.01%	0.001%
58	9.686	2685	2689	2692	rVB2	242	187	0.01%	0.001%
59	9.789	2717	2721	2725	rBV2	293	281	0.01%	0.002%
60	9.931	2763	2765	2769	rVV2	320	217	0.01%	0.001%
61	10.024	2791	2794	2799	rVB2	274	199	0.01%	0.001%
62	10.114	2820	2822	2828	rVB2	333	255	0.01%	0.002%
63	10.162	2828	2837	2841	rBV2	21192	30214	0.91%	0.208%
64	10.207	2841	2851	2872	rVB	464384	725414	21.92%	5.004%
65	10.361	2897	2899	2901	rBV2	399	254	0.01%	0.002%
66	10.529	2947	2951	2953	rVV2	561	388	0.01%	0.003%
67	10.567	2954	2963	2980	rVB2	9895	16447	0.50%	0.113%
68	10.699	3001	3004	3007	rBV3	377	301	0.01%	0.002%
69	10.821	3039	3042	3045	rVB	274	198	0.01%	0.001%
70	10.882	3058	3061	3064	rVV2	333	251	0.01%	0.002%
71	10.911	3064	3070	3076	rVB4	772	1032	0.03%	0.007%
72	10.943	3076	3080	3083	rBV3	286	259	0.01%	0.002%
73	11.059	3112	3116	3119	rBV2	225	190	0.01%	0.001%
74	11.111	3129	3132	3136	rBV3	348	275	0.01%	0.002%
75	11.168	3145	3150	3153	rBV4	1339	1241	0.04%	0.009%
76	11.236	3159	3171	3201	rBV	793305	1246643	37.67%	8.600%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029551.D
 Acq On : 10 Dec 2022 03:06
 Operator : SY/MD
 Sample : N5915-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N00DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.390	3217	3219	3222	rBV2	366	277	0.01%	0.002%
78	11.432	3229	3232	3235	rBV2	326	196	0.01%	0.001%
79	11.538	3261	3265	3266	rBV	355	225	0.01%	0.002%
80	11.612	3274	3288	3309	rBV	701884	1120393	33.86%	7.729%
81	11.831	3350	3356	3360	rVB3	448	456	0.01%	0.003%
82	11.857	3361	3364	3366	rBV2	313	203	0.01%	0.001%
83	11.873	3366	3369	3372	rVV2	326	235	0.01%	0.002%
84	11.969	3396	3399	3402	rBV	251	198	0.01%	0.001%
85	12.037	3415	3420	3422	rBV2	302	247	0.01%	0.002%
86	12.178	3461	3464	3465	rBV	411	186	0.01%	0.001%
87	12.236	3477	3482	3483	rBV	510	436	0.01%	0.003%
88	12.631	3602	3605	3611	rBV3	551	541	0.02%	0.004%
89	12.676	3615	3619	3622	rBV2	364	312	0.01%	0.002%
90	12.750	3639	3642	3647	rBV2	359	233	0.01%	0.002%
91	12.879	3680	3682	3688	rVB2	473	484	0.01%	0.003%
92	13.004	3718	3721	3724	rBV3	357	292	0.01%	0.002%
93	13.085	3744	3746	3750	rVB3	402	310	0.01%	0.002%
94	13.114	3750	3755	3758	rBV2	392	356	0.01%	0.002%
95	13.371	3832	3835	3840	rBV4	471	401	0.01%	0.003%
96	13.416	3845	3849	3851	rBV2	360	373	0.01%	0.003%
97	13.721	3939	3944	3946	rBV4	537	492	0.01%	0.003%
98	13.818	3970	3974	3978	rBV3	510	494	0.01%	0.003%
99	14.281	4116	4118	4121	rBV2	399	240	0.01%	0.002%
100	14.387	4149	4151	4154	rVB3	675	297	0.01%	0.002%




Sum of corrected areas: 14495883

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029551.D
Acq On : 10 Dec 2022 03:06
Operator : SY/MD
Sample : N5915-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

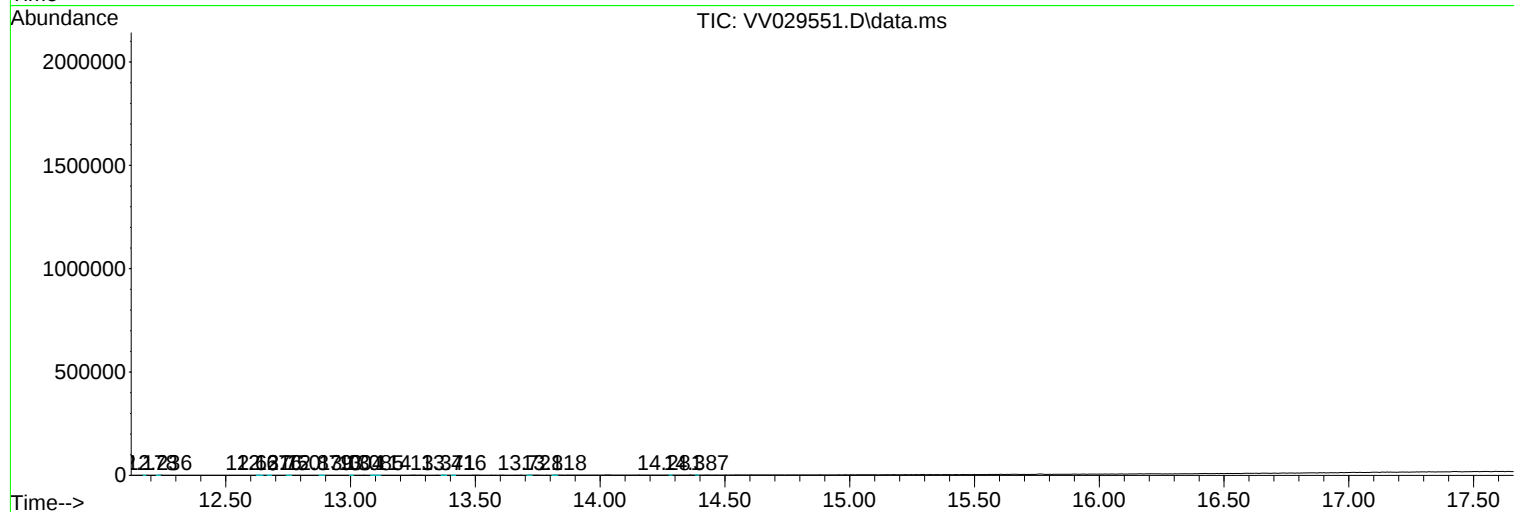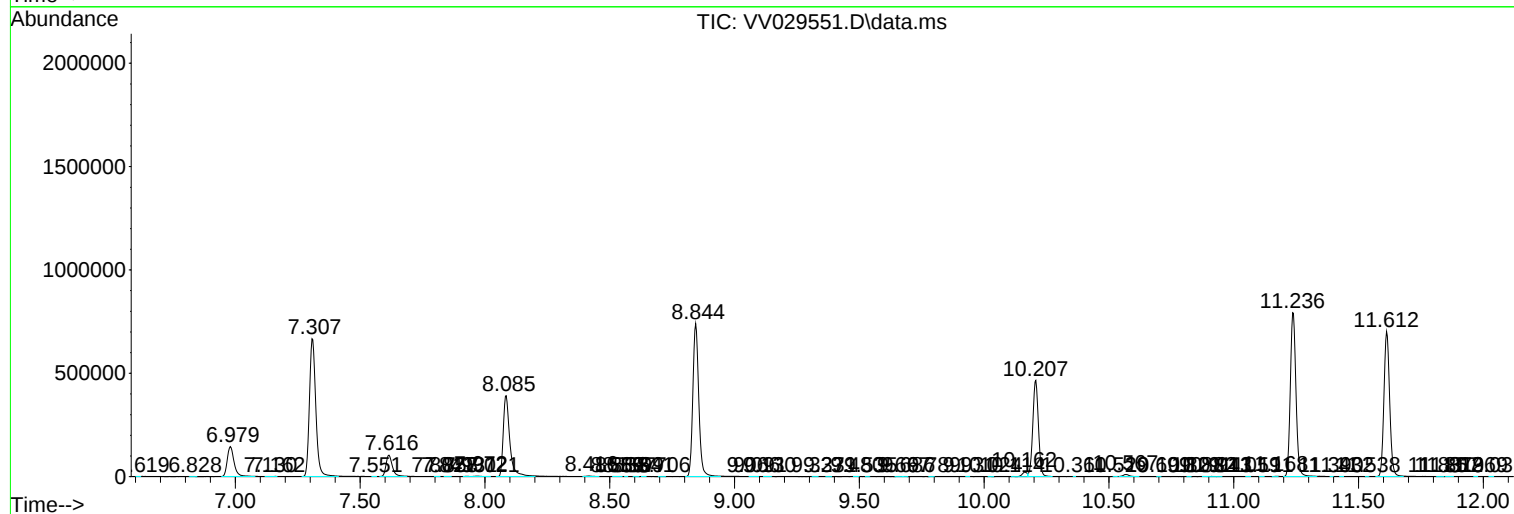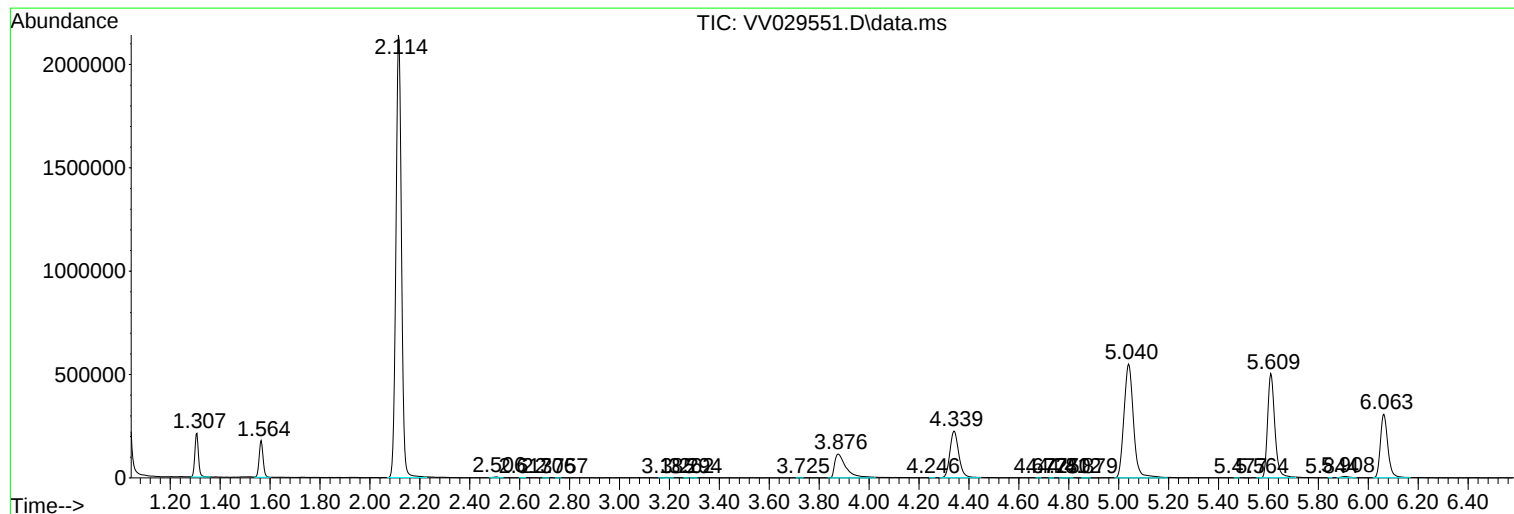

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029551.D
Acq On : 10 Dec 2022 03:06
Operator : SY/MD
Sample : N5915-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029551.D
Acq On : 10 Dec 2022 03:06
Operator : SY/MD
Sample : N5915-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc