

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029552.D
 Acq On : 10 Dec 2022 03:30
 Operator : SY/MD
 Sample : N5915-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N03DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	212318	212938	13.12%	1.448%
2	1.564	156	163	175	rVB	183611	206125	12.70%	1.402%
3	2.105	320	331	349	rBV	349413	505442	31.14%	3.438%
4	2.503	447	455	468	rBV3	4893	7852	0.48%	0.053%
5	2.699	514	516	518	rBV2	217	135	0.01%	0.001%
6	2.728	522	525	527	rVV3	345	216	0.01%	0.001%
7	2.764	527	536	547	rVB5	2289	4031	0.25%	0.027%
8	2.863	565	567	571	rVB	244	155	0.01%	0.001%
9	2.918	582	584	588	rBV	131	124	0.01%	0.001%
10	3.111	642	644	648	rBV2	176	81	0.00%	0.001%
11	3.159	654	659	661	rBV2	202	183	0.01%	0.001%
12	3.172	661	663	667	rVV2	284	178	0.01%	0.001%
13	3.198	669	671	675	rVB2	203	116	0.01%	0.001%
14	3.227	677	680	682	rVB2	217	120	0.01%	0.001%
15	3.259	686	690	693	rBV	113	113	0.01%	0.001%
16	3.381	724	728	730	rBV	137	106	0.01%	0.001%
17	3.449	746	749	752	rVV	147	98	0.01%	0.001%
18	3.490	759	762	764	rBV	145	90	0.01%	0.001%
19	3.577	786	789	790	rBV	207	80	0.00%	0.001%
20	3.638	803	808	811	rBV	278	227	0.01%	0.002%
21	3.677	817	820	825	rVB2	181	150	0.01%	0.001%
22	3.706	825	829	833	rBV	175	176	0.01%	0.001%
23	3.728	833	836	840	rVB	178	125	0.01%	0.001%
24	3.809	858	861	864	rBV2	135	96	0.01%	0.001%
25	3.876	869	882	936	rBV3	131391	480498	29.60%	3.268%
26	4.339	1009	1026	1059	rBV	236847	587404	36.19%	3.996%
27	4.590	1102	1104	1106	rBV2	282	124	0.01%	0.001%
28	4.735	1146	1149	1151	rVB2	155	83	0.01%	0.001%
29	4.751	1151	1154	1157	rBV	175	147	0.01%	0.001%
30	4.953	1213	1217	1221	rBV2	135	124	0.01%	0.001%
31	5.040	1226	1244	1271	rBV2	588701	1523343	93.85%	10.362%
32	5.394	1350	1354	1361	rBV2	386	480	0.03%	0.003%
33	5.468	1374	1377	1380	rBV	449	342	0.02%	0.002%
34	5.522	1390	1394	1397	rBV2	252	251	0.02%	0.002%
35	5.609	1408	1421	1452	rBV	545415	1113381	68.59%	7.573%
36	5.908	1500	1514	1544	rBV	274216	556508	34.28%	3.785%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029552.D
 Acq On : 10 Dec 2022 03:30
 Operator : SY/MD
 Sample : N5915-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N03DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1549	1562	1598	rVB	331485	678213	41.78%	4.613%
38	6.291	1631	1633	1635	rVB	278	108	0.01%	0.001%
39	6.336	1645	1647	1650	rBV2	123	81	0.00%	0.001%
40	6.474	1687	1690	1693	rBV	270	142	0.01%	0.001%
41	6.490	1693	1695	1698	rBV	209	134	0.01%	0.001%
42	6.551	1712	1714	1719	rVB3	261	203	0.01%	0.001%
43	6.619	1729	1735	1738	rBV3	950	1044	0.06%	0.007%
44	6.741	1770	1773	1774	rBV2	123	77	0.00%	0.001%
45	6.773	1780	1783	1785	rBV	113	82	0.01%	0.001%
46	6.831	1798	1801	1802	rBV	150	91	0.01%	0.001%
47	6.889	1816	1819	1822	rBV	165	84	0.01%	0.001%
48	6.979	1836	1847	1874	rBV	154425	287683	17.72%	1.957%
49	7.307	1937	1949	1976	rBV	712546	1266114	78.00%	8.612%
50	7.612	2034	2044	2066	rBV	108808	193605	11.93%	1.317%
51	7.876	2123	2126	2128	rBV2	410	239	0.01%	0.002%
52	7.966	2141	2154	2179	rBV	951325	1623219	100.00%	11.041%
53	8.082	2181	2190	2221	rBV	418674	748398	46.11%	5.091%
54	8.471	2309	2311	2318	rBV3	365	386	0.02%	0.003%
55	8.609	2351	2354	2356	rBV2	264	141	0.01%	0.001%
56	8.751	2394	2398	2402	rVB3	254	198	0.01%	0.001%
57	8.770	2402	2404	2406	rBV2	367	206	0.01%	0.001%
58	8.844	2414	2427	2463	rBV	807023	1322743	81.49%	8.997%
59	9.207	2534	2540	2543	rBV3	264	274	0.02%	0.002%
60	9.233	2546	2548	2551	rVB2	325	159	0.01%	0.001%
61	9.252	2551	2554	2557	rVB3	326	181	0.01%	0.001%
62	9.313	2569	2573	2576	rBV3	347	251	0.02%	0.002%
63	9.394	2596	2598	2605	rVB3	174	125	0.01%	0.001%
64	9.493	2625	2629	2633	rVB3	255	203	0.01%	0.001%
65	9.538	2638	2643	2644	rBV	507	376	0.02%	0.003%
66	9.577	2653	2655	2656	rBV	179	83	0.01%	0.001%
67	9.587	2656	2658	2661	rVB2	230	112	0.01%	0.001%
68	9.702	2691	2694	2695	rBV	202	95	0.01%	0.001%
69	9.767	2707	2714	2718	rBV3	292	365	0.02%	0.002%
70	9.805	2723	2726	2730	rBV2	235	113	0.01%	0.001%
71	9.828	2730	2733	2735	rBV2	192	115	0.01%	0.001%
72	9.918	2758	2761	2762	rBV	267	148	0.01%	0.001%
73	9.960	2771	2774	2776	rBV	163	94	0.01%	0.001%
74	10.037	2794	2798	2800	rBV2	228	172	0.01%	0.001%
75	10.050	2800	2802	2803	rBV	301	123	0.01%	0.001%
76	10.069	2806	2808	2810	rBV	192	89	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029552.D
 Acq On : 10 Dec 2022 03:30
 Operator : SY/MD
 Sample : N5915-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N03DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.120	2822	2824	2827	rBV	219	124	0.01%	0.001%
78	10.162	2828	2837	2841	rVV	21856	32734	2.02%	0.223%
79	10.207	2842	2851	2874	rVB	479652	762830	46.99%	5.189%
80	10.358	2896	2898	2899	rBV	312	97	0.01%	0.001%
81	10.490	2935	2939	2942	rBV2	217	157	0.01%	0.001%
82	10.567	2955	2963	2974	rVB	10646	16352	1.01%	0.111%
83	10.825	3038	3043	3046	rBV2	323	279	0.02%	0.002%
84	10.847	3046	3050	3053	rBV3	367	309	0.02%	0.002%
85	10.908	3060	3069	3072	rBV4	864	1149	0.07%	0.008%
86	11.008	3098	3100	3104	rBV3	187	140	0.01%	0.001%
87	11.079	3120	3122	3123	rBV2	266	90	0.01%	0.001%
88	11.165	3145	3149	3154	rBV5	548	628	0.04%	0.004%
89	11.239	3159	3172	3199	rBV	877895	1371807	84.51%	9.331%
90	11.509	3254	3256	3258	rBV	231	120	0.01%	0.001%
91	11.525	3258	3261	3262	rBV2	273	165	0.01%	0.001%
92	11.612	3276	3288	3308	rBV	760363	1184327	72.96%	8.056%
93	11.776	3336	3339	3346	rVB4	497	488	0.03%	0.003%
94	11.860	3361	3365	3368	rBV3	377	376	0.02%	0.003%
95	11.876	3368	3370	3373	rVB2	399	155	0.01%	0.001%
96	11.918	3379	3383	3388	rBV3	337	320	0.02%	0.002%
97	11.966	3395	3398	3400	rVB2	387	223	0.01%	0.002%
98	11.979	3400	3402	3404	rBV2	210	111	0.01%	0.001%
99	12.474	3553	3556	3557	rBV	230	139	0.01%	0.001%
100	13.046	3732	3734	3739	rBV3	480	307	0.02%	0.002%




Sum of corrected areas: 14701338

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029552.D
Acq On : 10 Dec 2022 03:30
Operator : SY/MD
Sample : N5915-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N03DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

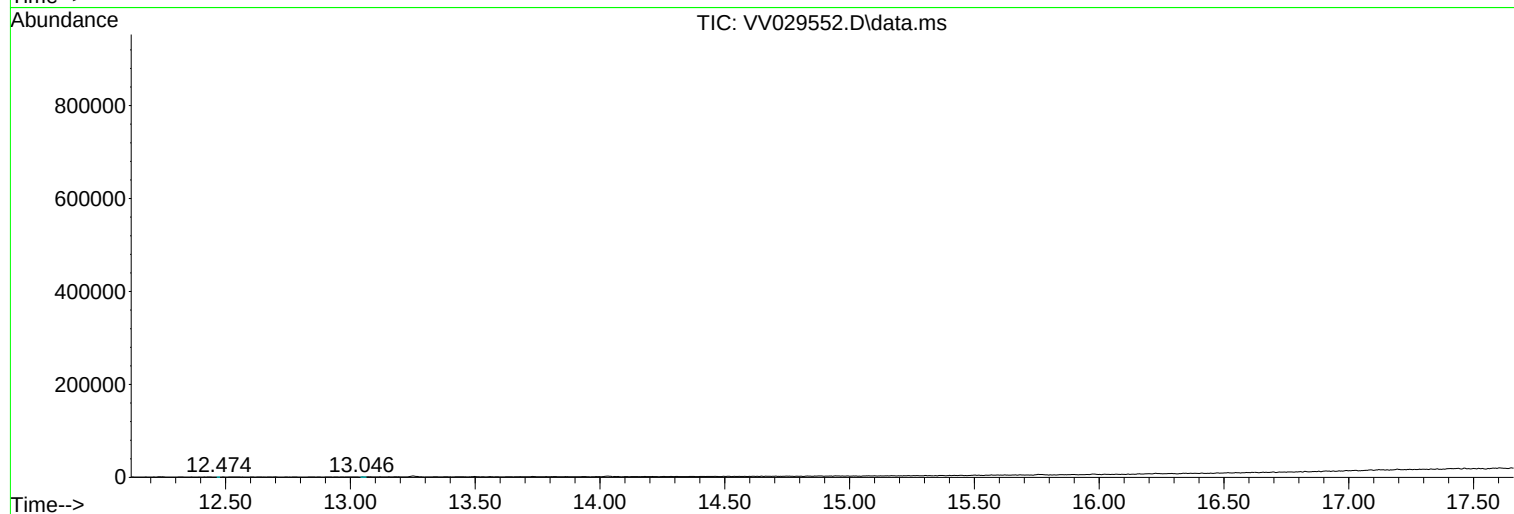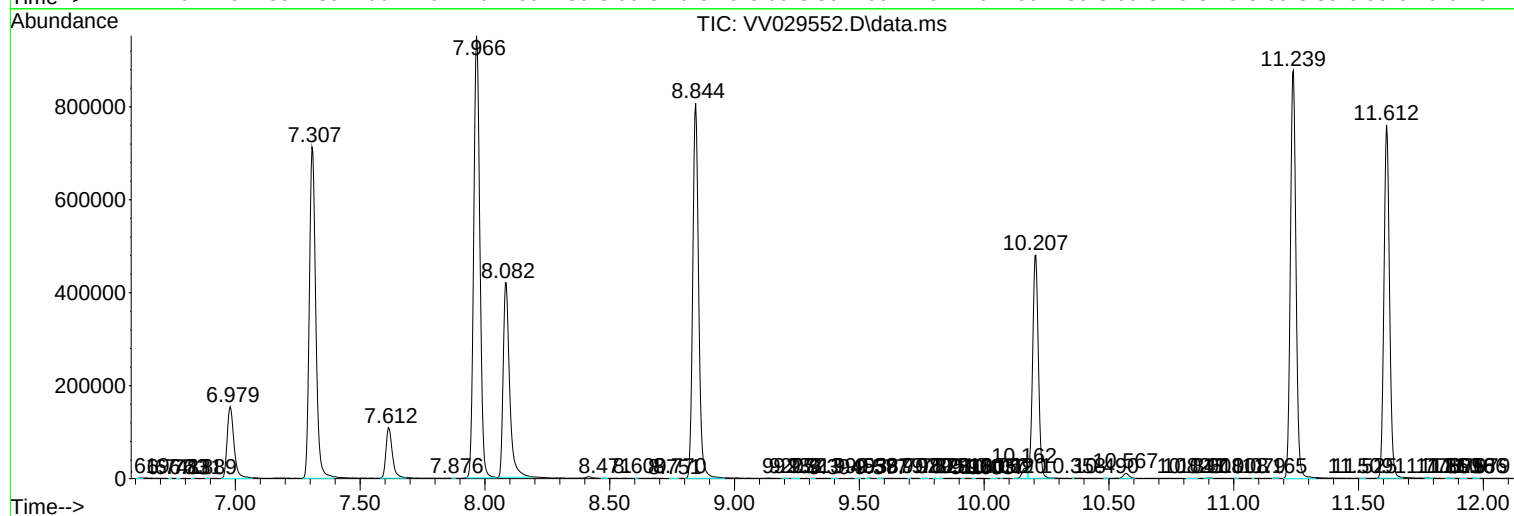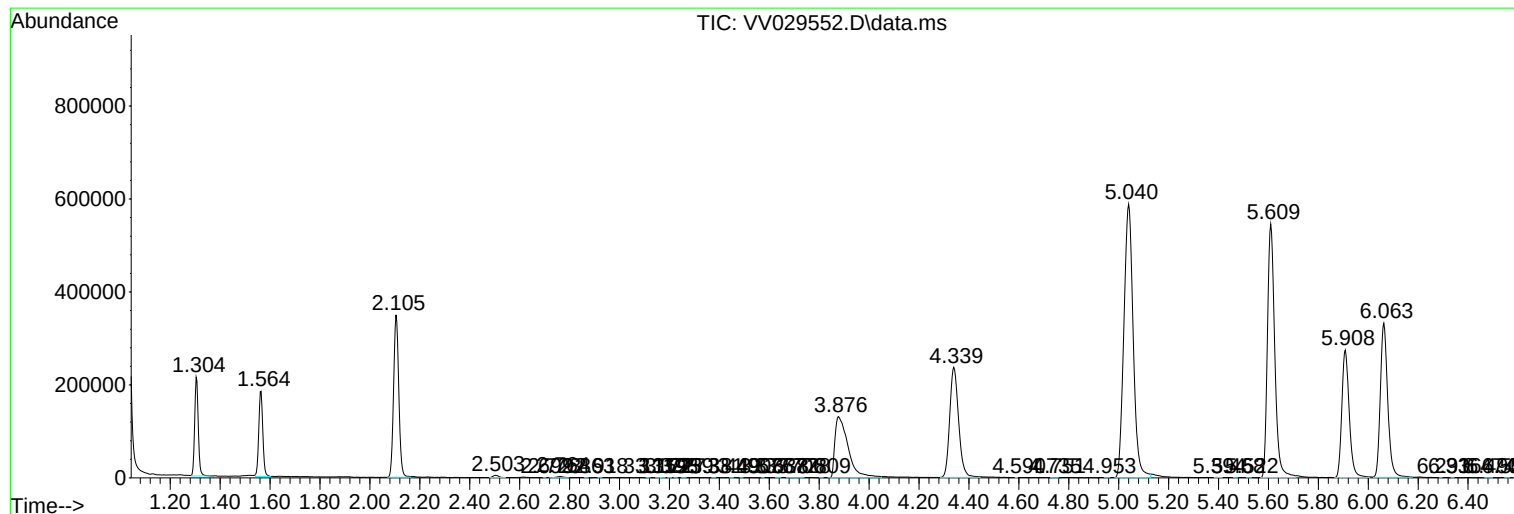

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029552.D
Acq On : 10 Dec 2022 03:30
Operator : SY/MD
Sample : N5915-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N03DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029552.D
Acq On : 10 Dec 2022 03:30
Operator : SY/MD
Sample : N5915-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N03DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------