

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029554.D
 Acq On : 10 Dec 2022 04:17
 Operator : SY/MD
 Sample : N5915-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	206775	207744	14.43%	1.769%
2	1.565	155	163	177	rVB	166762	192260	13.36%	1.638%
3	2.105	320	331	343	rBV	327900	470976	32.72%	4.011%
4	2.436	432	434	437	rBV	183	87	0.01%	0.001%
5	2.590	480	482	486	rVB	272	124	0.01%	0.001%
6	2.761	529	535	537	rBV2	333	363	0.03%	0.003%
7	3.163	658	660	666	rVB2	219	113	0.01%	0.001%
8	3.204	671	673	675	rBV	249	111	0.01%	0.001%
9	3.327	707	711	713	rBV	130	105	0.01%	0.001%
10	3.404	734	735	737	rBV	105	32	0.00%	0.000%
11	3.420	738	740	742	rVV	205	70	0.00%	0.001%
12	3.519	768	771	776	rVB	223	164	0.01%	0.001%
13	3.545	776	779	782	rBV2	178	125	0.01%	0.001%
14	3.613	797	800	801	rBV2	124	69	0.00%	0.001%
15	3.873	872	881	910	rBV	104799	295917	20.56%	2.520%
16	4.339	1010	1026	1059	rBV	225179	563727	39.16%	4.801%
17	4.677	1128	1131	1135	rBV3	275	265	0.02%	0.002%
18	4.709	1137	1141	1144	rVV2	283	217	0.02%	0.002%
19	4.745	1150	1152	1154	rBV2	166	99	0.01%	0.001%
20	4.796	1167	1168	1170	rVB	209	41	0.00%	0.000%
21	4.818	1171	1175	1177	rBV2	137	106	0.01%	0.001%
22	4.851	1183	1185	1188	rVB2	152	74	0.01%	0.001%
23	4.902	1196	1201	1204	rVB	322	225	0.02%	0.002%
24	4.925	1204	1208	1210	rBV2	121	109	0.01%	0.001%
25	5.040	1226	1244	1278	rBV2	545359	1439546	100.00%	12.261%
26	5.429	1363	1365	1366	rBV2	175	91	0.01%	0.001%
27	5.474	1374	1379	1385	rBV2	523	545	0.04%	0.005%
28	5.526	1393	1395	1397	rBV	174	50	0.00%	0.000%
29	5.539	1397	1399	1401	rBV	185	87	0.01%	0.001%
30	5.609	1408	1421	1460	rBV	524919	1071539	74.44%	9.127%
31	5.902	1502	1512	1528	rVB6	4753	9886	0.69%	0.084%
32	5.989	1538	1539	1540	rBV	132	35	0.00%	0.000%
33	6.063	1548	1562	1602	rBV	311825	641302	44.55%	5.462%
34	6.359	1650	1654	1655	rBV	348	240	0.02%	0.002%
35	6.426	1672	1675	1680	rBV3	423	388	0.03%	0.003%
36	6.452	1680	1683	1685	rVV2	311	181	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029554.D
 Acq On : 10 Dec 2022 04:17
 Operator : SY/MD
 Sample : N5915-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.500	1693	1698	1700	rBV	240	164	0.01%	0.001%
38	6.558	1713	1716	1718	rBV3	139	83	0.01%	0.001%
39	6.725	1766	1768	1771	rBV	166	108	0.01%	0.001%
40	6.825	1795	1799	1804	rBV2	247	167	0.01%	0.001%
41	6.879	1815	1816	1819	rBV	318	185	0.01%	0.002%
42	6.979	1835	1847	1880	rBV	145413	269871	18.75%	2.299%
43	7.307	1936	1949	1986	rBV	678432	1201836	83.49%	10.236%
44	7.574	2030	2032	2034	rBV3	434	240	0.02%	0.002%
45	7.613	2034	2044	2071	rVV	102011	179474	12.47%	1.529%
46	7.809	2102	2105	2107	rBV	335	210	0.01%	0.002%
47	7.934	2136	2144	2152	rBV3	4075	6967	0.48%	0.059%
48	8.082	2180	2190	2223	rBV	386049	707719	49.16%	6.028%
49	8.477	2312	2313	2316	rBV3	327	205	0.01%	0.002%
50	8.532	2329	2330	2331	rBV3	192	52	0.00%	0.000%
51	8.584	2343	2346	2348	rBV	424	203	0.01%	0.002%
52	8.596	2348	2350	2353	rVV2	346	177	0.01%	0.002%
53	8.728	2389	2391	2395	rBV2	186	149	0.01%	0.001%
54	8.748	2395	2397	2399	rBV	207	132	0.01%	0.001%
55	8.786	2406	2409	2414	rVB2	453	371	0.03%	0.003%
56	8.844	2414	2427	2459	rBV	763567	1266199	87.96%	10.784%
57	9.095	2503	2505	2506	rVB	290	69	0.00%	0.001%
58	9.127	2511	2515	2518	rBV4	411	357	0.02%	0.003%
59	9.227	2544	2546	2552	rVB	266	138	0.01%	0.001%
60	9.256	2552	2555	2559	rBV	218	168	0.01%	0.001%
61	9.272	2559	2560	2561	rBV	101	27	0.00%	0.000%
62	9.352	2582	2585	2587	rBV2	309	228	0.02%	0.002%
63	9.384	2593	2595	2599	rBV2	244	167	0.01%	0.001%
64	9.468	2612	2621	2624	rBV2	186	266	0.02%	0.002%
65	9.484	2624	2626	2628	rBV	177	80	0.01%	0.001%
66	9.645	2672	2676	2679	rBV3	377	217	0.02%	0.002%
67	9.690	2688	2690	2695	rBV	197	94	0.01%	0.001%
68	9.731	2700	2703	2705	rBV	183	112	0.01%	0.001%
69	9.902	2753	2756	2758	rBV2	184	115	0.01%	0.001%
70	9.947	2768	2770	2772	rVB	141	35	0.00%	0.000%
71	10.063	2802	2806	2810	rBV2	252	209	0.01%	0.002%
72	10.162	2823	2837	2841	rBV2	21662	32223	2.24%	0.274%
73	10.204	2842	2850	2875	rVB	459643	719968	50.01%	6.132%
74	10.375	2895	2903	2916	rVB2	4445	7370	0.51%	0.063%
75	10.445	2924	2925	2928	rVB	355	128	0.01%	0.001%
76	10.461	2928	2930	2931	rBV	134	35	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029554.D
 Acq On : 10 Dec 2022 04:17
 Operator : SY/MD
 Sample : N5915-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

77	10.532	2941	2952	2954	rBV6	805	1104	0.08%	0.009%
78	10.567	2955	2963	2976	rVB	10453	16299	1.13%	0.139%
79	10.731	3012	3014	3019	rBV	263	152	0.01%	0.001%
80	10.905	3062	3068	3079	rVB5	903	1588	0.11%	0.014%
81	11.034	3105	3108	3110	rBV	180	126	0.01%	0.001%
82	11.169	3147	3150	3159	rVB7	1148	1508	0.10%	0.013%
83	11.239	3159	3172	3192	rBV	829071	1306339	90.75%	11.126%
84	11.612	3275	3288	3309	rBV	713630	1119925	77.80%	9.539%
85	13.159	3767	3769	3771	rBV2	418	197	0.01%	0.002%
86	13.239	3792	3794	3795	rBV	399	171	0.01%	0.001%


Sum of corrected areas: 11740940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029554.D
Acq On : 10 Dec 2022 04:17
Operator : SY/MD
Sample : N5915-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

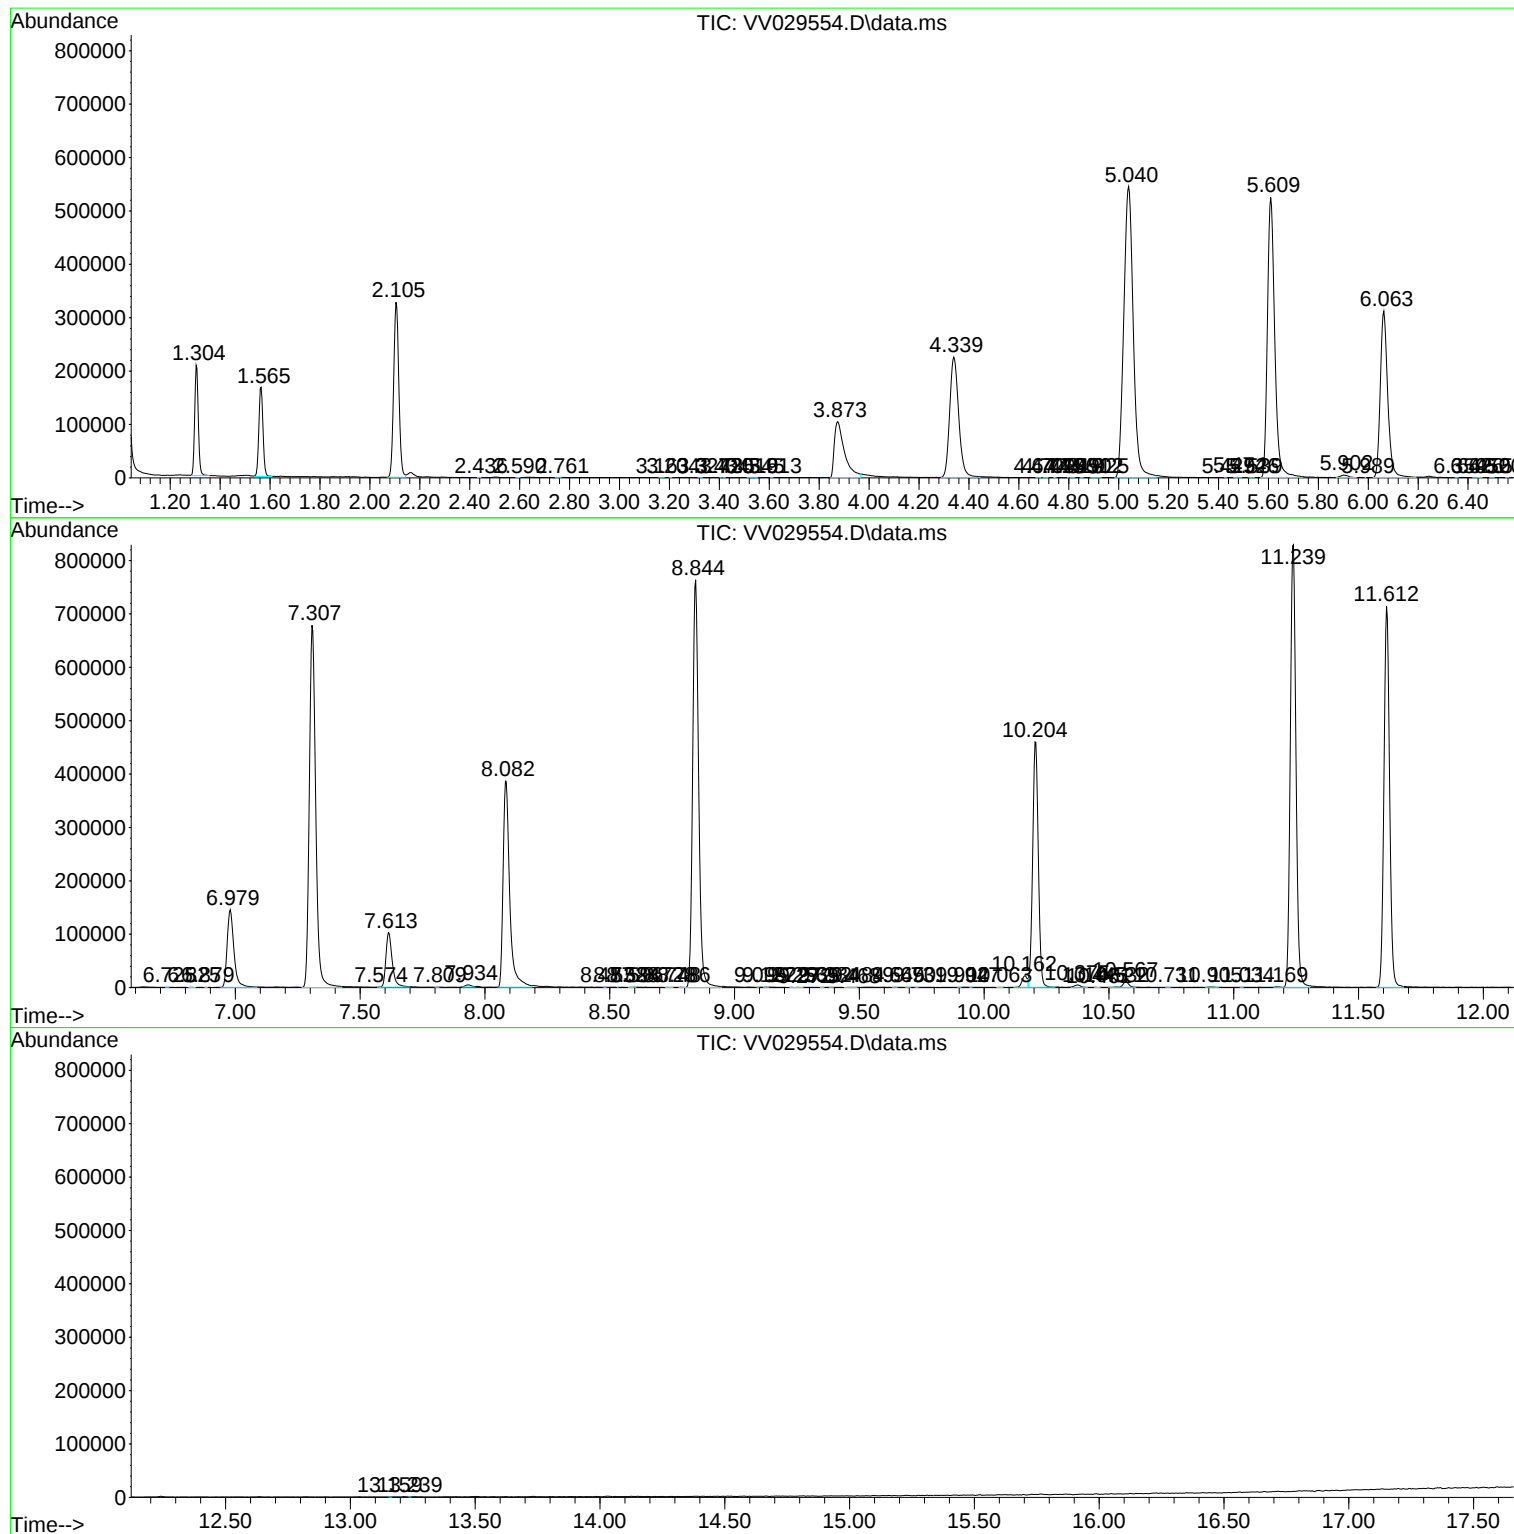

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029554.D
Acq On : 10 Dec 2022 04:17
Operator : SY/MD
Sample : N5915-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029554.D
Acq On : 10 Dec 2022 04:17
Operator : SY/MD
Sample : N5915-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------