

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029555.D
 Acq On : 10 Dec 2022 04:41
 Operator : SY/MD
 Sample : N5915-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	201301	202683	13.62%	1.709%
2	1.564	155	163	177	rVB	177265	199259	13.39%	1.680%
3	2.105	321	331	350	rBV	329135	472129	31.73%	3.981%
4	2.429	428	432	434	rBV2	196	137	0.01%	0.001%
5	2.503	447	455	466	rVV3	4983	8049	0.54%	0.068%
6	2.587	477	481	483	rBV2	344	240	0.02%	0.002%
7	2.728	522	525	531	rVB	296	237	0.02%	0.002%
8	2.764	531	536	539	rBV3	528	544	0.04%	0.005%
9	2.879	570	572	576	rBV2	109	96	0.01%	0.001%
10	3.304	701	704	706	rBV	387	239	0.02%	0.002%
11	3.442	744	747	750	rBV	140	104	0.01%	0.001%
12	3.587	786	792	795	rBV2	151	189	0.01%	0.002%
13	3.664	811	816	818	rBV2	207	159	0.01%	0.001%
14	3.715	829	832	836	rVB2	123	91	0.01%	0.001%
15	3.738	836	839	840	rBV	143	85	0.01%	0.001%
16	3.773	847	850	854	rVB2	168	123	0.01%	0.001%
17	3.805	854	860	863	rBV	251	271	0.02%	0.002%
18	3.873	868	881	920	rBV2	125342	390935	26.27%	3.297%
19	4.339	1010	1026	1051	rBV	230562	569943	38.30%	4.806%
20	4.558	1092	1094	1098	rBV3	369	284	0.02%	0.002%
21	4.613	1106	1111	1112	rBV2	233	173	0.01%	0.001%
22	4.661	1124	1126	1129	rBV2	169	95	0.01%	0.001%
23	4.828	1175	1178	1182	rBV3	367	192	0.01%	0.002%
24	4.857	1182	1187	1191	rBV	138	170	0.01%	0.001%
25	5.040	1226	1244	1288	rBV2	563563	1487956	100.00%	12.547%
26	5.420	1360	1362	1368	rBV3	278	267	0.02%	0.002%
27	5.539	1396	1399	1402	rBV2	115	93	0.01%	0.001%
28	5.609	1407	1421	1450	rBV	519087	1058142	71.11%	8.923%
29	6.063	1548	1562	1591	rBV	319683	657568	44.19%	5.545%
30	6.281	1628	1630	1632	rBV	275	151	0.01%	0.001%
31	6.378	1657	1660	1665	rVB	287	165	0.01%	0.001%
32	6.407	1666	1669	1672	rBV2	199	115	0.01%	0.001%
33	6.455	1680	1684	1686	rBV2	324	190	0.01%	0.002%
34	6.526	1703	1706	1711	rVB2	196	156	0.01%	0.001%
35	6.558	1713	1716	1718	rBV2	124	88	0.01%	0.001%
36	6.574	1719	1721	1724	rVB2	234	136	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029555.D
 Acq On : 10 Dec 2022 04:41
 Operator : SY/MD
 Sample : N5915-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.612	1731	1733	1735	rBV	655	353	0.02%	0.003%
38	6.728	1765	1769	1774	rBV2	261	239	0.02%	0.002%
39	6.751	1774	1776	1779	rVB3	216	140	0.01%	0.001%
40	6.783	1783	1786	1790	rVB4	504	402	0.03%	0.003%
41	6.809	1790	1794	1795	rBV	204	102	0.01%	0.001%
42	6.834	1799	1802	1804	rBV2	303	133	0.01%	0.001%
43	6.886	1815	1818	1819	rBV2	240	132	0.01%	0.001%
44	6.979	1836	1847	1872	rBV	148469	277095	18.62%	2.337%
45	7.307	1935	1949	1980	rBV	667588	1193504	80.21%	10.064%
46	7.616	2034	2045	2073	rBV	105020	188830	12.69%	1.592%
47	8.021	2168	2171	2172	rBV2	245	131	0.01%	0.001%
48	8.085	2180	2191	2232	rBV	409799	752748	50.59%	6.347%
49	8.410	2287	2292	2304	rBV4	1918	3618	0.24%	0.031%
50	8.654	2366	2368	2372	rVB	295	164	0.01%	0.001%
51	8.728	2389	2391	2393	rBV	254	170	0.01%	0.001%
52	8.757	2397	2400	2408	rVB3	402	449	0.03%	0.004%
53	8.789	2408	2410	2415	rBV2	246	297	0.02%	0.003%
54	8.844	2415	2427	2467	rBV	761210	1246164	83.75%	10.508%
55	9.140	2513	2519	2530	rBV6	769	1218	0.08%	0.010%
56	9.185	2530	2533	2536	rVB2	428	280	0.02%	0.002%
57	9.246	2549	2552	2556	rBV2	319	268	0.02%	0.002%
58	9.278	2556	2562	2565	rVV2	439	409	0.03%	0.003%
59	9.313	2565	2573	2576	rBV3	391	487	0.03%	0.004%
60	9.374	2591	2592	2597	rBV2	206	134	0.01%	0.001%
61	9.490	2626	2628	2631	rVB	337	168	0.01%	0.001%
62	9.506	2631	2633	2637	rVB2	264	136	0.01%	0.001%
63	9.542	2637	2644	2647	rBV3	535	581	0.04%	0.005%
64	9.564	2647	2651	2653	rBV3	303	229	0.02%	0.002%
65	9.619	2665	2668	2672	rBV3	211	177	0.01%	0.001%
66	9.641	2672	2675	2677	rBV	168	94	0.01%	0.001%
67	9.667	2682	2683	2689	rVV2	169	125	0.01%	0.001%
68	9.696	2689	2692	2696	rVB2	283	179	0.01%	0.002%
69	9.763	2709	2713	2714	rBV	166	103	0.01%	0.001%
70	9.847	2736	2739	2741	rBV2	267	169	0.01%	0.001%
71	9.898	2751	2755	2758	rBV2	212	201	0.01%	0.002%
72	10.046	2796	2801	2804	rBV2	273	282	0.02%	0.002%
73	10.162	2827	2837	2841	rBV	22047	31804	2.14%	0.268%
74	10.207	2842	2851	2876	rVB	475409	755807	50.79%	6.373%
75	10.371	2895	2902	2912	rBV4	1575	2327	0.16%	0.020%
76	10.426	2916	2919	2926	rVB3	346	345	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029555.D
 Acq On : 10 Dec 2022 04:41
 Operator : SY/MD
 Sample : N5915-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.509	2942	2945	2947	rBV	255	154	0.01%	0.001%
78	10.567	2954	2963	2976	rBV	9963	15828	1.06%	0.133%
79	10.648	2986	2988	2989	rBV	257	131	0.01%	0.001%
80	10.744	3015	3018	3021	rBV2	236	138	0.01%	0.001%
81	10.821	3038	3042	3047	rBV2	272	223	0.01%	0.002%
82	10.943	3078	3080	3084	rBV	259	213	0.01%	0.002%
83	11.027	3103	3106	3107	rBV	497	194	0.01%	0.002%
84	11.056	3111	3115	3117	rBV2	248	225	0.02%	0.002%
85	11.088	3122	3125	3128	rBV2	297	200	0.01%	0.002%
86	11.159	3141	3147	3148	rBV	393	314	0.02%	0.003%
87	11.175	3148	3152	3159	rVB3	948	889	0.06%	0.007%
88	11.239	3159	3172	3198	rBV	804759	1256284	84.43%	10.593%
89	11.474	3243	3245	3250	rVB2	285	158	0.01%	0.001%
90	11.503	3251	3254	3255	rBV	192	94	0.01%	0.001%
91	11.532	3260	3263	3269	rBV	388	358	0.02%	0.003%
92	11.558	3269	3271	3274	rVB	200	86	0.01%	0.001%
93	11.612	3274	3288	3310	rBV	675337	1068515	71.81%	9.010%
94	11.831	3354	3356	3359	rBV3	264	115	0.01%	0.001%
95	11.927	3384	3386	3388	rBV2	402	202	0.01%	0.002%
96	11.959	3394	3396	3398	rBV2	221	137	0.01%	0.001%
97	12.030	3413	3418	3420	rVB2	382	337	0.02%	0.003%
98	12.136	3448	3451	3454	rBV2	241	212	0.01%	0.002%
99	12.172	3460	3462	3464	rBV	156	86	0.01%	0.001%
100	12.242	3474	3484	3494	rBV5	1099	2328	0.16%	0.020%




Sum of corrected areas: 11859069

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029555.D
Acq On : 10 Dec 2022 04:41
Operator : SY/MD
Sample : N5915-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

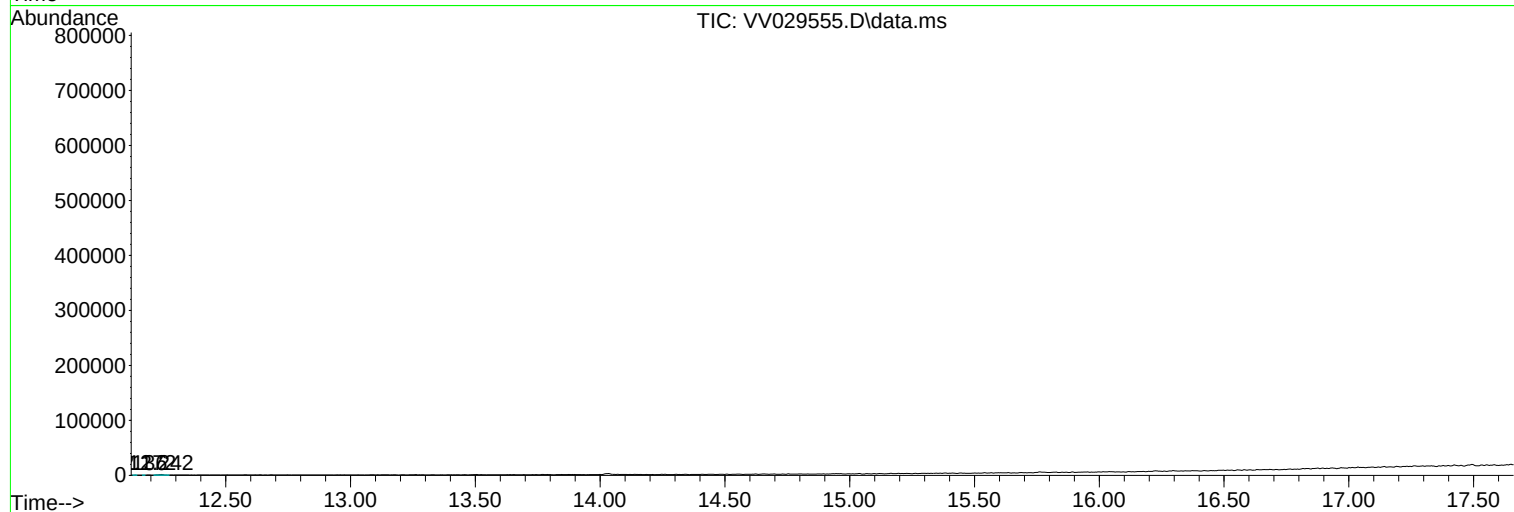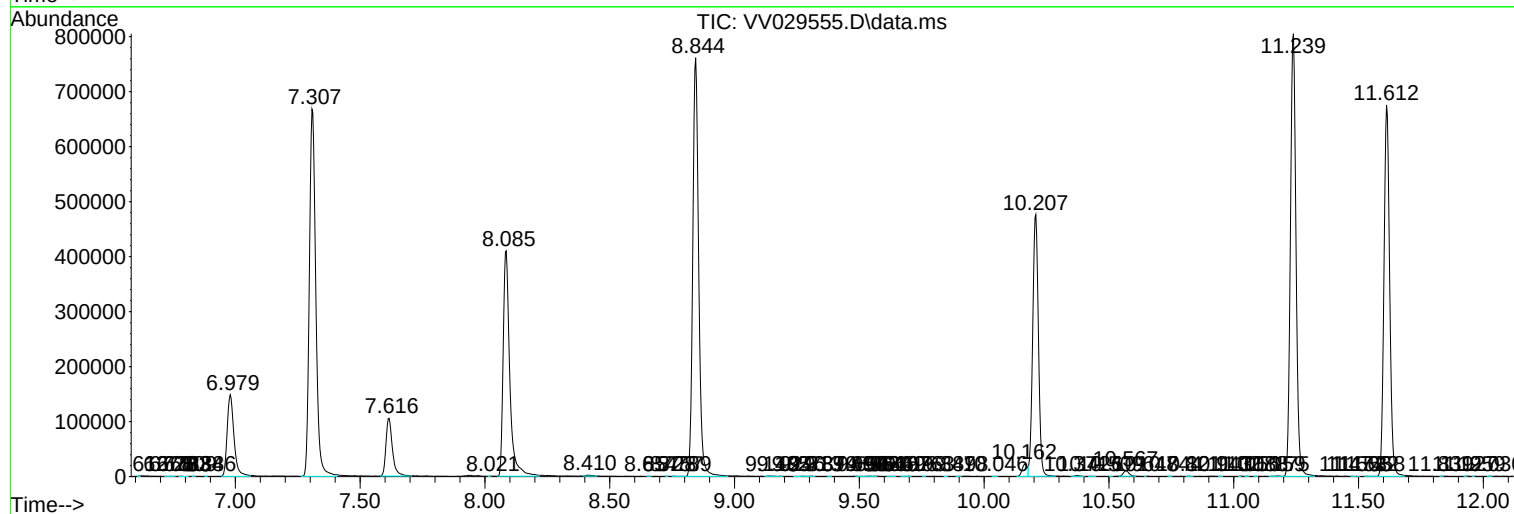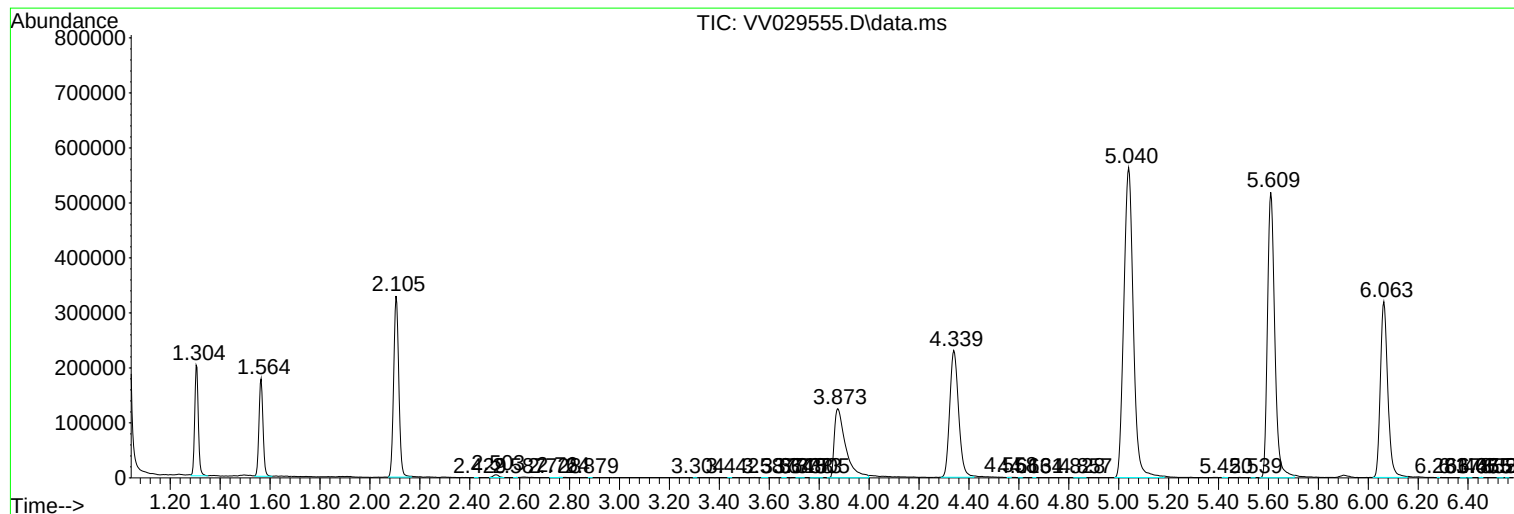

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029555.D
Acq On : 10 Dec 2022 04:41
Operator : SY/MD
Sample : N5915-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029555.D
Acq On : 10 Dec 2022 04:41
Operator : SY/MD
Sample : N5915-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc