

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029556.D
 Acq On : 10 Dec 2022 05:04
 Operator : SY/MD
 Sample : N5915-17 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	202960	203943	14.54%	1.824%
2	1.561	155	162	180	rVB	170077	191617	13.66%	1.713%
3	2.105	320	331	347	rBV	304883	441258	31.46%	3.946%
4	2.407	423	425	429	rBV2	208	87	0.01%	0.001%
5	2.503	446	455	466	rVB3	4871	8270	0.59%	0.074%
6	2.552	466	470	474	rBV2	296	279	0.02%	0.002%
7	2.593	481	483	484	rBV2	416	176	0.01%	0.002%
8	2.658	501	503	514	rVB2	271	246	0.02%	0.002%
9	2.728	523	525	528	rBV2	236	150	0.01%	0.001%
10	2.761	532	535	538	rBV	293	230	0.02%	0.002%
11	2.863	555	567	572	rBV2	360	509	0.04%	0.005%
12	2.995	605	608	614	rBV2	150	149	0.01%	0.001%
13	3.352	714	719	722	rBV2	142	147	0.01%	0.001%
14	3.400	729	734	736	rBV	147	155	0.01%	0.001%
15	3.439	742	746	749	rBV2	166	126	0.01%	0.001%
16	3.535	773	776	780	rBV	180	125	0.01%	0.001%
17	3.568	785	786	792	rVB2	121	94	0.01%	0.001%
18	3.597	792	795	798	rVB2	142	86	0.01%	0.001%
19	3.716	827	832	836	rVB2	201	173	0.01%	0.002%
20	3.780	850	852	855	rVB	205	93	0.01%	0.001%
21	3.873	871	881	919	rBV2	113328	344734	24.58%	3.083%
22	4.339	1010	1026	1064	rBV	220669	552139	39.37%	4.937%
23	4.635	1116	1118	1123	rVB2	203	153	0.01%	0.001%
24	4.696	1135	1137	1140	rVB	279	152	0.01%	0.001%
25	4.748	1150	1153	1157	rBV	168	110	0.01%	0.001%
26	4.770	1158	1160	1162	rBV	177	88	0.01%	0.001%
27	4.831	1173	1179	1181	rBV	104	93	0.01%	0.001%
28	4.908	1198	1203	1205	rBV	200	157	0.01%	0.001%
29	4.960	1215	1219	1221	rBV	171	151	0.01%	0.001%
30	5.040	1226	1244	1275	rBV2	539835	1402597	100.00%	12.542%
31	5.365	1343	1345	1350	rBV3	264	181	0.01%	0.002%
32	5.407	1355	1358	1362	rVB2	522	420	0.03%	0.004%
33	5.442	1366	1369	1373	rBV3	188	126	0.01%	0.001%
34	5.461	1373	1375	1377	rBV2	309	206	0.01%	0.002%
35	5.523	1392	1394	1397	rVB2	221	105	0.01%	0.001%
36	5.542	1397	1400	1403	rBV2	229	159	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029556.D
 Acq On : 10 Dec 2022 05:04
 Operator : SY/MD
 Sample : N5915-17 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1409	1421	1448	rBV	494490	984449	70.19%	8.803%
38	5.902	1502	1512	1526	rVB6	4274	8962	0.64%	0.080%
39	6.063	1547	1562	1587	rBV	306026	629580	44.89%	5.630%
40	6.294	1631	1634	1635	rBV	276	102	0.01%	0.001%
41	6.304	1635	1637	1644	rVB2	205	196	0.01%	0.002%
42	6.336	1644	1647	1648	rBV2	153	85	0.01%	0.001%
43	6.355	1651	1653	1656	rBV	184	97	0.01%	0.001%
44	6.477	1689	1691	1694	rBV	152	89	0.01%	0.001%
45	6.590	1722	1726	1727	rBV	228	167	0.01%	0.001%
46	6.629	1732	1738	1746	rVV5	1005	1611	0.11%	0.014%
47	6.696	1757	1759	1763	rVB3	281	175	0.01%	0.002%
48	6.825	1797	1799	1802	rBV2	242	118	0.01%	0.001%
49	6.854	1806	1808	1810	rBV3	213	120	0.01%	0.001%
50	6.867	1810	1812	1815	rVB2	241	125	0.01%	0.001%
51	6.921	1827	1829	1833	rVB	240	121	0.01%	0.001%
52	6.979	1834	1847	1874	rBV	140374	264338	18.85%	2.364%
53	7.240	1926	1928	1936	rVB3	462	380	0.03%	0.003%
54	7.307	1936	1949	1981	rBV	626877	1117206	79.65%	9.990%
55	7.612	2034	2044	2072	rBV	100968	178819	12.75%	1.599%
56	8.024	2170	2172	2177	rVB	342	169	0.01%	0.002%
57	8.082	2180	2190	2224	rBV	395433	723201	51.56%	6.467%
58	8.522	2324	2327	2332	rVB3	324	258	0.02%	0.002%
59	8.545	2332	2334	2336	rBV	305	154	0.01%	0.001%
60	8.593	2347	2349	2354	rVB3	370	315	0.02%	0.003%
61	8.619	2354	2357	2360	rBV2	268	235	0.02%	0.002%
62	8.764	2398	2402	2405	rBV2	360	259	0.02%	0.002%
63	8.799	2408	2413	2415	rBV2	465	396	0.03%	0.004%
64	8.844	2415	2427	2459	rBV	702130	1148255	81.87%	10.268%
65	9.088	2500	2503	2504	rBV	273	151	0.01%	0.001%
66	9.111	2507	2510	2512	rBV4	385	264	0.02%	0.002%
67	9.236	2546	2549	2551	rVB2	181	131	0.01%	0.001%
68	9.249	2551	2553	2554	rBV	220	95	0.01%	0.001%
69	9.284	2561	2564	2568	rVB	303	174	0.01%	0.002%
70	9.336	2577	2580	2588	rVB2	291	242	0.02%	0.002%
71	9.519	2634	2637	2639	rVV2	247	157	0.01%	0.001%
72	9.538	2639	2643	2648	rVB	727	722	0.05%	0.006%
73	9.564	2648	2651	2652	rBV2	469	249	0.02%	0.002%
74	9.725	2698	2701	2706	rVB2	303	249	0.02%	0.002%
75	9.751	2706	2709	2712	rBV2	185	112	0.01%	0.001%
76	9.834	2733	2735	2740	rVB	204	128	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029556.D
 Acq On : 10 Dec 2022 05:04
 Operator : SY/MD
 Sample : N5915-17 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.873	2745	2747	2750	rVB2	238	156	0.01%	0.001%
78	9.924	2759	2763	2767	rBV	510	443	0.03%	0.004%
79	10.050	2800	2802	2804	rBV2	190	101	0.01%	0.001%
80	10.063	2804	2806	2809	rVB	312	133	0.01%	0.001%
81	10.095	2813	2816	2817	rBV	270	134	0.01%	0.001%
82	10.162	2827	2837	2841	rBV2	21610	31578	2.25%	0.282%
83	10.207	2842	2851	2868	rVB	460000	722057	51.48%	6.457%
84	10.358	2896	2898	2904	rBV3	337	370	0.03%	0.003%
85	10.448	2923	2926	2931	rVB3	264	222	0.02%	0.002%
86	10.503	2939	2943	2945	rBV	182	136	0.01%	0.001%
87	10.526	2947	2950	2951	rVV2	475	289	0.02%	0.003%
88	10.567	2955	2963	2980	rVB2	10350	16477	1.17%	0.147%
89	10.690	2998	3001	3007	rBV3	265	250	0.02%	0.002%
90	10.796	3031	3034	3036	rBV2	251	165	0.01%	0.001%
91	10.908	3062	3069	3079	rVB5	629	1060	0.08%	0.009%
92	10.995	3093	3096	3099	rBV2	212	149	0.01%	0.001%
93	11.194	3156	3158	3159	rBV	186	85	0.01%	0.001%
94	11.236	3159	3171	3201	rVV	746765	1146783	81.76%	10.255%
95	11.464	3238	3242	3243	rBV2	366	289	0.02%	0.003%
96	11.612	3275	3288	3313	rBV	666007	1048720	74.77%	9.378%
97	12.455	3548	3550	3554	rBV	361	295	0.02%	0.003%
98	12.503	3563	3565	3566	rBV2	379	133	0.01%	0.001%
99	12.551	3578	3580	3583	rBV2	485	313	0.02%	0.003%
100	13.079	3741	3744	3747	rBV2	386	321	0.02%	0.003%




Sum of corrected areas: 11182799

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029556.D
Acq On : 10 Dec 2022 05:04
Operator : SY/MD
Sample : N5915-17 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

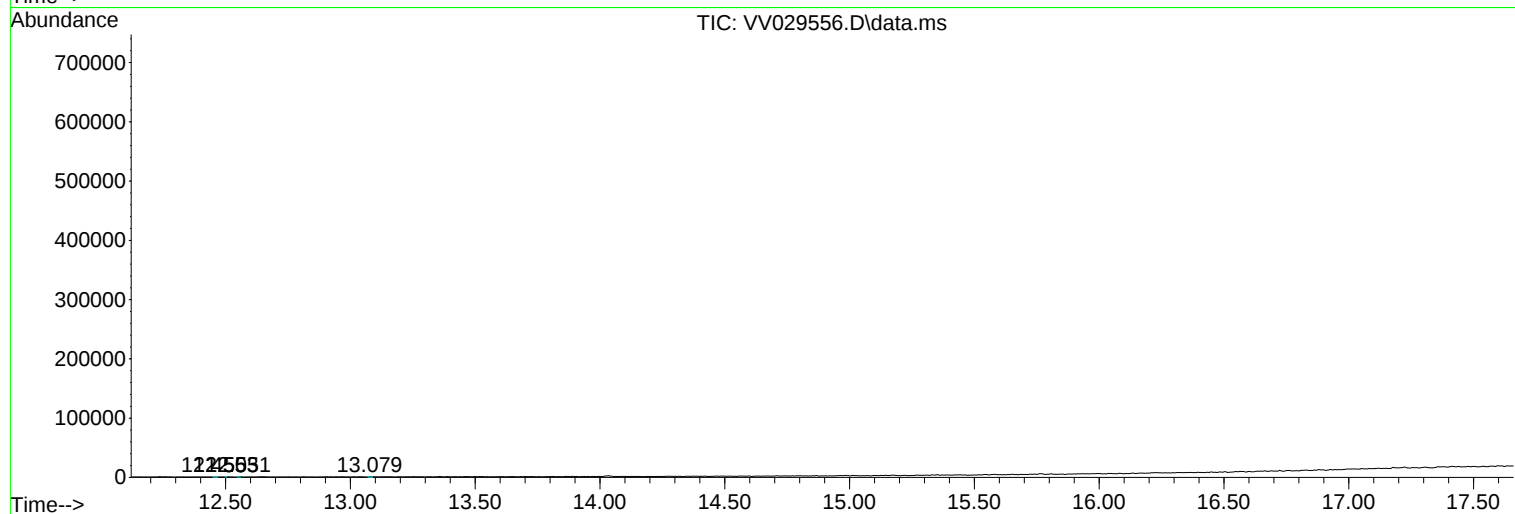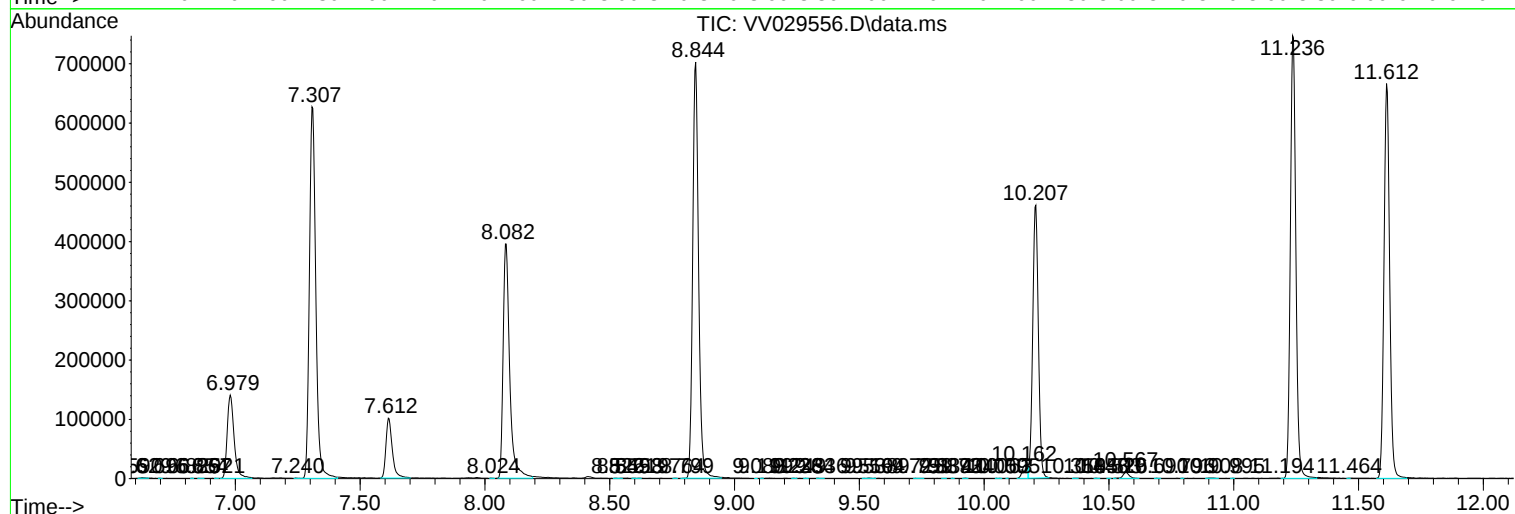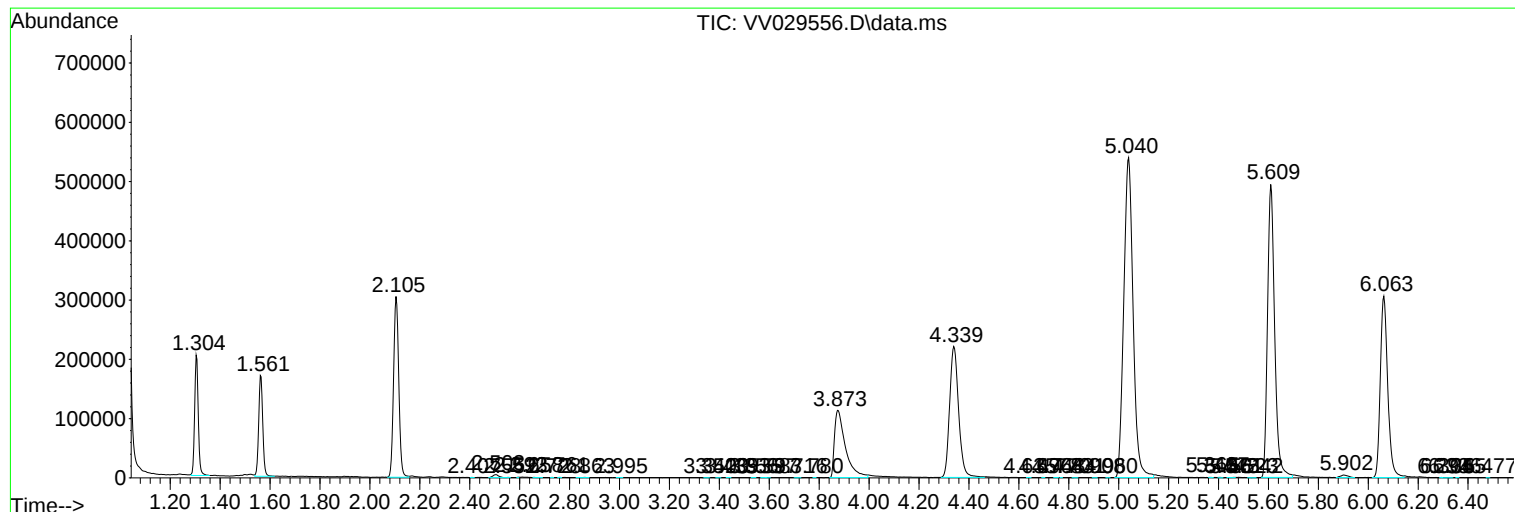

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029556.D
Acq On : 10 Dec 2022 05:04
Operator : SY/MD
Sample : N5915-17 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029556.D
Acq On : 10 Dec 2022 05:04
Operator : SY/MD
Sample : N5915-17 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------