

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029558.D
 Acq On : 10 Dec 2022 05:51
 Operator : SY/MD
 Sample : N5929-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB2	247287	253479	15.22%	1.916%
2	1.565	156	163	176	rVB	142165	160207	9.62%	1.211%
3	2.105	321	331	344	rBV	280807	408919	24.55%	3.092%
4	2.433	430	433	435	rBV2	226	171	0.01%	0.001%
5	2.500	449	454	463	rBV3	991	1378	0.08%	0.010%
6	2.574	473	477	483	rVB4	697	655	0.04%	0.005%
7	2.635	485	496	500	rBV2	1034	1728	0.10%	0.013%
8	2.703	514	517	519	rBV2	134	76	0.00%	0.001%
9	2.757	524	534	559	rVB	26462	48490	2.91%	0.367%
10	2.896	575	577	578	rBV2	166	50	0.00%	0.000%
11	2.941	589	591	596	rBV2	255	230	0.01%	0.002%
12	2.999	607	609	613	rVB2	288	153	0.01%	0.001%
13	3.114	642	645	650	rBV	179	136	0.01%	0.001%
14	3.182	650	666	687	rBV	357556	749861	45.02%	5.669%
15	3.449	746	749	752	rVB2	301	177	0.01%	0.001%
16	3.468	753	755	757	rBV	239	84	0.01%	0.001%
17	3.532	773	775	780	rVB2	204	108	0.01%	0.001%
18	3.597	793	795	798	rBV2	135	83	0.00%	0.001%
19	3.671	815	818	819	rBV2	58	28	0.00%	0.000%
20	3.687	821	823	828	rBV2	164	140	0.01%	0.001%
21	3.786	852	854	855	rBV	79	38	0.00%	0.000%
22	3.828	866	867	870	rVB2	180	94	0.01%	0.001%
23	3.902	871	890	928	rBV2	610746	1665728	100.00%	12.594%
24	4.339	1008	1026	1054	rBV	186272	466744	28.02%	3.529%
25	4.600	1091	1107	1129	rBV	150369	377068	22.64%	2.851%
26	4.806	1168	1171	1173	rBV2	186	132	0.01%	0.001%
27	4.831	1177	1179	1181	rVB	290	155	0.01%	0.001%
28	4.854	1181	1186	1189	rBV	156	168	0.01%	0.001%
29	4.941	1211	1213	1219	rBV	223	137	0.01%	0.001%
30	5.040	1225	1244	1289	rBV2	457466	1230358	73.86%	9.302%
31	5.391	1350	1353	1355	rBV	286	190	0.01%	0.001%
32	5.426	1361	1364	1367	rBV2	173	103	0.01%	0.001%
33	5.445	1368	1370	1373	rVB	256	128	0.01%	0.001%
34	5.461	1373	1375	1376	rBV	128	51	0.00%	0.000%
35	5.478	1376	1380	1382	rBV2	222	220	0.01%	0.002%
36	5.539	1398	1399	1400	rBV2	115	28	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029558.D
 Acq On : 10 Dec 2022 05:51
 Operator : SY/MD
 Sample : N5929-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1408	1421	1448	rBV	516465	1042206	62.57%	7.879%
38	5.912	1502	1515	1541	rBV	74446	154589	9.28%	1.169%
39	6.063	1548	1562	1595	rBV	258578	534132	32.07%	4.038%
40	6.252	1619	1621	1624	rVB2	342	162	0.01%	0.001%
41	6.269	1624	1626	1628	rBV	115	64	0.00%	0.000%
42	6.281	1628	1630	1632	rBV	176	72	0.00%	0.001%
43	6.310	1637	1639	1643	rVB2	188	89	0.01%	0.001%
44	6.336	1644	1647	1649	rBV2	172	110	0.01%	0.001%
45	6.391	1655	1664	1671	rBV4	1500	2608	0.16%	0.020%
46	6.452	1680	1683	1686	rBV2	88	56	0.00%	0.000%
47	6.539	1709	1710	1714	rVB	187	118	0.01%	0.001%
48	6.584	1721	1724	1727	rBV	199	156	0.01%	0.001%
49	6.625	1731	1737	1742	rBV4	712	838	0.05%	0.006%
50	6.738	1770	1772	1774	rVB2	217	72	0.00%	0.001%
51	6.751	1774	1776	1778	rBV	184	96	0.01%	0.001%
52	6.812	1793	1795	1796	rBV	147	48	0.00%	0.000%
53	6.854	1803	1808	1811	rBV2	131	135	0.01%	0.001%
54	6.905	1820	1824	1825	rBV2	182	94	0.01%	0.001%
55	6.979	1834	1847	1878	rBV	121674	229031	13.75%	1.732%
56	7.191	1909	1913	1916	rBV2	406	443	0.03%	0.003%
57	7.307	1937	1949	1982	rBV	557586	1000729	60.08%	7.566%
58	7.616	2034	2045	2069	rBV	85470	153541	9.22%	1.161%
59	7.834	2105	2113	2114	rBV4	2599	2588	0.16%	0.020%
60	7.937	2129	2145	2146	rBV	7684	10730	0.64%	0.081%
61	8.085	2181	2191	2226	rBV	294905	549311	32.98%	4.153%
62	8.403	2288	2290	2292	rVB	290	123	0.01%	0.001%
63	8.606	2348	2353	2355	rBV2	402	296	0.02%	0.002%
64	8.844	2414	2427	2472	rBV	750136	1251890	75.16%	9.465%
65	9.069	2495	2497	2501	rVB2	578	257	0.02%	0.002%
66	9.133	2512	2517	2518	rBV4	464	378	0.02%	0.003%
67	9.191	2529	2535	2536	rBV2	157	133	0.01%	0.001%
68	9.217	2541	2543	2544	rBV	133	40	0.00%	0.000%
69	9.259	2552	2556	2557	rBV	182	118	0.01%	0.001%
70	9.346	2582	2583	2585	rVB	269	98	0.01%	0.001%
71	9.436	2609	2611	2614	rBV	104	87	0.01%	0.001%
72	9.477	2621	2624	2627	rVB	317	176	0.01%	0.001%
73	9.510	2632	2634	2636	rBV2	112	51	0.00%	0.000%
74	9.625	2668	2670	2672	rBV	185	79	0.00%	0.001%
75	9.802	2722	2725	2726	rBV	212	76	0.00%	0.001%
76	9.831	2731	2734	2737	rBV	365	214	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029558.D
 Acq On : 10 Dec 2022 05:51
 Operator : SY/MD
 Sample : N5929-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.998	2784	2786	2787	rBV	188	85	0.01%	0.001%
78	10.008	2787	2789	2791	rVB2	227	105	0.01%	0.001%
79	10.165	2828	2838	2841	rBV2	17598	25702	1.54%	0.194%
80	10.204	2842	2850	2870	rVB	378303	599298	35.98%	4.531%
81	10.371	2894	2902	2912	rBV2	9023	13870	0.83%	0.105%
82	10.493	2939	2940	2941	rBV	192	49	0.00%	0.000%
83	10.522	2947	2949	2951	rBV3	441	167	0.01%	0.001%
84	10.567	2955	2963	2975	rVV2	7948	12688	0.76%	0.096%
85	10.648	2986	2988	2992	rBV2	233	114	0.01%	0.001%
86	10.667	2992	2994	2998	rBV	189	123	0.01%	0.001%
87	10.902	3064	3067	3068	rBV3	510	353	0.02%	0.003%
88	11.027	3104	3106	3111	rVB	380	230	0.01%	0.002%
89	11.127	3135	3137	3140	rBV2	167	109	0.01%	0.001%
90	11.236	3159	3171	3205	rBV	827448	1301531	78.14%	9.840%
91	11.612	3276	3288	3313	rBV	606556	962775	57.80%	7.279%
92	11.982	3400	3403	3406	rBV3	268	235	0.01%	0.002%
93	11.998	3406	3408	3411	rBV2	288	206	0.01%	0.002%
94	12.034	3416	3419	3420	rBV	231	125	0.01%	0.001%
95	12.075	3429	3432	3434	rBV2	262	182	0.01%	0.001%
96	12.149	3451	3455	3459	rBV3	603	438	0.03%	0.003%
97	12.239	3473	3483	3494	rBV3	2195	4088	0.25%	0.031%
98	12.638	3603	3607	3609	rBV2	495	425	0.03%	0.003%
99	12.702	3625	3627	3629	rBV	329	149	0.01%	0.001%
100	12.773	3645	3649	3650	rBV	339	242	0.01%	0.002%




Sum of corrected areas: 13226818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029558.D
Acq On : 10 Dec 2022 05:51
Operator : SY/MD
Sample : N5929-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

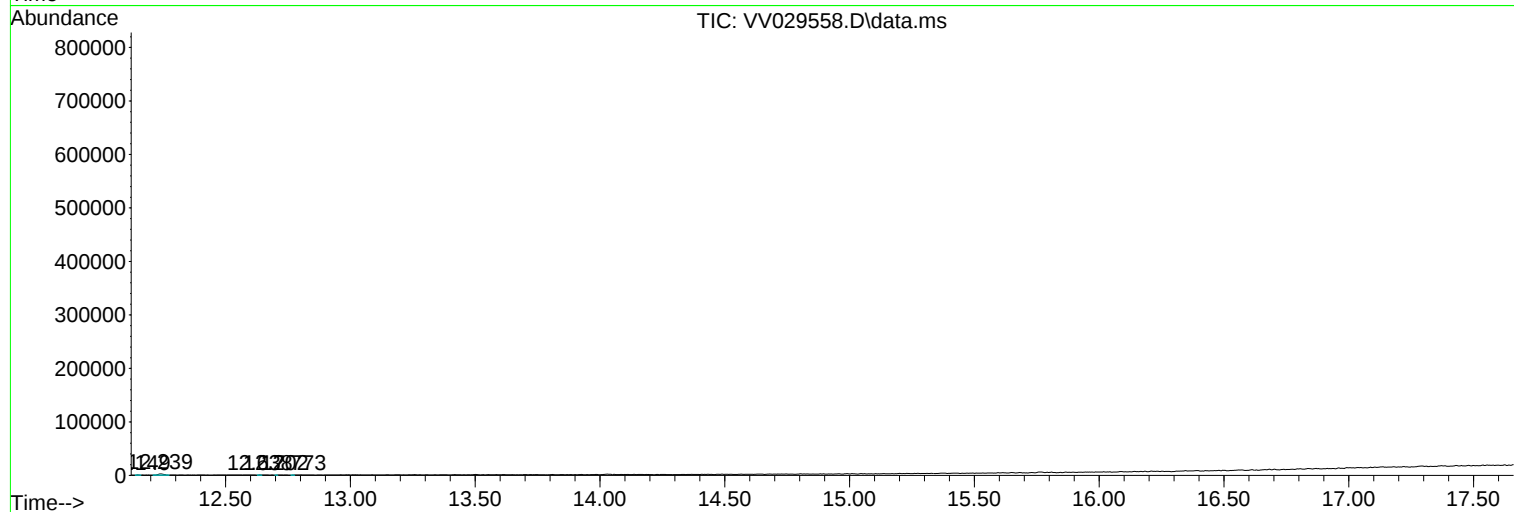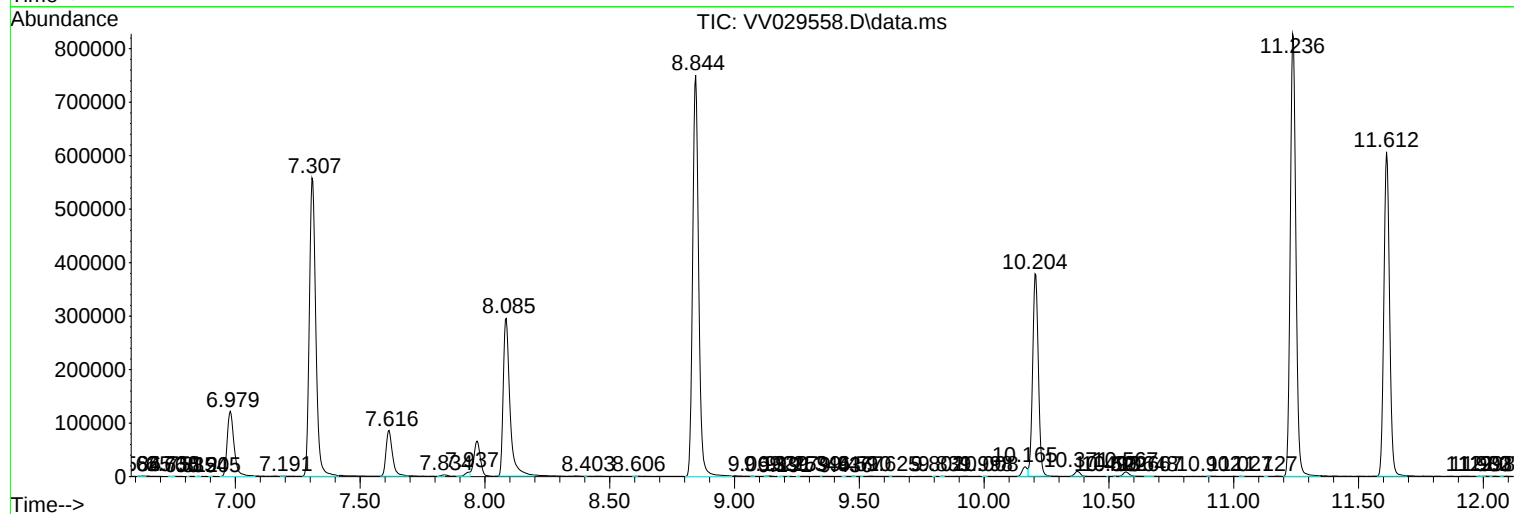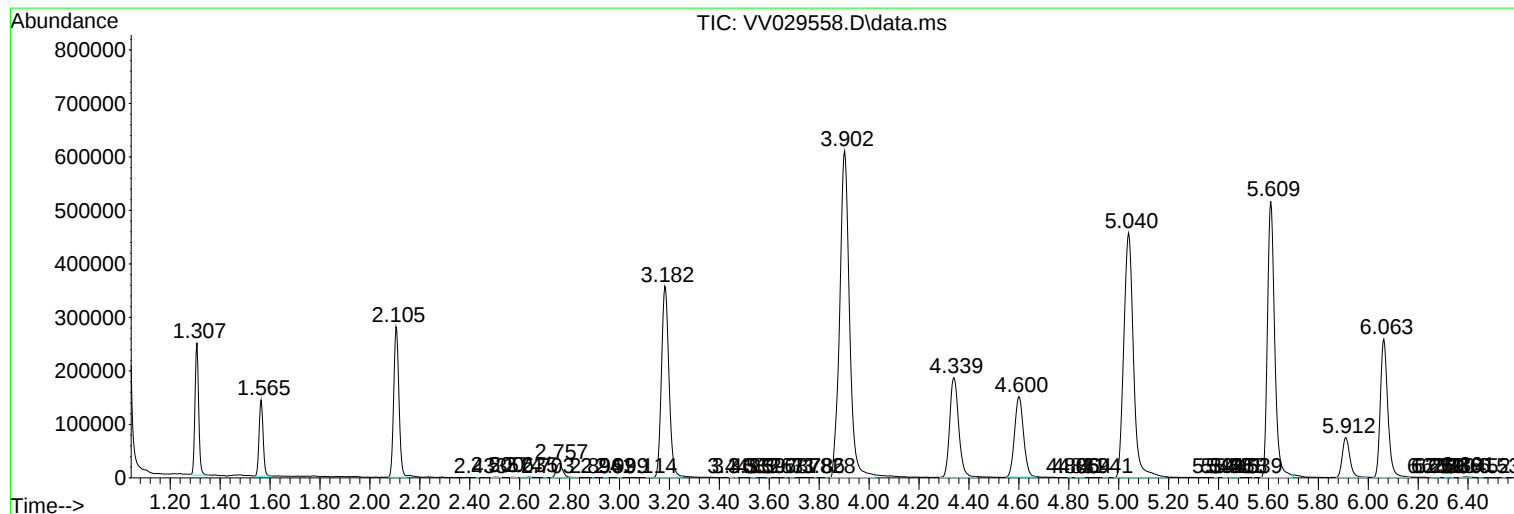

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029558.D
Acq On : 10 Dec 2022 05:51
Operator : SY/MD
Sample : N5929-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029558.D
Acq On : 10 Dec 2022 05:51
Operator : SY/MD
Sample : N5929-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------