

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029559.D
 Acq On : 10 Dec 2022 06:14
 Operator : SY/MD
 Sample : N5929-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029559.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	215728	219962	14.69%	1.680%
2	1.565	156	163	180	rVB	176291	193761	12.94%	1.480%
3	2.105	321	331	345	rBV	336786	483949	32.32%	3.696%
4	2.352	406	408	411	rBV2	306	223	0.01%	0.002%
5	2.426	429	431	433	rVB	300	98	0.01%	0.001%
6	2.507	446	456	462	rBV5	1049	1777	0.12%	0.014%
7	2.555	469	471	476	rBV3	183	166	0.01%	0.001%
8	2.677	504	509	513	rBV2	298	257	0.02%	0.002%
9	2.696	513	515	518	rBV2	276	122	0.01%	0.001%
10	2.761	526	535	546	rBV2	8581	14653	0.98%	0.112%
11	2.838	556	559	560	rBV2	196	114	0.01%	0.001%
12	2.915	580	583	586	rBV	155	119	0.01%	0.001%
13	3.185	653	667	691	rBV	135747	285786	19.09%	2.183%
14	3.404	731	735	738	rBV2	233	178	0.01%	0.001%
15	3.497	762	764	770	rVB2	249	165	0.01%	0.001%
16	3.529	772	774	781	rVB2	232	182	0.01%	0.001%
17	3.613	797	800	806	rBV2	168	193	0.01%	0.001%
18	3.645	806	810	813	rBV	275	177	0.01%	0.001%
19	3.835	864	869	871	rBV	178	106	0.01%	0.001%
20	3.902	871	890	937	rBV2	221226	753032	50.30%	5.751%
21	4.339	1009	1026	1059	rBV	233156	576175	38.48%	4.401%
22	4.600	1092	1107	1125	rBV2	60695	149905	10.01%	1.145%
23	4.696	1135	1137	1141	rBV3	420	274	0.02%	0.002%
24	4.719	1141	1144	1147	rVB2	451	302	0.02%	0.002%
25	4.735	1147	1149	1152	rBV	168	82	0.01%	0.001%
26	4.751	1152	1154	1158	rVB2	287	142	0.01%	0.001%
27	4.773	1158	1161	1164	rBV2	280	170	0.01%	0.001%
28	4.809	1169	1172	1173	rBV	180	97	0.01%	0.001%
29	4.857	1186	1187	1191	rVB2	229	102	0.01%	0.001%
30	4.883	1194	1195	1199	rVB	186	87	0.01%	0.001%
31	4.902	1199	1201	1205	rBV	166	79	0.01%	0.001%
32	4.934	1205	1211	1213	rBV3	172	178	0.01%	0.001%
33	4.976	1221	1224	1225	rBV	219	98	0.01%	0.001%
34	5.040	1226	1244	1288	rVV2	565987	1497188	100.00%	11.435%
35	5.465	1372	1376	1379	rBV3	479	348	0.02%	0.003%
36	5.500	1385	1387	1393	rBV3	244	184	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029559.D
 Acq On : 10 Dec 2022 06:14
 Operator : SY/MD
 Sample : N5929-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.529	1393	1396	1400	rVB3	315	284	0.02%	0.002%
38	5.548	1400	1402	1404	rBV	192	91	0.01%	0.001%
39	5.609	1404	1421	1447	rBV	551937	1111928	74.27%	8.493%
40	5.912	1504	1515	1538	rVB4	22602	50017	3.34%	0.382%
41	6.063	1548	1562	1587	rBV	320722	659156	44.03%	5.034%
42	6.252	1619	1621	1624	rVB3	344	190	0.01%	0.001%
43	6.397	1657	1666	1675	rBV4	1239	2483	0.17%	0.019%
44	6.468	1686	1688	1690	rBV	126	72	0.00%	0.001%
45	6.555	1712	1715	1718	rBV2	164	143	0.01%	0.001%
46	6.568	1718	1719	1723	rBV	265	178	0.01%	0.001%
47	6.619	1729	1735	1736	rBV2	816	696	0.05%	0.005%
48	6.715	1763	1765	1768	rVB2	309	125	0.01%	0.001%
49	6.760	1776	1779	1781	rVB	164	94	0.01%	0.001%
50	6.793	1786	1789	1792	rBV2	197	156	0.01%	0.001%
51	6.825	1794	1799	1802	rBV2	250	264	0.02%	0.002%
52	6.931	1831	1832	1835	rBV2	174	97	0.01%	0.001%
53	6.979	1835	1847	1882	rVV	149436	279948	18.70%	2.138%
54	7.149	1897	1900	1901	rBV2	537	311	0.02%	0.002%
55	7.230	1923	1925	1928	rBV3	361	232	0.02%	0.002%
56	7.307	1937	1949	1977	rBV	697554	1228572	82.06%	9.383%
57	7.613	2034	2044	2073	rBV	105406	190517	12.72%	1.455%
58	7.793	2098	2100	2102	rVB3	513	194	0.01%	0.001%
59	7.931	2134	2143	2148	rBV3	10200	17074	1.14%	0.130%
60	8.082	2180	2190	2234	rBV	368320	682533	45.59%	5.213%
61	8.545	2331	2334	2337	rBV2	452	285	0.02%	0.002%
62	8.564	2338	2340	2342	rBV	317	147	0.01%	0.001%
63	8.645	2363	2365	2368	rVB3	233	126	0.01%	0.001%
64	8.719	2385	2388	2389	rBV3	238	127	0.01%	0.001%
65	8.844	2414	2427	2455	rBV	816842	1330666	88.88%	10.163%
66	9.178	2528	2531	2532	rBV	154	81	0.01%	0.001%
67	9.210	2538	2541	2543	rBV2	296	191	0.01%	0.001%
68	9.342	2579	2582	2584	rBV	239	173	0.01%	0.001%
69	9.410	2601	2603	2606	rBV2	157	90	0.01%	0.001%
70	9.445	2611	2614	2617	rVV	253	148	0.01%	0.001%
71	9.519	2635	2637	2638	rBV	253	106	0.01%	0.001%
72	9.564	2648	2651	2654	rVB2	536	330	0.02%	0.003%
73	9.587	2656	2658	2661	rVB2	222	97	0.01%	0.001%
74	9.638	2672	2674	2677	rVB	224	94	0.01%	0.001%
75	9.664	2677	2682	2684	rBV	309	247	0.02%	0.002%
76	9.722	2697	2700	2702	rBV2	361	209	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029559.D
 Acq On : 10 Dec 2022 06:14
 Operator : SY/MD
 Sample : N5929-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.735	2702	2704	2710	rVV2	294	251	0.02%	0.002%
78	9.834	2732	2735	2738	rBV2	336	253	0.02%	0.002%
79	9.921	2756	2762	2769	rBV3	416	658	0.04%	0.005%
80	9.953	2769	2772	2775	rVV2	185	131	0.01%	0.001%
81	10.059	2802	2805	2811	rVB2	240	208	0.01%	0.002%
82	10.114	2817	2822	2825	rBV2	233	207	0.01%	0.002%
83	10.162	2827	2837	2841	rVV2	21799	31945	2.13%	0.244%
84	10.204	2842	2850	2873	rVB	465081	738530	49.33%	5.641%
85	10.371	2892	2902	2915	rBV2	14320	23042	1.54%	0.176%
86	10.423	2916	2918	2925	rVB2	495	352	0.02%	0.003%
87	10.500	2939	2942	2945	rBV2	210	176	0.01%	0.001%
88	10.526	2947	2950	2952	rBV2	489	295	0.02%	0.002%
89	10.567	2955	2963	2974	rVB2	9555	15412	1.03%	0.118%
90	10.661	2989	2992	2995	rBV	266	149	0.01%	0.001%
91	10.715	3007	3009	3013	rVB	250	132	0.01%	0.001%
92	10.783	3028	3030	3034	rVB	271	134	0.01%	0.001%
93	10.805	3034	3037	3040	rBV2	214	166	0.01%	0.001%
94	10.834	3041	3046	3047	rBV3	296	239	0.02%	0.002%
95	11.018	3101	3103	3106	rBV	185	94	0.01%	0.001%
96	11.236	3159	3171	3201	rBV	892191	1381274	92.26%	10.550%
97	11.558	3265	3271	3273	rBV3	806	863	0.06%	0.007%
98	11.612	3276	3288	3313	rVV	738865	1159194	77.42%	8.854%
99	12.040	3419	3421	3424	rBV	259	108	0.01%	0.001%
100	12.802	3656	3658	3662	rVB3	415	195	0.01%	0.001%




Sum of corrected areas: 13092911

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029559.D
Acq On : 10 Dec 2022 06:14
Operator : SY/MD
Sample : N5929-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

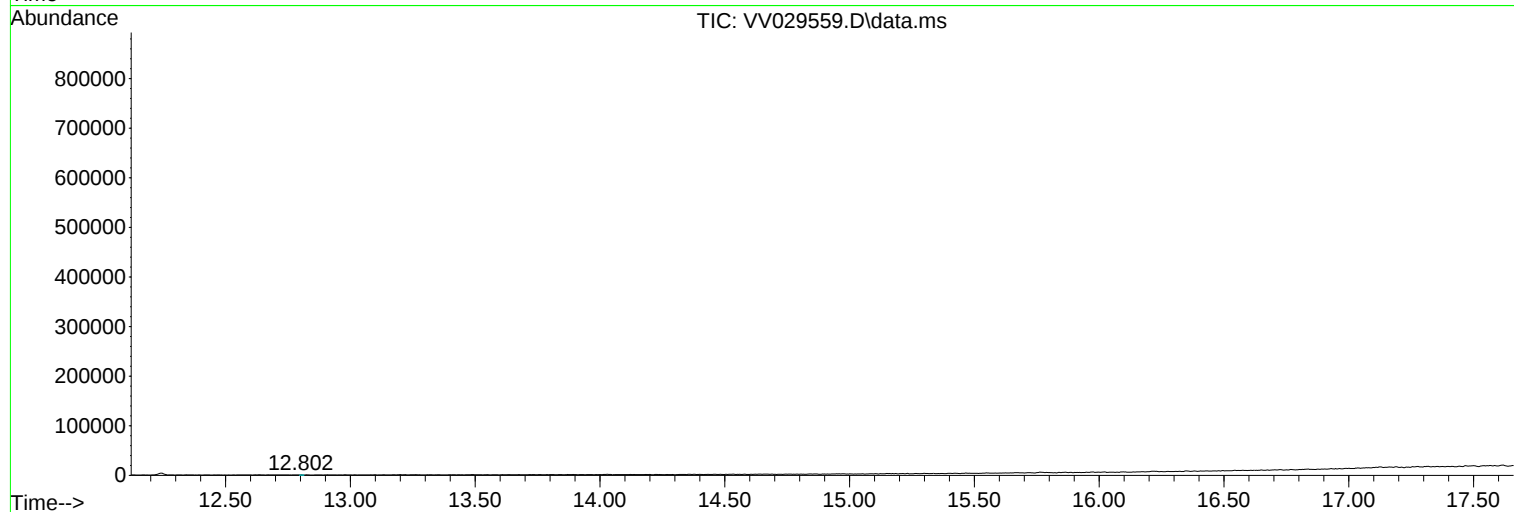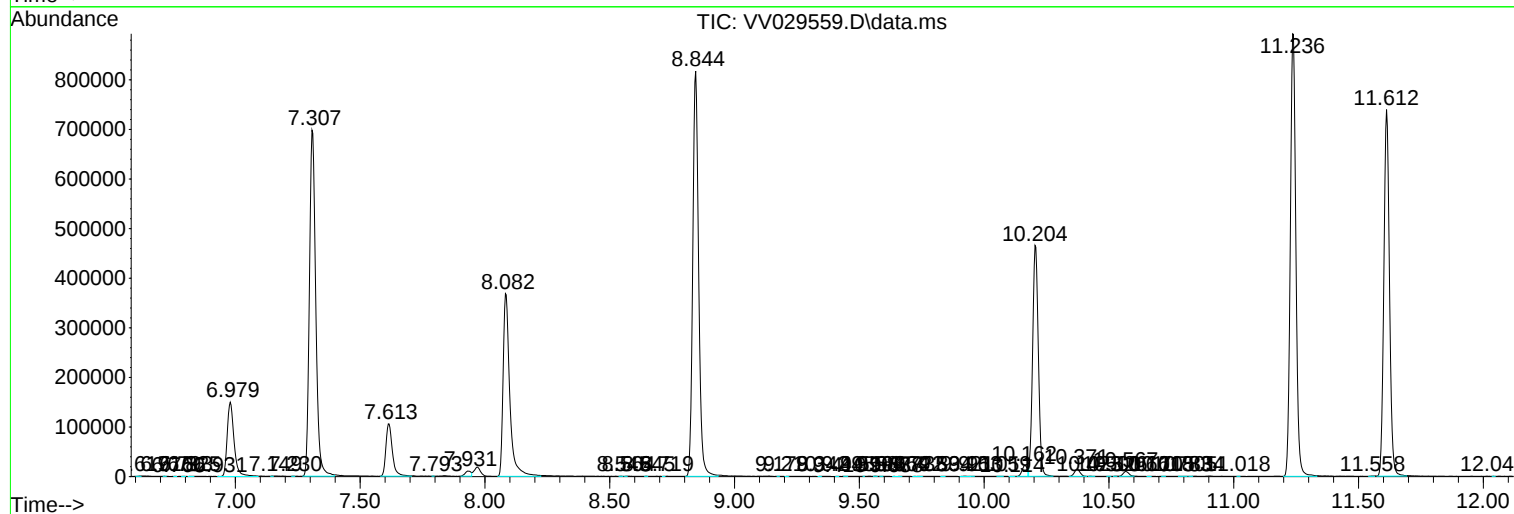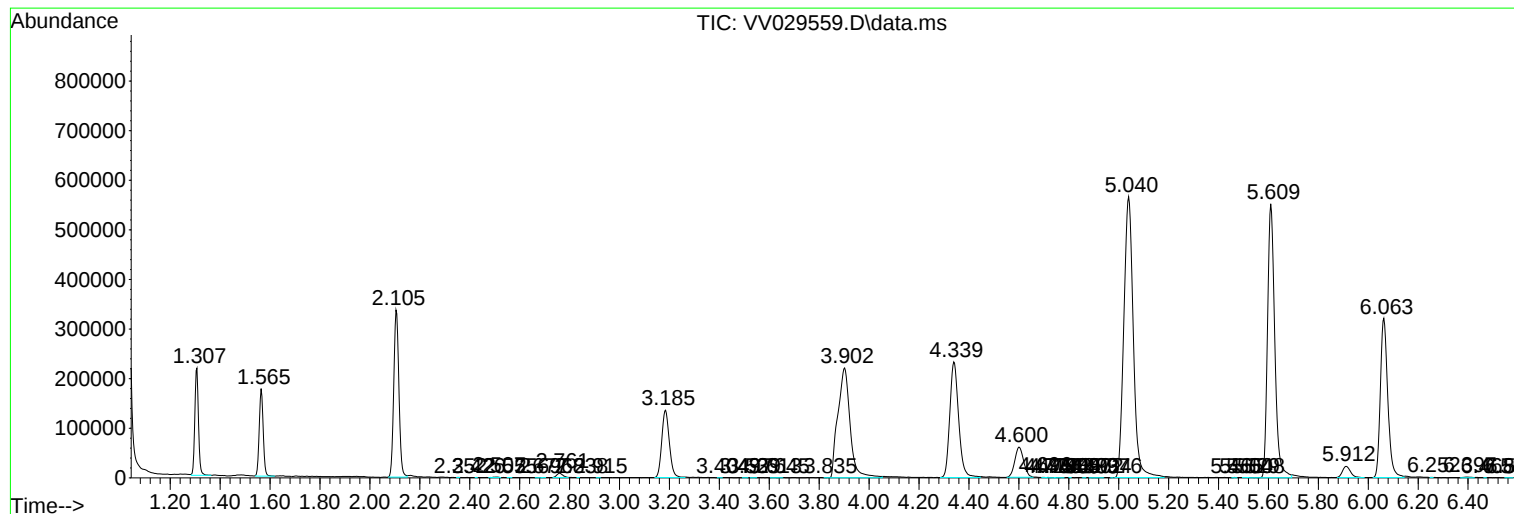

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029559.D
Acq On : 10 Dec 2022 06:14
Operator : SY/MD
Sample : N5929-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029559.D
Acq On : 10 Dec 2022 06:14
Operator : SY/MD
Sample : N5929-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------