

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029560.D
 Acq On : 10 Dec 2022 06:38
 Operator : SY/MD
 Sample : N5929-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	210581	212902	14.14%	1.693%
2	1.564	156	163	175	rVB	178677	197692	13.13%	1.572%
3	2.105	321	331	345	rBV	334213	483224	32.10%	3.842%
4	2.506	449	456	463	rVB4	897	1457	0.10%	0.012%
5	2.703	514	517	520	rBV2	157	117	0.01%	0.001%
6	2.764	525	536	550	rVV3	4949	9431	0.63%	0.075%
7	2.915	581	583	585	rBV	130	74	0.00%	0.001%
8	2.976	598	602	606	rBV2	215	163	0.01%	0.001%
9	3.188	654	668	682	rBV	20244	43101	2.86%	0.343%
10	3.297	700	702	703	rBV	172	79	0.01%	0.001%
11	3.375	723	726	729	rBV2	196	140	0.01%	0.001%
12	3.690	821	824	827	rBV2	245	151	0.01%	0.001%
13	3.725	832	835	842	rBV3	276	289	0.02%	0.002%
14	3.873	871	881	920	rBV	106980	328383	21.82%	2.611%
15	4.214	986	987	990	rBV2	296	146	0.01%	0.001%
16	4.339	1011	1026	1054	rBV2	232305	571809	37.99%	4.547%
17	4.603	1094	1108	1126	rVB2	43849	108756	7.23%	0.865%
18	4.744	1149	1152	1157	rBV2	342	197	0.01%	0.002%
19	4.841	1179	1182	1186	rVB	231	158	0.01%	0.001%
20	4.873	1186	1192	1193	rBV2	166	185	0.01%	0.001%
21	4.902	1198	1201	1203	rBV2	194	130	0.01%	0.001%
22	4.931	1208	1210	1214	rVB2	241	125	0.01%	0.001%
23	5.040	1226	1244	1283	rBV2	571448	1505201	100.00%	11.969%
24	5.362	1342	1344	1348	rBV3	205	119	0.01%	0.001%
25	5.420	1361	1362	1366	rVB	248	96	0.01%	0.001%
26	5.551	1400	1403	1404	rBV2	108	62	0.00%	0.000%
27	5.609	1408	1421	1455	rBV	548266	1115134	74.09%	8.867%
28	5.911	1502	1515	1533	rBV3	30744	67044	4.45%	0.533%
29	6.063	1548	1562	1592	rBV	323526	670244	44.53%	5.329%
30	6.320	1637	1642	1647	rBB2	160	136	0.01%	0.001%
31	6.355	1650	1653	1654	rBV	137	59	0.00%	0.000%
32	6.436	1674	1678	1681	rBV2	173	184	0.01%	0.001%
33	6.481	1688	1692	1697	rVB2	192	156	0.01%	0.001%
34	6.503	1697	1699	1703	rBV3	335	205	0.01%	0.002%
35	6.522	1703	1705	1709	rVV2	195	108	0.01%	0.001%
36	6.555	1713	1715	1719	rBV	171	109	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029560.D
 Acq On : 10 Dec 2022 06:38
 Operator : SY/MD
 Sample : N5929-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.628	1730	1738	1743	rBV5	1210	1764	0.12%	0.014%
38	6.702	1760	1761	1768	rBV3	307	242	0.02%	0.002%
39	6.741	1771	1773	1776	rVB	194	78	0.01%	0.001%
40	6.767	1776	1781	1784	rBV2	177	179	0.01%	0.001%
41	6.796	1787	1790	1792	rBV	196	97	0.01%	0.001%
42	6.841	1801	1804	1808	rVB2	371	241	0.02%	0.002%
43	6.876	1812	1815	1816	rBV2	185	95	0.01%	0.001%
44	6.979	1836	1847	1875	rBV	149863	277749	18.45%	2.209%
45	7.143	1896	1898	1899	rBV	274	115	0.01%	0.001%
46	7.159	1899	1903	1904	rBV2	646	413	0.03%	0.003%
47	7.220	1919	1922	1923	rBV2	322	151	0.01%	0.001%
48	7.307	1937	1949	1980	rBV	699058	1239499	82.35%	9.856%
49	7.616	2035	2045	2069	rBV	105994	188575	12.53%	1.499%
50	7.754	2086	2088	2092	rVB3	648	481	0.03%	0.004%
51	7.776	2092	2095	2098	rBV2	623	394	0.03%	0.003%
52	7.934	2135	2144	2151	rBV4	7405	13479	0.90%	0.107%
53	8.014	2167	2169	2172	rBV3	304	159	0.01%	0.001%
54	8.085	2180	2191	2230	rBV	391832	717321	47.66%	5.704%
55	8.519	2324	2326	2329	rBV2	321	234	0.02%	0.002%
56	8.622	2355	2358	2362	rBV2	334	241	0.02%	0.002%
57	8.702	2380	2383	2386	rBV3	233	173	0.01%	0.001%
58	8.760	2398	2401	2404	rBB3	174	110	0.01%	0.001%
59	8.792	2408	2411	2415	rBV3	307	256	0.02%	0.002%
60	8.844	2415	2427	2449	rBV	804667	1317428	87.53%	10.476%
61	9.127	2511	2515	2516	rBV4	1277	831	0.06%	0.007%
62	9.217	2541	2543	2545	rBV2	210	128	0.01%	0.001%
63	9.233	2545	2548	2555	rVB2	527	447	0.03%	0.004%
64	9.262	2555	2557	2560	rBV2	293	184	0.01%	0.001%
65	9.307	2569	2571	2578	rVB3	807	563	0.04%	0.004%
66	9.406	2599	2602	2606	rVB2	299	200	0.01%	0.002%
67	9.461	2608	2619	2620	rBV4	1753	2180	0.14%	0.017%
68	9.542	2637	2644	2650	rBV4	1586	2397	0.16%	0.019%
69	9.667	2676	2683	2684	rBV2	1352	1398	0.09%	0.011%
70	9.796	2714	2723	2733	rVB8	3429	5860	0.39%	0.047%
71	9.841	2734	2737	2740	rVV2	285	193	0.01%	0.002%
72	9.860	2740	2743	2750	rVB3	463	555	0.04%	0.004%
73	9.924	2752	2763	2770	rBV4	1507	2479	0.16%	0.020%
74	9.972	2773	2778	2781	rBV4	292	259	0.02%	0.002%
75	10.021	2790	2793	2796	rBV2	253	193	0.01%	0.002%
76	10.046	2798	2801	2807	rVB2	329	252	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029560.D
 Acq On : 10 Dec 2022 06:38
 Operator : SY/MD
 Sample : N5929-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.117	2815	2823	2829	rBV6	3438	5166	0.34%	0.041%
78	10.162	2829	2837	2841	rVV	21310	31124	2.07%	0.247%
79	10.207	2842	2851	2877	rVB	473880	756000	50.23%	6.011%
80	10.352	2886	2896	2897	rBV2	5985	7946	0.53%	0.063%
81	10.529	2942	2951	2957	rBV	7690	11286	0.75%	0.090%
82	10.728	3004	3013	3024	rBV4	9694	14566	0.97%	0.116%
83	10.905	3056	3068	3084	rBV2	22723	35872	2.38%	0.285%
84	11.046	3106	3112	3115	rBV2	2158	2538	0.17%	0.020%
85	11.185	3148	3155	3160	rBV5	2946	4153	0.28%	0.033%
86	11.239	3160	3172	3193	rBV	884028	1364672	90.66%	10.851%
87	11.442	3231	3235	3238	rBV5	741	648	0.04%	0.005%
88	11.538	3252	3265	3266	rBV6	4696	7800	0.52%	0.062%
89	11.612	3277	3288	3310	rVB	750398	1196692	79.50%	9.516%
90	11.808	3343	3349	3358	rVB2	6460	8773	0.58%	0.070%
91	11.902	3371	3378	3382	rBV2	4688	6213	0.41%	0.049%
92	11.972	3397	3400	3401	rBV2	663	407	0.03%	0.003%
93	12.004	3404	3410	3417	rVV	6311	8368	0.56%	0.067%
94	12.107	3434	3442	3445	rBV2	2519	3524	0.23%	0.028%
95	12.361	3519	3521	3522	rBV	854	368	0.02%	0.003%
96	12.455	3543	3550	3560	rVB	7150	10149	0.67%	0.081%
97	12.538	3571	3576	3582	rBV6	2175	2661	0.18%	0.021%
98	12.773	3647	3649	3650	rBV	595	247	0.02%	0.002%
99	12.834	3663	3668	3670	rBV3	1172	1016	0.07%	0.008%
100	12.988	3713	3716	3721	rBV4	1021	871	0.06%	0.007%




Sum of corrected areas: 12576219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029560.D
Acq On : 10 Dec 2022 06:38
Operator : SY/MD
Sample : N5929-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

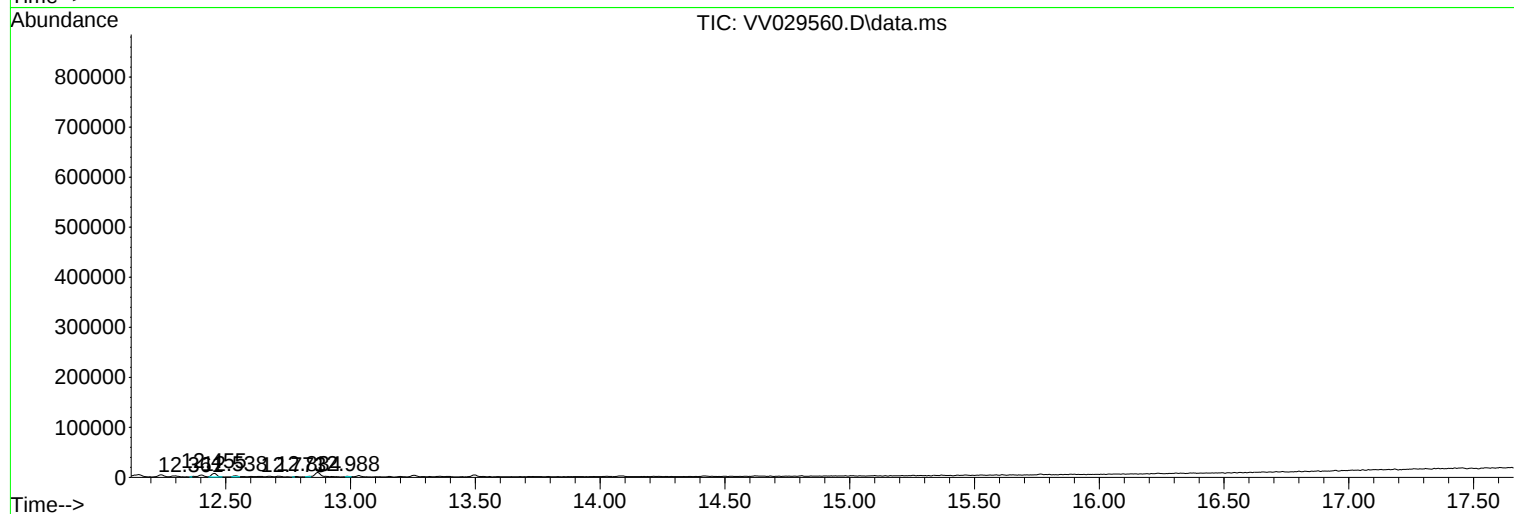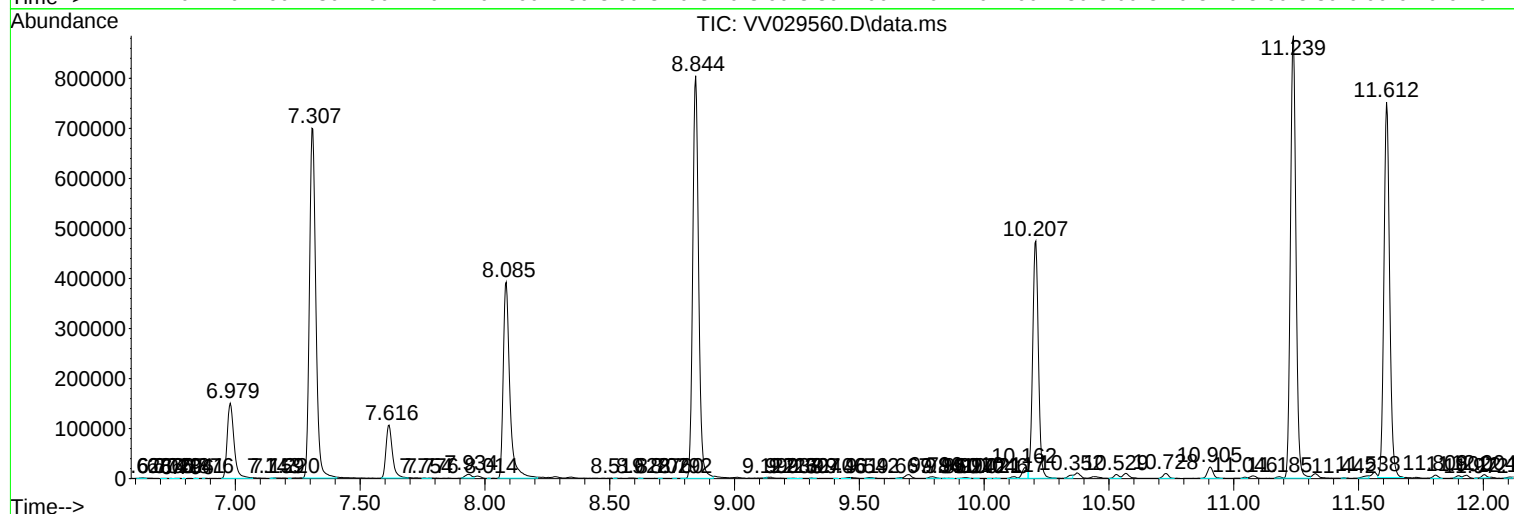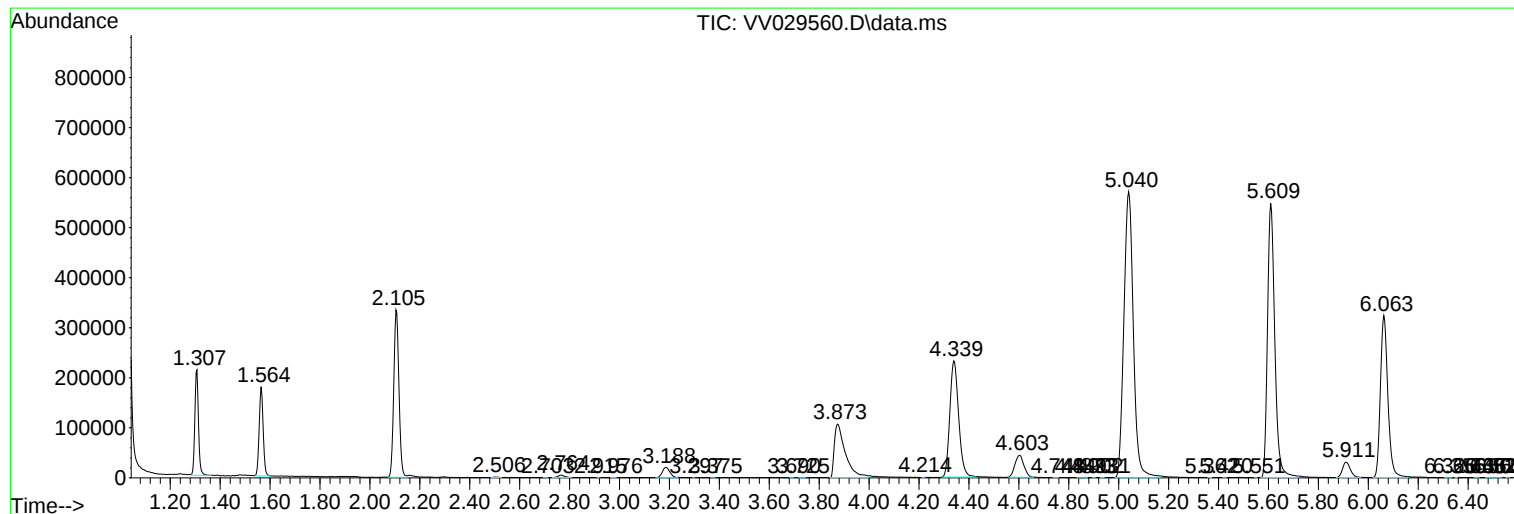

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029560.D
Acq On : 10 Dec 2022 06:38
Operator : SY/MD
Sample : N5929-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029560.D
Acq On : 10 Dec 2022 06:38
Operator : SY/MD
Sample : N5929-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc