

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029564.D
 Acq On : 10 Dec 2022 08:35
 Operator : SY/MD
 Sample : N5929-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rVB	192837	195574	14.15%	1.601%
2	1.564	156	163	175	rVB	165314	185836	13.45%	1.522%
3	2.108	321	332	353	rBV3	336780	536825	38.85%	4.396%
4	2.291	382	389	396	rVB4	998	1492	0.11%	0.012%
5	2.503	447	455	465	rVV2	4193	6828	0.49%	0.056%
6	2.609	481	488	495	rBV5	1137	1528	0.11%	0.013%
7	2.667	504	506	508	rBV	161	60	0.00%	0.000%
8	2.761	528	535	547	rVB3	3107	5051	0.37%	0.041%
9	2.925	582	586	588	rBV2	178	138	0.01%	0.001%
10	3.082	632	635	640	rBV	169	120	0.01%	0.001%
11	3.127	647	649	652	rVB	190	70	0.01%	0.001%
12	3.185	652	667	690	rBV	71221	151418	10.96%	1.240%
13	3.516	766	770	771	rBV2	100	74	0.01%	0.001%
14	3.529	771	774	777	rVB2	190	105	0.01%	0.001%
15	3.658	809	814	816	rBV2	217	152	0.01%	0.001%
16	3.706	826	829	832	rVB	284	180	0.01%	0.001%
17	3.735	832	838	842	rBV	325	302	0.02%	0.002%
18	3.879	871	883	918	rBV3	124639	455632	32.97%	3.731%
19	4.339	1009	1026	1055	rBV	218192	544490	39.40%	4.458%
20	4.600	1089	1107	1130	rBV2	189884	480285	34.76%	3.933%
21	4.793	1165	1167	1172	rBV2	179	178	0.01%	0.001%
22	4.876	1189	1193	1195	rBV	114	85	0.01%	0.001%
23	4.921	1203	1207	1209	rVB	196	140	0.01%	0.001%
24	5.040	1226	1244	1277	rBV2	521482	1381829	100.00%	11.315%
25	5.432	1364	1366	1370	rBV2	248	218	0.02%	0.002%
26	5.487	1382	1383	1389	rVB	438	236	0.02%	0.002%
27	5.609	1407	1421	1466	rBV	515887	1057775	76.55%	8.661%
28	5.908	1501	1514	1536	rBV3	41609	88670	6.42%	0.726%
29	6.063	1548	1562	1600	rBV	304580	626626	45.35%	5.131%
30	6.281	1628	1630	1632	rBV	168	85	0.01%	0.001%
31	6.291	1632	1633	1637	rBV	244	158	0.01%	0.001%
32	6.336	1643	1647	1650	rBV	281	164	0.01%	0.001%
33	6.355	1650	1653	1655	rBV2	98	67	0.00%	0.001%
34	6.503	1698	1699	1704	rVB	173	93	0.01%	0.001%
35	6.558	1713	1716	1720	rBV3	192	102	0.01%	0.001%
36	6.625	1731	1737	1738	rBV2	914	789	0.06%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029564.D
 Acq On : 10 Dec 2022 08:35
 Operator : SY/MD
 Sample : N5929-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.699	1757	1760	1762	rVB2	403	204	0.01%	0.002%
38	6.712	1762	1764	1769	rVB3	219	177	0.01%	0.001%
39	6.735	1769	1771	1776	rVB2	197	136	0.01%	0.001%
40	6.773	1777	1783	1785	rBV3	208	162	0.01%	0.001%
41	6.789	1785	1788	1790	rBV2	107	72	0.01%	0.001%
42	6.821	1795	1798	1800	rVB2	126	76	0.01%	0.001%
43	6.841	1802	1804	1807	rBV2	213	145	0.01%	0.001%
44	6.895	1817	1821	1822	rBV	348	164	0.01%	0.001%
45	6.979	1835	1847	1872	rBV	141214	259074	18.75%	2.121%
46	7.149	1898	1900	1902	rBV2	312	136	0.01%	0.001%
47	7.233	1924	1926	1929	rVB2	351	165	0.01%	0.001%
48	7.307	1937	1949	1990	rBV	592688	1063674	76.98%	8.710%
49	7.612	2034	2044	2065	rBV	99898	177827	12.87%	1.456%
50	7.969	2146	2155	2176	rVB	65553	111087	8.04%	0.910%
51	8.085	2180	2191	2224	rBV	389320	707505	51.20%	5.793%
52	8.439	2297	2301	2303	rBV2	395	348	0.03%	0.003%
53	8.510	2321	2323	2325	rVB2	351	136	0.01%	0.001%
54	8.654	2365	2368	2370	rBV	321	209	0.02%	0.002%
55	8.667	2370	2372	2375	rVB2	317	179	0.01%	0.001%
56	8.690	2375	2379	2380	rBV2	279	184	0.01%	0.002%
57	8.747	2395	2397	2402	rBV2	244	189	0.01%	0.002%
58	8.844	2415	2427	2452	rBV	728648	1207560	87.39%	9.888%
59	9.124	2511	2514	2516	rBV3	551	344	0.02%	0.003%
60	9.182	2530	2532	2534	rBV	195	127	0.01%	0.001%
61	9.333	2576	2579	2582	rVB2	179	118	0.01%	0.001%
62	9.355	2582	2586	2587	rBV2	318	227	0.02%	0.002%
63	9.413	2591	2604	2609	rBV2	313	556	0.04%	0.005%
64	9.529	2636	2640	2642	rVB2	288	177	0.01%	0.001%
65	9.571	2647	2653	2660	rBV4	578	736	0.05%	0.006%
66	9.628	2666	2671	2676	rBV3	268	301	0.02%	0.002%
67	9.661	2677	2681	2684	rBV2	246	192	0.01%	0.002%
68	9.799	2721	2724	2729	rBV	309	254	0.02%	0.002%
69	9.854	2739	2741	2743	rBV2	181	112	0.01%	0.001%
70	9.876	2747	2748	2751	rBV	156	86	0.01%	0.001%
71	9.892	2751	2753	2755	rVB2	264	103	0.01%	0.001%
72	9.918	2759	2761	2765	rBV	211	185	0.01%	0.002%
73	10.162	2828	2837	2841	rBV	20491	28934	2.09%	0.237%
74	10.207	2842	2851	2873	rVB	456402	719752	52.09%	5.893%
75	10.362	2897	2899	2900	rBV2	215	122	0.01%	0.001%
76	10.403	2909	2912	2914	rBV2	279	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029564.D
 Acq On : 10 Dec 2022 08:35
 Operator : SY/MD
 Sample : N5929-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.471	2931	2933	2935	rBV2	226	89	0.01%	0.001%
78	10.567	2955	2963	2976	rVB2	8956	14256	1.03%	0.117%
79	10.661	2990	2992	2993	rVB2	215	65	0.00%	0.001%
80	10.686	2994	3000	3004	rBV3	415	472	0.03%	0.004%
81	10.744	3014	3018	3023	rBV2	346	435	0.03%	0.004%
82	10.799	3033	3035	3037	rBV2	146	74	0.01%	0.001%
83	10.825	3039	3043	3046	rVB	186	112	0.01%	0.001%
84	10.870	3056	3057	3059	rBV	167	63	0.00%	0.001%
85	10.953	3079	3083	3085	rBV2	376	268	0.02%	0.002%
86	11.175	3145	3152	3157	rBV3	1144	1466	0.11%	0.012%
87	11.239	3160	3172	3201	rBV	773464	1196497	86.59%	9.797%
88	11.474	3242	3245	3251	rBV3	438	379	0.03%	0.003%
89	11.612	3274	3288	3309	rBV	628157	989689	71.62%	8.104%
90	11.847	3359	3361	3362	rVB	332	91	0.01%	0.001%
91	11.863	3362	3366	3368	rBV2	185	137	0.01%	0.001%
92	11.924	3383	3385	3387	rBV2	304	153	0.01%	0.001%
93	12.066	3426	3429	3430	rBV	320	159	0.01%	0.001%
94	12.098	3435	3439	3445	rBV3	272	334	0.02%	0.003%
95	12.239	3476	3483	3485	rBV3	539	606	0.04%	0.005%
96	12.329	3509	3511	3513	rBV	286	123	0.01%	0.001%
97	12.516	3567	3569	3570	rBV2	289	68	0.00%	0.001%
98	12.857	3673	3675	3676	rBV	182	61	0.00%	0.000%
99	13.320	3818	3819	3820	rBV	391	92	0.01%	0.001%
100	13.734	3943	3948	3953	rBV4	1800	1778	0.13%	0.015%




Sum of corrected areas: 12212766

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029564.D
Acq On : 10 Dec 2022 08:35
Operator : SY/MD
Sample : N5929-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ96DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

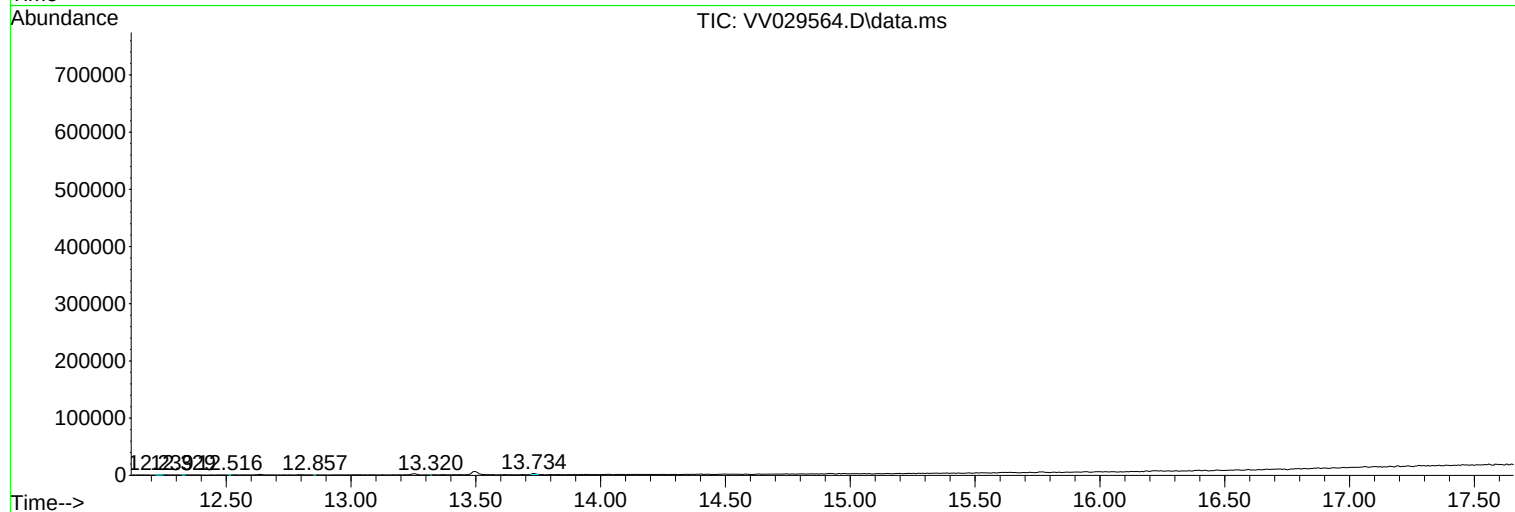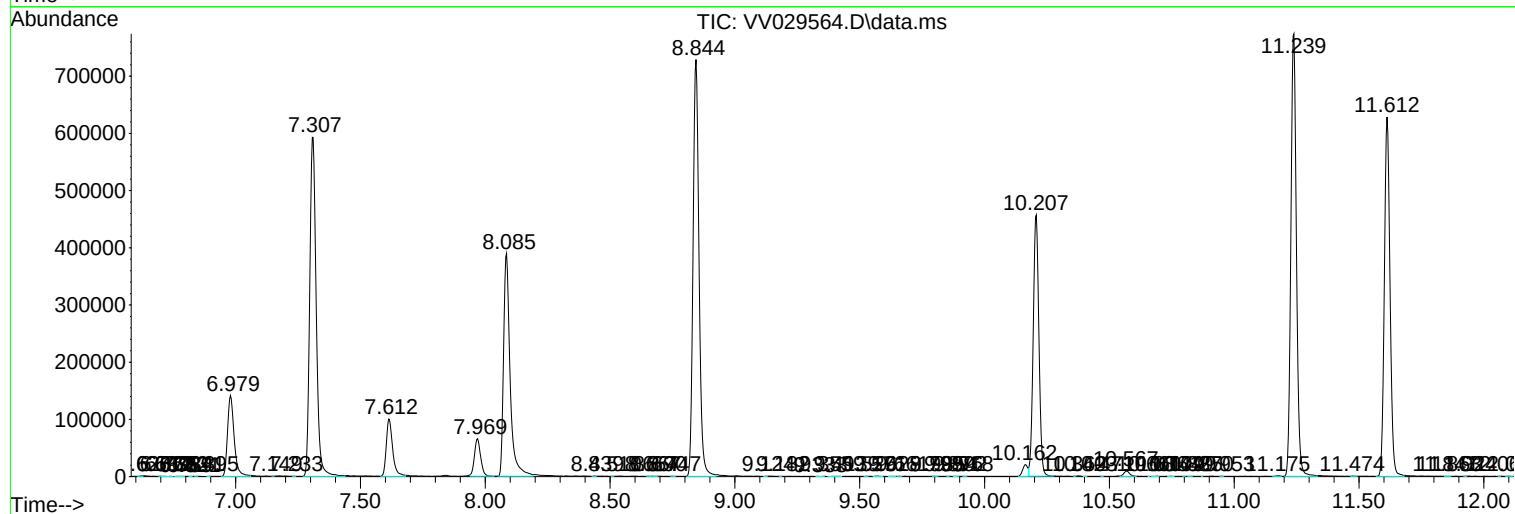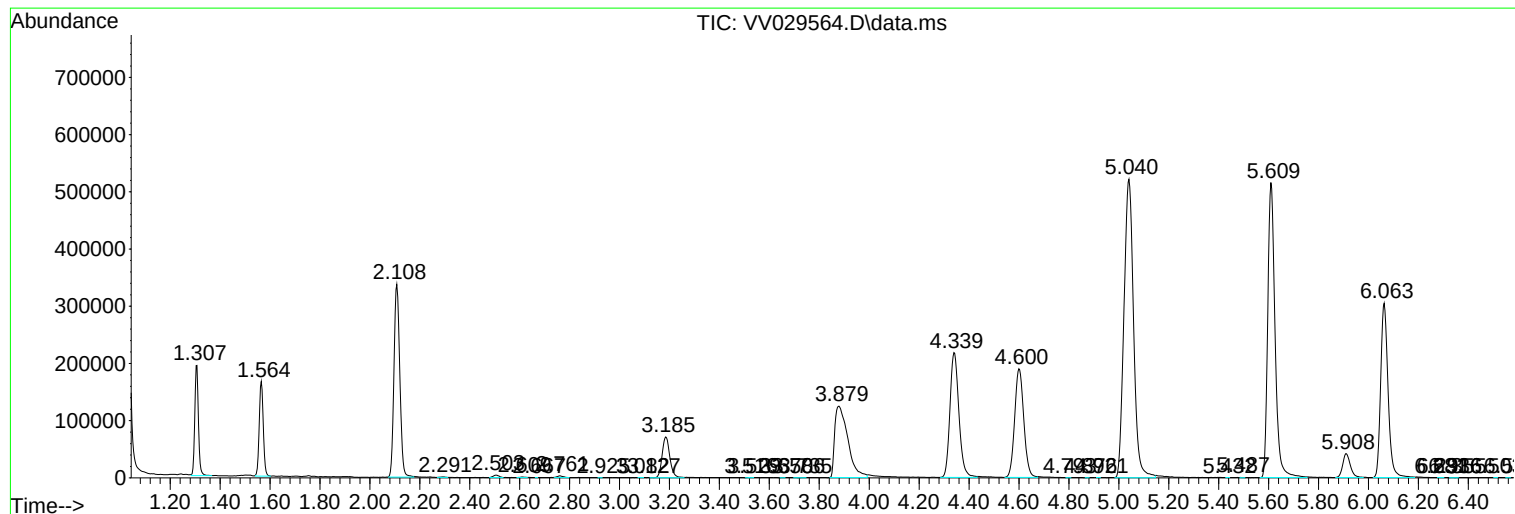

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029564.D
Acq On : 10 Dec 2022 08:35
Operator : SY/MD
Sample : N5929-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ96DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029564.D
Acq On : 10 Dec 2022 08:35
Operator : SY/MD
Sample : N5929-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ96DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc