

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029565.D
 Acq On : 10 Dec 2022 08:59
 Operator : SY/MD
 Sample : N5929-02DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ97DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	215101	217162	13.67%	1.395%
2	1.564	156	163	181	rVB	194717	214942	13.53%	1.381%
3	2.108	320	332	363	rBV2	472852	795495	50.09%	5.112%
4	2.507	445	456	465	rBV2	4061	6712	0.42%	0.043%
5	2.593	479	483	484	rBV	389	205	0.01%	0.001%
6	2.613	485	489	494	rVV2	867	941	0.06%	0.006%
7	2.761	526	535	547	rVB	4190	7442	0.47%	0.048%
8	2.847	558	562	567	rBV	266	196	0.01%	0.001%
9	2.873	567	570	571	rBV	191	103	0.01%	0.001%
10	3.050	619	625	628	rBV2	224	244	0.02%	0.002%
11	3.089	635	637	639	rBV	159	80	0.01%	0.001%
12	3.108	642	643	646	rVB	325	80	0.01%	0.001%
13	3.185	653	667	689	rBV	113588	238266	15.00%	1.531%
14	3.426	739	742	746	rVB	241	195	0.01%	0.001%
15	3.593	791	794	796	rBV	139	99	0.01%	0.001%
16	3.667	813	817	822	rBV2	221	241	0.02%	0.002%
17	3.754	841	844	846	rBV	141	85	0.01%	0.001%
18	3.767	846	848	850	rVB	177	78	0.00%	0.001%
19	3.899	869	889	934	rBV3	186727	700209	44.09%	4.500%
20	4.339	1009	1026	1056	rBV	243577	616649	38.83%	3.963%
21	4.600	1089	1107	1151	rBV	380777	962394	60.60%	6.184%
22	4.902	1198	1201	1204	rVB	135	74	0.00%	0.000%
23	4.944	1212	1214	1219	rVB	174	127	0.01%	0.001%
24	4.966	1219	1221	1223	rVB	220	70	0.00%	0.000%
25	5.040	1223	1244	1297	rBV2	597006	1588068	100.00%	10.205%
26	5.426	1362	1364	1367	rVB	307	117	0.01%	0.001%
27	5.474	1371	1379	1381	rBV2	548	655	0.04%	0.004%
28	5.609	1408	1421	1450	rBV	605898	1230254	77.47%	7.906%
29	5.908	1501	1514	1545	rBV	187446	380010	23.93%	2.442%
30	6.063	1548	1562	1583	rBV	333795	690238	43.46%	4.435%
31	6.294	1627	1634	1637	rBV2	205	216	0.01%	0.001%
32	6.310	1637	1639	1643	rVV2	283	164	0.01%	0.001%
33	6.330	1643	1645	1647	rVV2	184	79	0.00%	0.001%
34	6.371	1655	1658	1661	rVB2	124	77	0.00%	0.000%
35	6.391	1661	1664	1666	rBV2	442	226	0.01%	0.001%
36	6.410	1666	1670	1673	rBV	230	122	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029565.D
 Acq On : 10 Dec 2022 08:59
 Operator : SY/MD
 Sample : N5929-02DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ97DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.474	1688	1690	1695	rVB2	232	148	0.01%	0.001%
38	6.500	1695	1698	1703	rBV	215	155	0.01%	0.001%
39	6.539	1708	1710	1712	rVB	252	117	0.01%	0.001%
40	6.622	1728	1736	1738	rBV3	1426	1390	0.09%	0.009%
41	6.783	1785	1786	1789	rBV	247	107	0.01%	0.001%
42	6.802	1789	1792	1796	rVV2	141	125	0.01%	0.001%
43	6.867	1808	1812	1814	rBV2	228	190	0.01%	0.001%
44	6.905	1819	1824	1826	rBV2	192	157	0.01%	0.001%
45	6.979	1836	1847	1876	rBV	156830	294026	18.51%	1.889%
46	7.256	1931	1933	1937	rVB3	381	157	0.01%	0.001%
47	7.310	1937	1950	1982	rBV	737051	1304532	82.15%	8.383%
48	7.612	2034	2044	2083	rVB	112982	202738	12.77%	1.303%
49	7.838	2104	2114	2123	rBV4	4467	8018	0.50%	0.052%
50	7.966	2143	2154	2179	rVB	159099	273056	17.19%	1.755%
51	8.085	2180	2191	2227	rBV	428763	783362	49.33%	5.034%
52	8.471	2309	2311	2313	rBV2	342	122	0.01%	0.001%
53	8.542	2328	2333	2337	rVB3	493	464	0.03%	0.003%
54	8.558	2337	2338	2341	rVB	337	140	0.01%	0.001%
55	8.580	2341	2345	2348	rBV2	419	290	0.02%	0.002%
56	8.600	2348	2351	2353	rBV2	295	193	0.01%	0.001%
57	8.651	2362	2367	2369	rBV3	406	426	0.03%	0.003%
58	8.696	2378	2381	2384	rBV3	229	158	0.01%	0.001%
59	8.844	2414	2427	2467	rBV	899298	1469472	92.53%	9.443%
60	9.088	2500	2503	2507	rBV3	265	229	0.01%	0.001%
61	9.143	2518	2520	2523	rBV	298	150	0.01%	0.001%
62	9.204	2535	2539	2544	rVB4	431	467	0.03%	0.003%
63	9.230	2544	2547	2550	rVB3	468	323	0.02%	0.002%
64	9.246	2550	2552	2553	rBV3	184	80	0.01%	0.001%
65	9.272	2558	2560	2563	rVV2	458	220	0.01%	0.001%
66	9.432	2605	2610	2614	rBV2	370	308	0.02%	0.002%
67	9.542	2641	2644	2647	rBV2	392	250	0.02%	0.002%
68	9.571	2650	2653	2657	rVV3	337	240	0.02%	0.002%
69	9.593	2657	2660	2661	rVV2	260	162	0.01%	0.001%
70	9.619	2664	2668	2671	rBV2	305	199	0.01%	0.001%
71	9.661	2678	2681	2682	rBV2	146	79	0.00%	0.001%
72	9.709	2695	2696	2701	rVB2	168	98	0.01%	0.001%
73	9.744	2704	2707	2708	rBV	187	86	0.01%	0.001%
74	9.757	2708	2711	2717	rVB2	198	154	0.01%	0.001%
75	9.786	2717	2720	2723	rBV2	362	261	0.02%	0.002%
76	9.899	2751	2755	2760	rBV2	240	181	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029565.D
 Acq On : 10 Dec 2022 08:59
 Operator : SY/MD
 Sample : N5929-02DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ97DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.924	2760	2763	2764	rBV	311	175	0.01%	0.001%
78	9.972	2774	2778	2780	rBV2	284	190	0.01%	0.001%
79	10.030	2793	2796	2798	rBV2	306	181	0.01%	0.001%
80	10.114	2819	2822	2823	rBV	205	116	0.01%	0.001%
81	10.162	2826	2837	2841	rBV	22008	32196	2.03%	0.207%
82	10.207	2842	2851	2870	rVB	501679	788461	49.65%	5.067%
83	10.413	2910	2915	2920	rVB2	302	248	0.02%	0.002%
84	10.442	2920	2924	2928	rBV2	369	351	0.02%	0.002%
85	10.532	2948	2952	2954	rBV2	331	284	0.02%	0.002%
86	10.567	2955	2963	2980	rVB	10251	16608	1.05%	0.107%
87	10.792	3031	3033	3037	rVB2	253	161	0.01%	0.001%
88	10.812	3037	3039	3041	rBV2	140	77	0.00%	0.000%
89	10.844	3046	3049	3053	rVV2	479	259	0.02%	0.002%
90	10.985	3087	3093	3094	rBV2	251	187	0.01%	0.001%
91	11.046	3108	3112	3118	rBV2	267	329	0.02%	0.002%
92	11.127	3134	3137	3138	rBV	195	87	0.01%	0.001%
93	11.175	3146	3152	3153	rBV4	658	620	0.04%	0.004%
94	11.239	3159	3172	3204	rBV	986378	1510595	95.12%	9.707%
95	11.612	3276	3288	3311	rBV	777381	1213264	76.40%	7.796%
96	11.850	3359	3362	3363	rBV	269	171	0.01%	0.001%
97	11.950	3390	3393	3396	rBV	336	235	0.01%	0.002%
98	12.130	3447	3449	3453	rBV	373	243	0.02%	0.002%
99	12.246	3478	3485	3491	rBV5	688	1052	0.07%	0.007%
100	13.085	3743	3746	3751	rBV4	433	388	0.02%	0.002%


Sum of corrected areas: 15561823

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029565.D
Acq On : 10 Dec 2022 08:59
Operator : SY/MD
Sample : N5929-02DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ97DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

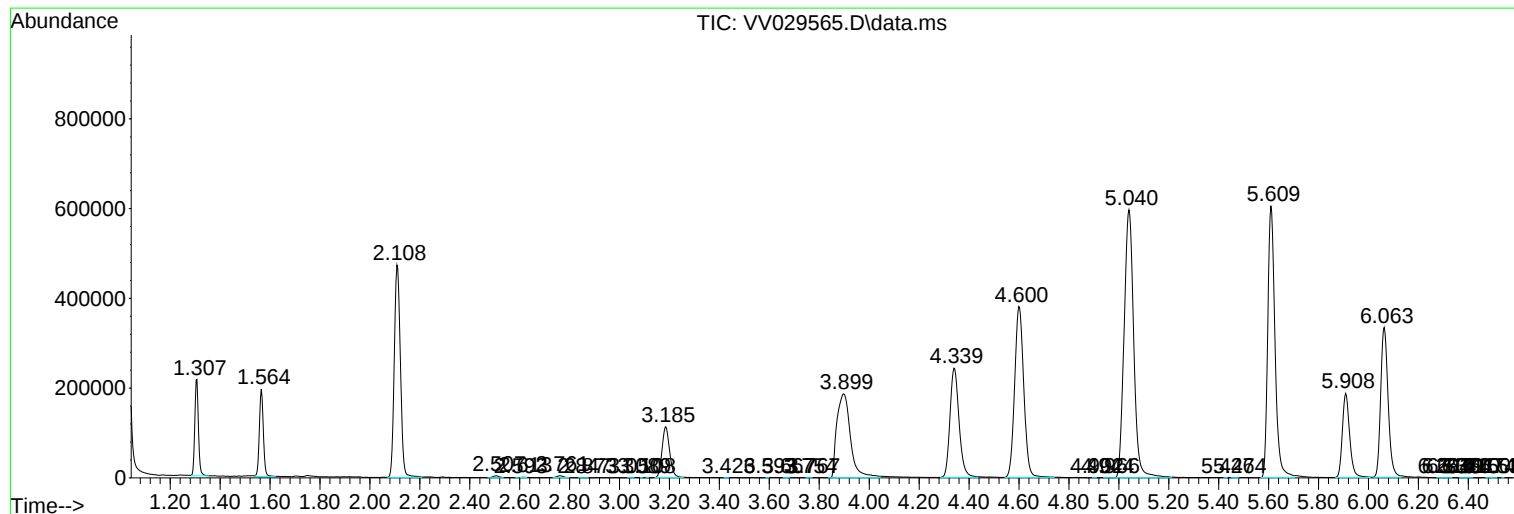

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029565.D
Acq On : 10 Dec 2022 08:59
Operator : SY/MD
Sample : N5929-02DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ97DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029565.D
Acq On : 10 Dec 2022 08:59
Operator : SY/MD
Sample : N5929-02DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ97DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------