

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029566.D
 Acq On : 10 Dec 2022 09:22
 Operator : SY/MD
 Sample : N5929-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	207433	205602	13.39%	1.515%
2	1.564	156	163	175	rVB	181820	199906	13.02%	1.473%
3	2.105	320	331	346	rBV	342397	499860	32.55%	3.684%
4	2.600	483	485	487	rBV2	155	100	0.01%	0.001%
5	2.616	487	490	492	rBV2	289	237	0.02%	0.002%
6	2.725	520	524	525	rVV2	224	164	0.01%	0.001%
7	2.761	525	535	555	rVB2	21064	39520	2.57%	0.291%
8	3.072	629	632	637	rVB2	235	157	0.01%	0.001%
9	3.101	637	641	644	rBV	164	120	0.01%	0.001%
10	3.185	653	667	689	rVV2	34739	73958	4.82%	0.545%
11	3.291	697	700	702	rVB	273	144	0.01%	0.001%
12	3.375	722	726	729	rVB2	167	108	0.01%	0.001%
13	3.551	775	781	783	rBV	468	320	0.02%	0.002%
14	3.606	795	798	801	rVB	210	120	0.01%	0.001%
15	3.696	822	826	830	rBV2	176	153	0.01%	0.001%
16	3.777	845	851	855	rBV2	107	139	0.01%	0.001%
17	3.899	872	889	931	rBV3	172748	640134	41.69%	4.718%
18	4.339	1009	1026	1067	rBV	236533	604612	39.37%	4.456%
19	4.600	1092	1107	1136	rVB3	69084	172881	11.26%	1.274%
20	4.822	1170	1176	1177	rBV	216	209	0.01%	0.002%
21	4.850	1182	1185	1187	rVV2	164	119	0.01%	0.001%
22	4.860	1187	1188	1192	rVV	217	126	0.01%	0.001%
23	5.040	1226	1244	1281	rBV2	583681	1535632	100.00%	11.317%
24	5.436	1363	1367	1370	rVB	285	235	0.02%	0.002%
25	5.468	1374	1377	1378	rBV2	384	272	0.02%	0.002%
26	5.609	1407	1421	1455	rBV	590028	1203471	78.37%	8.869%
27	5.912	1503	1515	1533	rBV2	74380	152486	9.93%	1.124%
28	6.063	1549	1562	1585	rBV	327710	672357	43.78%	4.955%
29	6.278	1626	1629	1633	rVB4	462	362	0.02%	0.003%
30	6.474	1688	1690	1691	rBV	188	100	0.01%	0.001%
31	6.481	1691	1692	1696	rVB2	290	117	0.01%	0.001%
32	6.503	1697	1699	1701	rBV2	372	218	0.01%	0.002%
33	6.625	1732	1737	1738	rBV2	931	726	0.05%	0.005%
34	6.873	1812	1814	1817	rVB	297	124	0.01%	0.001%
35	6.892	1817	1820	1824	rBV	262	204	0.01%	0.002%
36	6.921	1826	1829	1833	rBV2	112	115	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029566.D
 Acq On : 10 Dec 2022 09:22
 Operator : SY/MD
 Sample : N5929-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.979	1836	1847	1878	rBV	154539	286719	18.67%	2.113%
38	7.307	1937	1949	1981	rBV	710086	1261439	82.14%	9.296%
39	7.612	2033	2044	2069	rBV	114586	208273	13.56%	1.535%
40	7.873	2121	2125	2130	rBV3	352	404	0.03%	0.003%
41	7.969	2146	2155	2173	rVB2	105986	182025	11.85%	1.341%
42	8.085	2180	2191	2221	rBV	398144	724797	47.20%	5.341%
43	8.484	2313	2315	2319	rVB2	678	446	0.03%	0.003%
44	8.503	2319	2321	2322	rBV	401	201	0.01%	0.001%
45	8.590	2345	2348	2350	rBV	229	117	0.01%	0.001%
46	8.651	2365	2367	2371	rVB3	483	249	0.02%	0.002%
47	8.673	2371	2374	2377	rBV2	164	99	0.01%	0.001%
48	8.693	2377	2380	2382	rVB	285	140	0.01%	0.001%
49	8.709	2382	2385	2386	rBV	363	200	0.01%	0.001%
50	8.747	2395	2397	2398	rBV	227	112	0.01%	0.001%
51	8.776	2404	2406	2407	rBV	204	109	0.01%	0.001%
52	8.844	2414	2427	2461	rBV	869245	1431179	93.20%	10.547%
53	9.091	2502	2504	2509	rVB2	372	241	0.02%	0.002%
54	9.140	2515	2519	2522	rVB5	355	291	0.02%	0.002%
55	9.201	2535	2538	2539	rBV	173	101	0.01%	0.001%
56	9.226	2543	2546	2552	rVB2	327	186	0.01%	0.001%
57	9.320	2573	2575	2583	rBV3	381	321	0.02%	0.002%
58	9.435	2609	2611	2614	rVB	344	147	0.01%	0.001%
59	9.458	2614	2618	2619	rBV2	208	143	0.01%	0.001%
60	9.532	2639	2641	2645	rVB2	293	138	0.01%	0.001%
61	9.554	2645	2648	2653	rBV3	217	182	0.01%	0.001%
62	9.583	2655	2657	2659	rBV2	215	100	0.01%	0.001%
63	9.612	2664	2666	2671	rVB2	252	125	0.01%	0.001%
64	9.648	2671	2677	2682	rBV4	408	371	0.02%	0.003%
65	9.670	2682	2684	2687	rBV2	198	111	0.01%	0.001%
66	9.706	2691	2695	2697	rBV	150	116	0.01%	0.001%
67	9.718	2697	2699	2700	rBV2	199	103	0.01%	0.001%
68	9.763	2705	2713	2714	rBV3	295	287	0.02%	0.002%
69	9.789	2718	2721	2726	rBV2	230	173	0.01%	0.001%
70	9.815	2726	2729	2732	rBV	246	247	0.02%	0.002%
71	9.915	2758	2760	2763	rVB	280	118	0.01%	0.001%
72	9.950	2768	2771	2773	rBV2	196	135	0.01%	0.001%
73	10.124	2821	2825	2827	rBV3	259	194	0.01%	0.001%
74	10.162	2827	2837	2841	rVV	22683	32335	2.11%	0.238%
75	10.207	2842	2851	2871	rVB	480755	760713	49.54%	5.606%
76	10.371	2895	2902	2913	rVB2	3220	5621	0.37%	0.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029566.D
 Acq On : 10 Dec 2022 09:22
 Operator : SY/MD
 Sample : N5929-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.455	2924	2928	2929	rBV	187	105	0.01%	0.001%
78	10.532	2949	2952	2954	rBV2	254	184	0.01%	0.001%
79	10.567	2954	2963	2975	rVV2	10092	16667	1.09%	0.123%
80	10.625	2979	2981	2984	rBV2	251	160	0.01%	0.001%
81	10.683	2997	2999	3003	rBV3	159	112	0.01%	0.001%
82	10.725	3010	3012	3015	rVB	217	112	0.01%	0.001%
83	10.789	3030	3032	3036	rVB2	191	127	0.01%	0.001%
84	10.821	3036	3042	3044	rBV2	371	273	0.02%	0.002%
85	10.841	3045	3048	3053	rVV3	507	357	0.02%	0.003%
86	10.905	3064	3068	3073	rBV2	483	531	0.03%	0.004%
87	10.940	3077	3079	3081	rVV	197	133	0.01%	0.001%
88	10.969	3085	3088	3090	rVB2	347	190	0.01%	0.001%
89	10.982	3090	3092	3096	rBV	174	143	0.01%	0.001%
90	11.091	3122	3126	3129	rBV3	226	180	0.01%	0.001%
91	11.120	3132	3135	3138	rBV2	199	159	0.01%	0.001%
92	11.172	3147	3151	3159	rBV4	647	915	0.06%	0.007%
93	11.239	3159	3172	3200	rBV	949807	1466331	95.49%	10.806%
94	11.612	3276	3288	3311	rBV	739383	1176909	76.64%	8.673%
95	11.824	3352	3354	3357	rBV3	485	180	0.01%	0.001%
96	11.892	3372	3375	3379	rBV2	479	342	0.02%	0.003%
97	12.021	3412	3415	3419	rBV3	401	318	0.02%	0.002%
98	12.204	3470	3472	3474	rBV	304	136	0.01%	0.001%
99	12.705	3625	3628	3630	rBV3	337	173	0.01%	0.001%
100	13.059	3734	3738	3742	rBV2	459	363	0.02%	0.003%




Sum of corrected areas: 13569216

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029566.D
Acq On : 10 Dec 2022 09:22
Operator : SY/MD
Sample : N5929-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

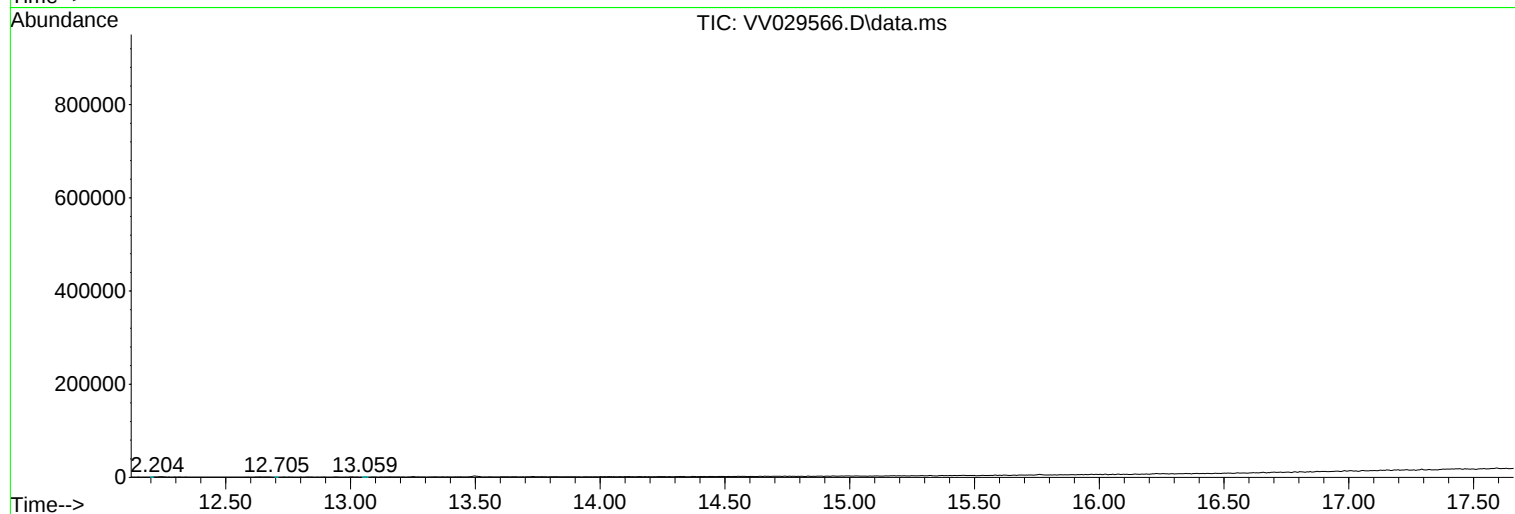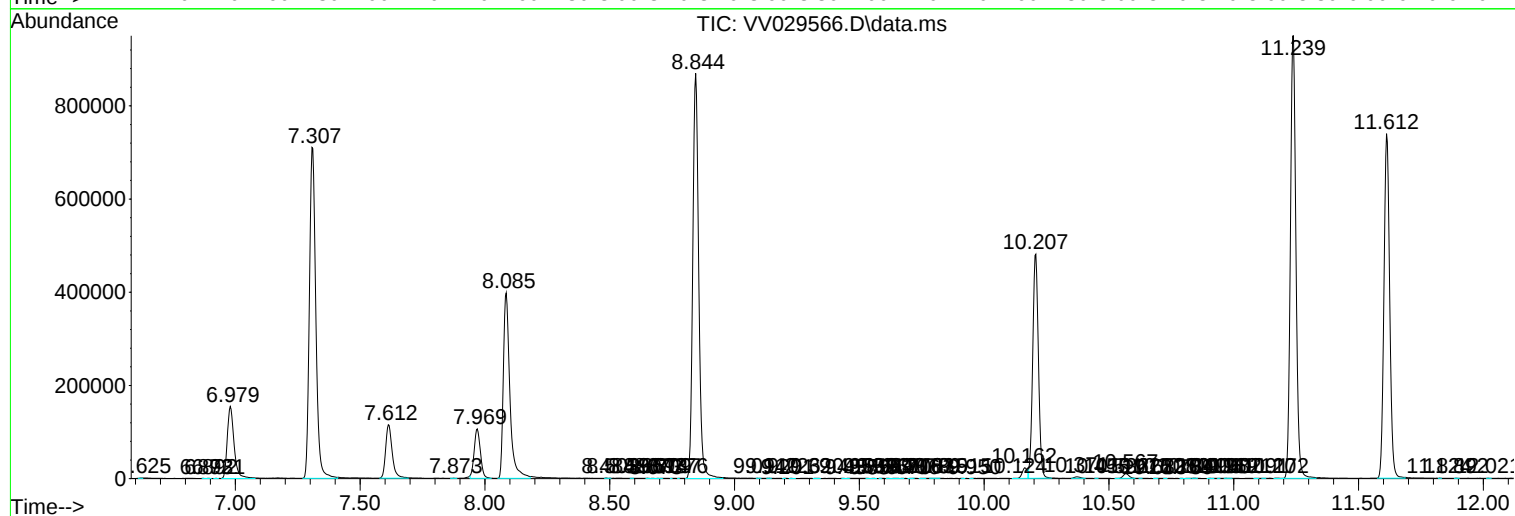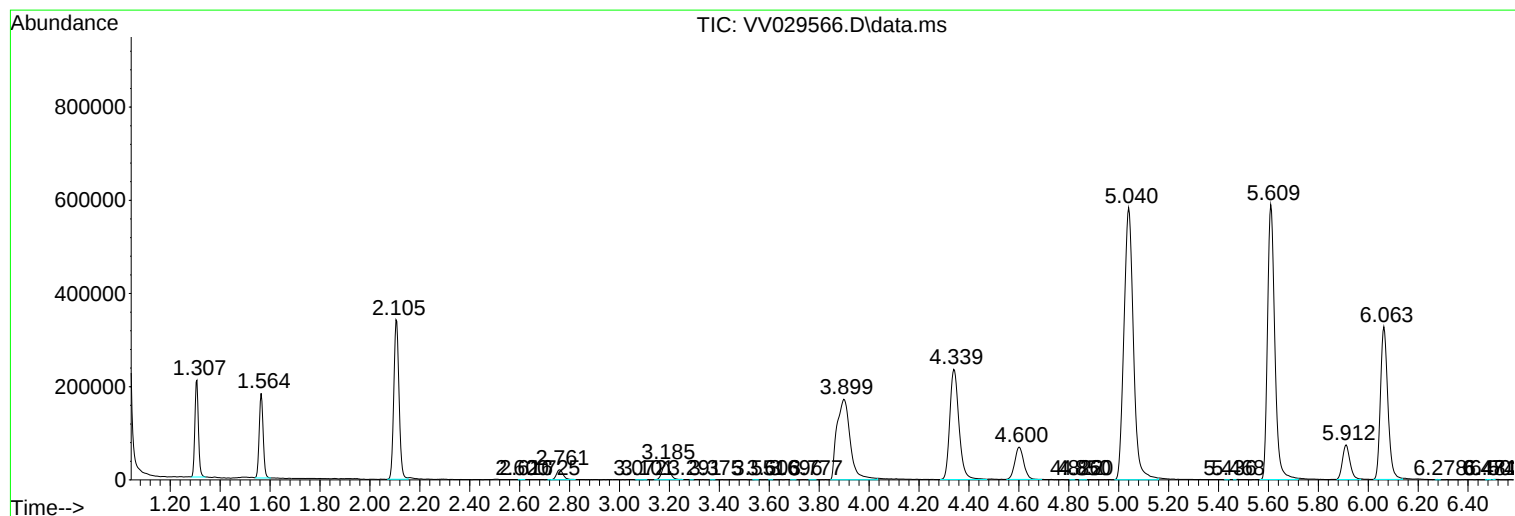

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029566.D
Acq On : 10 Dec 2022 09:22
Operator : SY/MD
Sample : N5929-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029566.D
Acq On : 10 Dec 2022 09:22
Operator : SY/MD
Sample : N5929-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------