

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029567.D
 Acq On : 10 Dec 2022 09:46
 Operator : SY/MD
 Sample : N5929-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	200243	200989	13.73%	1.632%
2	1.564	156	163	181	rVB	176577	195823	13.38%	1.590%
3	2.105	320	331	346	rBV	325613	478912	32.72%	3.889%
4	2.455	438	440	443	rBV	231	109	0.01%	0.001%
5	2.474	443	446	450	rVV2	353	300	0.02%	0.002%
6	2.503	450	455	464	rVB3	782	1000	0.07%	0.008%
7	2.767	533	537	542	rVB	430	354	0.02%	0.003%
8	2.863	564	567	573	rBV2	235	219	0.01%	0.002%
9	2.963	593	598	601	rBV2	138	149	0.01%	0.001%
10	2.995	603	608	612	rVB2	214	216	0.01%	0.002%
11	3.095	635	639	642	rBV2	232	254	0.02%	0.002%
12	3.185	659	667	683	rVB2	2972	6234	0.43%	0.051%
13	3.259	686	690	692	rBV	220	101	0.01%	0.001%
14	3.285	695	698	704	rVB2	176	97	0.01%	0.001%
15	3.314	704	707	709	rBV	161	107	0.01%	0.001%
16	3.371	723	725	728	rVB2	225	86	0.01%	0.001%
17	3.616	795	801	804	rBV2	212	200	0.01%	0.002%
18	3.696	823	826	831	rBV2	132	94	0.01%	0.001%
19	3.754	839	844	846	rBV2	144	145	0.01%	0.001%
20	3.789	852	855	859	rBV2	190	132	0.01%	0.001%
21	3.818	861	864	867	rBV2	109	86	0.01%	0.001%
22	3.873	871	881	918	rBV	103099	295490	20.19%	2.400%
23	4.339	1010	1026	1054	rBV	225667	560187	38.27%	4.550%
24	4.600	1090	1107	1132	rBV2	95155	238848	16.32%	1.940%
25	4.783	1161	1164	1165	rBV2	205	101	0.01%	0.001%
26	4.822	1173	1176	1178	rBV	193	114	0.01%	0.001%
27	4.867	1187	1190	1195	rVB2	184	167	0.01%	0.001%
28	4.934	1205	1211	1214	rBV	190	200	0.01%	0.002%
29	4.960	1214	1219	1221	rBV	115	117	0.01%	0.001%
30	5.040	1226	1244	1278	rBV2	557818	1463596	100.00%	11.887%
31	5.516	1391	1392	1395	rBV	210	129	0.01%	0.001%
32	5.609	1408	1421	1463	rBV	561501	1149884	78.57%	9.339%
33	5.911	1503	1515	1529	rBV10	5838	13239	0.90%	0.108%
34	6.063	1547	1562	1588	rBV	318790	652590	44.59%	5.300%
35	6.294	1632	1634	1637	rBV2	289	142	0.01%	0.001%
36	6.336	1643	1647	1649	rVB2	279	132	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029567.D
 Acq On : 10 Dec 2022 09:46
 Operator : SY/MD
 Sample : N5929-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.365	1654	1656	1659	rVB2	194	98	0.01%	0.001%
38	6.436	1675	1678	1680	rBV	240	146	0.01%	0.001%
39	6.526	1702	1706	1709	rBV2	265	237	0.02%	0.002%
40	6.590	1724	1726	1728	rVB	271	85	0.01%	0.001%
41	6.635	1729	1740	1741	rBV3	1114	1517	0.10%	0.012%
42	6.751	1773	1776	1780	rVB	218	138	0.01%	0.001%
43	6.776	1780	1784	1786	rBV	206	125	0.01%	0.001%
44	6.834	1799	1802	1805	rVV2	418	237	0.02%	0.002%
45	6.850	1805	1807	1809	rVV	204	105	0.01%	0.001%
46	6.866	1809	1812	1815	rVB	371	187	0.01%	0.002%
47	6.979	1835	1847	1875	rVV	146061	271711	18.56%	2.207%
48	7.310	1937	1950	1978	rBV	680851	1213977	82.94%	9.859%
49	7.612	2034	2044	2070	rBV	102272	183121	12.51%	1.487%
50	7.828	2108	2111	2112	rBV	348	188	0.01%	0.002%
51	7.850	2117	2118	2119	rBV	447	147	0.01%	0.001%
52	8.085	2180	2191	2225	rBV	379999	693131	47.36%	5.629%
53	8.442	2300	2302	2308	rBV3	363	437	0.03%	0.004%
54	8.509	2319	2323	2328	rVB4	629	534	0.04%	0.004%
55	8.558	2336	2338	2339	rBV	154	81	0.01%	0.001%
56	8.603	2349	2352	2354	rBV	246	171	0.01%	0.001%
57	8.673	2369	2374	2377	rBV3	321	333	0.02%	0.003%
58	8.718	2385	2388	2394	rBV3	364	357	0.02%	0.003%
59	8.786	2406	2409	2411	rBV	288	159	0.01%	0.001%
60	8.844	2413	2427	2456	rBV	829111	1358567	92.82%	11.034%
61	9.104	2504	2508	2510	rBV3	471	348	0.02%	0.003%
62	9.136	2515	2518	2519	rBV3	316	186	0.01%	0.002%
63	9.201	2536	2538	2541	rBV2	256	152	0.01%	0.001%
64	9.230	2544	2547	2551	rBV2	217	163	0.01%	0.001%
65	9.378	2591	2593	2594	rBV2	207	82	0.01%	0.001%
66	9.429	2606	2609	2610	rBV	167	84	0.01%	0.001%
67	9.564	2648	2651	2653	rBV	127	81	0.01%	0.001%
68	9.664	2679	2682	2686	rBV2	214	112	0.01%	0.001%
69	9.754	2707	2710	2713	rBV	241	166	0.01%	0.001%
70	9.825	2729	2732	2737	rVB2	198	113	0.01%	0.001%
71	9.931	2762	2765	2767	rBV2	209	148	0.01%	0.001%
72	9.985	2778	2782	2786	rBV2	221	152	0.01%	0.001%
73	10.107	2816	2820	2823	rBV2	216	184	0.01%	0.001%
74	10.162	2827	2837	2841	rBV	22051	32083	2.19%	0.261%
75	10.207	2842	2851	2879	rVB	465453	729151	49.82%	5.922%
76	10.326	2886	2888	2891	rVB	370	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029567.D
 Acq On : 10 Dec 2022 09:46
 Operator : SY/MD
 Sample : N5929-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.374	2891	2903	2917	rBV3	3546	5906	0.40%	0.048%
78	10.439	2921	2923	2929	rVB2	299	247	0.02%	0.002%
79	10.468	2929	2932	2935	rBV	313	205	0.01%	0.002%
80	10.500	2940	2942	2947	rBV2	240	220	0.02%	0.002%
81	10.567	2954	2963	2974	rBV	10717	16811	1.15%	0.137%
82	10.670	2992	2995	3000	rBV2	318	328	0.02%	0.003%
83	10.709	3004	3007	3009	rBV2	226	136	0.01%	0.001%
84	10.841	3042	3048	3052	rBV2	376	273	0.02%	0.002%
85	10.905	3064	3068	3072	rVB2	481	447	0.03%	0.004%
86	10.940	3073	3079	3080	rBV2	254	239	0.02%	0.002%
87	10.972	3085	3089	3095	rBV2	178	185	0.01%	0.002%
88	11.069	3115	3119	3120	rBV	208	164	0.01%	0.001%
89	11.156	3143	3146	3147	rBV	196	93	0.01%	0.001%
90	11.197	3156	3159	3160	rBV2	263	153	0.01%	0.001%
91	11.236	3160	3171	3194	rBV	905642	1396768	95.43%	11.344%
92	11.525	3259	3261	3262	rBV	257	95	0.01%	0.001%
93	11.558	3268	3271	3275	rBV4	837	712	0.05%	0.006%
94	11.612	3276	3288	3312	rVV	717293	1132887	77.40%	9.201%
95	11.834	3352	3357	3360	rBV3	419	381	0.03%	0.003%
96	11.853	3361	3363	3365	rVB	495	158	0.01%	0.001%
97	12.050	3421	3424	3428	rBV2	243	205	0.01%	0.002%
98	12.307	3500	3504	3507	rBV2	455	365	0.02%	0.003%
99	13.149	3761	3766	3768	rBV3	539	501	0.03%	0.004%
100	14.911	4310	4314	4319	rBV	8328	5770	0.39%	0.047%




Sum of corrected areas: 12312977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029567.D
Acq On : 10 Dec 2022 09:46
Operator : SY/MD
Sample : N5929-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

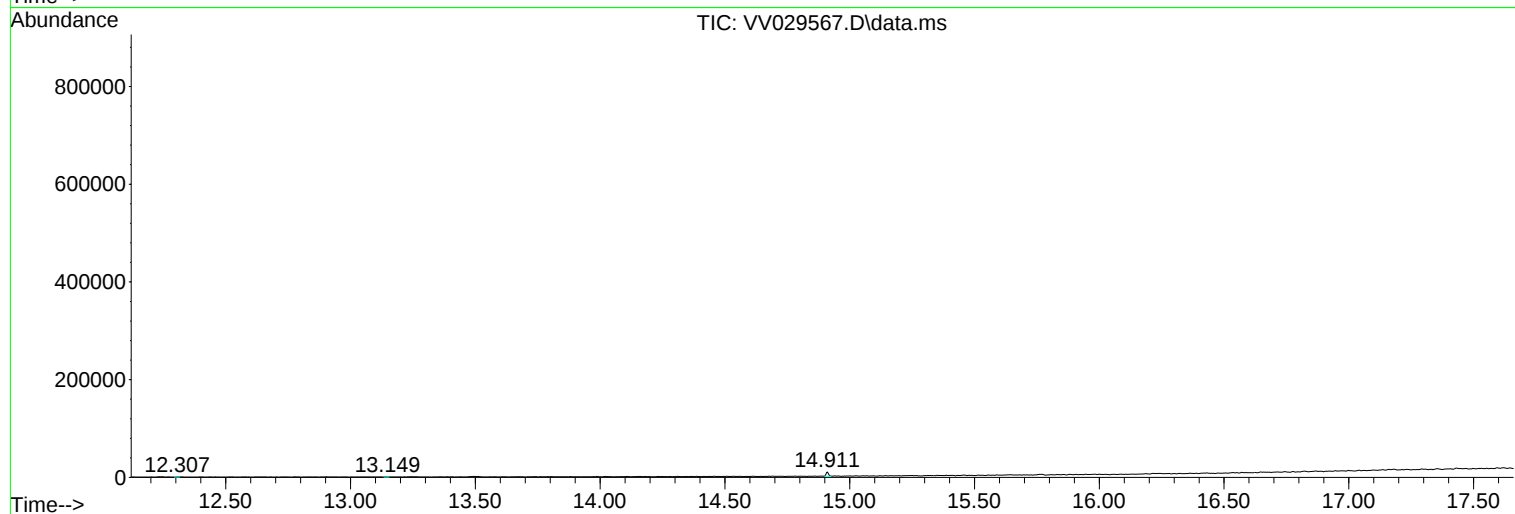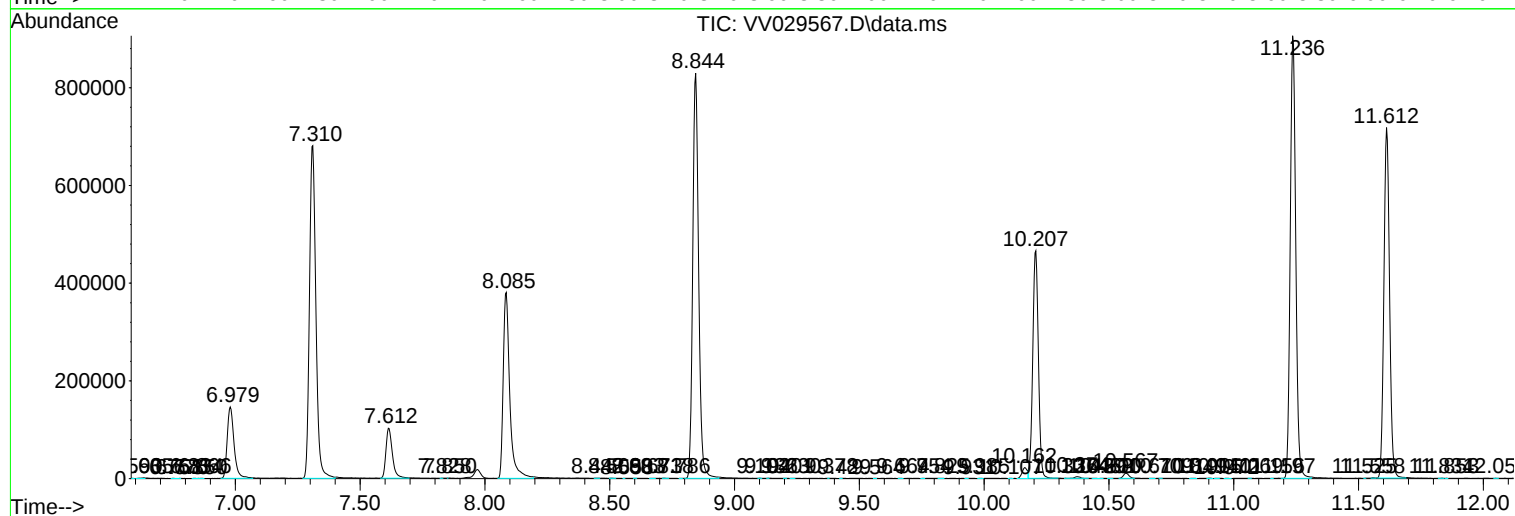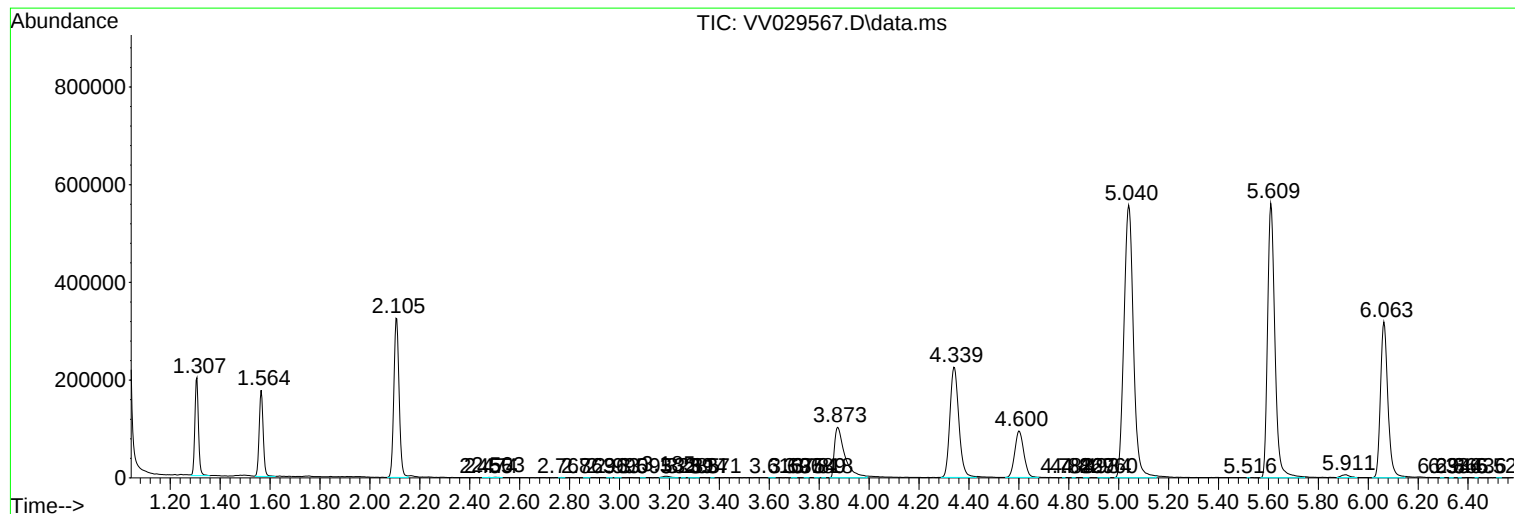

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029567.D
Acq On : 10 Dec 2022 09:46
Operator : SY/MD
Sample : N5929-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029567.D
Acq On : 10 Dec 2022 09:46
Operator : SY/MD
Sample : N5929-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc