

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029568.D
 Acq On : 10 Dec 2022 10:09
 Operator : SY/MD
 Sample : N5929-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029568.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	207921	210446	13.59%	1.591%
2	1.564	156	163	180	rVB	186597	206579	13.34%	1.562%
3	2.105	321	331	345	rBV2	346571	513753	33.16%	3.884%
4	2.426	429	431	432	rBV2	202	78	0.01%	0.001%
5	2.825	551	555	558	rBV2	212	162	0.01%	0.001%
6	2.960	596	597	602	rVB	218	124	0.01%	0.001%
7	3.185	655	667	681	rBV2	9397	20241	1.31%	0.153%
8	3.532	771	775	779	rVB2	319	286	0.02%	0.002%
9	3.696	823	826	830	rBV	151	154	0.01%	0.001%
10	3.876	872	882	928	rBV	108403	343502	22.17%	2.597%
11	4.339	1009	1026	1052	rBV2	238735	588998	38.02%	4.453%
12	4.600	1091	1107	1135	rBV	223900	561173	36.23%	4.242%
13	4.828	1176	1178	1181	rVB2	271	116	0.01%	0.001%
14	4.928	1206	1209	1210	rBV	91	54	0.00%	0.000%
15	4.941	1210	1213	1217	rVV2	139	131	0.01%	0.001%
16	5.040	1223	1244	1308	rBV2	585675	1549103	100.00%	11.711%
17	5.336	1333	1336	1337	rBV	244	134	0.01%	0.001%
18	5.375	1343	1348	1350	rBV3	254	289	0.02%	0.002%
19	5.484	1380	1382	1388	rVB2	544	409	0.03%	0.003%
20	5.523	1388	1394	1399	rBV3	424	484	0.03%	0.004%
21	5.609	1408	1421	1449	rBV	590117	1185404	76.52%	8.961%
22	5.912	1502	1515	1529	rVB7	7614	17947	1.16%	0.136%
23	5.976	1529	1535	1541	rVB3	308	420	0.03%	0.003%
24	6.008	1541	1545	1548	rBV	305	281	0.02%	0.002%
25	6.063	1548	1562	1597	rBV	332220	682402	44.05%	5.159%
26	6.346	1647	1650	1651	rBV	188	87	0.01%	0.001%
27	6.355	1651	1653	1657	rVB2	220	121	0.01%	0.001%
28	6.378	1657	1660	1663	rBV	167	113	0.01%	0.001%
29	6.455	1681	1684	1687	rBV	127	96	0.01%	0.001%
30	6.497	1693	1697	1700	rBV3	290	258	0.02%	0.002%
31	6.532	1705	1708	1709	rBV	138	61	0.00%	0.000%
32	6.587	1723	1725	1728	rBV2	145	85	0.01%	0.001%
33	6.622	1728	1736	1737	rBV3	1129	968	0.06%	0.007%
34	6.728	1766	1769	1771	rBV2	421	222	0.01%	0.002%
35	6.789	1784	1788	1794	rVB2	277	279	0.02%	0.002%
36	6.815	1794	1796	1799	rBV	170	102	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029568.D
 Acq On : 10 Dec 2022 10:09
 Operator : SY/MD
 Sample : N5929-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.841	1802	1804	1806	rVV	155	64	0.00%	0.000%
38	6.912	1822	1826	1829	rVB2	280	236	0.02%	0.002%
39	6.979	1833	1847	1877	rBV	154458	289525	18.69%	2.189%
40	7.307	1937	1949	1990	rBV	718039	1270861	82.04%	9.607%
41	7.612	2034	2044	2072	rBV	110072	195956	12.65%	1.481%
42	7.828	2109	2111	2114	rBV2	457	357	0.02%	0.003%
43	7.969	2148	2155	2170	rVB2	22937	39801	2.57%	0.301%
44	8.085	2180	2191	2223	rBV	400496	730846	47.18%	5.525%
45	8.564	2338	2340	2343	rVB2	372	193	0.01%	0.001%
46	8.580	2343	2345	2350	rVB3	358	208	0.01%	0.002%
47	8.606	2350	2353	2358	rBV2	377	350	0.02%	0.003%
48	8.629	2358	2360	2363	rBV	198	154	0.01%	0.001%
49	8.693	2376	2380	2382	rBV2	427	283	0.02%	0.002%
50	8.728	2388	2391	2393	rBV2	284	154	0.01%	0.001%
51	8.776	2404	2406	2408	rBV2	167	85	0.01%	0.001%
52	8.844	2414	2427	2455	rBV	880832	1417012	91.47%	10.712%
53	9.091	2501	2504	2510	rVB2	526	558	0.04%	0.004%
54	9.127	2510	2515	2516	rBV3	812	665	0.04%	0.005%
55	9.191	2532	2535	2537	rBV2	189	106	0.01%	0.001%
56	9.223	2542	2545	2547	rVV2	193	108	0.01%	0.001%
57	9.255	2553	2555	2556	rBV	165	56	0.00%	0.000%
58	9.265	2556	2558	2560	rVV2	157	56	0.00%	0.000%
59	9.310	2568	2572	2575	rBV2	285	200	0.01%	0.002%
60	9.362	2586	2588	2589	rBV	163	66	0.00%	0.000%
61	9.381	2589	2594	2599	rVB2	240	280	0.02%	0.002%
62	9.400	2599	2600	2601	rBV	174	49	0.00%	0.000%
63	9.423	2605	2607	2609	rVV	275	114	0.01%	0.001%
64	9.455	2614	2617	2619	rBV	278	170	0.01%	0.001%
65	9.509	2631	2634	2636	rBV	152	91	0.01%	0.001%
66	9.538	2638	2643	2648	rVB2	575	576	0.04%	0.004%
67	9.567	2651	2652	2655	rVB2	373	143	0.01%	0.001%
68	9.590	2655	2659	2662	rBV2	252	184	0.01%	0.001%
69	9.612	2662	2666	2668	rBV	180	137	0.01%	0.001%
70	9.712	2695	2697	2698	rBV	122	57	0.00%	0.000%
71	9.722	2698	2700	2703	rVV2	270	137	0.01%	0.001%
72	9.738	2703	2705	2707	rVV2	185	73	0.00%	0.001%
73	9.754	2707	2710	2717	rVB3	360	321	0.02%	0.002%
74	9.792	2717	2722	2726	rBV3	272	291	0.02%	0.002%
75	9.921	2760	2762	2765	rVB2	213	122	0.01%	0.001%
76	10.027	2792	2795	2797	rBV	195	125	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029568.D
 Acq On : 10 Dec 2022 10:09
 Operator : SY/MD
 Sample : N5929-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.063	2803	2806	2807	rBV2	149	80	0.01%	0.001%
78	10.162	2827	2837	2841	rBV2	22757	32200	2.08%	0.243%
79	10.207	2842	2851	2871	rVB	487314	768598	49.62%	5.810%
80	10.352	2894	2896	2897	rBV	370	151	0.01%	0.001%
81	10.371	2897	2902	2920	rVB4	2355	3956	0.26%	0.030%
82	10.436	2920	2922	2923	rBV4	140	67	0.00%	0.001%
83	10.445	2923	2925	2927	rVB	342	129	0.01%	0.001%
84	10.464	2927	2931	2936	rBV2	312	339	0.02%	0.003%
85	10.567	2954	2963	2977	rVB2	10369	16166	1.04%	0.122%
86	10.754	3015	3021	3023	rBV2	401	367	0.02%	0.003%
87	10.895	3063	3065	3066	rBV2	344	128	0.01%	0.001%
88	11.037	3107	3109	3111	rBV2	275	130	0.01%	0.001%
89	11.114	3130	3133	3135	rBV2	251	136	0.01%	0.001%
90	11.236	3159	3171	3195	rBV	920842	1437973	92.83%	10.871%
91	11.419	3226	3228	3232	rVV2	507	319	0.02%	0.002%
92	11.448	3235	3237	3239	rVB2	285	96	0.01%	0.001%
93	11.548	3266	3268	3271	rBV2	381	208	0.01%	0.002%
94	11.612	3275	3288	3311	rVV	712524	1129606	72.92%	8.540%
95	11.825	3351	3354	3356	rBV3	415	340	0.02%	0.003%
96	11.882	3370	3372	3376	rBV3	304	222	0.01%	0.002%
97	12.136	3449	3451	3453	rBV2	306	168	0.01%	0.001%
98	12.149	3453	3455	3458	rVV2	176	107	0.01%	0.001%
99	12.323	3506	3509	3510	rBV2	413	254	0.02%	0.002%
100	12.558	3578	3582	3584	rBV2	518	364	0.02%	0.003%




Sum of corrected areas: 13227936

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029568.D
Acq On : 10 Dec 2022 10:09
Operator : SY/MD
Sample : N5929-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

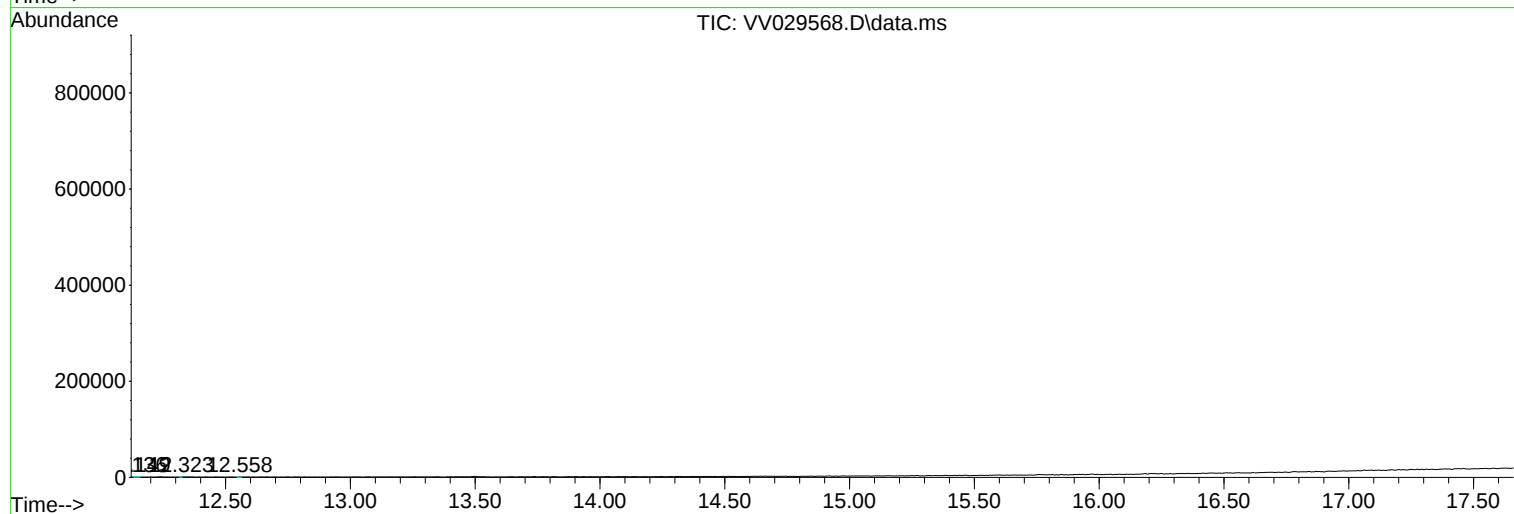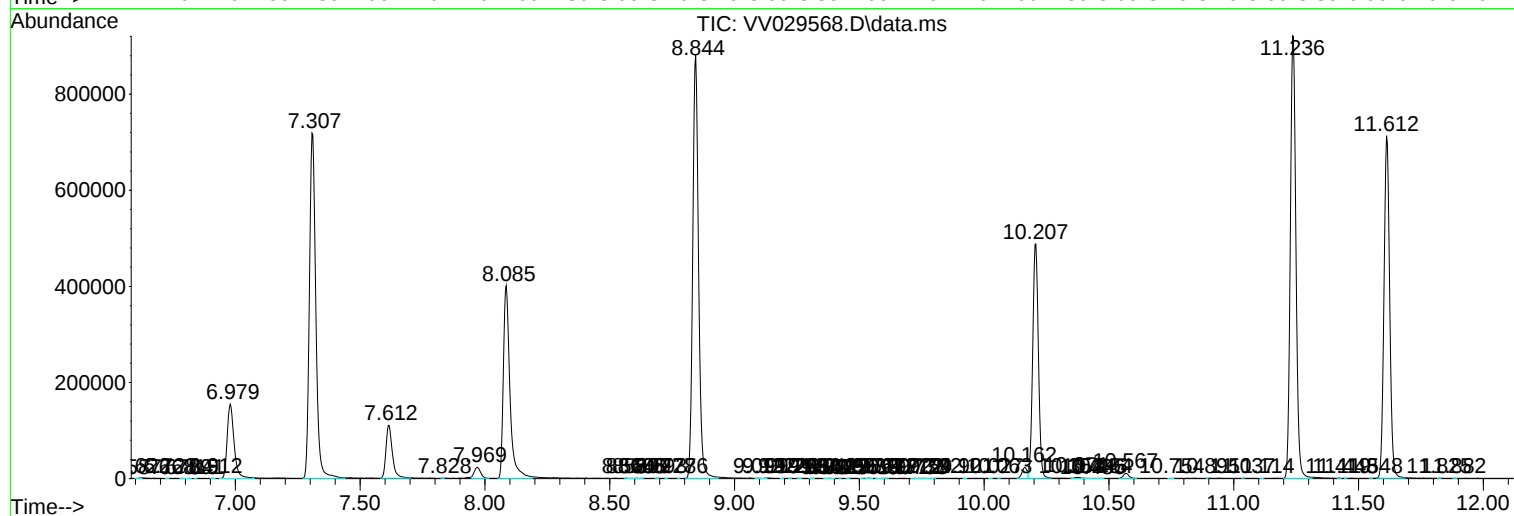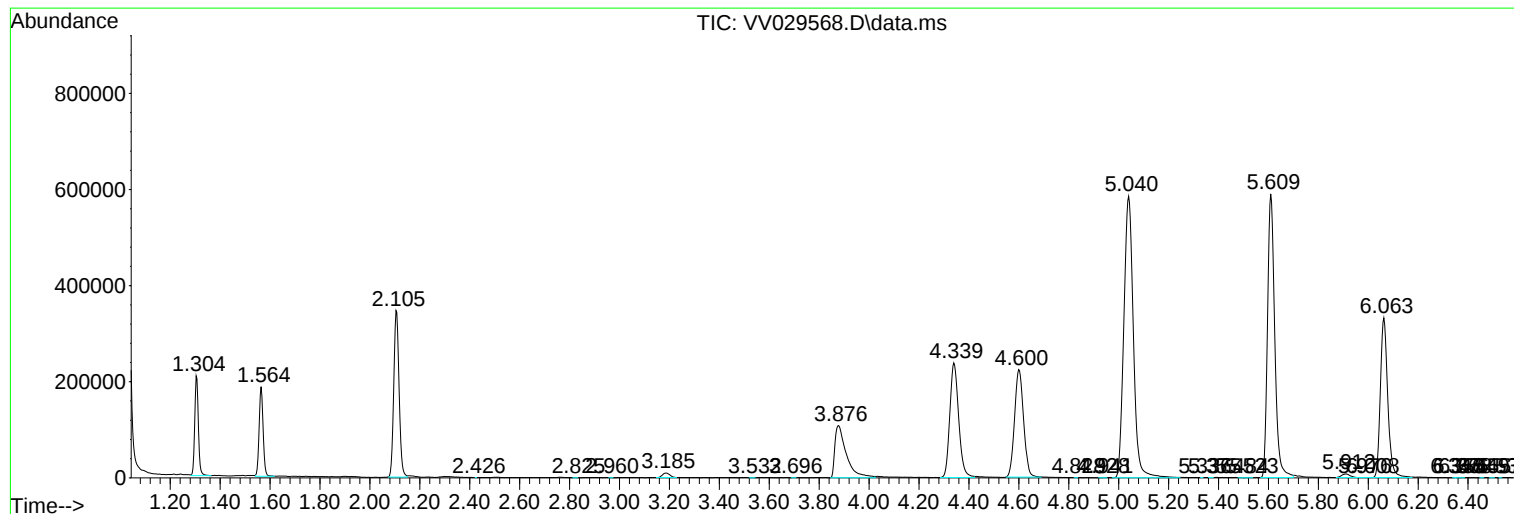

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029568.D
Acq On : 10 Dec 2022 10:09
Operator : SY/MD
Sample : N5929-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029568.D
Acq On : 10 Dec 2022 10:09
Operator : SY/MD
Sample : N5929-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------