

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029569.D
 Acq On : 10 Dec 2022 10:33
 Operator : SY/MD
 Sample : N5929-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029569.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	197198	199650	14.00%	1.515%
2	1.564	155	163	179	rVB	172290	192058	13.47%	1.457%
3	2.108	321	332	350	rBV3	353849	558472	39.17%	4.237%
4	2.397	419	422	425	rBV2	361	214	0.02%	0.002%
5	2.452	437	439	441	rBV	160	91	0.01%	0.001%
6	2.477	444	447	450	rBV2	241	172	0.01%	0.001%
7	2.503	450	455	461	rBV4	752	989	0.07%	0.008%
8	2.760	525	535	546	rBV4	5542	9732	0.68%	0.074%
9	2.953	592	595	597	rBV	225	105	0.01%	0.001%
10	3.111	641	644	646	rVB2	218	124	0.01%	0.001%
11	3.127	646	649	650	rBV	239	142	0.01%	0.001%
12	3.185	650	667	686	rBV	158451	333140	23.37%	2.528%
13	3.474	755	757	760	rVB	296	130	0.01%	0.001%
14	3.661	810	815	820	rBV2	114	133	0.01%	0.001%
15	3.876	872	882	919	rBV2	109623	399678	28.03%	3.032%
16	4.339	1010	1026	1050	rBV	224648	553097	38.79%	4.196%
17	4.600	1092	1107	1136	rVB	144944	364033	25.53%	2.762%
18	4.792	1164	1167	1172	rVB2	271	205	0.01%	0.002%
19	4.870	1189	1191	1195	rVB2	190	130	0.01%	0.001%
20	4.934	1209	1211	1216	rVB2	273	173	0.01%	0.001%
21	5.040	1222	1244	1268	rBV2	545216	1425772	100.00%	10.817%
22	5.429	1363	1365	1368	rBV3	229	142	0.01%	0.001%
23	5.474	1375	1379	1380	rBV2	407	294	0.02%	0.002%
24	5.509	1388	1390	1392	rVB	234	95	0.01%	0.001%
25	5.526	1392	1395	1397	rVB2	295	122	0.01%	0.001%
26	5.545	1397	1401	1405	rBV2	207	152	0.01%	0.001%
27	5.609	1407	1421	1452	rBV	566372	1147480	80.48%	8.706%
28	5.908	1502	1514	1538	rBV3	68094	141921	9.95%	1.077%
29	6.063	1548	1562	1595	rBV	311238	639572	44.86%	4.852%
30	6.268	1622	1626	1629	rVB3	537	360	0.03%	0.003%
31	6.300	1632	1636	1638	rBV3	243	205	0.01%	0.002%
32	6.394	1655	1665	1684	rBV3	3435	8694	0.61%	0.066%
33	6.603	1727	1730	1731	rBV2	408	187	0.01%	0.001%
34	6.776	1781	1784	1785	rBV	142	93	0.01%	0.001%
35	6.844	1801	1805	1807	rBV	184	147	0.01%	0.001%
36	6.879	1812	1816	1818	rBV2	291	198	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029569.D
 Acq On : 10 Dec 2022 10:33
 Operator : SY/MD
 Sample : N5929-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.979	1836	1847	1877	rVV	143967	267154	18.74%	2.027%
38	7.185	1908	1911	1914	rBV2	498	359	0.03%	0.003%
39	7.252	1928	1932	1935	rBV3	460	430	0.03%	0.003%
40	7.307	1937	1949	1978	rBV	673477	1192214	83.62%	9.045%
41	7.615	2034	2045	2070	rBV	104170	184470	12.94%	1.400%
42	7.799	2095	2102	2103	rBV4	583	631	0.04%	0.005%
43	7.831	2109	2112	2113	rBV3	859	422	0.03%	0.003%
44	7.911	2129	2137	2138	rBV2	614	648	0.05%	0.005%
45	7.969	2144	2155	2176	rVB	117609	199831	14.02%	1.516%
46	8.085	2180	2191	2225	rBV	375795	693725	48.66%	5.263%
47	8.506	2319	2322	2323	rVB2	336	162	0.01%	0.001%
48	8.525	2325	2328	2330	rBV	268	165	0.01%	0.001%
49	8.622	2353	2358	2363	rBV3	453	472	0.03%	0.004%
50	8.680	2372	2376	2377	rBV	279	193	0.01%	0.001%
51	8.722	2387	2389	2392	rBV3	280	136	0.01%	0.001%
52	8.741	2392	2395	2396	rBV	299	145	0.01%	0.001%
53	8.844	2415	2427	2468	rBV	833797	1367000	95.88%	10.371%
54	9.104	2505	2508	2513	rBV3	352	346	0.02%	0.003%
55	9.168	2524	2528	2531	rBV	366	272	0.02%	0.002%
56	9.185	2531	2533	2535	rVB	337	169	0.01%	0.001%
57	9.223	2543	2545	2551	rVB2	395	235	0.02%	0.002%
58	9.255	2551	2555	2561	rBV2	290	261	0.02%	0.002%
59	9.365	2586	2589	2593	rBV2	172	175	0.01%	0.001%
60	9.419	2603	2606	2610	rVB3	207	154	0.01%	0.001%
61	9.519	2634	2637	2639	rBV2	222	185	0.01%	0.001%
62	9.570	2650	2653	2655	rBV	285	161	0.01%	0.001%
63	9.612	2663	2666	2668	rBV2	165	125	0.01%	0.001%
64	9.673	2682	2685	2686	rBV	214	99	0.01%	0.001%
65	9.924	2755	2763	2765	rBV2	235	239	0.02%	0.002%
66	9.956	2771	2773	2776	rBV2	213	127	0.01%	0.001%
67	9.969	2776	2777	2781	rVV2	193	92	0.01%	0.001%
68	9.988	2781	2783	2786	rVV2	173	112	0.01%	0.001%
69	10.011	2786	2790	2793	rVV2	403	287	0.02%	0.002%
70	10.037	2795	2798	2802	rVB2	221	171	0.01%	0.001%
71	10.082	2810	2812	2815	rVB	331	134	0.01%	0.001%
72	10.162	2827	2837	2841	rVV2	20664	29823	2.09%	0.226%
73	10.207	2842	2851	2877	rVB	454348	717792	50.34%	5.446%
74	10.410	2912	2914	2916	rBV	156	92	0.01%	0.001%
75	10.484	2935	2937	2940	rBV	124	90	0.01%	0.001%
76	10.567	2954	2963	2977	rBV	9162	15324	1.07%	0.116%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029569.D
 Acq On : 10 Dec 2022 10:33
 Operator : SY/MD
 Sample : N5929-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.657	2989	2991	2994	rBV2	153	102	0.01%	0.001%
78	10.850	3048	3051	3053	rBV	175	114	0.01%	0.001%
79	10.937	3075	3078	3083	rBV2	259	281	0.02%	0.002%
80	10.979	3088	3091	3092	rBV	237	145	0.01%	0.001%
81	11.017	3101	3103	3106	rVB2	189	98	0.01%	0.001%
82	11.037	3106	3109	3112	rBV	157	126	0.01%	0.001%
83	11.117	3133	3134	3140	rVB	289	118	0.01%	0.001%
84	11.156	3143	3146	3148	rBV2	228	150	0.01%	0.001%
85	11.239	3158	3172	3196	rBV	914719	1401694	98.31%	10.635%
86	11.432	3230	3232	3234	rBV2	378	207	0.01%	0.002%
87	11.612	3276	3288	3313	rBV	714973	1120643	78.60%	8.502%
88	11.860	3363	3365	3368	rBV2	298	213	0.01%	0.002%
89	11.927	3384	3386	3389	rBV	342	227	0.02%	0.002%
90	11.975	3397	3401	3408	rBV2	334	443	0.03%	0.003%
91	12.075	3430	3432	3440	rBV3	336	397	0.03%	0.003%
92	12.226	3476	3479	3481	rBV	371	275	0.02%	0.002%
93	12.281	3493	3496	3497	rBV2	356	194	0.01%	0.001%
94	12.445	3544	3547	3548	rBV2	287	135	0.01%	0.001%
95	12.590	3589	3592	3597	rBV2	408	349	0.02%	0.003%
96	12.667	3614	3616	3617	rBV2	270	102	0.01%	0.001%
97	12.683	3617	3621	3626	rVV2	398	423	0.03%	0.003%
98	12.770	3646	3648	3649	rBV2	300	122	0.01%	0.001%
99	12.982	3712	3714	3718	rBV3	447	247	0.02%	0.002%
100	13.252	3793	3798	3805	rBV4	827	1190	0.08%	0.009%


Sum of corrected areas: 13180519

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029569.D
Acq On : 10 Dec 2022 10:33
Operator : SY/MD
Sample : N5929-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

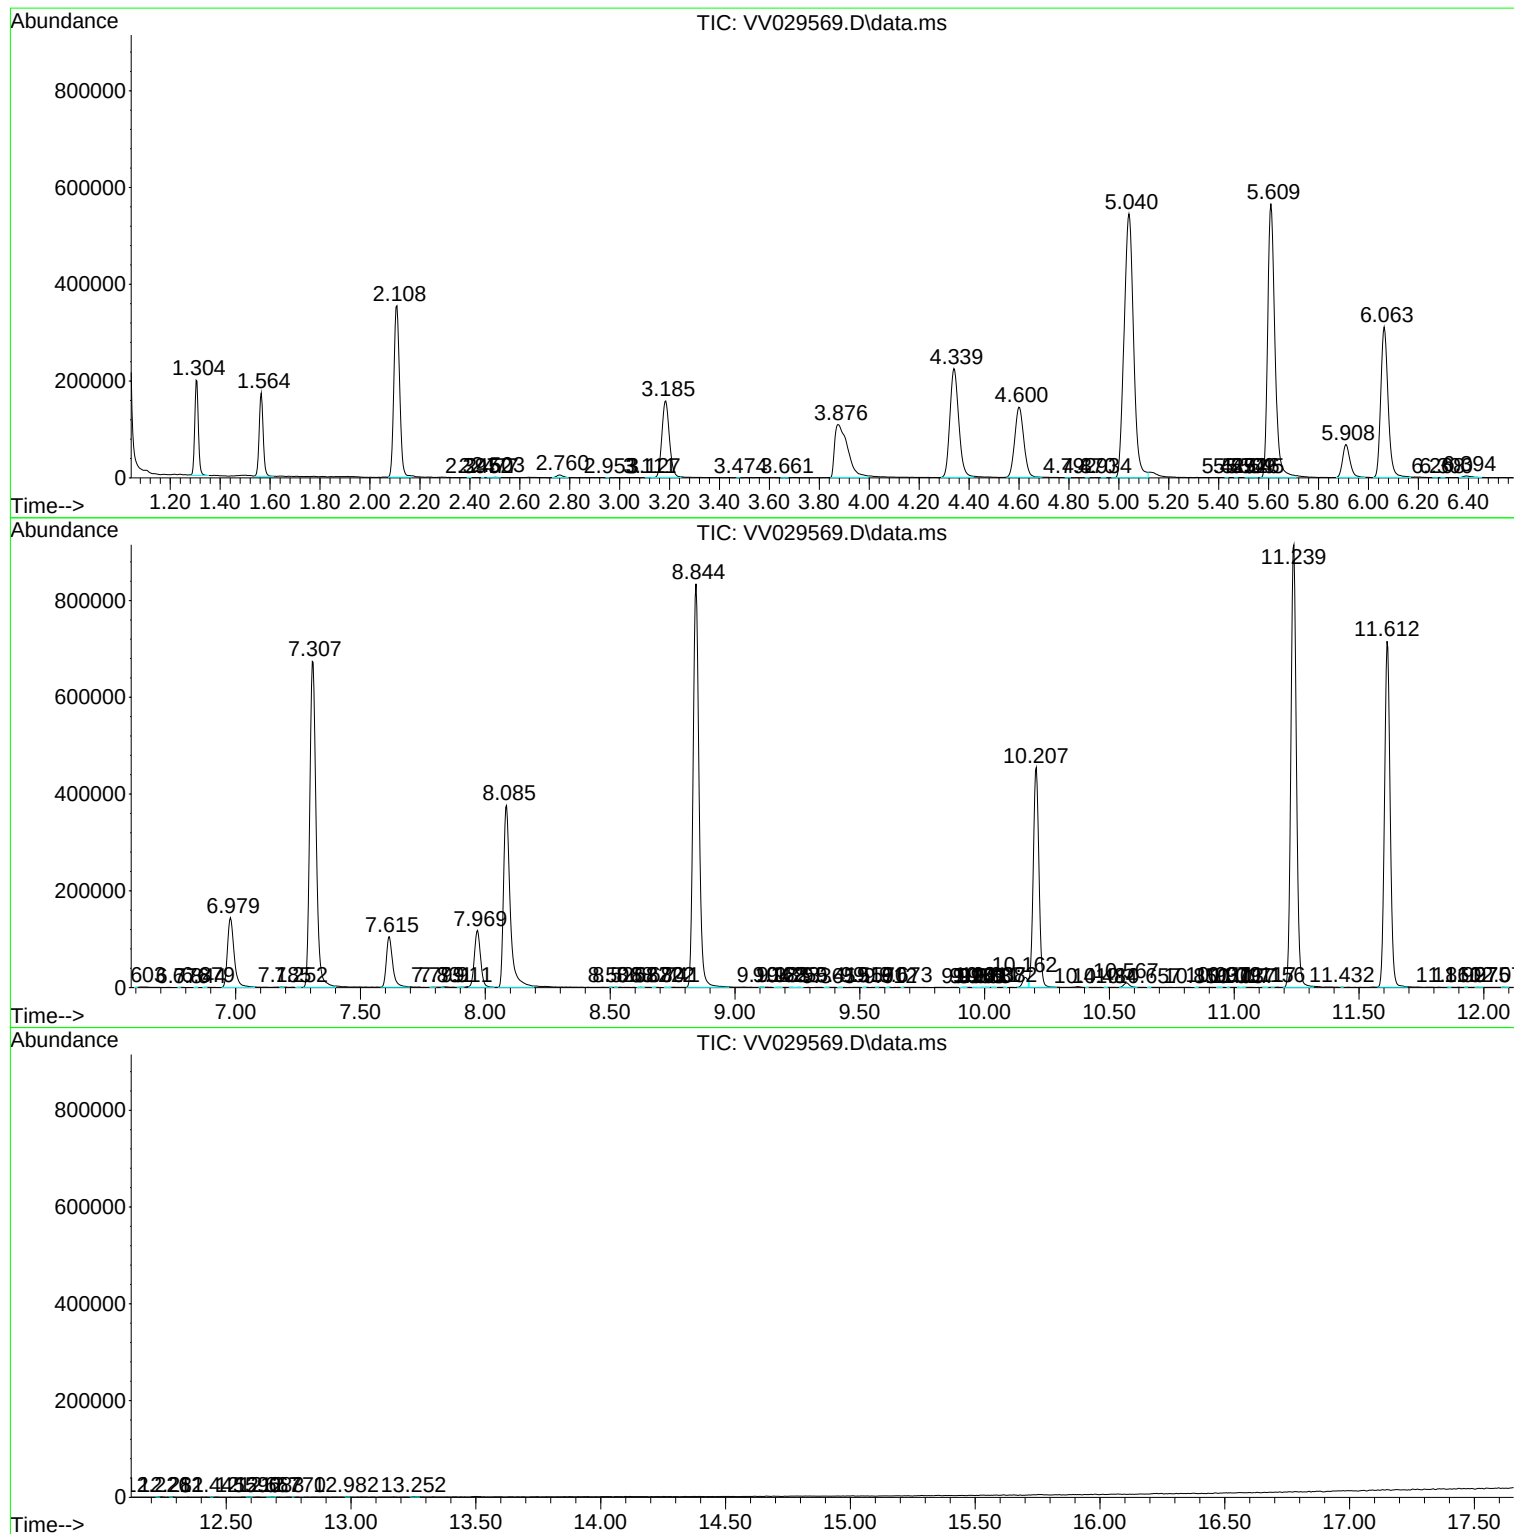

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029569.D
Acq On : 10 Dec 2022 10:33
Operator : SY/MD
Sample : N5929-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029569.D
Acq On : 10 Dec 2022 10:33
Operator : SY/MD
Sample : N5929-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------