

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029570.D
 Acq On : 10 Dec 2022 10:56
 Operator : SY/MD
 Sample : N5929-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	201739	204378	13.78%	1.445%
2	1.565	155	163	178	rVB	178470	199847	13.47%	1.413%
3	2.105	320	331	345	rBV	336915	493975	33.30%	3.492%
4	2.436	432	434	437	rBV2	315	164	0.01%	0.001%
5	2.761	525	535	551	rVB3	12864	23202	1.56%	0.164%
6	2.883	571	573	575	rBV	282	100	0.01%	0.001%
7	2.912	580	582	586	rVB	149	81	0.01%	0.001%
8	3.053	624	626	630	rVB2	302	143	0.01%	0.001%
9	3.108	639	643	646	rVB2	244	160	0.01%	0.001%
10	3.185	649	667	692	rBV	194497	416059	28.05%	2.941%
11	3.458	749	752	755	rVB	204	133	0.01%	0.001%
12	3.474	755	757	760	rBV2	212	130	0.01%	0.001%
13	3.539	775	777	779	rVB	265	74	0.00%	0.001%
14	3.590	790	793	795	rVB	219	72	0.00%	0.001%
15	3.626	800	804	806	rBV	123	93	0.01%	0.001%
16	3.741	836	840	846	rBV2	341	269	0.02%	0.002%
17	3.793	853	856	858	rBV	112	83	0.01%	0.001%
18	3.899	871	889	914	rBV3	203236	703267	47.41%	4.971%
19	4.339	1010	1026	1062	rBV	231496	575966	38.83%	4.071%
20	4.600	1088	1107	1131	rBV	316678	790213	53.28%	5.586%
21	4.815	1171	1174	1178	rBV3	325	200	0.01%	0.001%
22	4.892	1195	1198	1203	rBV2	125	120	0.01%	0.001%
23	5.040	1225	1244	1268	rBV2	571631	1483261	100.00%	10.484%
24	5.558	1402	1405	1408	rBV3	206	160	0.01%	0.001%
25	5.609	1408	1421	1468	rBV	581271	1186862	80.02%	8.389%
26	5.912	1502	1515	1539	rVB6	20832	46844	3.16%	0.331%
27	6.063	1548	1562	1596	rBV	325968	671043	45.24%	4.743%
28	6.365	1651	1656	1658	rBV2	158	133	0.01%	0.001%
29	6.400	1658	1667	1672	rBV6	984	1758	0.12%	0.012%
30	6.510	1696	1701	1703	rBV2	188	101	0.01%	0.001%
31	6.529	1703	1707	1710	rBV2	150	132	0.01%	0.001%
32	6.542	1710	1711	1714	rBV2	180	99	0.01%	0.001%
33	6.574	1718	1721	1725	rVB	162	107	0.01%	0.001%
34	6.625	1731	1737	1739	rBV4	790	891	0.06%	0.006%
35	6.789	1785	1788	1790	rBV2	237	154	0.01%	0.001%
36	6.892	1818	1820	1824	rVB2	148	105	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029570.D
 Acq On : 10 Dec 2022 10:56
 Operator : SY/MD
 Sample : N5929-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.918	1825	1828	1831	rBV3	187	127	0.01%	0.001%
38	6.979	1835	1847	1879	rBV	152183	279705	18.86%	1.977%
39	7.307	1936	1949	1978	rBV	700180	1231673	83.04%	8.706%
40	7.613	2034	2044	2067	rBV	106046	188108	12.68%	1.330%
41	7.732	2078	2081	2082	rBV2	334	201	0.01%	0.001%
42	7.879	2124	2127	2130	rBV2	560	348	0.02%	0.002%
43	7.969	2145	2155	2176	rVB	63854	107887	7.27%	0.763%
44	8.082	2180	2190	2233	rBV	390159	720394	48.57%	5.092%
45	8.452	2303	2305	2307	rBV	299	143	0.01%	0.001%
46	8.484	2312	2315	2317	rBV	476	308	0.02%	0.002%
47	8.580	2343	2345	2347	rBV2	352	207	0.01%	0.001%
48	8.613	2353	2355	2358	rVB3	546	219	0.01%	0.002%
49	8.632	2358	2361	2366	rBV2	176	140	0.01%	0.001%
50	8.751	2396	2398	2399	rBV2	205	80	0.01%	0.001%
51	8.793	2408	2411	2412	rBV2	302	142	0.01%	0.001%
52	8.844	2414	2427	2458	rBV	859002	1402653	94.57%	9.914%
53	9.053	2490	2492	2495	rBV2	461	306	0.02%	0.002%
54	9.114	2508	2511	2513	rBV2	499	252	0.02%	0.002%
55	9.162	2522	2526	2533	rVB3	311	318	0.02%	0.002%
56	9.252	2552	2554	2556	rVB3	238	77	0.01%	0.001%
57	9.272	2556	2560	2562	rBV	332	229	0.02%	0.002%
58	9.407	2599	2602	2606	rVB2	314	193	0.01%	0.001%
59	9.494	2626	2629	2630	rBV	221	140	0.01%	0.001%
60	9.516	2635	2636	2638	rBV	190	73	0.00%	0.001%
61	9.529	2638	2640	2643	rBV2	183	142	0.01%	0.001%
62	9.690	2688	2690	2693	rBV	221	139	0.01%	0.001%
63	9.709	2693	2696	2698	rVV2	290	180	0.01%	0.001%
64	9.786	2717	2720	2722	rBV2	297	172	0.01%	0.001%
65	9.860	2740	2743	2745	rBV2	210	137	0.01%	0.001%
66	9.921	2758	2762	2763	rBV2	333	194	0.01%	0.001%
67	10.005	2786	2788	2791	rVB	186	77	0.01%	0.001%
68	10.027	2791	2795	2797	rBV2	152	125	0.01%	0.001%
69	10.072	2803	2809	2812	rBV2	256	304	0.02%	0.002%
70	10.108	2817	2820	2824	rBV2	190	144	0.01%	0.001%
71	10.162	2827	2837	2841	rVV2	21291	30848	2.08%	0.218%
72	10.207	2842	2851	2877	rVB	480097	754965	50.90%	5.336%
73	10.506	2941	2944	2948	rBV	172	176	0.01%	0.001%
74	10.529	2948	2951	2952	rVV	319	156	0.01%	0.001%
75	10.571	2955	2964	2978	rVB2	10145	16777	1.13%	0.119%
76	10.683	2994	2999	3005	rBV2	258	337	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029570.D
 Acq On : 10 Dec 2022 10:56
 Operator : SY/MD
 Sample : N5929-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.722	3008	3011	3015	rVB	322	224	0.02%	0.002%
78	10.751	3015	3020	3023	rBV2	272	248	0.02%	0.002%
79	10.847	3044	3050	3051	rBV	490	273	0.02%	0.002%
80	10.857	3051	3053	3059	rVB2	281	187	0.01%	0.001%
81	10.883	3059	3061	3064	rBB2	195	74	0.00%	0.001%
82	10.905	3064	3068	3069	rBV2	561	343	0.02%	0.002%
83	10.950	3079	3082	3083	rBV	198	100	0.01%	0.001%
84	10.995	3092	3096	3097	rBV	283	172	0.01%	0.001%
85	11.082	3121	3123	3125	rBV2	189	112	0.01%	0.001%
86	11.185	3152	3155	3157	rBV2	384	239	0.02%	0.002%
87	11.236	3159	3171	3196	rBV	928728	1444627	97.40%	10.211%
88	11.471	3240	3244	3247	rBV2	343	322	0.02%	0.002%
89	11.612	3276	3288	3311	rBV	745929	1159203	78.15%	8.194%
90	11.796	3342	3345	3347	rBV3	366	263	0.02%	0.002%
91	12.014	3410	3413	3414	rBV2	292	147	0.01%	0.001%
92	12.191	3463	3468	3471	rVB2	353	357	0.02%	0.003%
93	12.207	3471	3473	3475	rBV	385	215	0.01%	0.002%
94	12.339	3512	3514	3515	rBV	238	113	0.01%	0.001%
95	12.516	3567	3569	3570	rBV2	340	102	0.01%	0.001%
96	12.606	3595	3597	3599	rBV2	500	230	0.02%	0.002%
97	12.673	3617	3618	3619	rBV2	228	74	0.00%	0.001%
98	12.918	3692	3694	3698	rVB2	533	316	0.02%	0.002%
99	12.953	3701	3705	3706	rBV2	338	274	0.02%	0.002%
100	13.088	3745	3747	3750	rVB	323	113	0.01%	0.001%


Sum of corrected areas: 14147503

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029570.D
Acq On : 10 Dec 2022 10:56
Operator : SY/MD
Sample : N5929-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 64 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

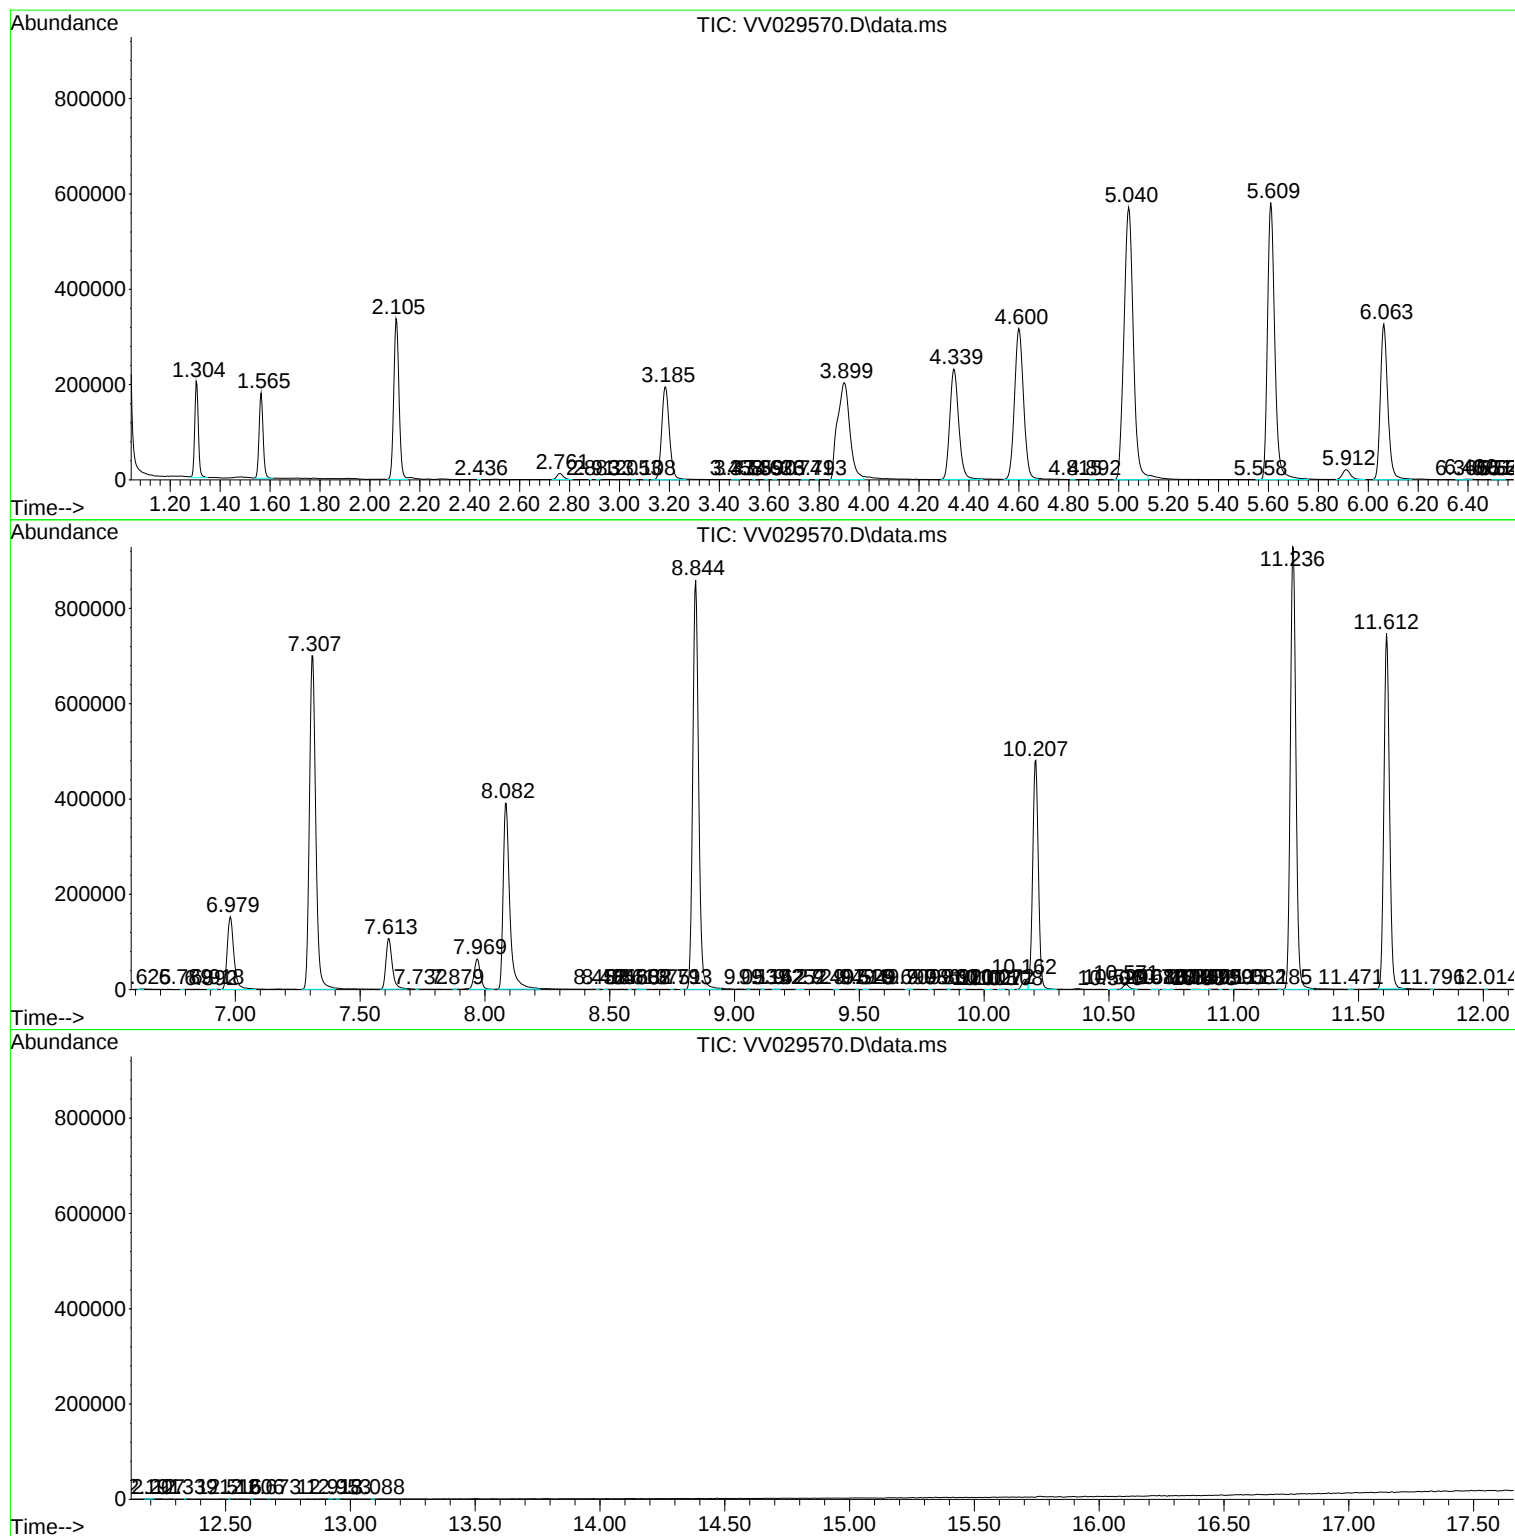

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029570.D
Acq On : 10 Dec 2022 10:56
Operator : SY/MD
Sample : N5929-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 64 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029570.D
Acq On : 10 Dec 2022 10:56
Operator : SY/MD
Sample : N5929-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 64 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------