

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029571.D
 Acq On : 10 Dec 2022 11:20
 Operator : SY/MD
 Sample : N5929-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	201710	202445	14.36%	1.523%
2	1.564	156	163	183	rVB	170266	192035	13.62%	1.444%
3	2.105	320	331	346	rBV	322784	475514	33.73%	3.577%
4	2.500	449	454	462	rVB4	975	1263	0.09%	0.009%
5	2.532	462	464	467	rBV	216	110	0.01%	0.001%
6	2.677	505	509	510	rBV	212	130	0.01%	0.001%
7	2.761	521	535	549	rBV3	11783	21932	1.56%	0.165%
8	2.957	590	596	600	rBV2	228	258	0.02%	0.002%
9	3.044	620	623	627	rBV2	121	95	0.01%	0.001%
10	3.066	627	630	632	rBV	181	103	0.01%	0.001%
11	3.098	638	640	642	rBV	205	110	0.01%	0.001%
12	3.108	642	643	646	rVB2	323	118	0.01%	0.001%
13	3.185	649	667	691	rBV	180687	387160	27.46%	2.912%
14	3.532	773	775	780	rVB	289	143	0.01%	0.001%
15	3.648	803	811	817	rBV2	169	283	0.02%	0.002%
16	3.899	872	889	925	rBV2	191829	672093	47.68%	5.055%
17	4.339	1010	1026	1053	rBV	219998	544585	38.63%	4.096%
18	4.600	1090	1107	1135	rBV2	296291	739917	52.49%	5.565%
19	4.815	1171	1174	1179	rVB2	158	127	0.01%	0.001%
20	4.854	1183	1186	1188	rBV2	183	94	0.01%	0.001%
21	5.040	1226	1244	1269	rBV3	537421	1409700	100.00%	10.603%
22	5.452	1369	1372	1373	rBV	284	121	0.01%	0.001%
23	5.503	1385	1388	1391	rVB2	303	204	0.01%	0.002%
24	5.551	1401	1403	1406	rVB	255	151	0.01%	0.001%
25	5.609	1406	1421	1462	rBV	540855	1103305	78.27%	8.299%
26	5.912	1504	1515	1538	rVB6	18708	42457	3.01%	0.319%
27	6.063	1547	1562	1597	rBV	301116	625889	44.40%	4.708%
28	6.240	1616	1617	1620	rVB2	664	288	0.02%	0.002%
29	6.265	1622	1625	1628	rVB	173	96	0.01%	0.001%
30	6.304	1635	1637	1641	rVB	289	143	0.01%	0.001%
31	6.487	1691	1694	1698	rBV2	221	148	0.01%	0.001%
32	6.584	1722	1724	1729	rVB2	263	200	0.01%	0.002%
33	6.622	1729	1736	1739	rBV2	1137	1358	0.10%	0.010%
34	6.821	1796	1798	1800	rBV	176	105	0.01%	0.001%
35	6.863	1808	1811	1816	rBV3	184	136	0.01%	0.001%
36	6.902	1820	1823	1826	rBV2	182	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029571.D
 Acq On : 10 Dec 2022 11:20
 Operator : SY/MD
 Sample : N5929-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.918	1826	1828	1834	rVB2	253	174	0.01%	0.001%
38	6.979	1835	1847	1887	rBV	142663	266567	18.91%	2.005%
39	7.156	1897	1902	1903	rBV2	837	513	0.04%	0.004%
40	7.307	1937	1949	1984	rBV	658130	1168605	82.90%	8.790%
41	7.612	2034	2044	2061	rBV	100583	175556	12.45%	1.320%
42	7.805	2099	2104	2106	rBV3	533	510	0.04%	0.004%
43	7.841	2111	2115	2116	rBV2	314	220	0.02%	0.002%
44	7.889	2128	2130	2131	rBV2	265	132	0.01%	0.001%
45	7.969	2144	2155	2176	rVB2	57948	100649	7.14%	0.757%
46	8.085	2180	2191	2221	rBV	371801	676758	48.01%	5.090%
47	8.397	2282	2288	2292	rBV4	562	546	0.04%	0.004%
48	8.471	2309	2311	2317	rVB3	461	362	0.03%	0.003%
49	8.577	2339	2344	2350	rVB4	501	466	0.03%	0.004%
50	8.606	2350	2353	2354	rBV2	228	134	0.01%	0.001%
51	8.651	2365	2367	2371	rBV2	347	182	0.01%	0.001%
52	8.686	2376	2378	2380	rVB	374	114	0.01%	0.001%
53	8.696	2380	2381	2385	rVB2	176	91	0.01%	0.001%
54	8.731	2388	2392	2393	rBV2	276	208	0.01%	0.002%
55	8.844	2414	2427	2459	rBV	791139	1300604	92.26%	9.783%
56	9.159	2523	2525	2528	rBB	306	130	0.01%	0.001%
57	9.207	2538	2540	2544	rVB2	248	152	0.01%	0.001%
58	9.230	2544	2547	2549	rBV	397	218	0.02%	0.002%
59	9.272	2554	2560	2563	rBV3	346	323	0.02%	0.002%
60	9.400	2596	2600	2603	rBV	333	199	0.01%	0.001%
61	9.423	2603	2607	2609	rBV2	319	234	0.02%	0.002%
62	9.458	2616	2618	2624	rVB2	204	134	0.01%	0.001%
63	9.542	2640	2644	2647	rBV2	245	198	0.01%	0.001%
64	9.593	2657	2660	2663	rVV2	177	141	0.01%	0.001%
65	9.609	2663	2665	2670	rVB2	276	190	0.01%	0.001%
66	9.638	2670	2674	2676	rBV	161	144	0.01%	0.001%
67	9.702	2688	2694	2697	rBV2	110	140	0.01%	0.001%
68	9.760	2709	2712	2716	rVB2	201	125	0.01%	0.001%
69	9.815	2726	2729	2733	rVB2	248	193	0.01%	0.001%
70	9.863	2741	2744	2747	rVB	289	178	0.01%	0.001%
71	9.886	2747	2751	2754	rBV2	110	121	0.01%	0.001%
72	9.924	2760	2763	2765	rBV	304	165	0.01%	0.001%
73	9.963	2773	2775	2780	rVB2	244	153	0.01%	0.001%
74	9.998	2784	2786	2791	rVB3	248	161	0.01%	0.001%
75	10.021	2791	2793	2796	rBV	189	90	0.01%	0.001%
76	10.079	2808	2811	2812	rBV2	243	139	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029571.D
 Acq On : 10 Dec 2022 11:20
 Operator : SY/MD
 Sample : N5929-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.120	2820	2824	2827	rVV3	230	218	0.02%	0.002%
78	10.162	2827	2837	2841	rVV2	20172	29374	2.08%	0.221%
79	10.207	2842	2851	2870	rVB	447647	704342	49.96%	5.298%
80	10.371	2896	2902	2911	rBV4	1291	1661	0.12%	0.012%
81	10.442	2922	2924	2927	rBV2	172	98	0.01%	0.001%
82	10.567	2955	2963	2973	rVV3	9411	14478	1.03%	0.109%
83	10.683	2996	2999	3001	rBV	425	245	0.02%	0.002%
84	10.712	3006	3008	3011	rVB2	304	119	0.01%	0.001%
85	10.731	3011	3014	3016	rBV2	175	118	0.01%	0.001%
86	10.789	3029	3032	3034	rVB	193	108	0.01%	0.001%
87	10.902	3065	3067	3070	rBV2	257	146	0.01%	0.001%
88	10.976	3087	3090	3093	rVB	196	140	0.01%	0.001%
89	11.011	3097	3101	3102	rBV2	192	112	0.01%	0.001%
90	11.149	3142	3144	3148	rVB2	281	197	0.01%	0.001%
91	11.172	3149	3151	3153	rBV2	227	108	0.01%	0.001%
92	11.236	3160	3171	3196	rBV	855092	1331578	94.46%	10.016%
93	11.484	3244	3248	3250	rBV2	292	245	0.02%	0.002%
94	11.612	3275	3288	3309	rBV	698914	1091197	77.41%	8.208%
95	11.847	3359	3361	3364	rBV	295	201	0.01%	0.002%
96	12.201	3468	3471	3474	rBV3	363	301	0.02%	0.002%
97	12.307	3500	3504	3506	rBV3	451	383	0.03%	0.003%
98	12.358	3518	3520	3523	rBV2	312	201	0.01%	0.002%
99	12.394	3529	3531	3534	rVB	443	166	0.01%	0.001%
100	12.921	3693	3695	3698	rBV3	356	199	0.01%	0.001%




Sum of corrected areas: 13294784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029571.D
Acq On : 10 Dec 2022 11:20
Operator : SY/MD
Sample : N5929-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

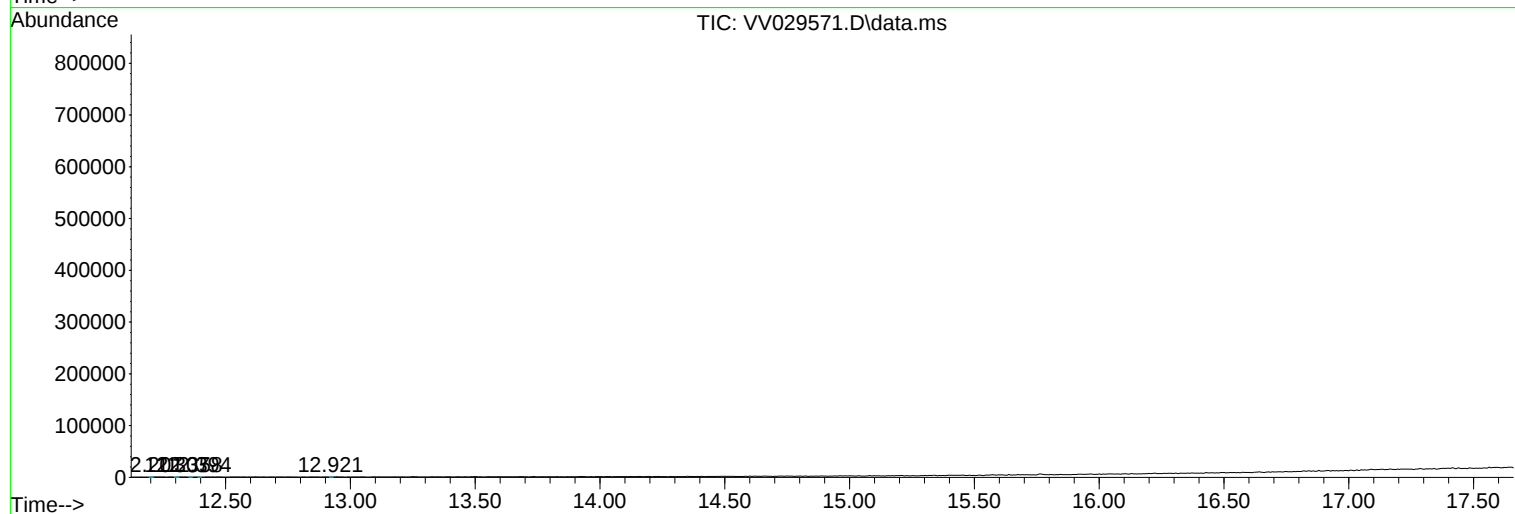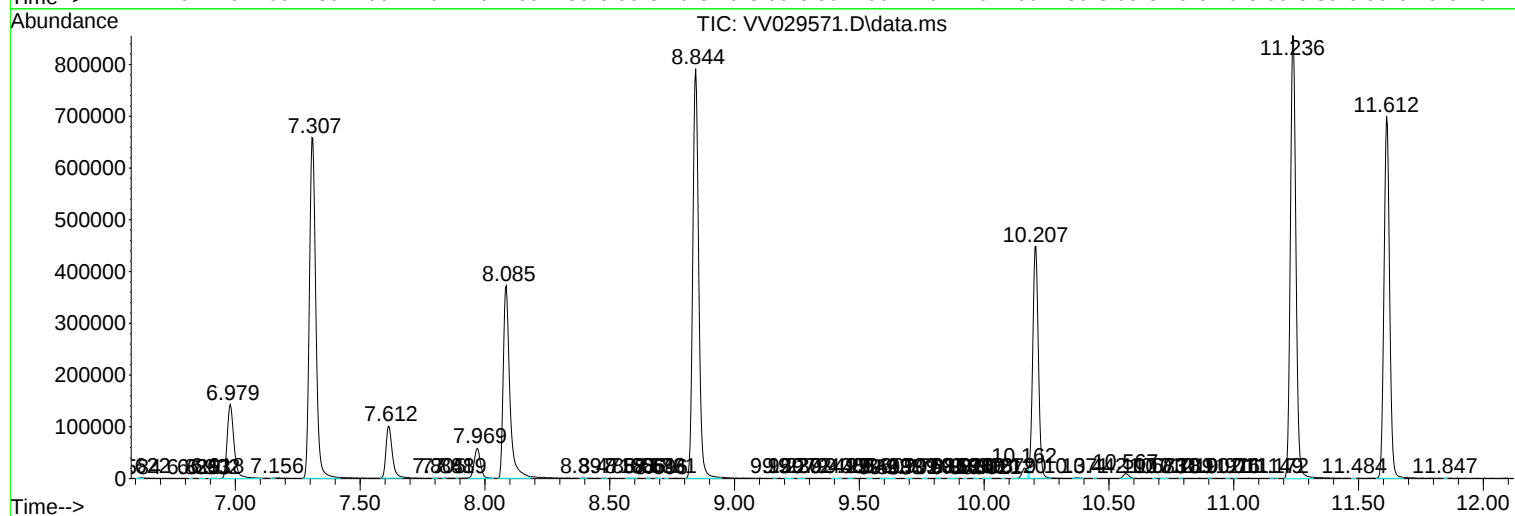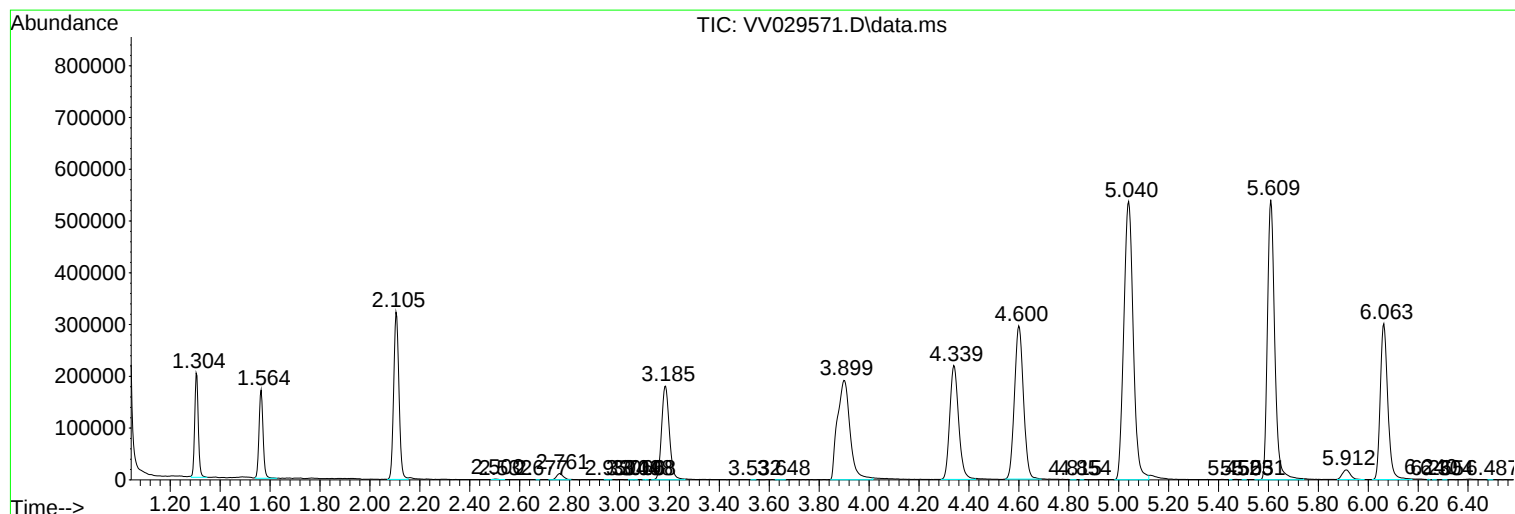

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029571.D
Acq On : 10 Dec 2022 11:20
Operator : SY/MD
Sample : N5929-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029571.D
Acq On : 10 Dec 2022 11:20
Operator : SY/MD
Sample : N5929-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc