

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029573.D
 Acq On : 10 Dec 2022 12:07
 Operator : SY/MD
 Sample : N5928-07 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	208333	213341	15.02%	1.745%
2	1.564	155	163	178	rVB	171955	191901	13.51%	1.570%
3	2.105	320	331	362	rBV	324565	470355	33.10%	3.848%
4	2.503	449	455	469	rVB3	2694	4520	0.32%	0.037%
5	2.609	482	488	490	rBV3	862	900	0.06%	0.007%
6	2.671	505	507	511	rVB2	224	139	0.01%	0.001%
7	2.764	527	536	541	rBV3	1485	2151	0.15%	0.018%
8	2.915	577	583	590	rBV2	416	523	0.04%	0.004%
9	2.947	590	593	595	rBV	152	105	0.01%	0.001%
10	2.989	603	606	610	rVB3	306	234	0.02%	0.002%
11	3.034	613	620	623	rBV3	253	264	0.02%	0.002%
12	3.185	653	667	686	rVV2	20728	43269	3.05%	0.354%
13	3.490	760	762	768	rVB3	297	290	0.02%	0.002%
14	3.593	791	794	799	rVB2	170	157	0.01%	0.001%
15	3.645	805	810	812	rBV2	164	135	0.01%	0.001%
16	3.741	837	840	845	rBV2	162	119	0.01%	0.001%
17	3.880	870	883	920	rBV4	132033	530875	37.36%	4.343%
18	4.339	1010	1026	1059	rBV	221043	545050	38.36%	4.459%
19	4.600	1097	1107	1124	rVB3	14279	34564	2.43%	0.283%
20	4.690	1131	1135	1140	rBV3	172	202	0.01%	0.002%
21	4.735	1146	1149	1153	rBV2	193	157	0.01%	0.001%
22	4.764	1153	1158	1162	rVB3	268	209	0.01%	0.002%
23	4.867	1187	1190	1194	rBV2	127	110	0.01%	0.001%
24	5.040	1226	1244	1274	rBV2	540726	1420825	100.00%	11.624%
25	5.285	1318	1320	1323	rVB	604	228	0.02%	0.002%
26	5.307	1324	1327	1333	rBV3	296	317	0.02%	0.003%
27	5.397	1348	1355	1359	rBV3	308	411	0.03%	0.003%
28	5.465	1373	1376	1377	rBV	163	108	0.01%	0.001%
29	5.513	1388	1391	1392	rBV2	177	118	0.01%	0.001%
30	5.609	1408	1421	1464	rVV	555050	1125166	79.19%	9.205%
31	5.902	1503	1512	1513	rBV2	5240	5879	0.41%	0.048%
32	5.963	1529	1531	1534	rBV2	278	175	0.01%	0.001%
33	6.005	1541	1544	1546	rBV3	190	113	0.01%	0.001%
34	6.063	1548	1562	1597	rBV	307244	632095	44.49%	5.171%
35	6.301	1632	1636	1640	rVB2	382	311	0.02%	0.003%
36	6.336	1644	1647	1652	rVB2	184	148	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029573.D
 Acq On : 10 Dec 2022 12:07
 Operator : SY/MD
 Sample : N5928-07 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.368	1652	1657	1659	rBV2	271	221	0.02%	0.002%
38	6.420	1670	1673	1675	rBV	235	146	0.01%	0.001%
39	6.551	1712	1714	1718	rBV2	171	103	0.01%	0.001%
40	6.603	1724	1730	1731	rBV2	351	250	0.02%	0.002%
41	6.619	1732	1735	1736	rBV	588	333	0.02%	0.003%
42	6.831	1796	1801	1802	rBV	292	240	0.02%	0.002%
43	6.850	1806	1807	1811	rVB2	221	111	0.01%	0.001%
44	6.979	1836	1847	1874	rBV	142230	262672	18.49%	2.149%
45	7.256	1930	1933	1934	rBV	396	157	0.01%	0.001%
46	7.307	1937	1949	1980	rVV	675480	1181790	83.18%	9.669%
47	7.616	2034	2045	2078	rBV	101734	182781	12.86%	1.495%
48	7.786	2096	2098	2104	rVB2	506	315	0.02%	0.003%
49	7.821	2104	2109	2110	rBV2	423	335	0.02%	0.003%
50	7.863	2120	2122	2125	rVB2	433	217	0.02%	0.002%
51	8.082	2180	2190	2231	rBV	381647	701360	49.36%	5.738%
52	8.548	2330	2335	2337	rBV2	412	301	0.02%	0.002%
53	8.609	2351	2354	2356	rBV2	311	192	0.01%	0.002%
54	8.622	2356	2358	2359	rVV2	399	176	0.01%	0.001%
55	8.648	2363	2366	2372	rBV4	417	324	0.02%	0.003%
56	8.738	2391	2394	2397	rVB2	219	116	0.01%	0.001%
57	8.764	2397	2402	2407	rBV3	335	325	0.02%	0.003%
58	8.844	2414	2427	2455	rBV	803851	1329352	93.56%	10.876%
59	9.104	2506	2508	2513	rVB2	370	286	0.02%	0.002%
60	9.133	2513	2517	2523	rBV5	613	717	0.05%	0.006%
61	9.194	2534	2536	2539	rVB	317	184	0.01%	0.002%
62	9.243	2548	2551	2554	rVB	259	185	0.01%	0.002%
63	9.452	2610	2616	2618	rBV	302	222	0.02%	0.002%
64	9.513	2632	2635	2636	rBV2	333	192	0.01%	0.002%
65	9.538	2636	2643	2649	rVV2	1780	2301	0.16%	0.019%
66	9.715	2695	2698	2702	rVB3	239	174	0.01%	0.001%
67	9.805	2723	2726	2731	rBV2	173	201	0.01%	0.002%
68	9.921	2758	2762	2765	rBV4	352	314	0.02%	0.003%
69	9.992	2781	2784	2785	rBV2	187	105	0.01%	0.001%
70	10.056	2802	2804	2807	rVV	203	120	0.01%	0.001%
71	10.075	2807	2810	2813	rVB	295	140	0.01%	0.001%
72	10.162	2825	2837	2841	rBV	20122	29011	2.04%	0.237%
73	10.207	2842	2851	2872	rVB	458017	716749	50.45%	5.864%
74	10.436	2918	2922	2933	rVV5	914	1744	0.12%	0.014%
75	10.474	2933	2934	2937	rVB2	422	165	0.01%	0.001%
76	10.500	2937	2942	2947	rBV2	383	256	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029573.D
 Acq On : 10 Dec 2022 12:07
 Operator : SY/MD
 Sample : N5928-07 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.532	2947	2952	2955	rBV4	807	854	0.06%	0.007%
78	10.567	2955	2963	2978	rVV2	9423	15116	1.06%	0.124%
79	10.645	2982	2987	2989	rBV3	184	151	0.01%	0.001%
80	10.725	3006	3012	3022	rBV5	1619	2351	0.17%	0.019%
81	10.821	3038	3042	3045	rBV2	279	238	0.02%	0.002%
82	10.908	3061	3069	3079	rVV2	3889	5906	0.42%	0.048%
83	10.950	3079	3082	3087	rVB3	421	321	0.02%	0.003%
84	11.027	3103	3106	3108	rBV2	347	214	0.02%	0.002%
85	11.072	3118	3120	3123	rVB2	219	125	0.01%	0.001%
86	11.159	3144	3147	3151	rVB	382	205	0.01%	0.002%
87	11.239	3159	3172	3192	rBV	891882	1392330	97.99%	11.391%
88	11.445	3232	3236	3238	rBV2	444	261	0.02%	0.002%
89	11.468	3241	3243	3245	rBV3	290	153	0.01%	0.001%
90	11.516	3253	3258	3265	rVB5	1168	1513	0.11%	0.012%
91	11.612	3276	3288	3313	rBV	707180	1113854	78.39%	9.113%
92	11.841	3357	3359	3364	rVB2	428	227	0.02%	0.002%
93	11.866	3364	3367	3369	rBV	197	127	0.01%	0.001%
94	11.915	3369	3382	3396	rBV3	26804	46620	3.28%	0.381%
95	12.027	3416	3417	3421	rBV2	388	244	0.02%	0.002%
96	12.233	3479	3481	3485	rBV2	356	208	0.01%	0.002%
97	12.352	3516	3518	3521	rBV2	313	210	0.01%	0.002%
98	12.628	3601	3604	3608	rBV3	416	342	0.02%	0.003%
99	13.143	3762	3764	3769	rBV	533	409	0.03%	0.003%
100	13.275	3801	3805	3807	rBV4	623	472	0.03%	0.004%




Sum of corrected areas: 12222798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029573.D
Acq On : 10 Dec 2022 12:07
Operator : SY/MD
Sample : N5928-07 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 67 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

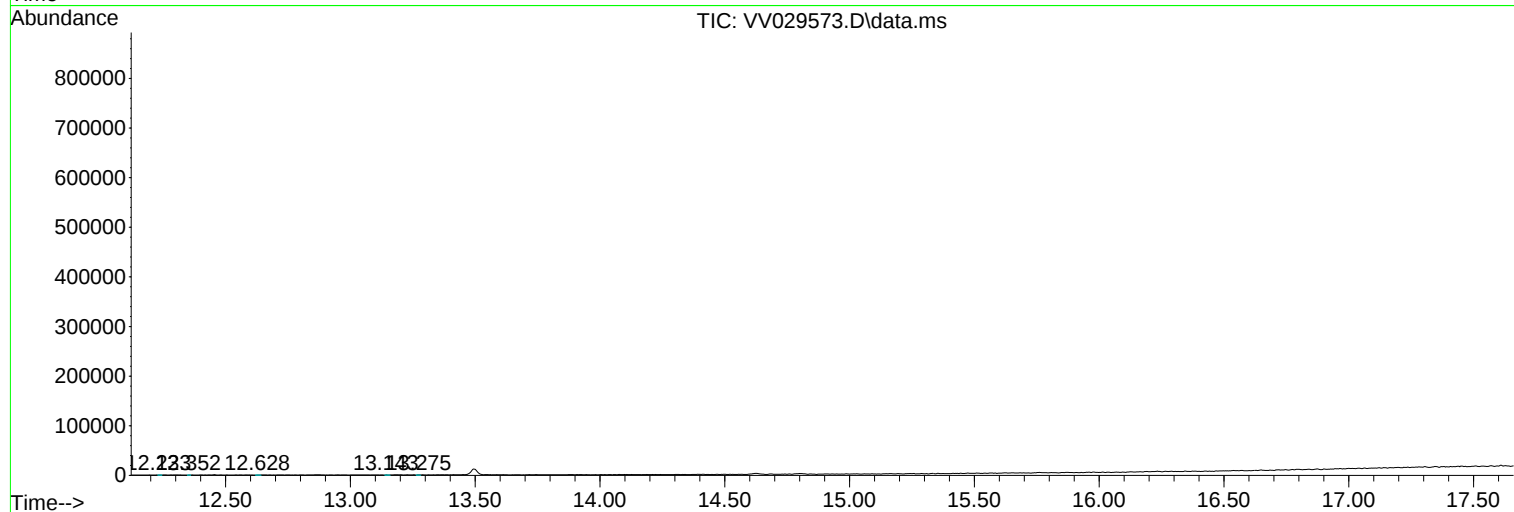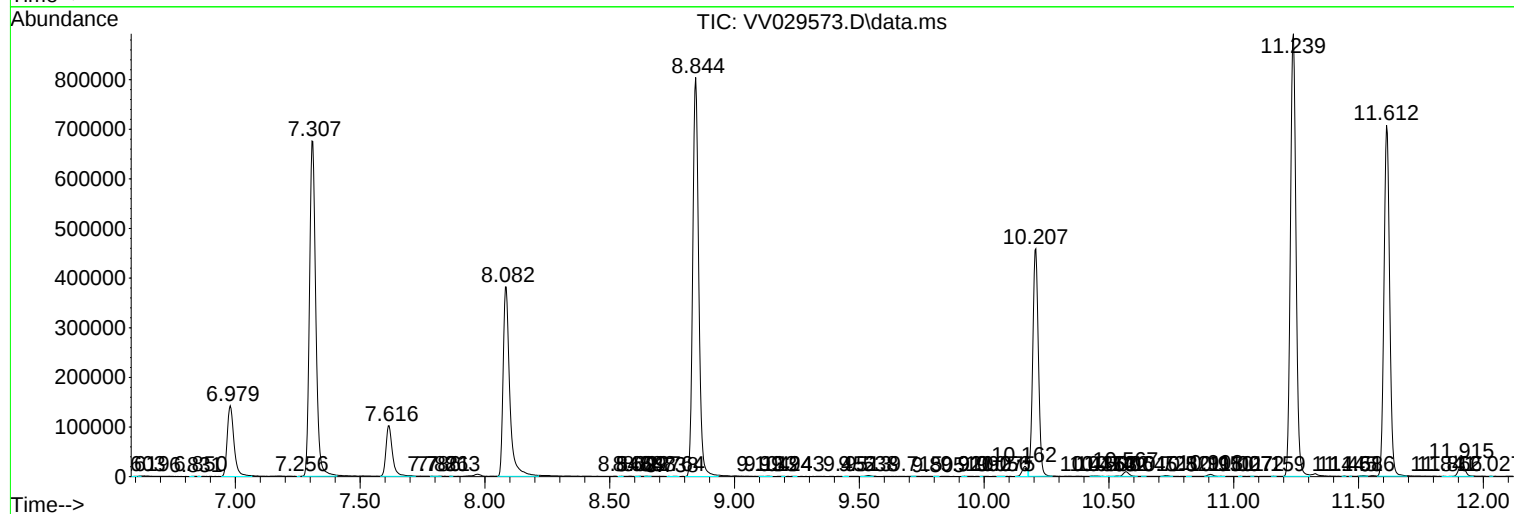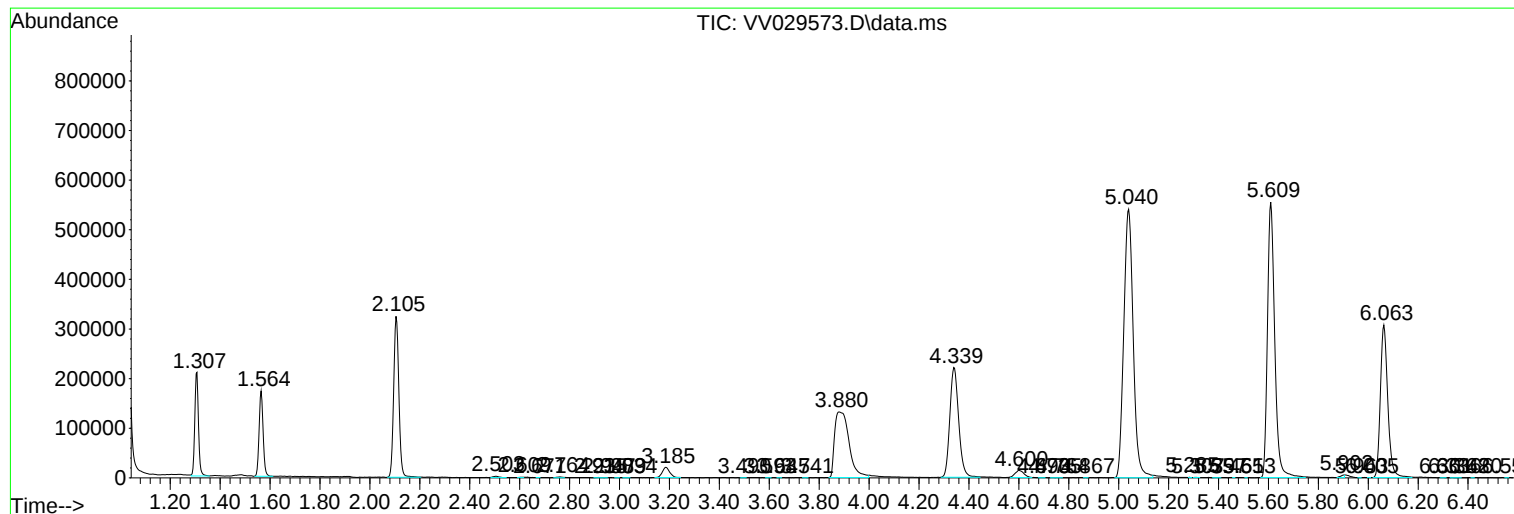

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029573.D
Acq On : 10 Dec 2022 12:07
Operator : SY/MD
Sample : N5928-07 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 67 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029573.D
Acq On : 10 Dec 2022 12:07
Operator : SY/MD
Sample : N5928-07 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 67 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------