

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029575.D
 Acq On : 10 Dec 2022 12:53
 Operator : SY/MD
 Sample : N5928-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	200337	202682	13.58%	1.614%
2	1.564	155	163	176	rVB	168428	192915	12.92%	1.537%
3	2.105	320	331	349	rBV	328229	475471	31.85%	3.787%
4	2.416	426	428	431	rBV2	405	277	0.02%	0.002%
5	2.503	448	455	466	rVB2	3042	4753	0.32%	0.038%
6	2.580	475	479	481	rBV2	319	225	0.02%	0.002%
7	2.751	529	532	533	rBV2	356	229	0.02%	0.002%
8	2.863	562	567	570	rBV2	153	154	0.01%	0.001%
9	2.915	577	583	587	rBV2	275	335	0.02%	0.003%
10	3.088	634	637	641	rVB2	324	289	0.02%	0.002%
11	3.114	641	645	650	rBV2	261	258	0.02%	0.002%
12	3.185	656	667	682	rVB2	7783	16996	1.14%	0.135%
13	3.391	727	731	735	rBV	169	164	0.01%	0.001%
14	3.413	735	738	741	rVB	238	151	0.01%	0.001%
15	3.432	741	744	749	rVB	196	130	0.01%	0.001%
16	3.513	763	769	772	rBV	171	194	0.01%	0.002%
17	3.751	839	843	847	rBV2	146	140	0.01%	0.001%
18	3.776	847	851	857	rVB3	203	250	0.02%	0.002%
19	3.873	871	881	924	rBV2	126332	423176	28.35%	3.371%
20	4.339	1009	1026	1059	rBV2	227629	568601	38.09%	4.529%
21	4.725	1142	1146	1148	rBV2	160	165	0.01%	0.001%
22	4.818	1172	1175	1178	rBV3	222	148	0.01%	0.001%
23	4.834	1178	1180	1184	rVB	284	162	0.01%	0.001%
24	4.857	1184	1187	1189	rBV	317	169	0.01%	0.001%
25	4.889	1192	1197	1202	rBV2	250	235	0.02%	0.002%
26	4.924	1205	1208	1213	rVB3	305	184	0.01%	0.001%
27	5.040	1223	1244	1293	rBV2	568959	1492629	100.00%	11.889%
28	5.410	1357	1359	1370	rVB3	488	539	0.04%	0.004%
29	5.455	1370	1373	1377	rBV	343	335	0.02%	0.003%
30	5.477	1377	1380	1384	rBV3	236	222	0.01%	0.002%
31	5.555	1401	1404	1407	rBV	287	207	0.01%	0.002%
32	5.609	1407	1421	1469	rBV	586013	1194686	80.04%	9.516%
33	5.908	1503	1514	1532	rVB7	11313	27319	1.83%	0.218%
34	6.063	1548	1562	1588	rBV	321828	659716	44.20%	5.255%
35	6.252	1620	1621	1625	rVB	406	209	0.01%	0.002%
36	6.307	1633	1638	1642	rBV2	243	224	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029575.D
 Acq On : 10 Dec 2022 12:53
 Operator : SY/MD
 Sample : N5928-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.436	1676	1678	1683	rVB	210	137	0.01%	0.001%
38	6.580	1718	1723	1725	rBV3	191	177	0.01%	0.001%
39	6.622	1729	1736	1739	rBV4	1214	1530	0.10%	0.012%
40	6.741	1769	1773	1775	rBV2	339	184	0.01%	0.001%
41	6.757	1775	1778	1784	rVB2	283	282	0.02%	0.002%
42	6.879	1814	1816	1823	rVB2	302	271	0.02%	0.002%
43	6.979	1834	1847	1875	rBV	146321	273371	18.31%	2.177%
44	7.149	1895	1900	1902	rBV3	459	414	0.03%	0.003%
45	7.243	1925	1929	1933	rBV3	489	431	0.03%	0.003%
46	7.307	1937	1949	1981	rBV	688122	1215597	81.44%	9.683%
47	7.616	2033	2045	2077	rBV	104989	189036	12.66%	1.506%
48	7.786	2095	2098	2102	rBV3	535	436	0.03%	0.003%
49	7.825	2107	2110	2112	rBV2	390	208	0.01%	0.002%
50	7.969	2147	2155	2166	rVB3	9536	16256	1.09%	0.129%
51	8.043	2175	2178	2180	rBV2	284	181	0.01%	0.001%
52	8.085	2180	2191	2230	rBV	411662	743872	49.84%	5.925%
53	8.419	2291	2295	2299	rBV2	679	548	0.04%	0.004%
54	8.564	2334	2340	2346	rBV4	408	469	0.03%	0.004%
55	8.680	2375	2376	2380	rBV2	266	141	0.01%	0.001%
56	8.706	2380	2384	2387	rBV3	309	256	0.02%	0.002%
57	8.754	2396	2399	2402	rVB3	347	246	0.02%	0.002%
58	8.773	2402	2405	2409	rBV2	283	272	0.02%	0.002%
59	8.796	2409	2412	2415	rBV2	366	227	0.02%	0.002%
60	8.844	2415	2427	2461	rBV	844224	1400210	93.81%	11.153%
61	9.095	2502	2505	2508	rVB	395	192	0.01%	0.002%
62	9.355	2584	2586	2592	rBV2	205	202	0.01%	0.002%
63	9.419	2603	2606	2609	rBV	204	133	0.01%	0.001%
64	9.448	2612	2615	2616	rBV	237	135	0.01%	0.001%
65	9.542	2637	2644	2646	rBV2	536	585	0.04%	0.005%
66	9.664	2678	2682	2685	rBV2	202	180	0.01%	0.001%
67	9.689	2688	2690	2694	rVB3	536	343	0.02%	0.003%
68	9.837	2733	2736	2741	rVB	230	185	0.01%	0.001%
69	9.902	2752	2756	2758	rBV	381	198	0.01%	0.002%
70	9.921	2758	2762	2764	rBV2	457	311	0.02%	0.002%
71	10.024	2791	2794	2797	rVB2	237	139	0.01%	0.001%
72	10.053	2797	2803	2805	rBV2	204	209	0.01%	0.002%
73	10.165	2827	2838	2841	rBV	21180	30306	2.03%	0.241%
74	10.207	2842	2851	2871	rVB	478059	750057	50.25%	5.974%
75	10.442	2919	2924	2927	rBV3	382	443	0.03%	0.004%
76	10.487	2935	2938	2942	rVB2	267	210	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029575.D
 Acq On : 10 Dec 2022 12:53
 Operator : SY/MD
 Sample : N5928-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.529	2942	2951	2957	rBV2	7089	9823	0.66%	0.078%
78	10.728	3005	3013	3023	rBV	7263	10988	0.74%	0.088%
79	10.799	3032	3035	3038	rBV2	401	287	0.02%	0.002%
80	10.837	3043	3047	3048	rBV	375	193	0.01%	0.002%
81	10.905	3059	3068	3077	rBV	15211	22146	1.48%	0.176%
82	10.979	3086	3091	3094	rBV2	322	285	0.02%	0.002%
83	11.043	3108	3111	3114	rVB3	277	170	0.01%	0.001%
84	11.072	3118	3120	3124	rVB	258	143	0.01%	0.001%
85	11.185	3148	3155	3160	rBV3	1615	1494	0.10%	0.012%
86	11.239	3160	3172	3192	rBV	934624	1457335	97.64%	11.608%
87	11.612	3277	3288	3306	rBV	727289	1145635	76.75%	9.125%
88	11.847	3359	3361	3364	rBV	187	148	0.01%	0.001%
89	11.866	3364	3367	3369	rVB2	330	186	0.01%	0.001%
90	11.902	3370	3378	3379	rBV4	2290	1983	0.13%	0.016%
91	12.001	3403	3409	3418	rBV3	2727	4319	0.29%	0.034%
92	12.098	3435	3439	3442	rBV3	1046	951	0.06%	0.008%
93	12.172	3460	3462	3465	rBV2	294	176	0.01%	0.001%
94	12.230	3475	3480	3482	rBV2	352	279	0.02%	0.002%
95	12.365	3519	3522	3524	rBV2	279	170	0.01%	0.001%
96	12.394	3528	3531	3532	rBV2	780	442	0.03%	0.004%
97	12.529	3570	3573	3576	rBV2	453	327	0.02%	0.003%
98	12.680	3616	3620	3622	rBV3	470	402	0.03%	0.003%
99	12.869	3673	3679	3685	rBV5	2019	2715	0.18%	0.022%
100	13.258	3795	3800	3803	rBV4	815	732	0.05%	0.006%


Sum of corrected areas: 12554448

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029575.D
Acq On : 10 Dec 2022 12:53
Operator : SY/MD
Sample : N5928-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

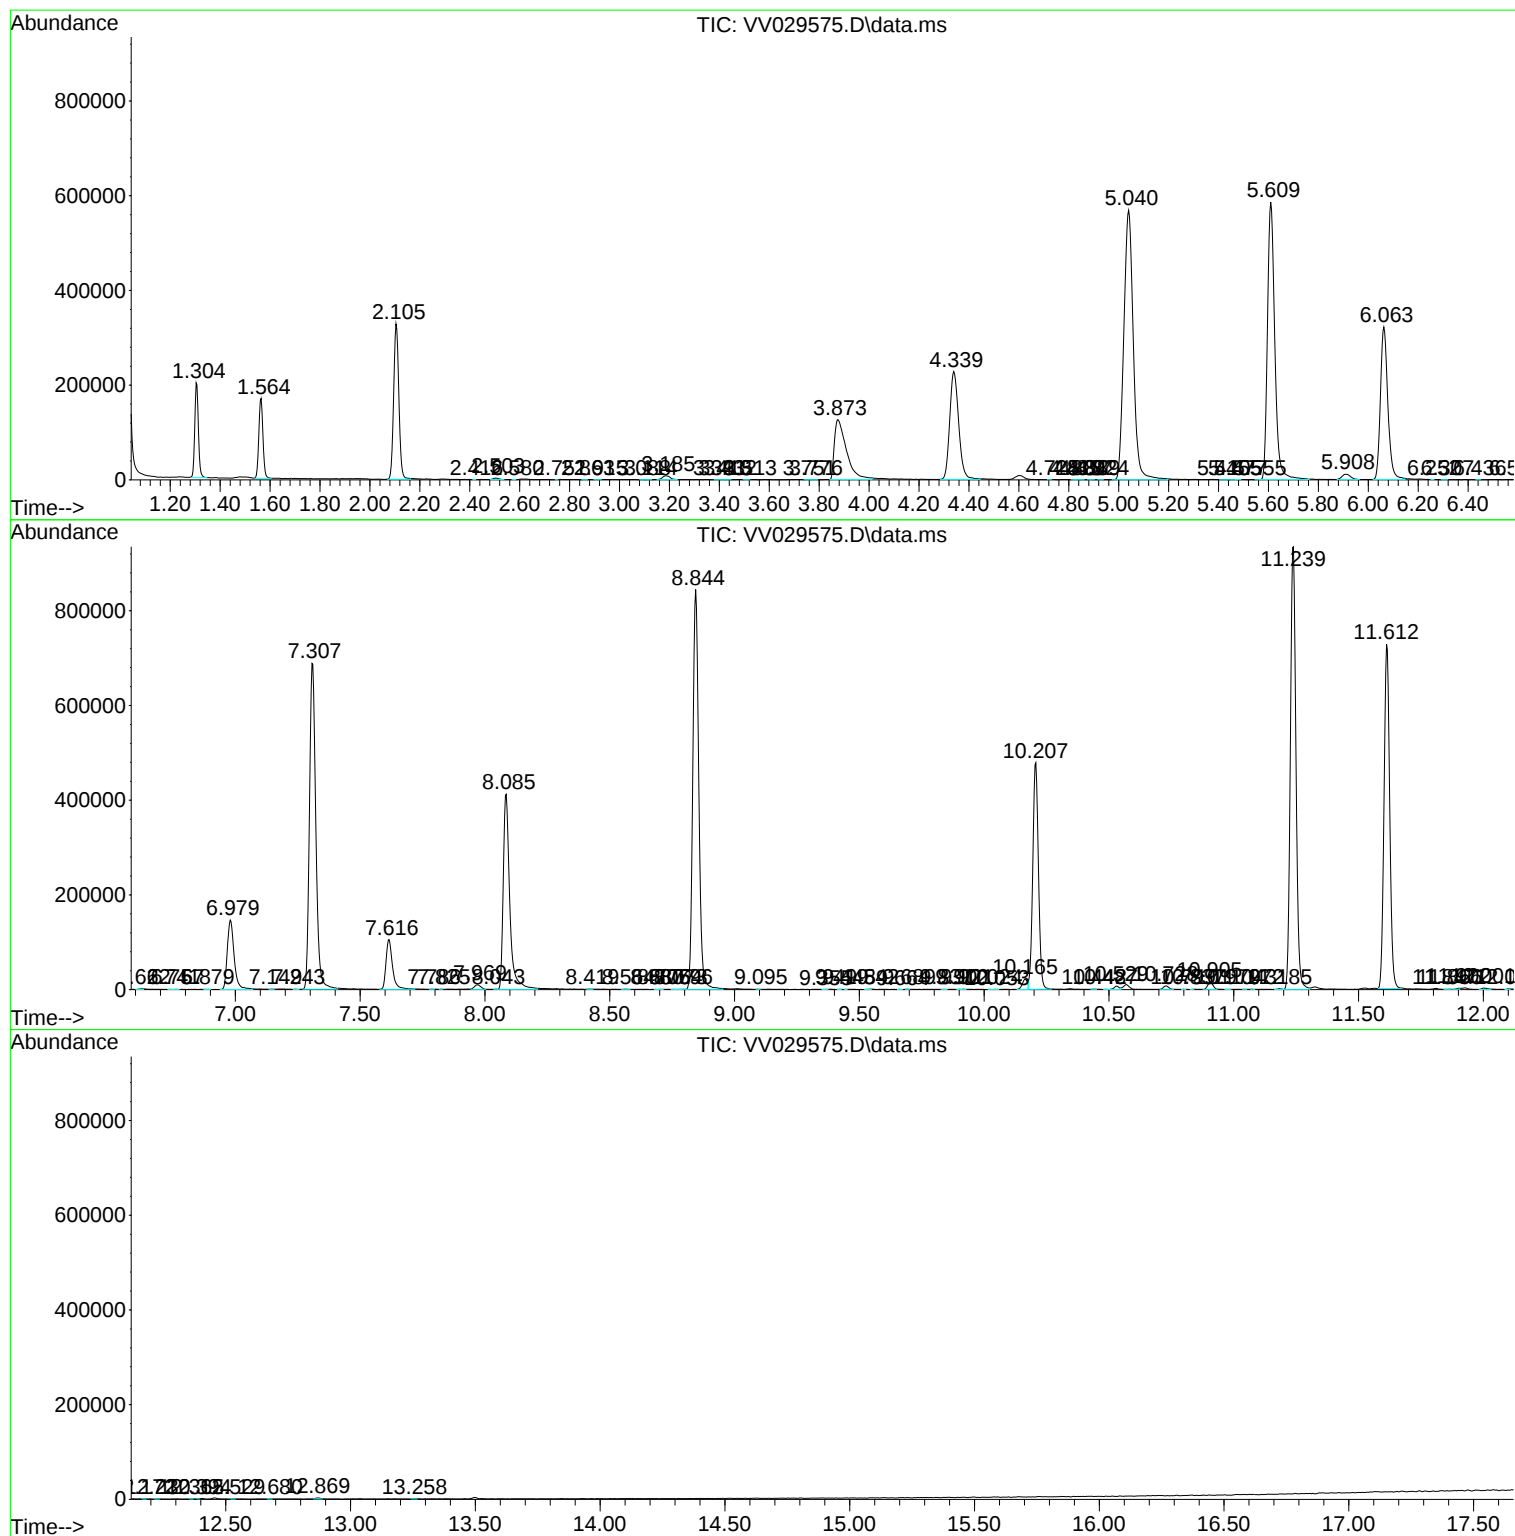

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029575.D
Acq On : 10 Dec 2022 12:53
Operator : SY/MD
Sample : N5928-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029575.D
Acq On : 10 Dec 2022 12:53
Operator : SY/MD
Sample : N5928-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------