

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029576.D
 Acq On : 10 Dec 2022 13:17
 Operator : SY/MD
 Sample : N5928-09 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	207944	209015	13.63%	1.646%
2	1.561	155	162	176	rVB	181627	204389	13.33%	1.609%
3	2.105	320	331	349	rBV	344774	495713	32.34%	3.903%
4	2.503	443	455	465	rBV4	3259	5768	0.38%	0.045%
5	2.719	518	522	524	rBV	136	92	0.01%	0.001%
6	2.921	581	585	589	rBV	160	158	0.01%	0.001%
7	2.998	607	609	613	rVB2	227	129	0.01%	0.001%
8	3.021	613	616	618	rBV	248	151	0.01%	0.001%
9	3.182	658	666	669	rBV3	1572	1949	0.13%	0.015%
10	3.333	710	713	715	rBV	140	91	0.01%	0.001%
11	3.394	730	732	733	rBV	137	47	0.00%	0.000%
12	3.445	746	748	750	rBV2	140	84	0.01%	0.001%
13	3.561	781	784	786	rBV	208	105	0.01%	0.001%
14	3.699	823	827	828	rBV	150	89	0.01%	0.001%
15	3.728	833	836	840	rVB2	207	153	0.01%	0.001%
16	3.873	868	881	923	rBV2	127583	405132	26.43%	3.190%
17	4.339	1011	1026	1063	rVB	236453	585452	38.19%	4.610%
18	4.693	1134	1136	1142	rVB3	294	221	0.01%	0.002%
19	4.725	1142	1146	1147	rBV	171	142	0.01%	0.001%
20	4.754	1154	1155	1156	rBV	118	25	0.00%	0.000%
21	4.764	1156	1158	1161	rBV2	222	179	0.01%	0.001%
22	4.915	1202	1205	1207	rBV2	166	110	0.01%	0.001%
23	5.040	1225	1244	1269	rBV2	589000	1533053	100.00%	12.071%
24	5.465	1373	1376	1377	rBV3	399	207	0.01%	0.002%
25	5.532	1394	1397	1402	rBV	287	274	0.02%	0.002%
26	5.558	1402	1405	1407	rBV	166	112	0.01%	0.001%
27	5.609	1407	1421	1461	rBV	592386	1205595	78.64%	9.492%
28	5.838	1490	1492	1496	rBV	358	227	0.01%	0.002%
29	6.063	1548	1562	1587	rBV	337209	687385	44.84%	5.412%
30	6.278	1628	1629	1631	rVB	277	66	0.00%	0.001%
31	6.288	1631	1632	1635	rBV2	179	95	0.01%	0.001%
32	6.394	1664	1665	1671	rVB2	512	259	0.02%	0.002%
33	6.468	1684	1688	1690	rBV2	207	153	0.01%	0.001%
34	6.481	1690	1692	1698	rVV2	290	199	0.01%	0.002%
35	6.522	1701	1705	1707	rBV2	190	115	0.01%	0.001%
36	6.574	1719	1721	1724	rVB2	193	72	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029576.D
 Acq On : 10 Dec 2022 13:17
 Operator : SY/MD
 Sample : N5928-09 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.590	1724	1726	1727	rBV2	168	79	0.01%	0.001%
38	6.622	1731	1736	1737	rBV2	956	777	0.05%	0.006%
39	6.728	1767	1769	1774	rVB	279	238	0.02%	0.002%
40	6.754	1774	1777	1779	rBV	437	257	0.02%	0.002%
41	6.770	1780	1782	1785	rVB2	423	247	0.02%	0.002%
42	6.789	1785	1788	1791	rBV2	108	101	0.01%	0.001%
43	6.821	1795	1798	1800	rBV2	235	145	0.01%	0.001%
44	6.838	1800	1803	1805	rBV2	227	161	0.01%	0.001%
45	6.886	1816	1818	1821	rBV	411	221	0.01%	0.002%
46	6.979	1833	1847	1874	rBV	158369	290909	18.98%	2.291%
47	7.307	1935	1949	1984	rBV	730505	1287089	83.96%	10.134%
48	7.612	2034	2044	2065	rBV	109433	195207	12.73%	1.537%
49	8.082	2180	2190	2228	rBV	422568	767021	50.03%	6.039%
50	8.616	2354	2356	2358	rBV2	321	154	0.01%	0.001%
51	8.657	2367	2369	2376	rVB2	404	404	0.03%	0.003%
52	8.696	2377	2381	2383	rBV2	356	310	0.02%	0.002%
53	8.780	2405	2407	2410	rVB2	230	109	0.01%	0.001%
54	8.796	2410	2412	2414	rBV	247	140	0.01%	0.001%
55	8.844	2415	2427	2457	rBV	868367	1411530	92.07%	11.114%
56	9.143	2517	2520	2522	rVB2	276	130	0.01%	0.001%
57	9.156	2522	2524	2529	rVB3	411	226	0.01%	0.002%
58	9.185	2530	2533	2534	rBV2	199	119	0.01%	0.001%
59	9.217	2541	2543	2546	rBV2	351	194	0.01%	0.002%
60	9.233	2546	2548	2551	rVV2	293	213	0.01%	0.002%
61	9.262	2555	2557	2560	rVB	284	93	0.01%	0.001%
62	9.281	2561	2563	2565	rBV	144	46	0.00%	0.000%
63	9.400	2598	2600	2601	rBV	170	72	0.00%	0.001%
64	9.616	2659	2667	2670	rBV2	275	364	0.02%	0.003%
65	9.638	2670	2674	2676	rBV2	249	183	0.01%	0.001%
66	9.709	2693	2696	2700	rBV	257	212	0.01%	0.002%
67	9.744	2704	2707	2710	rBV2	337	241	0.02%	0.002%
68	9.889	2748	2752	2755	rBV2	276	161	0.01%	0.001%
69	9.905	2755	2757	2759	rBV	169	84	0.01%	0.001%
70	10.063	2804	2806	2808	rBV	172	96	0.01%	0.001%
71	10.162	2828	2837	2841	rBV	21425	31457	2.05%	0.248%
72	10.207	2842	2851	2878	rVB	492192	780013	50.88%	6.142%
73	10.371	2896	2902	2904	rBV3	369	330	0.02%	0.003%
74	10.416	2913	2916	2917	rBV	195	92	0.01%	0.001%
75	10.448	2924	2926	2928	rVB	355	109	0.01%	0.001%
76	10.477	2929	2935	2940	rBV3	372	525	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029576.D
 Acq On : 10 Dec 2022 13:17
 Operator : SY/MD
 Sample : N5928-09 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.513	2943	2946	2949	rBV2	206	159	0.01%	0.001%
78	10.567	2954	2963	2973	rBV2	10355	16325	1.06%	0.129%
79	10.789	3030	3032	3034	rVB	211	88	0.01%	0.001%
80	10.805	3034	3037	3039	rBV	232	138	0.01%	0.001%
81	10.847	3046	3050	3054	rVB3	695	542	0.04%	0.004%
82	10.866	3054	3056	3059	rBV2	211	114	0.01%	0.001%
83	10.985	3090	3093	3094	rBV	265	127	0.01%	0.001%
84	11.030	3103	3107	3108	rBV	146	89	0.01%	0.001%
85	11.107	3129	3131	3132	rBV	216	86	0.01%	0.001%
86	11.159	3144	3147	3152	rVB2	325	232	0.02%	0.002%
87	11.236	3159	3171	3196	rBV	917755	1414727	92.28%	11.139%
88	11.413	3225	3226	3228	rBV2	349	149	0.01%	0.001%
89	11.509	3253	3256	3258	rBV2	269	159	0.01%	0.001%
90	11.525	3258	3261	3265	rVV2	286	201	0.01%	0.002%
91	11.612	3276	3288	3312	rBV	737479	1159006	75.60%	9.126%
92	11.911	3377	3381	3383	rBV2	661	571	0.04%	0.004%
93	12.197	3467	3470	3474	rBV2	353	328	0.02%	0.003%
94	12.625	3597	3603	3605	rBV2	453	450	0.03%	0.004%




Sum of corrected areas: 12700556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029576.D
Acq On : 10 Dec 2022 13:17
Operator : SY/MD
Sample : N5928-09 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

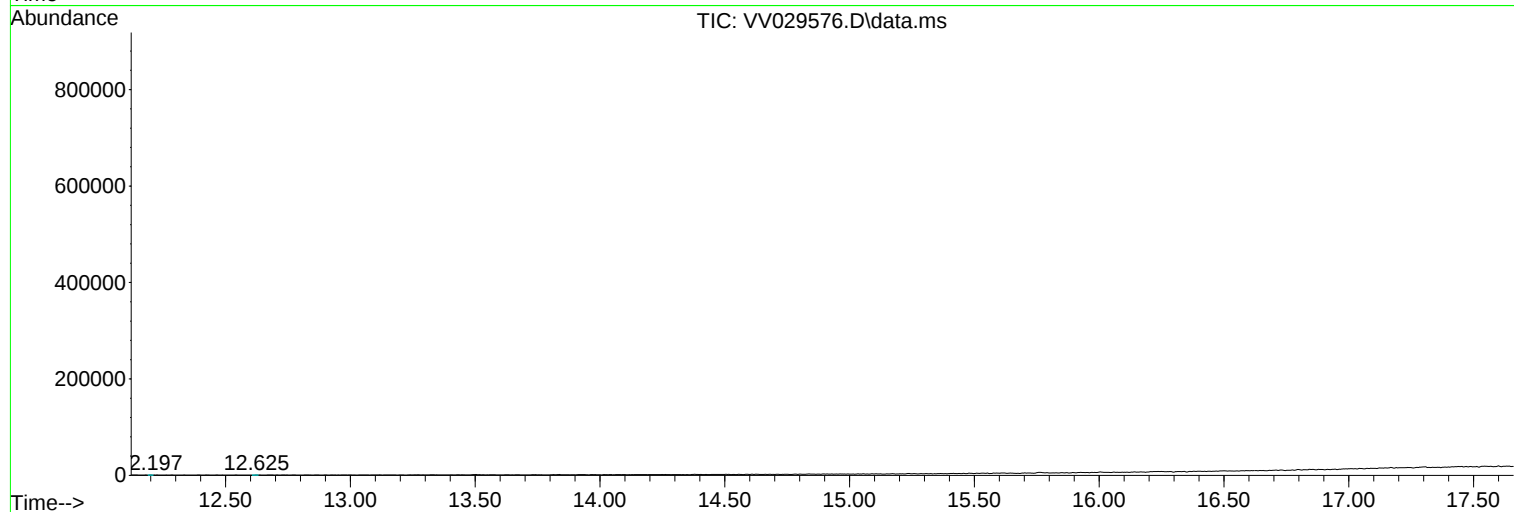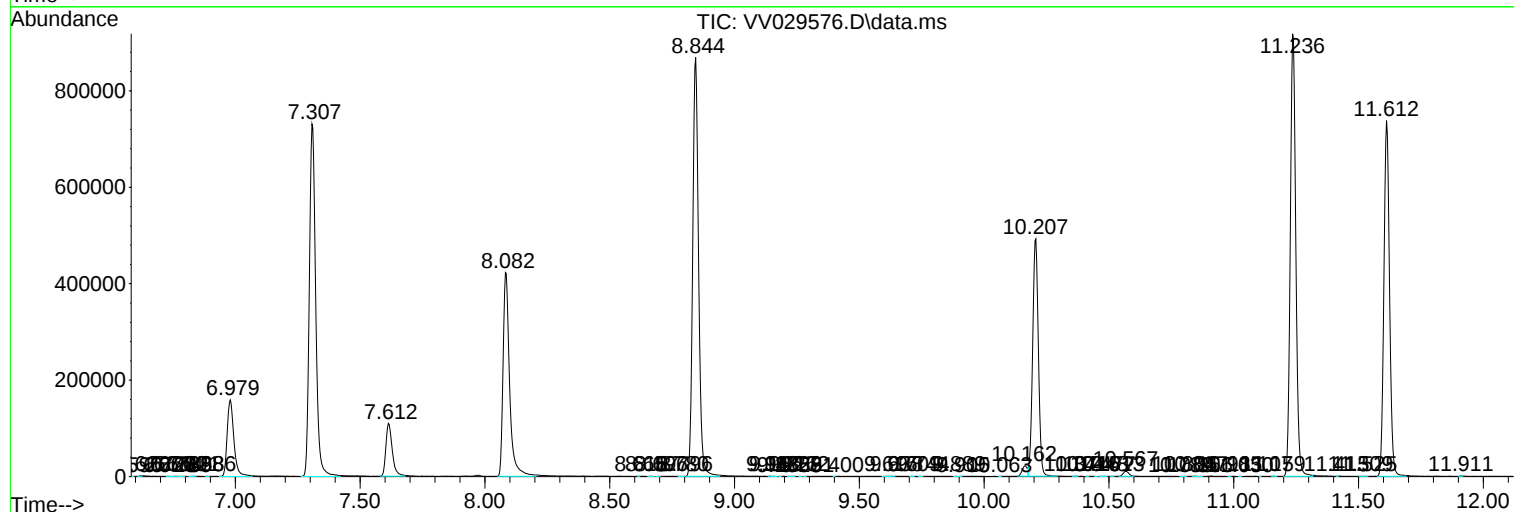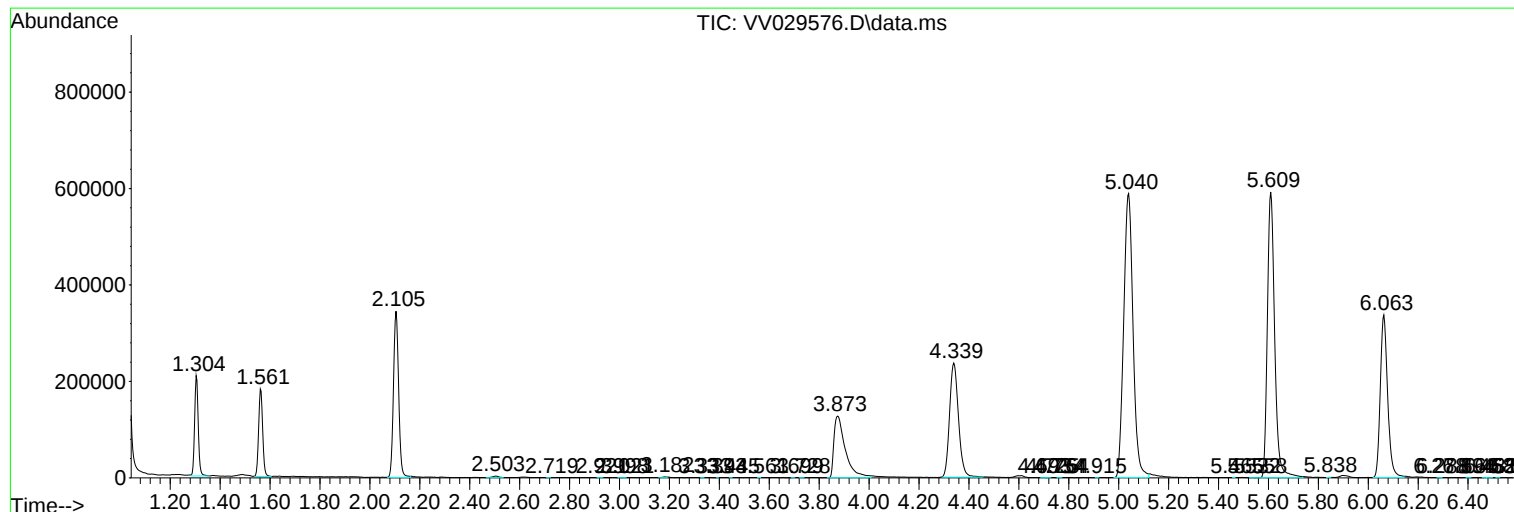

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029576.D
Acq On : 10 Dec 2022 13:17
Operator : SY/MD
Sample : N5928-09 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029576.D
Acq On : 10 Dec 2022 13:17
Operator : SY/MD
Sample : N5928-09 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------