

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029578.D
 Acq On : 10 Dec 2022 14:04
 Operator : SY/MD
 Sample : N5928-13 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	194633	197036	13.45%	1.594%
2	1.561	155	162	179	rVB	172188	195010	13.31%	1.577%
3	2.105	320	331	364	rBV	324370	471693	32.19%	3.815%
4	2.503	447	455	467	rVB4	3336	5303	0.36%	0.043%
5	2.558	468	472	475	rBV2	230	173	0.01%	0.001%
6	2.580	475	479	482	rBV2	408	342	0.02%	0.003%
7	2.696	512	515	518	rVB	318	200	0.01%	0.002%
8	2.789	540	544	547	rBV2	237	170	0.01%	0.001%
9	2.809	548	550	553	rVV2	262	143	0.01%	0.001%
10	2.854	561	564	565	rBV	269	128	0.01%	0.001%
11	3.185	655	667	683	rBV	19671	39993	2.73%	0.323%
12	3.400	731	734	738	rBV2	359	295	0.02%	0.002%
13	3.449	746	749	752	rVB	178	116	0.01%	0.001%
14	3.474	752	757	762	rBV2	201	196	0.01%	0.002%
15	3.503	762	766	768	rBV	178	130	0.01%	0.001%
16	3.568	783	786	789	rVV2	152	106	0.01%	0.001%
17	3.651	808	812	814	rBV	187	120	0.01%	0.001%
18	3.670	814	818	819	rVV	195	92	0.01%	0.001%
19	3.680	819	821	826	rVB2	216	163	0.01%	0.001%
20	3.876	868	882	933	rBV3	124344	474926	32.42%	3.841%
21	4.339	1010	1026	1054	rBV	229728	566112	38.64%	4.579%
22	4.603	1095	1108	1126	rVB2	30186	73761	5.03%	0.597%
23	4.703	1137	1139	1142	rVB2	317	135	0.01%	0.001%
24	4.732	1142	1148	1155	rBV3	420	526	0.04%	0.004%
25	4.777	1160	1162	1163	rVB2	321	93	0.01%	0.001%
26	4.793	1163	1167	1171	rBV	177	148	0.01%	0.001%
27	4.838	1178	1181	1182	rBV	149	88	0.01%	0.001%
28	4.873	1189	1192	1196	rVB	213	151	0.01%	0.001%
29	4.915	1202	1205	1208	rVB	226	137	0.01%	0.001%
30	4.931	1208	1210	1216	rBV2	239	219	0.01%	0.002%
31	4.963	1216	1220	1224	rBV	244	216	0.01%	0.002%
32	5.040	1226	1244	1271	rBV2	559023	1465134	100.00%	11.850%
33	5.375	1345	1348	1351	rBV	280	200	0.01%	0.002%
34	5.452	1369	1372	1374	rBV2	166	111	0.01%	0.001%
35	5.506	1386	1389	1391	rBV3	291	194	0.01%	0.002%
36	5.542	1396	1400	1402	rBV	400	219	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029578.D
 Acq On : 10 Dec 2022 14:04
 Operator : SY/MD
 Sample : N5928-13 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1408	1421	1453	rBV	569443	1163389	79.40%	9.409%
38	5.902	1503	1512	1526	rVB8	4413	9479	0.65%	0.077%
39	6.063	1548	1562	1597	rBV	316974	657649	44.89%	5.319%
40	6.307	1635	1638	1641	rBV2	203	126	0.01%	0.001%
41	6.346	1648	1650	1653	rBV2	213	116	0.01%	0.001%
42	6.429	1672	1676	1677	rBV	208	129	0.01%	0.001%
43	6.500	1695	1698	1699	rBV2	224	114	0.01%	0.001%
44	6.558	1712	1716	1718	rBV2	296	194	0.01%	0.002%
45	6.606	1727	1731	1733	rBV2	463	318	0.02%	0.003%
46	6.696	1756	1759	1763	rVV2	281	163	0.01%	0.001%
47	6.715	1763	1765	1768	rVB2	489	218	0.01%	0.002%
48	6.741	1768	1773	1774	rBV	231	178	0.01%	0.001%
49	6.825	1796	1799	1800	rBV	192	100	0.01%	0.001%
50	6.834	1800	1802	1808	rVB	246	246	0.02%	0.002%
51	6.889	1817	1819	1822	rVB	189	93	0.01%	0.001%
52	6.905	1822	1824	1827	rBV	231	94	0.01%	0.001%
53	6.979	1835	1847	1875	rBV	149932	274305	18.72%	2.219%
54	7.307	1936	1949	1988	rBV	678040	1213624	82.83%	9.816%
55	7.616	2034	2045	2066	rBV	104186	184140	12.57%	1.489%
56	7.837	2111	2114	2116	rBV2	338	208	0.01%	0.002%
57	7.911	2135	2137	2140	rBV2	396	211	0.01%	0.002%
58	7.966	2149	2154	2163	rVB4	2409	3646	0.25%	0.029%
59	8.085	2180	2191	2231	rBV	403117	737896	50.36%	5.968%
60	8.603	2347	2352	2356	rBV4	394	439	0.03%	0.004%
61	8.802	2412	2414	2415	rBV2	302	124	0.01%	0.001%
62	8.844	2415	2427	2457	rVV	833576	1376469	93.95%	11.133%
63	9.111	2508	2510	2513	rBV2	364	223	0.02%	0.002%
64	9.162	2523	2526	2529	rVB	342	184	0.01%	0.001%
65	9.230	2544	2547	2550	rBV	379	222	0.02%	0.002%
66	9.246	2550	2552	2559	rVV3	277	195	0.01%	0.002%
67	9.291	2562	2566	2570	rBV3	263	260	0.02%	0.002%
68	9.336	2576	2580	2581	rBV	155	105	0.01%	0.001%
69	9.407	2598	2602	2607	rVB3	304	387	0.03%	0.003%
70	9.435	2607	2611	2615	rBV	251	291	0.02%	0.002%
71	9.580	2649	2656	2660	rVB3	432	405	0.03%	0.003%
72	9.606	2661	2664	2667	rBV2	198	165	0.01%	0.001%
73	9.670	2682	2684	2690	rVB3	342	188	0.01%	0.002%
74	9.792	2718	2722	2724	rBV2	246	183	0.01%	0.001%
75	9.825	2729	2732	2734	rVV	173	92	0.01%	0.001%
76	9.911	2758	2759	2761	rBV	281	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029578.D
 Acq On : 10 Dec 2022 14:04
 Operator : SY/MD
 Sample : N5928-13 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.944	2766	2769	2775	rBV2	229	150	0.01%	0.001%
78	9.976	2777	2779	2782	rVV2	209	110	0.01%	0.001%
79	10.059	2803	2805	2809	rVV2	239	125	0.01%	0.001%
80	10.079	2809	2811	2815	rVV3	167	110	0.01%	0.001%
81	10.165	2825	2838	2841	rBV	21462	30670	2.09%	0.248%
82	10.207	2842	2851	2874	rVB	472015	747532	51.02%	6.046%
83	10.345	2890	2894	2898	rBV3	219	177	0.01%	0.001%
84	10.403	2909	2912	2914	rBV2	359	230	0.02%	0.002%
85	10.535	2950	2953	2954	rBV2	316	154	0.01%	0.001%
86	10.567	2955	2963	2977	rVB	9794	15743	1.07%	0.127%
87	10.725	3010	3012	3015	rBV3	302	241	0.02%	0.002%
88	10.776	3022	3028	3031	rBV3	204	240	0.02%	0.002%
89	10.844	3046	3049	3057	rVB4	645	562	0.04%	0.005%
90	10.882	3057	3061	3062	rBV	335	183	0.01%	0.001%
91	10.908	3063	3069	3075	rVB3	861	1173	0.08%	0.009%
92	11.124	3132	3136	3139	rVB	344	276	0.02%	0.002%
93	11.149	3142	3144	3145	rBV	291	93	0.01%	0.001%
94	11.236	3159	3171	3195	rBV	879637	1357928	92.68%	10.983%
95	11.612	3275	3288	3311	rBV	701011	1085840	74.11%	8.782%
96	11.834	3354	3357	3358	rBV	292	164	0.01%	0.001%
97	11.911	3376	3381	3390	rBV3	1299	1607	0.11%	0.013%
98	12.120	3443	3446	3447	rBV	314	157	0.01%	0.001%
99	12.300	3499	3502	3508	rBV2	308	222	0.02%	0.002%
100	12.561	3581	3583	3587	rBV2	298	183	0.01%	0.001%




Sum of corrected areas: 12364359

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029578.D
Acq On : 10 Dec 2022 14:04
Operator : SY/MD
Sample : N5928-13 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

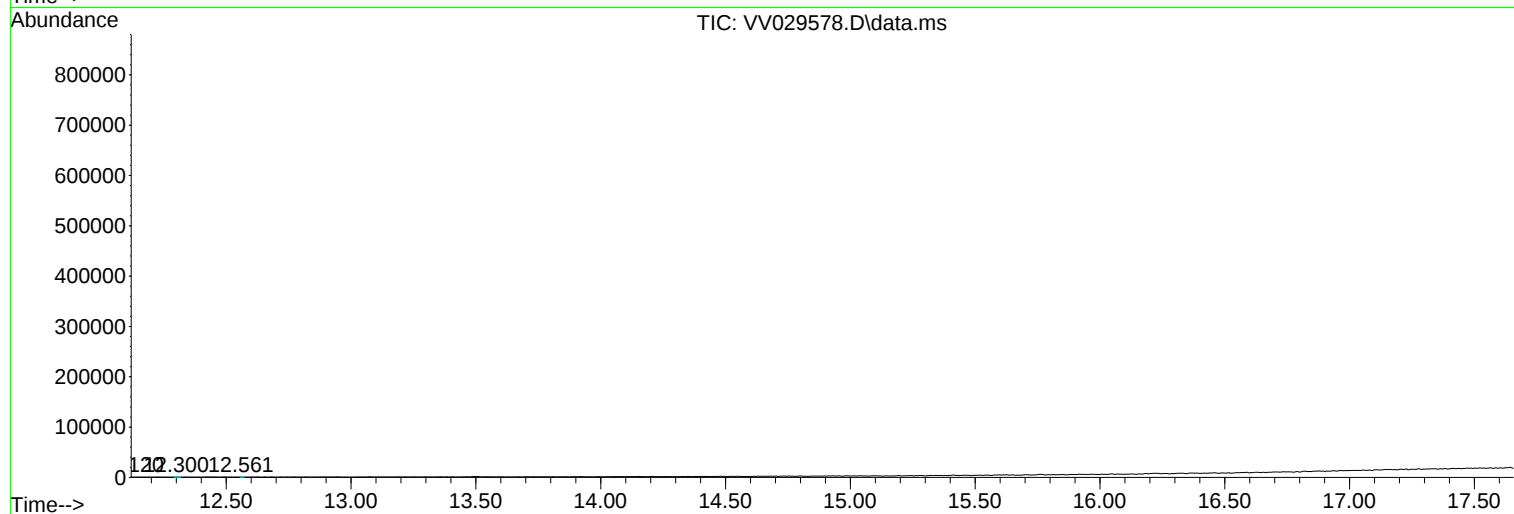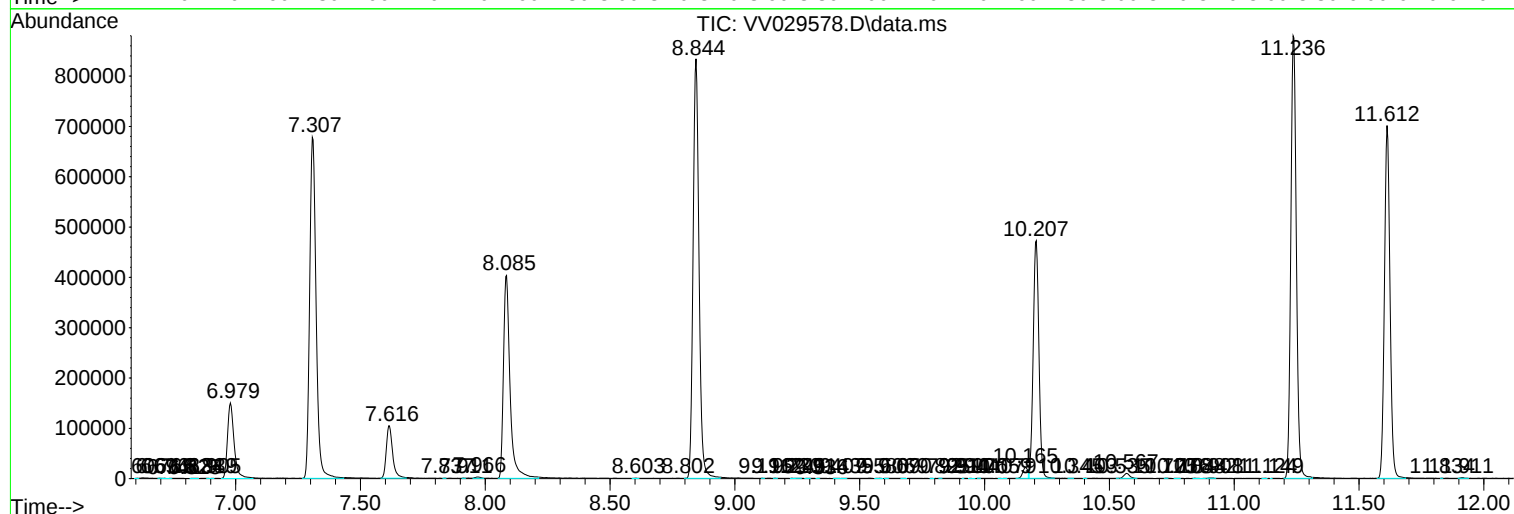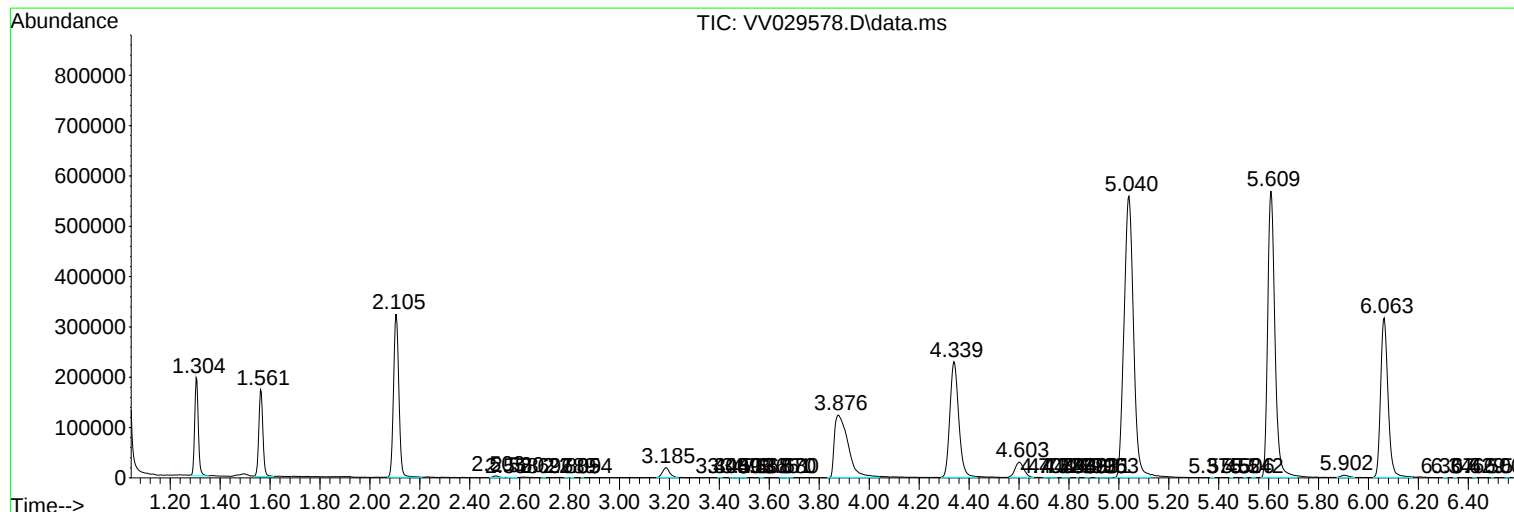

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029578.D
Acq On : 10 Dec 2022 14:04
Operator : SY/MD
Sample : N5928-13 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029578.D
Acq On : 10 Dec 2022 14:04
Operator : SY/MD
Sample : N5928-13 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc