

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029579.D
 Acq On : 10 Dec 2022 14:28
 Operator : SY/MD
 Sample : N5928-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	181211	182165	13.66%	1.561%
2	1.564	156	163	178	rVB	166035	188184	14.12%	1.613%
3	2.105	320	331	346	rBV	274286	395412	29.66%	3.388%
4	2.503	446	455	466	rVB2	5122	8298	0.62%	0.071%
5	2.545	466	468	469	rBV2	143	68	0.01%	0.001%
6	2.664	502	505	508	rBV	184	139	0.01%	0.001%
7	2.699	513	516	518	rBV3	193	122	0.01%	0.001%
8	2.761	527	535	545	rVB4	2445	4304	0.32%	0.037%
9	2.802	545	548	550	rBV2	255	187	0.01%	0.002%
10	3.185	653	667	688	rBV2	19782	42652	3.20%	0.366%
11	3.388	728	730	734	rVB	169	90	0.01%	0.001%
12	3.426	740	742	748	rVB	274	228	0.02%	0.002%
13	3.478	754	758	761	rBV	148	118	0.01%	0.001%
14	3.497	761	764	769	rVV	173	106	0.01%	0.001%
15	3.523	769	772	774	rBV	185	93	0.01%	0.001%
16	3.625	801	804	809	rVV	162	152	0.01%	0.001%
17	3.902	872	890	923	rBV2	313787	980507	73.55%	8.402%
18	4.339	1009	1026	1059	rBV	207569	523576	39.28%	4.487%
19	4.600	1092	1107	1139	rVB2	158668	400193	30.02%	3.429%
20	4.883	1192	1195	1198	rBV2	149	115	0.01%	0.001%
21	4.924	1203	1208	1210	rBV	219	150	0.01%	0.001%
22	4.953	1213	1217	1223	rVB	176	179	0.01%	0.002%
23	5.040	1223	1244	1281	rBV2	500777	1333094	100.00%	11.424%
24	5.397	1352	1355	1357	rBV	272	130	0.01%	0.001%
25	5.461	1373	1375	1378	rBV2	175	106	0.01%	0.001%
26	5.478	1378	1380	1383	rVB2	259	126	0.01%	0.001%
27	5.523	1391	1394	1398	rBV3	198	159	0.01%	0.001%
28	5.551	1402	1403	1404	rBV3	186	71	0.01%	0.001%
29	5.609	1408	1421	1449	rBV	491185	997012	74.79%	8.544%
30	5.899	1502	1511	1513	rBV6	3723	4829	0.36%	0.041%
31	6.002	1541	1543	1544	rBV	184	71	0.01%	0.001%
32	6.063	1548	1562	1600	rBV	291417	605551	45.42%	5.189%
33	6.246	1617	1619	1623	rVB2	607	337	0.03%	0.003%
34	6.278	1623	1629	1635	rBV4	345	360	0.03%	0.003%
35	6.381	1656	1661	1662	rBV	325	194	0.01%	0.002%
36	6.404	1665	1668	1672	rVB	144	104	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029579.D
 Acq On : 10 Dec 2022 14:28
 Operator : SY/MD
 Sample : N5928-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.542	1707	1711	1714	rBV2	212	160	0.01%	0.001%
38	6.577	1721	1722	1725	rVB	224	83	0.01%	0.001%
39	6.632	1728	1739	1746	rBV5	1345	2485	0.19%	0.021%
40	6.735	1768	1771	1773	rBV	288	169	0.01%	0.001%
41	6.764	1777	1780	1783	rVV3	221	138	0.01%	0.001%
42	6.783	1783	1786	1789	rVV2	305	195	0.01%	0.002%
43	6.857	1806	1809	1813	rBV2	207	179	0.01%	0.002%
44	6.892	1816	1820	1822	rVB2	168	98	0.01%	0.001%
45	6.915	1822	1827	1828	rBV2	314	237	0.02%	0.002%
46	6.979	1835	1847	1872	rBV	134303	248624	18.65%	2.131%
47	7.243	1920	1929	1932	rBV3	611	627	0.05%	0.005%
48	7.307	1937	1949	1970	rBV	552286	983369	73.77%	8.427%
49	7.612	2035	2044	2068	rBV	96593	169367	12.70%	1.451%
50	7.844	2114	2116	2118	rBV2	358	206	0.02%	0.002%
51	8.085	2180	2191	2229	rBV	390667	715160	53.65%	6.128%
52	8.455	2303	2306	2311	rBV4	419	384	0.03%	0.003%
53	8.555	2334	2337	2339	rVB	445	260	0.02%	0.002%
54	8.654	2365	2368	2371	rBV2	436	279	0.02%	0.002%
55	8.722	2384	2389	2390	rBV2	361	281	0.02%	0.002%
56	8.731	2390	2392	2396	rVB2	448	227	0.02%	0.002%
57	8.747	2396	2397	2403	rVB2	243	189	0.01%	0.002%
58	8.776	2403	2406	2409	rBV2	348	197	0.01%	0.002%
59	8.844	2412	2427	2468	rBV	689777	1127318	84.56%	9.660%
60	9.091	2502	2504	2505	rBV	316	117	0.01%	0.001%
61	9.104	2505	2508	2509	rVV2	422	241	0.02%	0.002%
62	9.133	2510	2517	2530	rVB3	3543	5611	0.42%	0.048%
63	9.182	2530	2532	2536	rBV3	225	175	0.01%	0.001%
64	9.201	2537	2538	2541	rVB	312	131	0.01%	0.001%
65	9.217	2541	2543	2545	rBV	179	104	0.01%	0.001%
66	9.249	2552	2553	2557	rBV2	160	61	0.00%	0.001%
67	9.407	2599	2602	2605	rBV	293	167	0.01%	0.001%
68	9.442	2610	2613	2614	rBV	243	146	0.01%	0.001%
69	9.474	2619	2623	2625	rBV2	245	151	0.01%	0.001%
70	9.538	2635	2643	2653	rBV2	3853	6146	0.46%	0.053%
71	9.603	2659	2663	2666	rVB2	314	218	0.02%	0.002%
72	9.622	2666	2669	2673	rBV2	133	116	0.01%	0.001%
73	9.664	2680	2682	2683	rBV2	260	93	0.01%	0.001%
74	9.747	2705	2708	2709	rBV2	170	97	0.01%	0.001%
75	9.780	2717	2718	2723	rBV2	154	101	0.01%	0.001%
76	9.818	2726	2730	2731	rBV	236	137	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029579.D
 Acq On : 10 Dec 2022 14:28
 Operator : SY/MD
 Sample : N5928-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.895	2749	2754	2758	rBV3	355	382	0.03%	0.003%
78	10.040	2797	2799	2800	rBV3	190	62	0.00%	0.001%
79	10.162	2828	2837	2841	rBV2	18394	26733	2.01%	0.229%
80	10.207	2842	2851	2871	rVB	446981	704966	52.88%	6.041%
81	10.442	2915	2924	2929	rBV5	2793	4770	0.36%	0.041%
82	10.532	2944	2952	2956	rBV5	2673	3875	0.29%	0.033%
83	10.728	3006	3013	3024	rVB4	2978	4195	0.31%	0.036%
84	10.773	3025	3027	3029	rBV2	283	127	0.01%	0.001%
85	10.815	3038	3040	3043	rVB2	224	111	0.01%	0.001%
86	10.831	3043	3045	3047	rBV	160	99	0.01%	0.001%
87	10.844	3047	3049	3053	rVB	255	161	0.01%	0.001%
88	10.866	3053	3056	3059	rBV2	238	176	0.01%	0.002%
89	10.905	3061	3068	3077	rVV3	7079	9623	0.72%	0.082%
90	11.017	3101	3103	3108	rBV2	306	204	0.02%	0.002%
91	11.046	3110	3112	3114	rBV	167	92	0.01%	0.001%
92	11.149	3142	3144	3148	rVB2	347	242	0.02%	0.002%
93	11.236	3160	3171	3192	rBV	694319	1073175	80.50%	9.196%
94	11.522	3253	3260	3266	rBV4	1515	2043	0.15%	0.018%
95	11.612	3277	3288	3312	rBV	578094	903080	67.74%	7.739%
96	11.773	3336	3338	3340	rBV	312	201	0.02%	0.002%
97	12.149	3453	3455	3459	rVB2	427	185	0.01%	0.002%
98	12.207	3471	3473	3475	rBV	320	217	0.02%	0.002%
99	12.349	3515	3517	3520	rBV2	326	207	0.02%	0.002%
100	12.455	3544	3550	3557	rBV3	928	1284	0.10%	0.011%




Sum of corrected areas: 11669436

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029579.D
Acq On : 10 Dec 2022 14:28
Operator : SY/MD
Sample : N5928-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

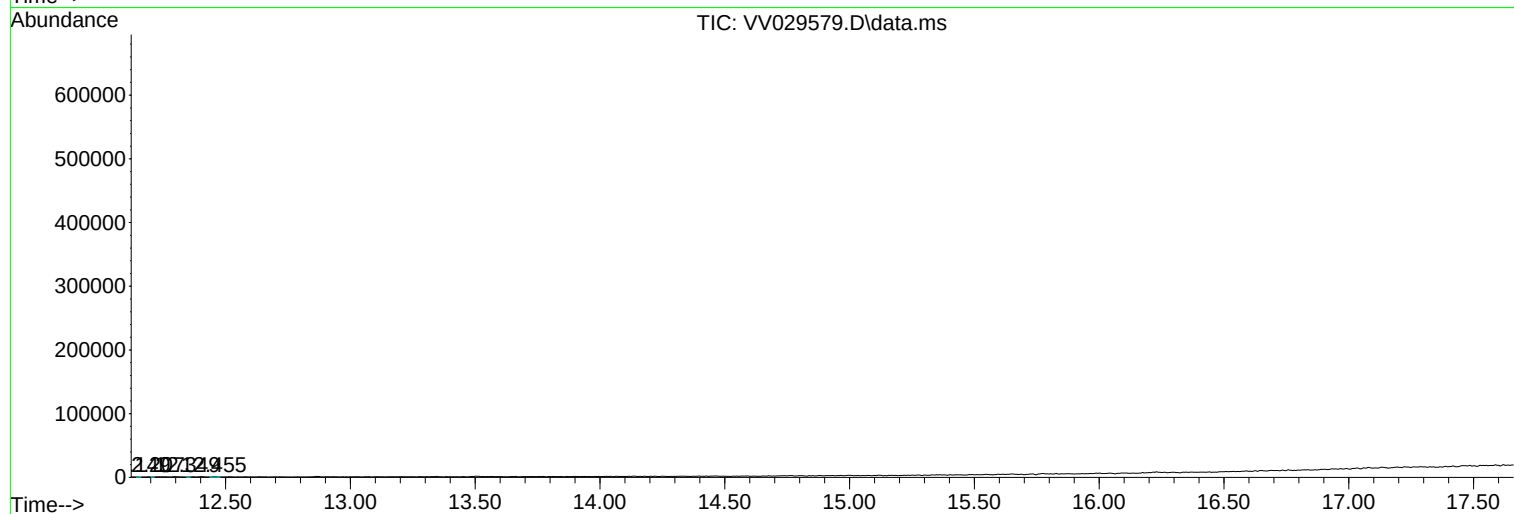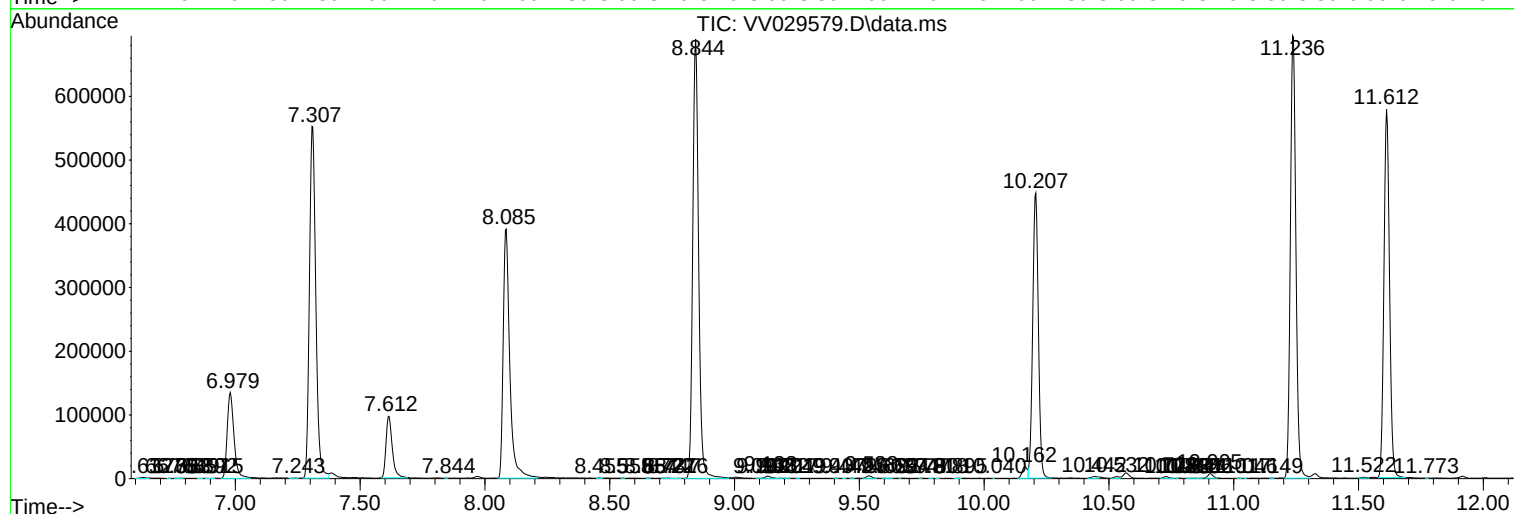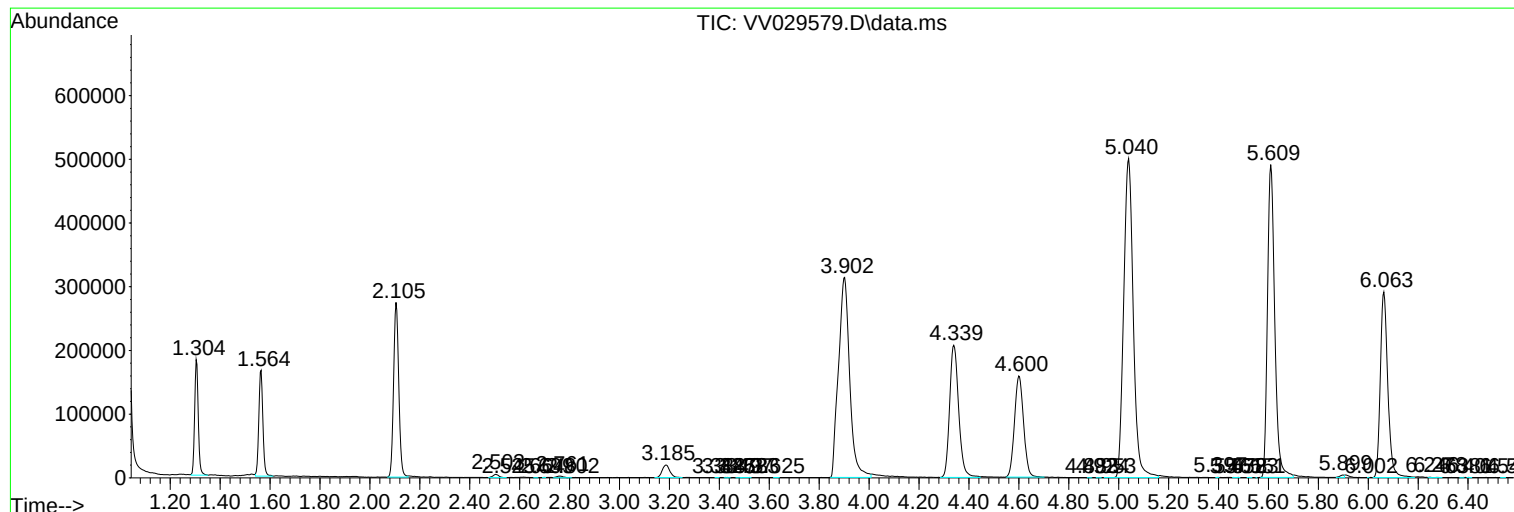

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029579.D
Acq On : 10 Dec 2022 14:28
Operator : SY/MD
Sample : N5928-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029579.D
Acq On : 10 Dec 2022 14:28
Operator : SY/MD
Sample : N5928-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc