

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029580.D
 Acq On : 10 Dec 2022 14:51
 Operator : SY/MD
 Sample : N5928-15 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	191322	194182	13.16%	1.589%
2	1.564	156	163	177	rVB	170019	191401	12.97%	1.566%
3	2.105	320	331	347	rBV	323108	467760	31.71%	3.827%
4	2.282	384	386	387	rBV	723	315	0.02%	0.003%
5	2.468	442	444	446	rBV2	312	201	0.01%	0.002%
6	2.507	448	456	465	rVB3	3283	5114	0.35%	0.042%
7	2.773	537	539	541	rVB	192	93	0.01%	0.001%
8	2.806	546	549	550	rBV	246	111	0.01%	0.001%
9	2.880	567	572	574	rBV	322	216	0.01%	0.002%
10	3.082	634	635	636	rBB	212	41	0.00%	0.000%
11	3.140	652	653	654	rBV	121	33	0.00%	0.000%
12	3.179	659	665	666	rBV2	884	742	0.05%	0.006%
13	3.233	680	682	684	rBV	104	63	0.00%	0.001%
14	3.281	694	697	698	rBV	155	91	0.01%	0.001%
15	3.542	777	778	780	rVB	112	40	0.00%	0.000%
16	3.600	791	796	798	rBV	124	126	0.01%	0.001%
17	3.835	865	869	871	rBV	318	245	0.02%	0.002%
18	3.873	871	881	921	rBV2	122883	379993	25.76%	3.109%
19	4.339	1011	1026	1065	rBV2	226846	562101	38.10%	4.599%
20	4.600	1094	1107	1127	rVB5	10748	27220	1.85%	0.223%
21	4.812	1171	1173	1174	rBV5	103	49	0.00%	0.000%
22	4.860	1185	1188	1193	rBV2	158	141	0.01%	0.001%
23	4.912	1202	1204	1207	rVB2	233	103	0.01%	0.001%
24	4.947	1213	1215	1217	rBV	112	67	0.00%	0.001%
25	4.960	1217	1219	1220	rBV	128	34	0.00%	0.000%
26	4.973	1221	1223	1225	rVB2	202	84	0.01%	0.001%
27	5.040	1226	1244	1281	rBV2	561596	1475153	100.00%	12.069%
28	5.458	1368	1374	1377	rBV3	338	367	0.02%	0.003%
29	5.523	1387	1394	1399	rBV3	260	371	0.03%	0.003%
30	5.609	1408	1421	1453	rBV	571025	1161145	78.71%	9.500%
31	6.063	1548	1562	1588	rBV	319331	654775	44.39%	5.357%
32	6.278	1627	1629	1634	rBV2	197	163	0.01%	0.001%
33	6.317	1640	1641	1644	rBV	230	83	0.01%	0.001%
34	6.333	1644	1646	1649	rBV	291	154	0.01%	0.001%
35	6.355	1651	1653	1659	rVB2	402	331	0.02%	0.003%
36	6.387	1659	1663	1666	rBV2	290	243	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029580.D
 Acq On : 10 Dec 2022 14:51
 Operator : SY/MD
 Sample : N5928-15 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.542	1708	1711	1717	rBV2	362	280	0.02%	0.002%
38	6.567	1717	1719	1721	rVB	247	84	0.01%	0.001%
39	6.584	1721	1724	1726	rBV2	157	88	0.01%	0.001%
40	6.603	1726	1730	1732	rBV	172	129	0.01%	0.001%
41	6.635	1733	1740	1745	rBV4	1119	1684	0.11%	0.014%
42	6.709	1761	1763	1764	rBV4	294	115	0.01%	0.001%
43	6.760	1776	1779	1782	rBV2	178	114	0.01%	0.001%
44	6.780	1782	1785	1786	rBV2	216	112	0.01%	0.001%
45	6.818	1794	1797	1798	rBV	188	115	0.01%	0.001%
46	6.850	1804	1807	1808	rBV2	159	98	0.01%	0.001%
47	6.883	1814	1817	1822	rVB2	330	234	0.02%	0.002%
48	6.915	1823	1827	1830	rBV2	240	187	0.01%	0.002%
49	6.979	1836	1847	1881	rBV	146979	270501	18.34%	2.213%
50	7.114	1888	1889	1891	rBV	497	158	0.01%	0.001%
51	7.307	1937	1949	1991	rBV	689261	1218817	82.62%	9.972%
52	7.616	2034	2045	2074	rBV	104917	185256	12.56%	1.516%
53	7.847	2114	2117	2119	rBV2	347	236	0.02%	0.002%
54	8.085	2180	2191	2230	rBV	411859	751022	50.91%	6.144%
55	8.645	2364	2365	2367	rBV2	222	97	0.01%	0.001%
56	8.696	2379	2381	2383	rBV	221	141	0.01%	0.001%
57	8.744	2389	2396	2401	rBV4	525	668	0.05%	0.005%
58	8.796	2409	2412	2415	rBV	156	123	0.01%	0.001%
59	8.844	2415	2427	2463	rBV	843228	1371918	93.00%	11.224%
60	9.056	2490	2493	2494	rBV2	410	218	0.01%	0.002%
61	9.178	2529	2531	2535	rBV2	264	181	0.01%	0.001%
62	9.268	2554	2559	2563	rBV3	401	367	0.02%	0.003%
63	9.329	2574	2578	2582	rBV3	254	242	0.02%	0.002%
64	9.371	2588	2591	2595	rBV3	254	191	0.01%	0.002%
65	9.789	2718	2721	2723	rBV	208	99	0.01%	0.001%
66	9.818	2729	2730	2733	rVB	149	41	0.00%	0.000%
67	9.847	2737	2739	2743	rVB2	339	207	0.01%	0.002%
68	9.895	2751	2754	2755	rBV	153	62	0.00%	0.001%
69	9.908	2756	2758	2760	rVV2	247	111	0.01%	0.001%
70	9.940	2765	2768	2775	rVV3	298	235	0.02%	0.002%
71	10.053	2801	2803	2806	rBV	144	87	0.01%	0.001%
72	10.085	2810	2813	2814	rBV2	170	110	0.01%	0.001%
73	10.162	2827	2837	2841	rBV	20587	30095	2.04%	0.246%
74	10.207	2842	2851	2872	rVB	477216	750205	50.86%	6.138%
75	10.352	2893	2896	2898	rBV2	231	181	0.01%	0.001%
76	10.429	2918	2920	2921	rBV2	248	87	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029580.D
 Acq On : 10 Dec 2022 14:51
 Operator : SY/MD
 Sample : N5928-15 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.464	2928	2931	2933	rBV	287	178	0.01%	0.001%
78	10.503	2941	2943	2946	rVB3	331	112	0.01%	0.001%
79	10.567	2955	2963	2976	rVB2	9448	14674	0.99%	0.120%
80	10.844	3048	3049	3052	rBV2	189	93	0.01%	0.001%
81	10.902	3062	3067	3073	rBV3	420	535	0.04%	0.004%
82	11.091	3120	3126	3129	rBV3	283	375	0.03%	0.003%
83	11.136	3138	3140	3144	rBV3	216	141	0.01%	0.001%
84	11.239	3159	3172	3194	rBV	902954	1400552	94.94%	11.459%
85	11.551	3267	3269	3274	rVB2	435	260	0.02%	0.002%
86	11.612	3275	3288	3317	rBV	700357	1097166	74.38%	8.976%
87	11.934	3385	3388	3389	rBV2	237	141	0.01%	0.001%
88	12.107	3440	3442	3444	rBV2	185	128	0.01%	0.001%
89	12.233	3479	3481	3482	rBV2	295	129	0.01%	0.001%
90	12.616	3598	3600	3602	rVB	220	71	0.00%	0.001%

Sum of corrected areas: 12222802




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029580.D
Acq On : 10 Dec 2022 14:51
Operator : SY/MD
Sample : N5928-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 74 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

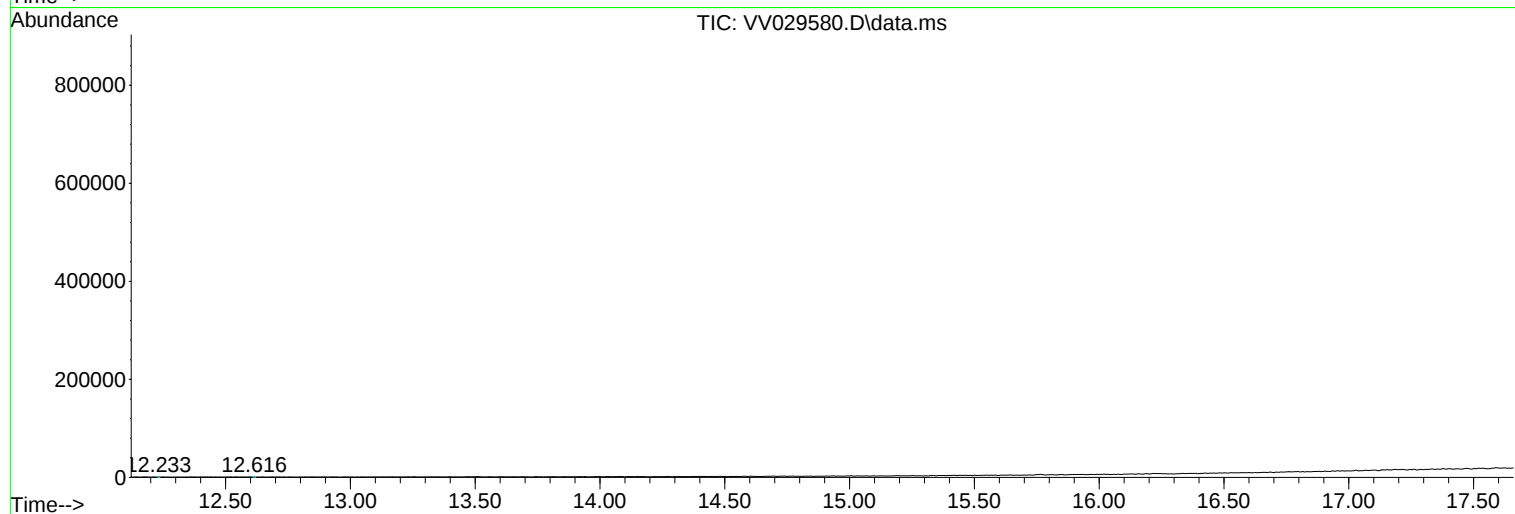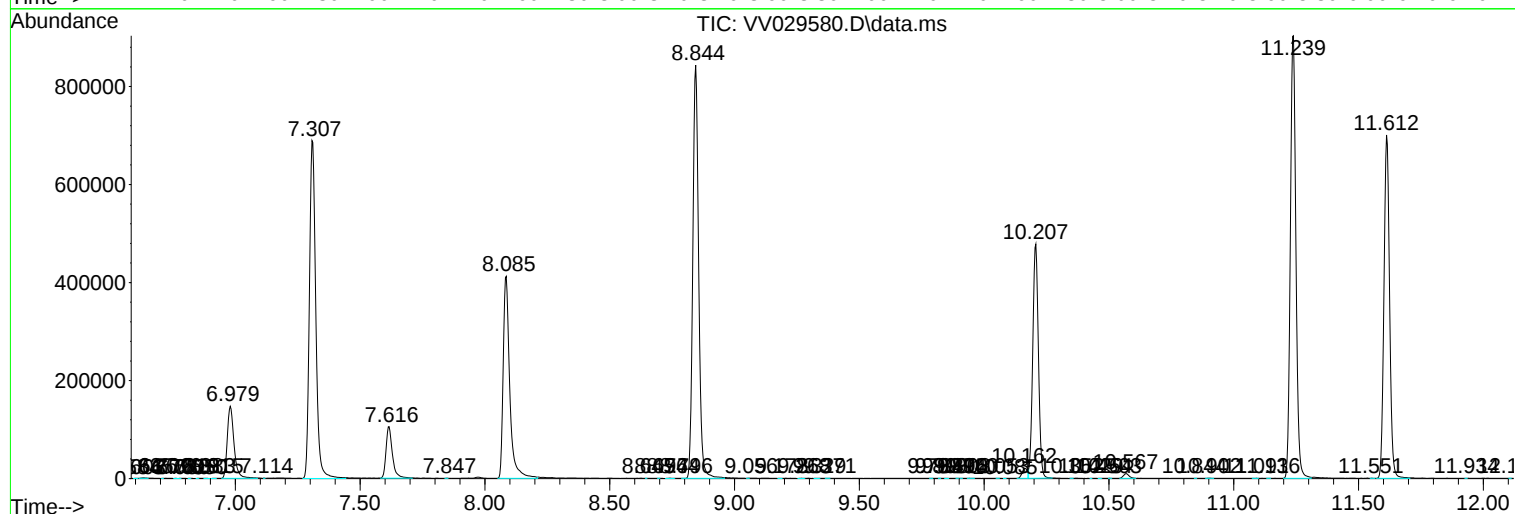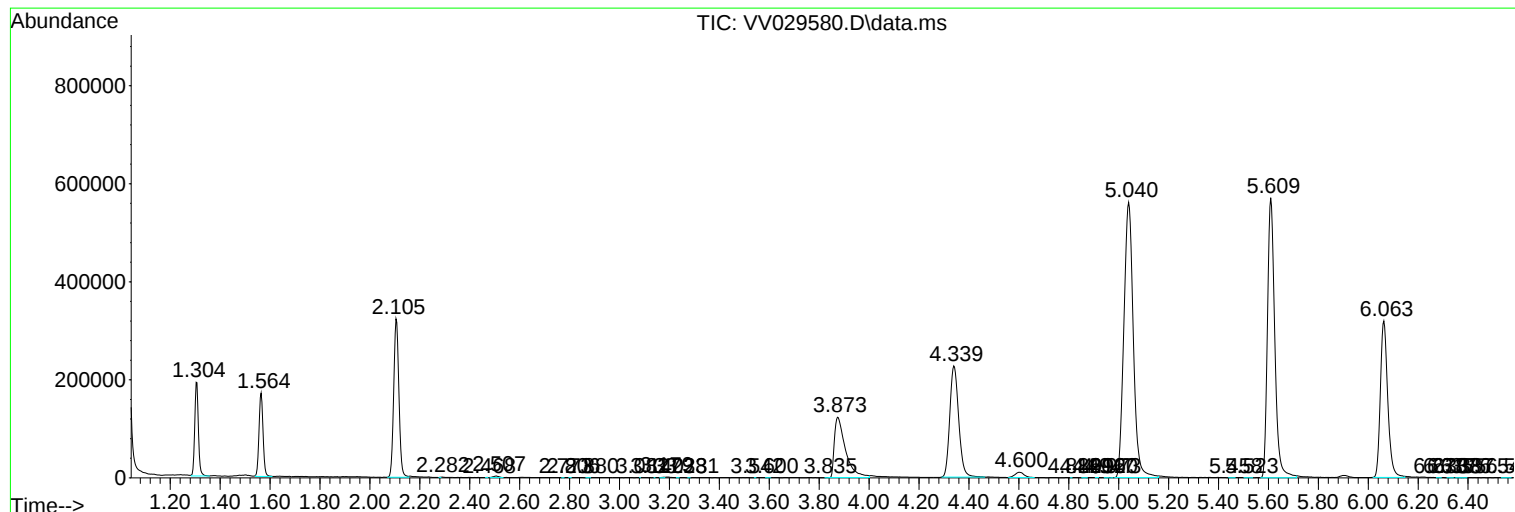

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029580.D
Acq On : 10 Dec 2022 14:51
Operator : SY/MD
Sample : N5928-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 74 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029580.D
Acq On : 10 Dec 2022 14:51
Operator : SY/MD
Sample : N5928-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 74 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------