

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029581.D
 Acq On : 10 Dec 2022 15:15
 Operator : SY/MD
 Sample : N5928-16 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	187535	190408	13.78%	1.633%
2	1.561	155	162	175	rVB	160881	181842	13.16%	1.560%
3	2.105	321	331	346	rBV	307900	441292	31.93%	3.785%
4	2.500	447	454	465	rVB3	3067	4489	0.32%	0.039%
5	2.584	477	480	481	rBV	255	145	0.01%	0.001%
6	2.600	482	485	486	rBV	575	336	0.02%	0.003%
7	2.686	506	512	515	rBV2	226	256	0.02%	0.002%
8	2.703	515	517	525	rVB2	251	251	0.02%	0.002%
9	2.767	534	537	540	rBV	174	129	0.01%	0.001%
10	2.818	550	553	557	rVB	174	126	0.01%	0.001%
11	2.847	557	562	564	rBV	179	159	0.01%	0.001%
12	2.876	569	571	577	rVB2	244	125	0.01%	0.001%
13	2.937	587	590	593	rBV2	212	158	0.01%	0.001%
14	2.973	598	601	606	rBV2	96	88	0.01%	0.001%
15	3.040	617	622	624	rBV2	206	173	0.01%	0.001%
16	3.178	660	665	666	rBV	669	491	0.04%	0.004%
17	3.223	677	679	681	rBV	262	119	0.01%	0.001%
18	3.288	695	699	700	rBV	203	133	0.01%	0.001%
19	3.436	743	745	751	rVB	201	148	0.01%	0.001%
20	3.465	751	754	757	rBV2	156	131	0.01%	0.001%
21	3.590	789	793	799	rVB	215	220	0.02%	0.002%
22	3.809	857	861	867	rVB	110	123	0.01%	0.001%
23	3.876	871	882	925	rBV3	113016	354629	25.66%	3.042%
24	4.339	1009	1026	1048	rBV	215606	529638	38.32%	4.543%
25	4.600	1096	1107	1123	rVB3	15847	37584	2.72%	0.322%
26	4.796	1165	1168	1170	rBV2	175	98	0.01%	0.001%
27	4.815	1170	1174	1175	rBV	197	89	0.01%	0.001%
28	4.866	1187	1190	1191	rBV	176	90	0.01%	0.001%
29	4.966	1218	1221	1223	rBV2	141	90	0.01%	0.001%
30	5.040	1226	1244	1283	rBV2	524885	1382076	100.00%	11.855%
31	5.391	1351	1353	1356	rBV	214	152	0.01%	0.001%
32	5.548	1399	1402	1405	rBV2	260	143	0.01%	0.001%
33	5.609	1408	1421	1450	rBV	544545	1109200	80.26%	9.514%
34	5.905	1503	1513	1529	rVB	6586	15492	1.12%	0.133%
35	6.063	1547	1562	1586	rBV	298437	614466	44.46%	5.271%
36	6.227	1612	1613	1617	rBV4	336	176	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029581.D
 Acq On : 10 Dec 2022 15:15
 Operator : SY/MD
 Sample : N5928-16 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.272	1625	1627	1631	rVB	325	184	0.01%	0.002%
38	6.294	1631	1634	1641	rVB3	257	221	0.02%	0.002%
39	6.323	1641	1643	1645	rBV	134	88	0.01%	0.001%
40	6.387	1658	1663	1669	rVB	224	200	0.01%	0.002%
41	6.442	1676	1680	1682	rBV2	301	248	0.02%	0.002%
42	6.471	1686	1689	1694	rVB3	229	163	0.01%	0.001%
43	6.529	1705	1707	1711	rBV3	183	114	0.01%	0.001%
44	6.554	1712	1715	1717	rBV	352	154	0.01%	0.001%
45	6.567	1717	1719	1723	rBV2	287	126	0.01%	0.001%
46	6.603	1726	1730	1731	rBV2	271	167	0.01%	0.001%
47	6.628	1732	1738	1743	rBV2	679	953	0.07%	0.008%
48	6.709	1761	1763	1768	rVB	201	121	0.01%	0.001%
49	6.763	1776	1780	1782	rVB3	269	183	0.01%	0.002%
50	6.892	1813	1820	1823	rBV	310	284	0.02%	0.002%
51	6.979	1836	1847	1878	rBV	138773	254631	18.42%	2.184%
52	7.226	1922	1924	1928	rVB	426	243	0.02%	0.002%
53	7.307	1937	1949	1983	rBV	638422	1140683	82.53%	9.784%
54	7.612	2034	2044	2069	rBV	99162	174931	12.66%	1.500%
55	7.969	2146	2155	2168	rVB3	14940	25231	1.83%	0.216%
56	8.085	2180	2191	2225	rBV	378911	697942	50.50%	5.987%
57	8.603	2350	2352	2355	rBV	241	169	0.01%	0.001%
58	8.648	2364	2366	2367	rBV	306	144	0.01%	0.001%
59	8.689	2375	2379	2380	rBV	251	172	0.01%	0.001%
60	8.731	2389	2392	2394	rBV	238	167	0.01%	0.001%
61	8.757	2397	2400	2403	rVV	379	253	0.02%	0.002%
62	8.770	2403	2404	2407	rVB2	201	106	0.01%	0.001%
63	8.844	2412	2427	2461	rBV	801273	1315525	95.18%	11.284%
64	9.140	2515	2519	2523	rBV3	357	361	0.03%	0.003%
65	9.230	2544	2547	2550	rBV3	319	231	0.02%	0.002%
66	9.329	2574	2578	2582	rVV2	265	268	0.02%	0.002%
67	9.435	2609	2611	2615	rVB2	247	129	0.01%	0.001%
68	9.542	2640	2644	2646	rBV2	269	183	0.01%	0.002%
69	9.574	2652	2654	2657	rBV2	220	157	0.01%	0.001%
70	9.615	2664	2667	2672	rVB2	243	182	0.01%	0.002%
71	9.705	2694	2695	2698	rVB2	240	92	0.01%	0.001%
72	9.805	2722	2726	2727	rBV2	200	126	0.01%	0.001%
73	9.860	2740	2743	2746	rBV	188	141	0.01%	0.001%
74	9.972	2777	2778	2782	rVB2	266	142	0.01%	0.001%
75	10.050	2799	2802	2806	rVB3	308	248	0.02%	0.002%
76	10.165	2827	2838	2841	rBV2	19079	27822	2.01%	0.239%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029581.D
 Acq On : 10 Dec 2022 15:15
 Operator : SY/MD
 Sample : N5928-16 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.207	2842	2851	2872	rVB	444919	702139	50.80%	6.023%
78	10.371	2898	2902	2905	rBV3	431	288	0.02%	0.002%
79	10.445	2924	2925	2929	rBV	159	88	0.01%	0.001%
80	10.493	2936	2940	2943	rBV2	208	152	0.01%	0.001%
81	10.567	2954	2963	2975	rBV	9374	15610	1.13%	0.134%
82	10.725	3009	3012	3014	rBV	190	87	0.01%	0.001%
83	10.792	3030	3033	3034	rBV2	210	122	0.01%	0.001%
84	10.892	3062	3064	3067	rBV2	139	89	0.01%	0.001%
85	10.908	3067	3069	3071	rVV	244	127	0.01%	0.001%
86	10.959	3082	3085	3091	rBV3	345	393	0.03%	0.003%
87	11.078	3118	3122	3125	rBV3	192	171	0.01%	0.001%
88	11.172	3149	3151	3153	rBV2	211	112	0.01%	0.001%
89	11.239	3159	3172	3202	rBV	869564	1355504	98.08%	11.627%
90	11.612	3276	3288	3310	rBV	681413	1072344	77.59%	9.198%
91	11.792	3342	3344	3350	rBV3	265	231	0.02%	0.002%
92	11.863	3363	3366	3370	rBV2	311	283	0.02%	0.002%
93	12.011	3408	3412	3414	rBV2	350	224	0.02%	0.002%
94	12.130	3447	3449	3455	rVB4	266	168	0.01%	0.001%
95	12.236	3479	3482	3483	rBV	391	185	0.01%	0.002%
96	12.365	3518	3522	3526	rBV3	361	371	0.03%	0.003%
97	12.541	3575	3577	3583	rBV2	319	203	0.01%	0.002%
98	12.651	3608	3611	3614	rBV3	391	269	0.02%	0.002%
99	12.863	3673	3677	3678	rBV2	377	261	0.02%	0.002%
100	13.053	3734	3736	3738	rBV2	474	188	0.01%	0.002%




Sum of corrected areas: 11658359

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029581.D
Acq On : 10 Dec 2022 15:15
Operator : SY/MD
Sample : N5928-16 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

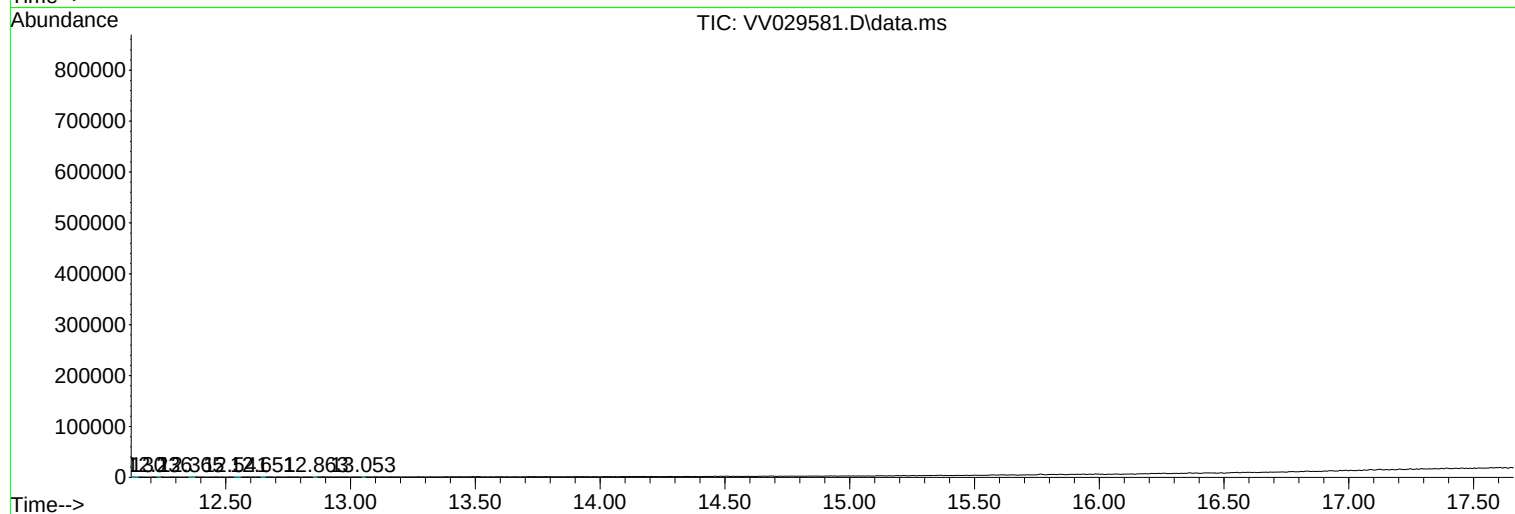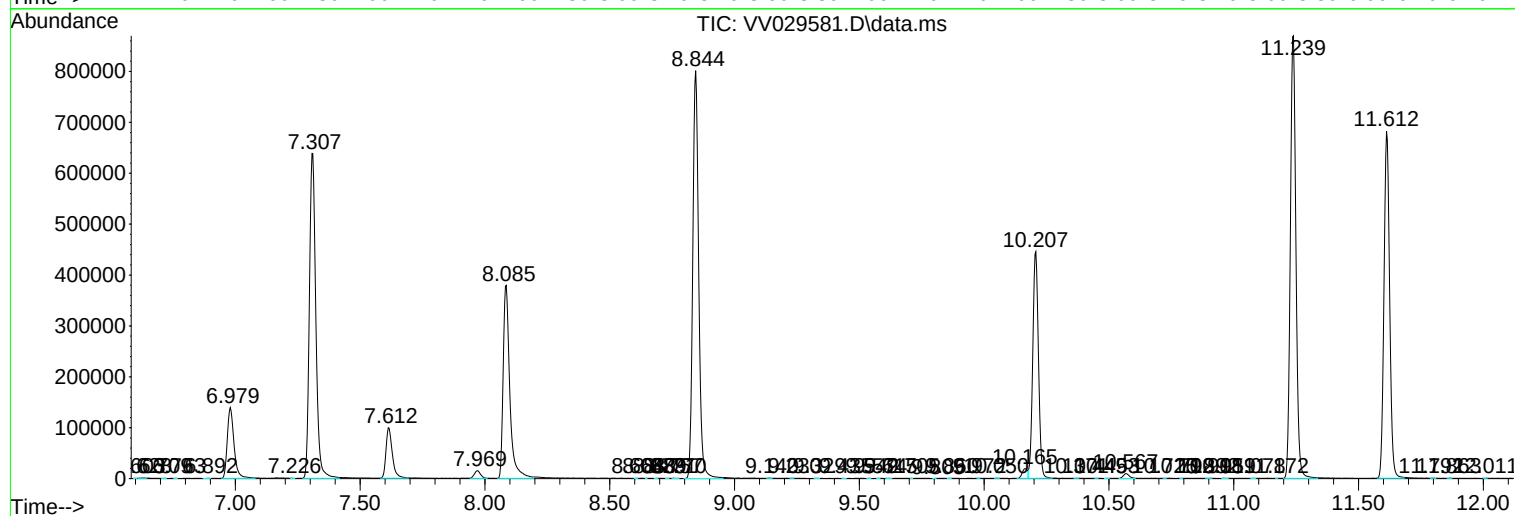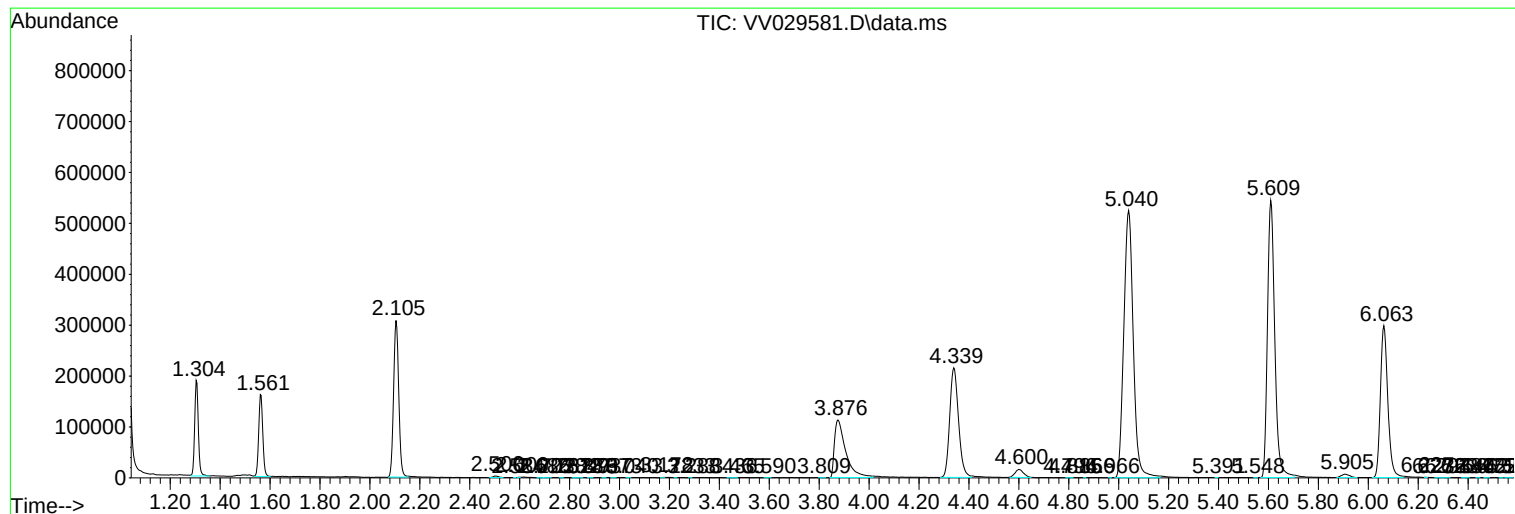

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029581.D
Acq On : 10 Dec 2022 15:15
Operator : SY/MD
Sample : N5928-16 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029581.D
Acq On : 10 Dec 2022 15:15
Operator : SY/MD
Sample : N5928-16 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------