

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029582.D
 Acq On : 10 Dec 2022 15:38
 Operator : SY/MD
 Sample : N5928-17 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	201878	200786	13.68%	1.617%
2	1.561	155	162	178	rVB2	169682	219081	14.93%	1.765%
3	2.104	320	331	347	rBV	325367	466144	31.76%	3.755%
4	2.500	447	454	465	rBV6	3058	5437	0.37%	0.044%
5	2.719	516	522	528	rBV2	163	202	0.01%	0.002%
6	2.754	528	533	546	rBV6	1016	1683	0.11%	0.014%
7	2.921	582	585	586	rBV	209	103	0.01%	0.001%
8	3.008	609	612	617	rBV	136	128	0.01%	0.001%
9	3.185	653	667	684	rBV	36252	75325	5.13%	0.607%
10	3.339	710	715	718	rBV2	353	297	0.02%	0.002%
11	3.368	721	724	727	rVB2	254	174	0.01%	0.001%
12	3.468	752	755	759	rBV2	171	139	0.01%	0.001%
13	3.522	769	772	775	rBV2	143	105	0.01%	0.001%
14	3.545	776	779	782	rVB2	234	136	0.01%	0.001%
15	3.709	826	830	832	rBV2	135	105	0.01%	0.001%
16	3.793	851	856	859	rBV2	144	147	0.01%	0.001%
17	3.873	871	881	929	rBV2	126827	453103	30.87%	3.650%
18	4.339	1010	1026	1061	rBV	224076	559095	38.10%	4.504%
19	4.600	1096	1107	1125	rVB3	16711	41260	2.81%	0.332%
20	4.702	1134	1139	1141	rBV2	191	158	0.01%	0.001%
21	4.728	1143	1147	1150	rVV2	161	130	0.01%	0.001%
22	4.767	1157	1159	1163	rBV2	214	111	0.01%	0.001%
23	4.844	1179	1183	1185	rBV	121	98	0.01%	0.001%
24	4.921	1203	1207	1214	rBV2	136	190	0.01%	0.002%
25	4.960	1216	1219	1222	rVB2	221	114	0.01%	0.001%
26	5.040	1223	1244	1292	rBV2	552075	1467558	100.00%	11.822%
27	5.468	1374	1377	1379	rBV2	345	210	0.01%	0.002%
28	5.548	1400	1402	1408	rVB2	173	141	0.01%	0.001%
29	5.609	1408	1421	1446	rBV	573433	1149454	78.32%	9.259%
30	5.902	1503	1512	1522	rBV4	4711	10006	0.68%	0.081%
31	6.063	1548	1562	1597	rBV	313251	649528	44.26%	5.232%
32	6.243	1615	1618	1622	rVV2	502	377	0.03%	0.003%
33	6.262	1622	1624	1627	rVB	326	137	0.01%	0.001%
34	6.313	1635	1640	1642	rBV2	117	106	0.01%	0.001%
35	6.358	1649	1654	1656	rVB	183	121	0.01%	0.001%
36	6.374	1656	1659	1661	rBV	213	117	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029582.D
 Acq On : 10 Dec 2022 15:38
 Operator : SY/MD
 Sample : N5928-17 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.493	1693	1696	1698	rBV2	321	167	0.01%	0.001%
38	6.545	1708	1712	1714	rBV2	282	182	0.01%	0.001%
39	6.558	1714	1716	1723	rVB2	248	144	0.01%	0.001%
40	6.628	1727	1738	1741	rBV4	1133	1536	0.10%	0.012%
41	6.725	1764	1768	1771	rBV4	256	229	0.02%	0.002%
42	6.757	1776	1778	1781	rVB	216	103	0.01%	0.001%
43	6.780	1782	1785	1787	rBV2	278	163	0.01%	0.001%
44	6.847	1803	1806	1810	rVB2	196	109	0.01%	0.001%
45	6.873	1812	1814	1820	rVB2	319	275	0.02%	0.002%
46	6.915	1822	1827	1830	rBV2	241	195	0.01%	0.002%
47	6.979	1836	1847	1876	rBV	143552	266604	18.17%	2.148%
48	7.307	1936	1949	1968	rBV	674265	1188430	80.98%	9.573%
49	7.616	2034	2045	2070	rBV	102800	182135	12.41%	1.467%
50	7.815	2106	2107	2109	rBV	294	127	0.01%	0.001%
51	7.889	2128	2130	2132	rVB	249	116	0.01%	0.001%
52	7.927	2135	2142	2144	rBV3	537	722	0.05%	0.006%
53	8.082	2180	2190	2225	rBV	405795	733189	49.96%	5.906%
54	8.529	2323	2329	2331	rBV4	389	399	0.03%	0.003%
55	8.545	2332	2334	2335	rBV	347	149	0.01%	0.001%
56	8.680	2374	2376	2378	rVB	233	100	0.01%	0.001%
57	8.728	2387	2391	2398	rVB3	478	455	0.03%	0.004%
58	8.757	2398	2400	2403	rBV2	324	216	0.01%	0.002%
59	8.773	2403	2405	2409	rVB3	426	267	0.02%	0.002%
60	8.792	2409	2411	2412	rBV3	323	151	0.01%	0.001%
61	8.844	2414	2427	2453	rBV	825475	1365881	93.07%	11.003%
62	9.098	2502	2506	2509	rBV3	293	238	0.02%	0.002%
63	9.133	2509	2517	2525	rVV2	4209	6946	0.47%	0.056%
64	9.181	2529	2532	2539	rVB3	404	419	0.03%	0.003%
65	9.268	2557	2559	2563	rVB2	366	183	0.01%	0.001%
66	9.297	2563	2568	2571	rBV	265	280	0.02%	0.002%
67	9.384	2593	2595	2598	rBV	269	160	0.01%	0.001%
68	9.455	2613	2617	2619	rBV3	238	154	0.01%	0.001%
69	9.471	2619	2622	2624	rBV2	306	190	0.01%	0.002%
70	9.535	2635	2642	2655	rVB4	2483	3984	0.27%	0.032%
71	9.587	2655	2658	2660	rBV	251	184	0.01%	0.001%
72	9.657	2677	2680	2685	rBV3	282	217	0.01%	0.002%
73	9.882	2748	2750	2756	rBV3	246	208	0.01%	0.002%
74	9.921	2759	2762	2766	rBV3	591	447	0.03%	0.004%
75	10.082	2809	2812	2815	rBV	279	190	0.01%	0.002%
76	10.162	2825	2837	2841	rBV	21029	30337	2.07%	0.244%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029582.D
 Acq On : 10 Dec 2022 15:38
 Operator : SY/MD
 Sample : N5928-17 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.207	2842	2851	2870	rVB	468772	739089	50.36%	5.954%
78	10.336	2888	2891	2893	rBV2	758	560	0.04%	0.005%
79	10.442	2918	2924	2928	rBV5	991	1360	0.09%	0.011%
80	10.506	2942	2944	2946	rBV2	195	116	0.01%	0.001%
81	10.570	2956	2964	2976	rVB	9628	15281	1.04%	0.123%
82	10.628	2980	2982	2987	rVB2	517	385	0.03%	0.003%
83	10.654	2987	2990	2992	rBV	251	135	0.01%	0.001%
84	10.725	3005	3012	3013	rBV4	1514	1145	0.08%	0.009%
85	10.776	3025	3028	3031	rBV	188	165	0.01%	0.001%
86	10.905	3060	3068	3082	rVV3	5839	8447	0.58%	0.068%
87	10.966	3083	3087	3092	rVB2	298	261	0.02%	0.002%
88	11.008	3098	3100	3104	rVB2	243	175	0.01%	0.001%
89	11.133	3135	3139	3140	rBV	202	131	0.01%	0.001%
90	11.156	3144	3146	3148	rVV	226	109	0.01%	0.001%
91	11.236	3159	3171	3192	rBV	908391	1420559	96.80%	11.443%
92	11.522	3252	3260	3267	rBV6	1211	1929	0.13%	0.016%
93	11.612	3276	3288	3309	rBV	716045	1134431	77.30%	9.138%
94	11.847	3359	3361	3364	rBV3	294	131	0.01%	0.001%
95	11.969	3396	3399	3400	rBV2	217	134	0.01%	0.001%
96	11.998	3404	3408	3410	rBV	454	358	0.02%	0.003%
97	12.069	3428	3430	3435	rBV2	276	163	0.01%	0.001%
98	12.300	3501	3502	3503	rBV	385	108	0.01%	0.001%
99	12.734	3635	3637	3642	rBV3	345	367	0.03%	0.003%
100	13.278	3804	3806	3809	rBV3	485	303	0.02%	0.002%




Sum of corrected areas: 12414029

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029582.D
Acq On : 10 Dec 2022 15:38
Operator : SY/MD
Sample : N5928-17 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 76 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

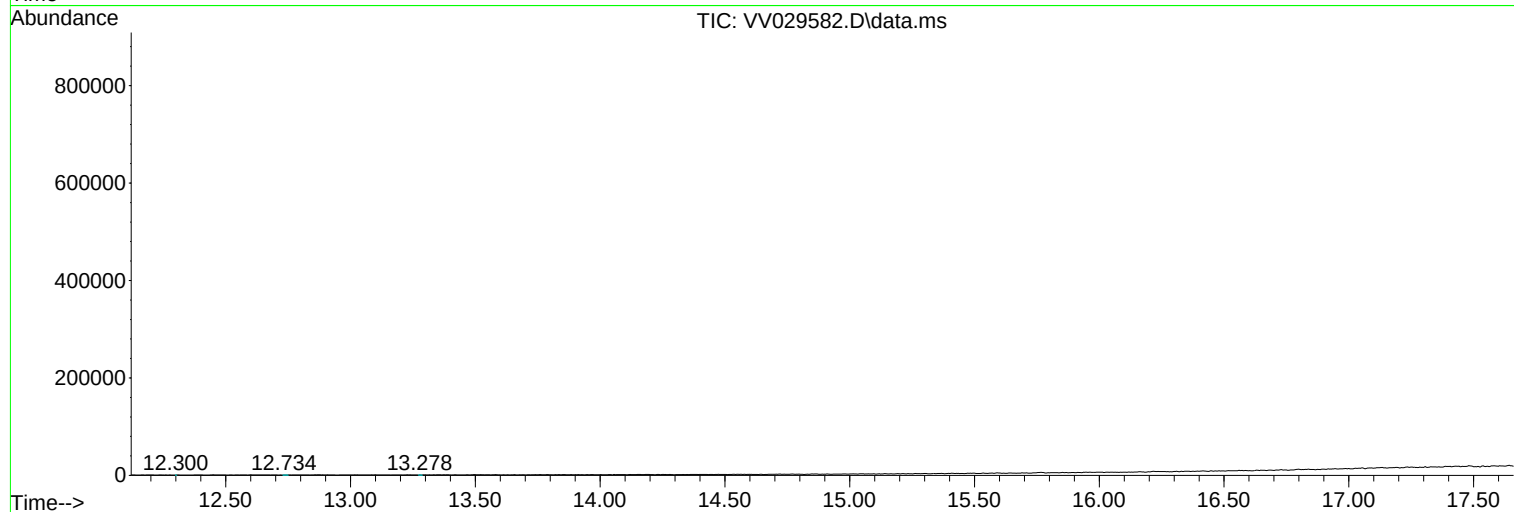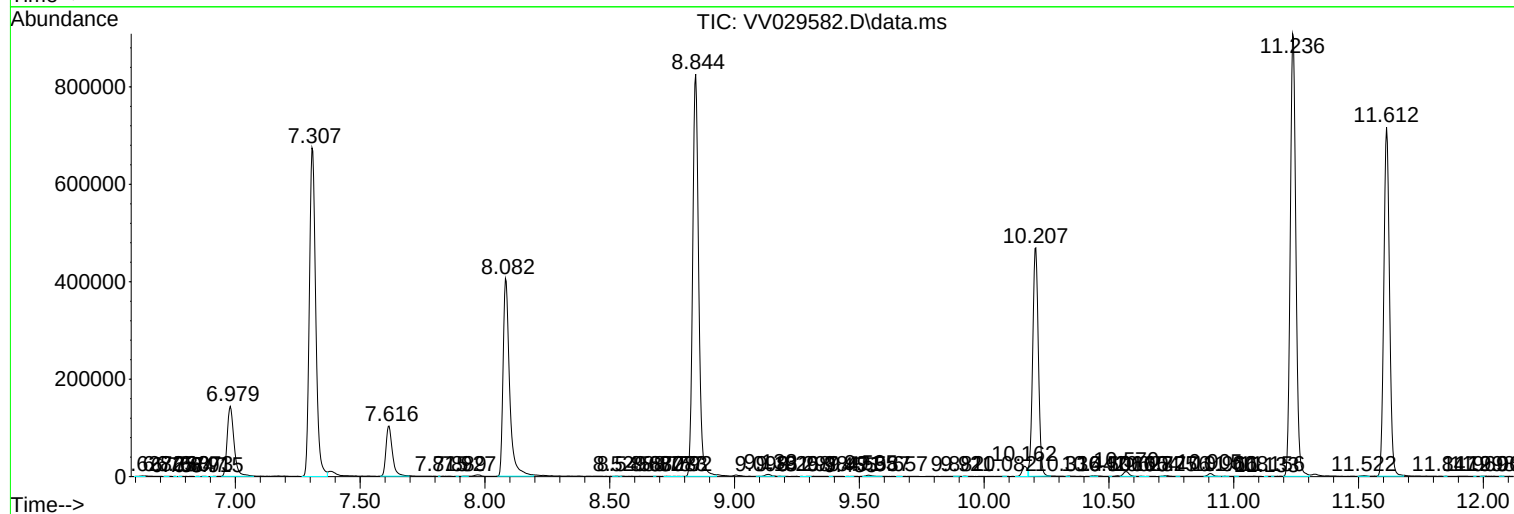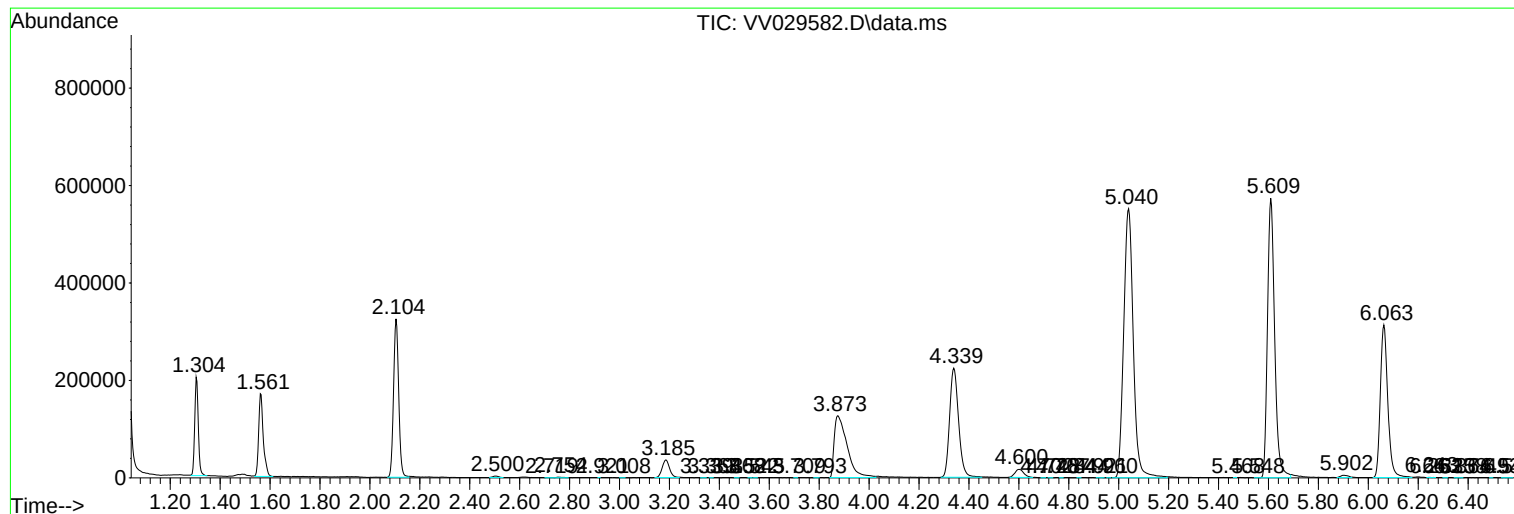

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029582.D
Acq On : 10 Dec 2022 15:38
Operator : SY/MD
Sample : N5928-17 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 76 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029582.D
Acq On : 10 Dec 2022 15:38
Operator : SY/MD
Sample : N5928-17 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 76 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc