

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029583.D
 Acq On : 10 Dec 2022 16:01
 Operator : SY/MD
 Sample : N5928-18 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	190137	190635	12.99%	1.556%
2	1.561	155	162	175	rVB	169045	190008	12.95%	1.550%
3	2.105	320	331	346	rBV	325080	465706	31.73%	3.800%
4	2.503	446	455	465	rVB3	4778	7359	0.50%	0.060%
5	2.571	473	476	477	rBV2	194	114	0.01%	0.001%
6	2.619	482	491	499	rBV4	937	2054	0.14%	0.017%
7	2.690	510	513	517	rBV2	223	222	0.02%	0.002%
8	2.754	530	533	534	rBV	137	76	0.01%	0.001%
9	2.995	605	608	613	rBV	300	195	0.01%	0.002%
10	3.108	640	643	646	rVB2	256	141	0.01%	0.001%
11	3.185	659	667	674	rBV4	928	1712	0.12%	0.014%
12	3.301	698	703	705	rBV2	153	143	0.01%	0.001%
13	3.336	712	714	718	rVB2	288	138	0.01%	0.001%
14	3.458	747	752	759	rBV2	245	303	0.02%	0.002%
15	3.500	759	765	768	rBV	215	185	0.01%	0.002%
16	3.523	769	772	774	rBV2	114	81	0.01%	0.001%
17	3.690	821	824	830	rBV2	206	180	0.01%	0.001%
18	3.809	856	861	862	rBV	124	102	0.01%	0.001%
19	3.873	869	881	929	rBV2	122238	382443	26.06%	3.121%
20	4.339	1010	1026	1049	rBV	227746	560345	38.18%	4.573%
21	4.722	1141	1145	1148	rVB2	204	138	0.01%	0.001%
22	4.802	1168	1170	1173	rVB2	208	118	0.01%	0.001%
23	4.847	1179	1184	1185	rBV	156	115	0.01%	0.001%
24	4.892	1195	1198	1200	rVB	129	72	0.00%	0.001%
25	4.937	1208	1212	1214	rBV2	107	76	0.01%	0.001%
26	4.970	1219	1222	1226	rBV2	343	308	0.02%	0.003%
27	5.040	1227	1244	1296	rBV2	556324	1467595	100.00%	11.976%
28	5.346	1337	1339	1341	rVB	271	109	0.01%	0.001%
29	5.513	1388	1391	1392	rBV	313	144	0.01%	0.001%
30	5.548	1398	1402	1404	rBV2	179	105	0.01%	0.001%
31	5.561	1404	1406	1407	rBV2	189	90	0.01%	0.001%
32	5.609	1407	1421	1469	rBV	571029	1178129	80.28%	9.614%
33	5.905	1505	1513	1528	rVB6	4264	9646	0.66%	0.079%
34	6.063	1548	1562	1588	rBV	316300	650434	44.32%	5.308%
35	6.330	1642	1645	1650	rVV2	227	163	0.01%	0.001%
36	6.426	1672	1675	1678	rVB	137	83	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029583.D
 Acq On : 10 Dec 2022 16:01
 Operator : SY/MD
 Sample : N5928-18 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.449	1678	1682	1685	rBV2	226	155	0.01%	0.001%
38	6.465	1685	1687	1692	rVB2	273	208	0.01%	0.002%
39	6.490	1692	1695	1698	rBV	203	159	0.01%	0.001%
40	6.619	1730	1735	1740	rBV2	937	1132	0.08%	0.009%
41	6.703	1759	1761	1767	rVB3	467	350	0.02%	0.003%
42	6.748	1768	1775	1778	rVB4	347	478	0.03%	0.004%
43	6.780	1782	1785	1789	rBV2	306	155	0.01%	0.001%
44	6.815	1794	1796	1799	rBV	224	118	0.01%	0.001%
45	6.841	1802	1804	1808	rVB2	390	218	0.01%	0.002%
46	6.876	1812	1815	1818	rBV3	222	154	0.01%	0.001%
47	6.979	1835	1847	1873	rBV	146709	269099	18.34%	2.196%
48	7.262	1931	1935	1937	rBV3	420	371	0.03%	0.003%
49	7.307	1937	1949	1980	rBV	684357	1200874	81.83%	9.799%
50	7.616	2033	2045	2075	rBV	102461	185678	12.65%	1.515%
51	7.760	2087	2090	2092	rBV3	298	235	0.02%	0.002%
52	7.786	2095	2098	2100	rBV3	324	155	0.01%	0.001%
53	7.818	2106	2108	2111	rBV3	453	269	0.02%	0.002%
54	7.883	2126	2128	2130	rBV2	252	147	0.01%	0.001%
55	8.002	2163	2165	2167	rBV2	286	140	0.01%	0.001%
56	8.085	2180	2191	2225	rBV	402823	731785	49.86%	5.971%
57	8.477	2310	2313	2315	rBV	256	168	0.01%	0.001%
58	8.574	2339	2343	2344	rBV3	260	226	0.02%	0.002%
59	8.632	2359	2361	2363	rVB	296	122	0.01%	0.001%
60	8.654	2363	2368	2371	rBV2	383	308	0.02%	0.003%
61	8.674	2371	2374	2376	rBV	221	121	0.01%	0.001%
62	8.796	2409	2412	2414	rBV	232	173	0.01%	0.001%
63	8.844	2414	2427	2455	rBV	845806	1387780	94.56%	11.324%
64	9.153	2521	2523	2529	rBV2	293	193	0.01%	0.002%
65	9.178	2529	2531	2535	rVB2	298	120	0.01%	0.001%
66	9.211	2538	2541	2543	rBV	250	156	0.01%	0.001%
67	9.262	2555	2557	2559	rVB	422	187	0.01%	0.002%
68	9.281	2560	2563	2566	rVB	190	121	0.01%	0.001%
69	9.301	2566	2569	2571	rBV	337	187	0.01%	0.002%
70	9.320	2571	2575	2580	rVB3	233	236	0.02%	0.002%
71	9.497	2625	2630	2632	rBV2	261	204	0.01%	0.002%
72	9.538	2639	2643	2645	rVB2	240	163	0.01%	0.001%
73	9.638	2671	2674	2675	rBV	240	100	0.01%	0.001%
74	9.725	2698	2701	2702	rBV	207	92	0.01%	0.001%
75	9.895	2751	2754	2757	rBV	196	160	0.01%	0.001%
76	9.937	2764	2767	2768	rBV	242	145	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029583.D
 Acq On : 10 Dec 2022 16:01
 Operator : SY/MD
 Sample : N5928-18 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.976	2777	2779	2781	rBV	208	70	0.00%	0.001%
78	10.162	2826	2837	2841	rBV3	19876	29115	1.98%	0.238%
79	10.207	2842	2851	2871	rVB	467504	739056	50.36%	6.031%
80	10.339	2889	2892	2895	rBV2	139	78	0.01%	0.001%
81	10.358	2895	2898	2901	rBV2	320	187	0.01%	0.002%
82	10.458	2927	2929	2931	rBV	164	106	0.01%	0.001%
83	10.567	2955	2963	2976	rBV3	9332	14777	1.01%	0.121%
84	10.764	3019	3024	3028	rBV2	265	254	0.02%	0.002%
85	10.818	3039	3041	3043	rBV	181	107	0.01%	0.001%
86	10.844	3047	3049	3053	rVB2	280	146	0.01%	0.001%
87	10.902	3061	3067	3070	rBV4	450	469	0.03%	0.004%
88	10.918	3070	3072	3078	rVB3	444	357	0.02%	0.003%
89	10.966	3085	3087	3089	rBV	179	77	0.01%	0.001%
90	11.178	3151	3153	3158	rVB2	188	116	0.01%	0.001%
91	11.236	3159	3171	3199	rBV	923985	1431650	97.55%	11.682%
92	11.432	3231	3232	3236	rVB2	460	283	0.02%	0.002%
93	11.452	3236	3238	3242	rVB2	549	295	0.02%	0.002%
94	11.612	3274	3288	3317	rBV	727275	1143380	77.91%	9.330%
95	12.005	3407	3410	3413	rBV2	337	242	0.02%	0.002%
96	12.075	3429	3432	3436	rBV3	305	269	0.02%	0.002%
97	12.220	3475	3477	3480	rBV2	389	208	0.01%	0.002%
98	12.297	3498	3501	3503	rBV2	411	213	0.01%	0.002%
99	12.435	3541	3544	3546	rBV2	309	210	0.01%	0.002%
100	12.587	3584	3591	3593	rBV3	575	698	0.05%	0.006%




Sum of corrected areas: 12254672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029583.D
Acq On : 10 Dec 2022 16:01
Operator : SY/MD
Sample : N5928-18 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 77 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

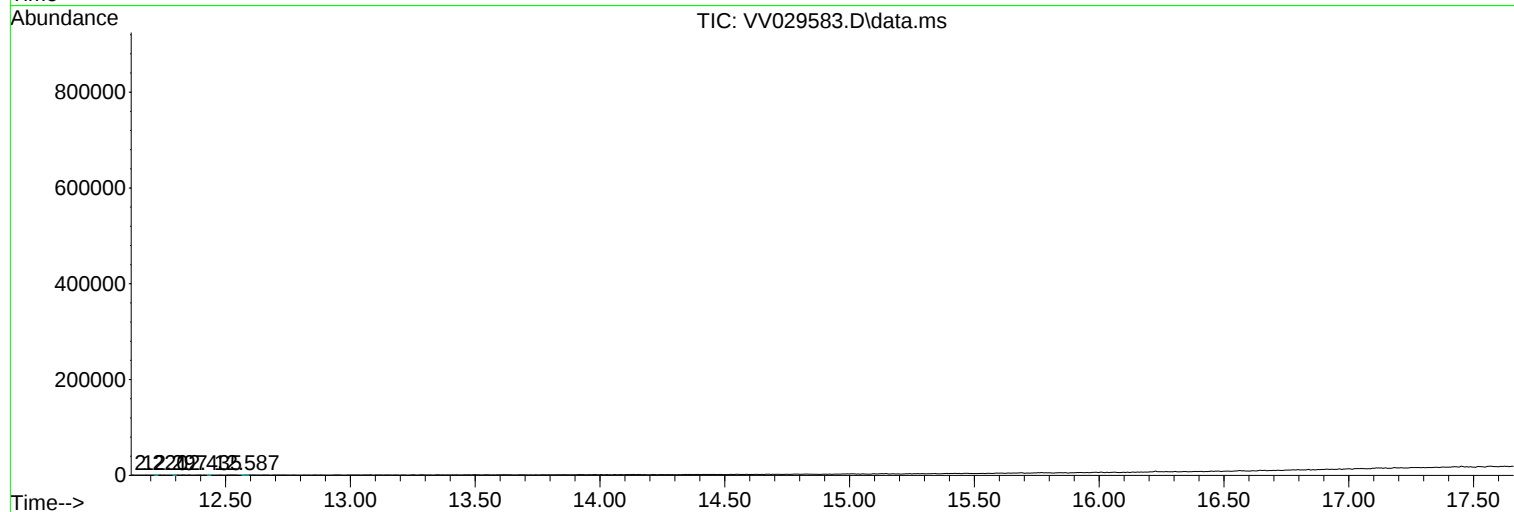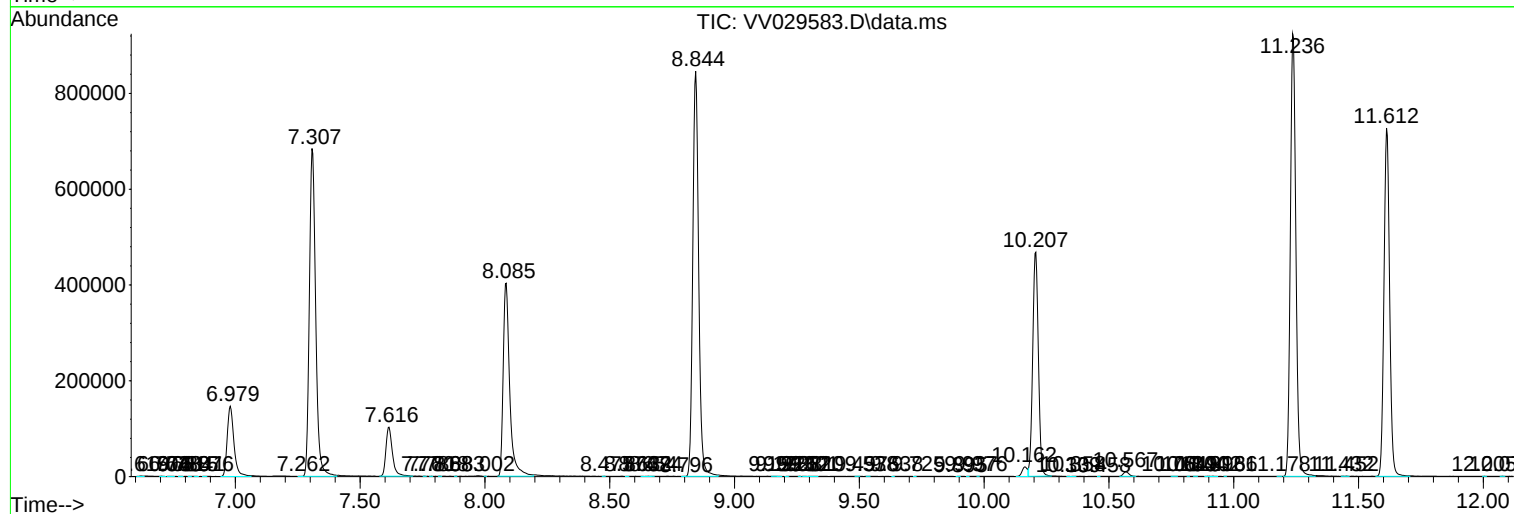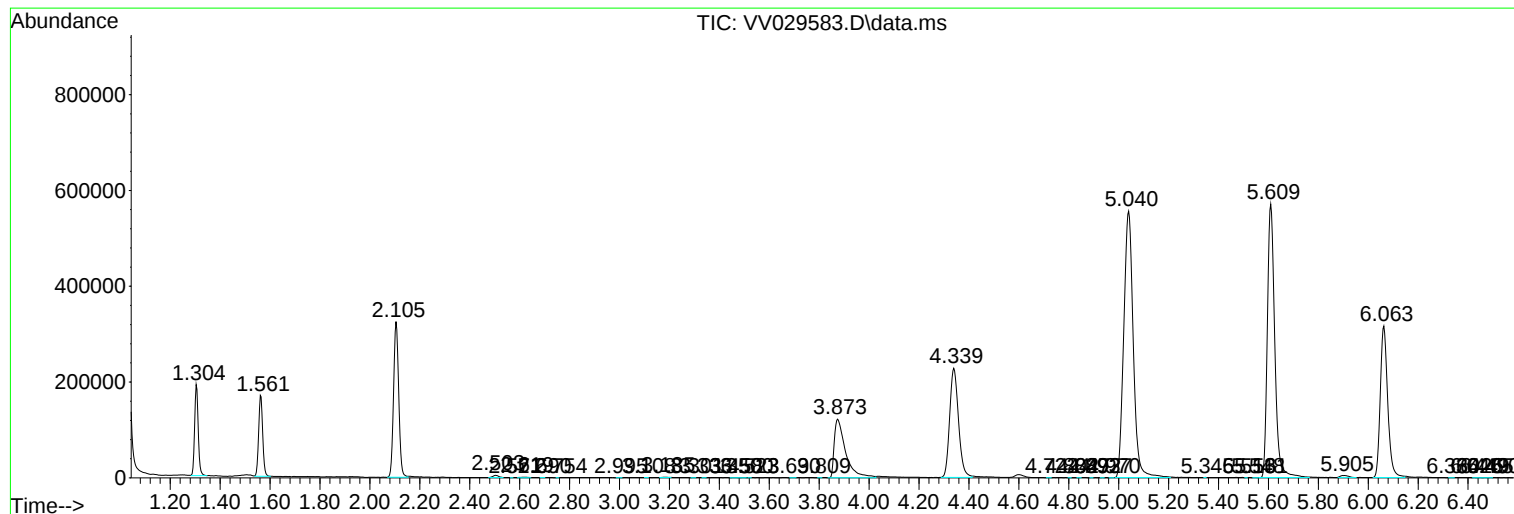

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029583.D
Acq On : 10 Dec 2022 16:01
Operator : SY/MD
Sample : N5928-18 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 77 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029583.D
Acq On : 10 Dec 2022 16:01
Operator : SY/MD
Sample : N5928-18 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 77 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc