

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029584.D
 Acq On : 10 Dec 2022 16:25
 Operator : SY/MD
 Sample : N5928-19 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	195356	198169	13.89%	1.591%
2	1.565	155	163	177	rVB	161599	190352	13.34%	1.528%
3	2.105	321	331	346	rBV	312305	450482	31.58%	3.616%
4	2.372	409	414	418	rBV	289	271	0.02%	0.002%
5	2.507	447	456	464	rBV4	3256	5187	0.36%	0.042%
6	2.577	475	478	481	rVB2	287	218	0.02%	0.002%
7	2.725	522	524	529	rVB2	225	142	0.01%	0.001%
8	2.761	529	535	539	rBV4	1218	1595	0.11%	0.013%
9	2.954	591	595	597	rBV2	180	168	0.01%	0.001%
10	2.995	606	608	613	rVB2	448	220	0.02%	0.002%
11	3.027	613	618	620	rBV2	171	146	0.01%	0.001%
12	3.063	626	629	635	rVB	195	119	0.01%	0.001%
13	3.185	653	667	688	rBV2	34726	74076	5.19%	0.595%
14	3.352	716	719	721	rBV2	232	106	0.01%	0.001%
15	3.436	740	745	748	rBV2	222	240	0.02%	0.002%
16	3.516	766	770	774	rBV	157	172	0.01%	0.001%
17	3.600	793	796	799	rBV	169	109	0.01%	0.001%
18	3.725	833	835	838	rVB2	230	113	0.01%	0.001%
19	3.744	838	841	844	rVB	208	111	0.01%	0.001%
20	3.777	844	851	855	rBV2	179	192	0.01%	0.002%
21	3.815	860	863	866	rBV	172	113	0.01%	0.001%
22	3.899	869	889	932	rBV3	174411	659132	46.20%	5.291%
23	4.339	1011	1026	1054	rBV2	216747	536651	37.62%	4.308%
24	4.600	1093	1107	1128	rVB	50276	124652	8.74%	1.001%
25	4.741	1147	1151	1154	rBV2	289	213	0.01%	0.002%
26	4.818	1172	1175	1177	rBV2	202	135	0.01%	0.001%
27	5.040	1224	1244	1289	rBV2	539975	1406746	98.61%	11.292%
28	5.397	1352	1355	1358	rBV3	298	229	0.02%	0.002%
29	5.442	1365	1369	1371	rBV2	231	169	0.01%	0.001%
30	5.471	1376	1378	1382	rVV2	290	215	0.02%	0.002%
31	5.516	1389	1392	1396	rVB	152	124	0.01%	0.001%
32	5.561	1402	1406	1408	rBV2	159	111	0.01%	0.001%
33	5.609	1408	1421	1451	rBV	574143	1169609	81.99%	9.388%
34	5.902	1505	1512	1525	rVB6	5422	11181	0.78%	0.090%
35	6.063	1547	1562	1599	rBV	301136	626074	43.89%	5.025%
36	6.320	1639	1642	1646	rBV2	303	237	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029584.D
 Acq On : 10 Dec 2022 16:25
 Operator : SY/MD
 Sample : N5928-19 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.423	1670	1674	1676	rBV2	162	117	0.01%	0.001%
38	6.487	1691	1694	1697	rVB2	269	139	0.01%	0.001%
39	6.510	1697	1701	1703	rBV2	198	122	0.01%	0.001%
40	6.619	1730	1735	1738	rBV4	723	827	0.06%	0.007%
41	6.706	1759	1762	1764	rBV2	216	123	0.01%	0.001%
42	6.760	1774	1779	1782	rVB3	462	325	0.02%	0.003%
43	6.783	1782	1786	1793	rVB2	228	232	0.02%	0.002%
44	6.831	1793	1801	1803	rBV2	231	232	0.02%	0.002%
45	6.857	1807	1809	1813	rVB3	292	187	0.01%	0.002%
46	6.979	1836	1847	1873	rBV	138981	256677	17.99%	2.060%
47	7.124	1889	1892	1893	rBV	332	173	0.01%	0.001%
48	7.307	1937	1949	1970	rBV	654154	1154822	80.95%	9.269%
49	7.616	2034	2045	2065	rBV	98622	175451	12.30%	1.408%
50	7.780	2092	2096	2099	rBV	634	548	0.04%	0.004%
51	7.866	2120	2123	2129	rBV4	294	276	0.02%	0.002%
52	7.892	2129	2131	2132	rBV4	314	140	0.01%	0.001%
53	7.973	2148	2156	2164	rBV5	2905	4635	0.32%	0.037%
54	8.082	2180	2190	2228	rBV	388284	700637	49.11%	5.624%
55	8.571	2335	2342	2347	rBV3	490	558	0.04%	0.004%
56	8.596	2348	2350	2352	rBV	218	118	0.01%	0.001%
57	8.629	2358	2360	2364	rBV2	374	169	0.01%	0.001%
58	8.674	2368	2374	2377	rBV2	309	316	0.02%	0.003%
59	8.754	2395	2399	2401	rBV2	252	173	0.01%	0.001%
60	8.786	2406	2409	2411	rBV	276	129	0.01%	0.001%
61	8.844	2414	2427	2451	rBV	847645	1385349	97.11%	11.120%
62	9.137	2510	2518	2530	rVB	3591	5923	0.42%	0.048%
63	9.301	2567	2569	2574	rVB2	262	176	0.01%	0.001%
64	9.352	2581	2585	2591	rBV2	263	265	0.02%	0.002%
65	9.535	2635	2642	2651	rBV	4944	7504	0.53%	0.060%
66	9.616	2663	2667	2670	rBV2	204	184	0.01%	0.001%
67	9.709	2692	2696	2703	rVB3	230	301	0.02%	0.002%
68	9.747	2703	2708	2712	rBV3	231	230	0.02%	0.002%
69	9.802	2722	2725	2731	rVB	276	261	0.02%	0.002%
70	9.831	2731	2734	2739	rVB2	176	151	0.01%	0.001%
71	9.860	2739	2743	2744	rBV	268	156	0.01%	0.001%
72	9.915	2758	2760	2763	rBV2	233	152	0.01%	0.001%
73	10.001	2782	2787	2788	rBV	249	182	0.01%	0.001%
74	10.162	2828	2837	2841	rBV	18664	27693	1.94%	0.222%
75	10.207	2842	2851	2874	rVB	454401	708092	49.64%	5.684%
76	10.342	2888	2893	2899	rBV3	754	1014	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029584.D
 Acq On : 10 Dec 2022 16:25
 Operator : SY/MD
 Sample : N5928-19 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.532	2942	2952	2956	rBV2	2873	3959	0.28%	0.032%
78	10.567	2957	2963	2975	rVB2	8842	13782	0.97%	0.111%
79	10.667	2992	2994	2999	rVB2	235	146	0.01%	0.001%
80	10.731	3003	3014	3022	rBV2	3649	5257	0.37%	0.042%
81	10.841	3043	3048	3049	rBV2	355	281	0.02%	0.002%
82	10.908	3060	3069	3079	rVB2	7396	10931	0.77%	0.088%
83	10.953	3081	3083	3090	rVB2	221	153	0.01%	0.001%
84	10.998	3094	3097	3098	rBV2	208	107	0.01%	0.001%
85	11.037	3107	3109	3112	rVB	240	142	0.01%	0.001%
86	11.114	3127	3133	3134	rBV2	289	264	0.02%	0.002%
87	11.143	3138	3142	3143	rBV2	254	149	0.01%	0.001%
88	11.185	3150	3155	3159	rBV3	535	530	0.04%	0.004%
89	11.236	3159	3171	3192	rBV	917374	1426593	100.00%	11.451%
90	11.513	3252	3257	3268	rBV3	1625	2629	0.18%	0.021%
91	11.612	3276	3288	3315	rBV	696228	1095709	76.81%	8.795%
92	11.911	3377	3381	3391	rVB7	1975	2847	0.20%	0.023%
93	12.040	3418	3421	3424	rBV2	187	176	0.01%	0.001%
94	12.098	3435	3439	3441	rBV	384	303	0.02%	0.002%
95	12.156	3455	3457	3460	rBV2	365	227	0.02%	0.002%
96	12.207	3470	3473	3475	rBV	318	213	0.01%	0.002%
97	12.249	3484	3486	3489	rBV3	465	207	0.01%	0.002%
98	12.304	3500	3503	3508	rBV4	597	597	0.04%	0.005%
99	12.744	3637	3640	3645	rBV2	366	367	0.03%	0.003%
100	13.120	3754	3757	3760	rBV2	405	256	0.02%	0.002%




Sum of corrected areas: 12458363

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029584.D
Acq On : 10 Dec 2022 16:25
Operator : SY/MD
Sample : N5928-19 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 78 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

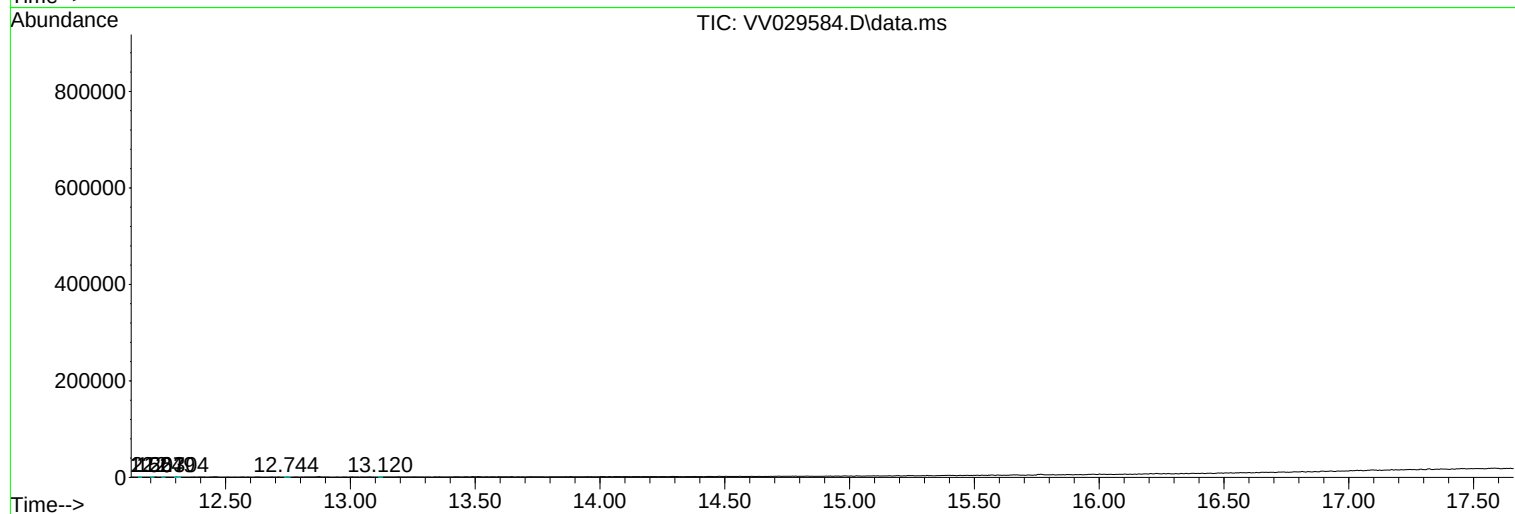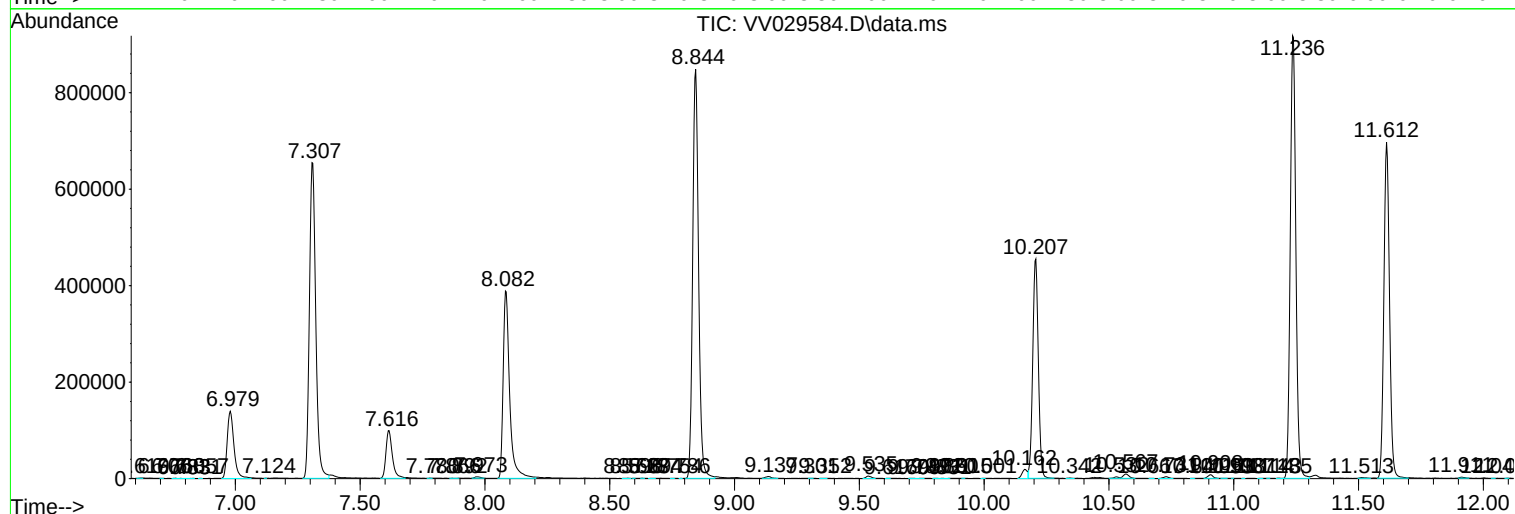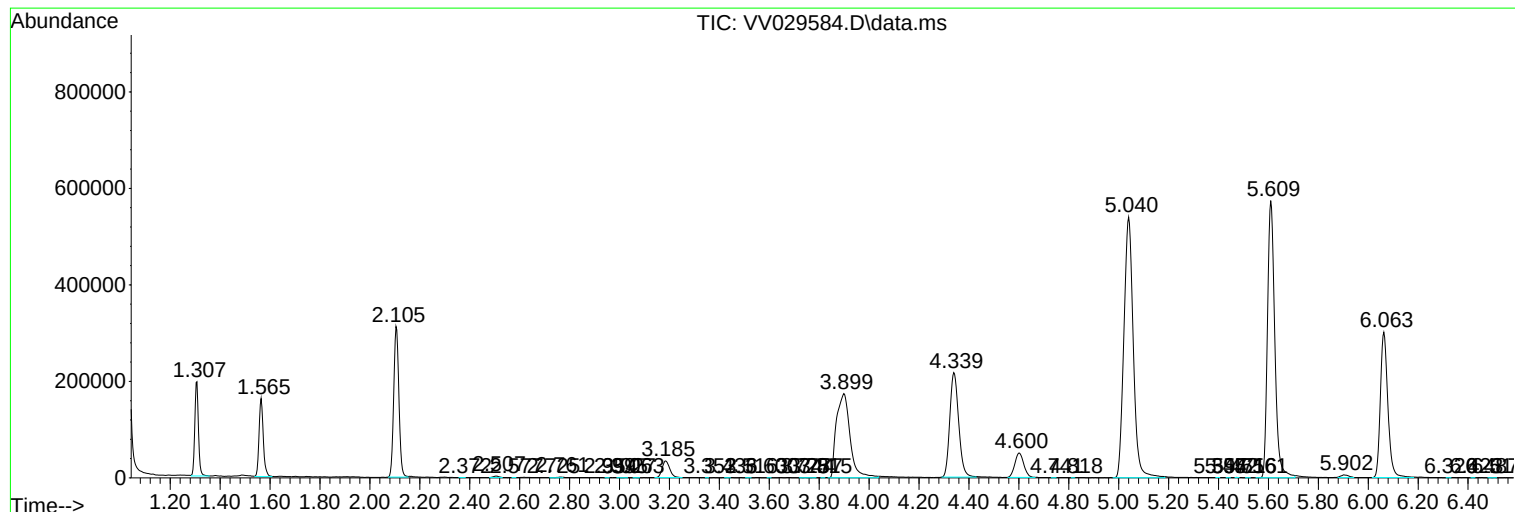

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029584.D
Acq On : 10 Dec 2022 16:25
Operator : SY/MD
Sample : N5928-19 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 78 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029584.D
Acq On : 10 Dec 2022 16:25
Operator : SY/MD
Sample : N5928-19 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 78 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------